

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102821\
 Data File : P0082291.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 12:40
 Operator : AJ\MA
 Sample : M4342-06 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-4-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 04:14:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.976	3.970	139542	48994	1.727	1.661
2) SA Decachlor...	11.092	9.292	92427	58965	1.663	2.315m#

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
Data File : PO082291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 12:40
Operator : AJ\MA
Sample : M4342-06 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-4-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 04:14:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

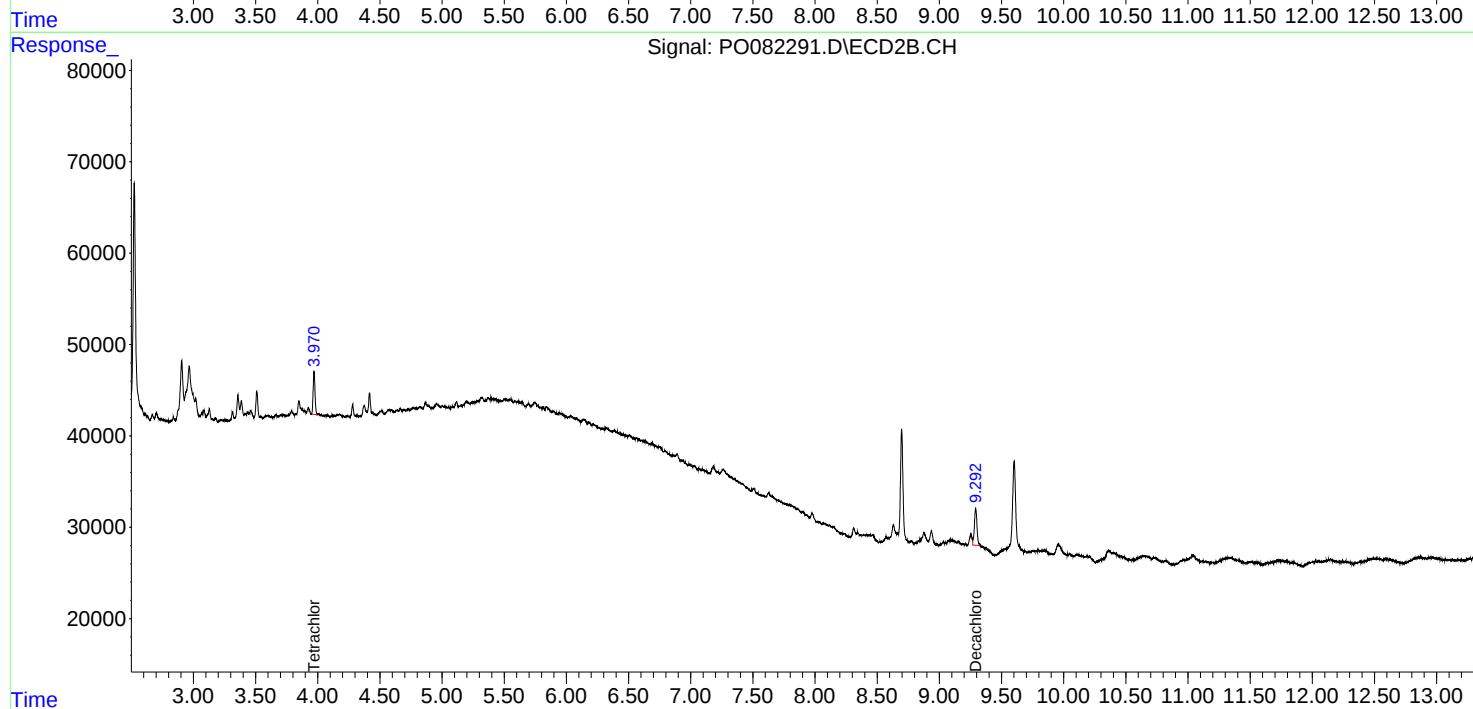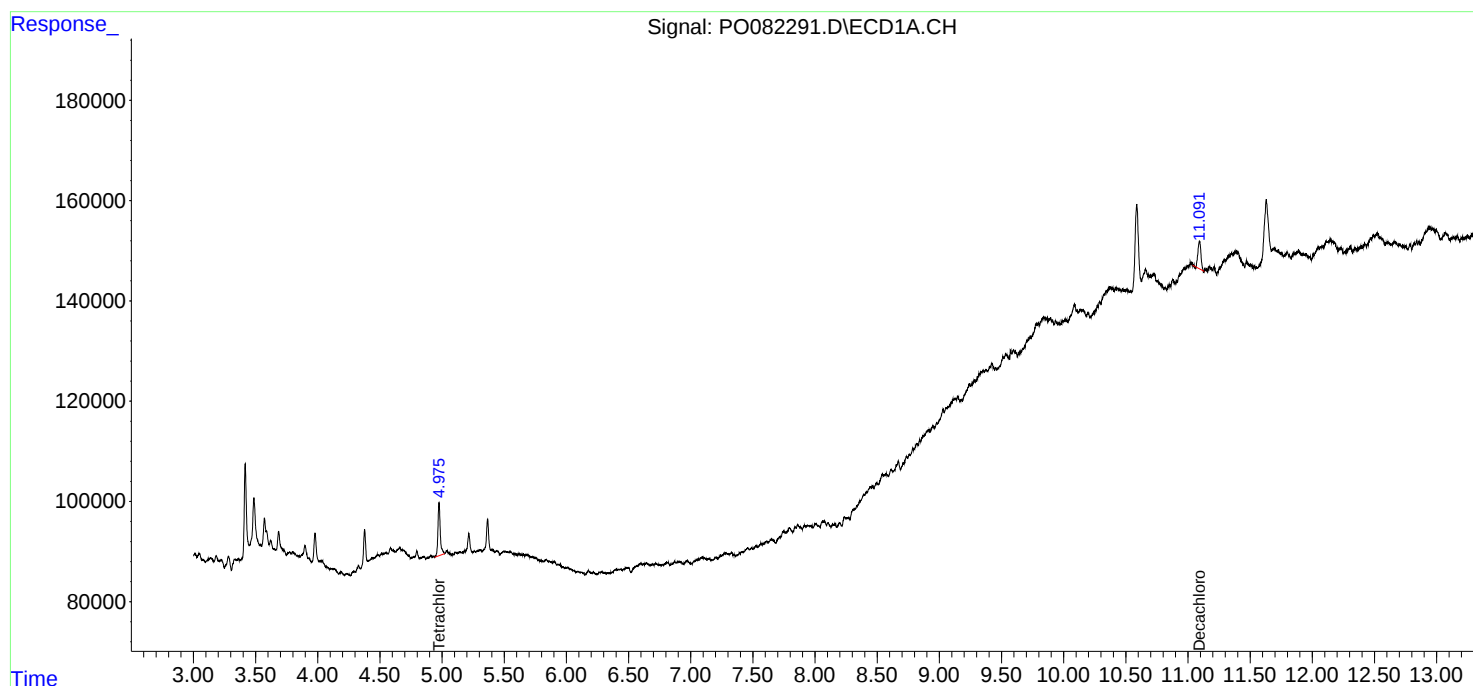


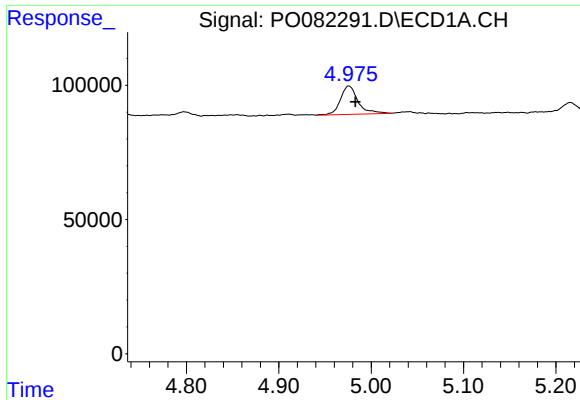

#1 Tetrachloro-m-xylene


R.T.: 4.976 min
Delta R.T.: -0.007 min
Response: 139542
Conc: 1.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-4-A

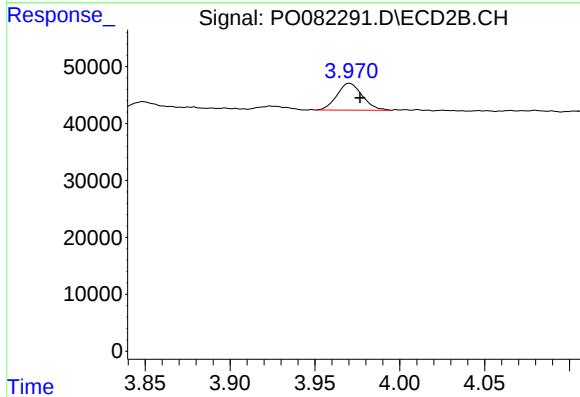


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: -0.006 min
Response: 48994
Conc: 1.66 ng/ml

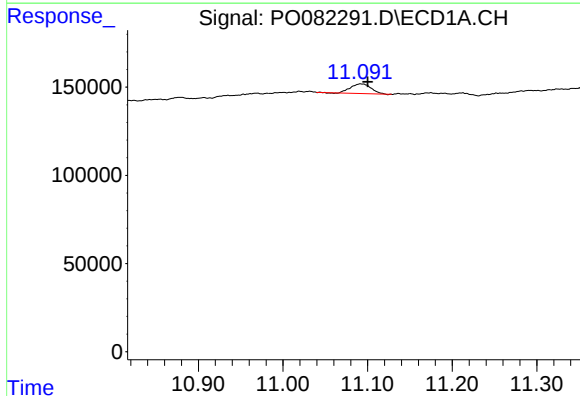

#2 Decachlorobiphenyl

R.T.: 11.092 min
Delta R.T.: -0.008 min
Response: 92427
Conc: 1.66 ng/ml

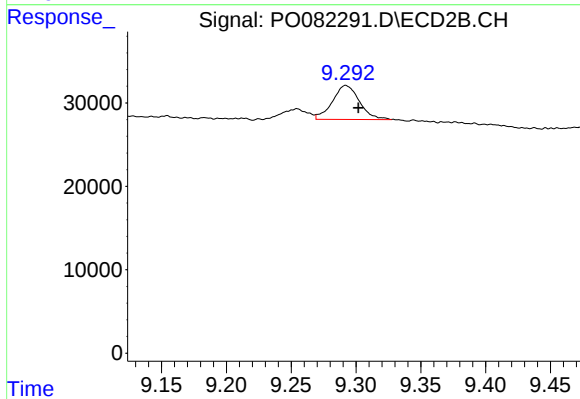

#2 Decachlorobiphenyl

R.T.: 9.292 min
Delta R.T.: -0.010 min
Response: 58965
Conc: 2.32 ng/ml m