

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102821\
 Data File : P0082293.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 13:15
 Operator : AJ\MA
 Sample : M4342-08 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-5-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:23:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.977	3.970	130088	50833	1.610	1.723
2) SA Decachlor...	11.091	9.295	194156	45431	3.493	1.784m#
Target Compounds						
41) L9 AR-1268-1	9.531	8.203	653630	306543	87.501	72.747
42) L9 AR-1268-2	9.630	8.268	744393	380877	110.034	100.265
43) L9 AR-1268-3	9.863	8.476	157152	66402	26.612	20.476
44) L9 AR-1268-4	10.317	8.766	452541	191794	178.831	138.068
45) L9 AR-1268-5	10.746	9.048	623995	261784	31.022	27.043



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
Data File : PO082293.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 13:15
Operator : AJ\MA
Sample : M4342-08 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
CLI-2021-5-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:23:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

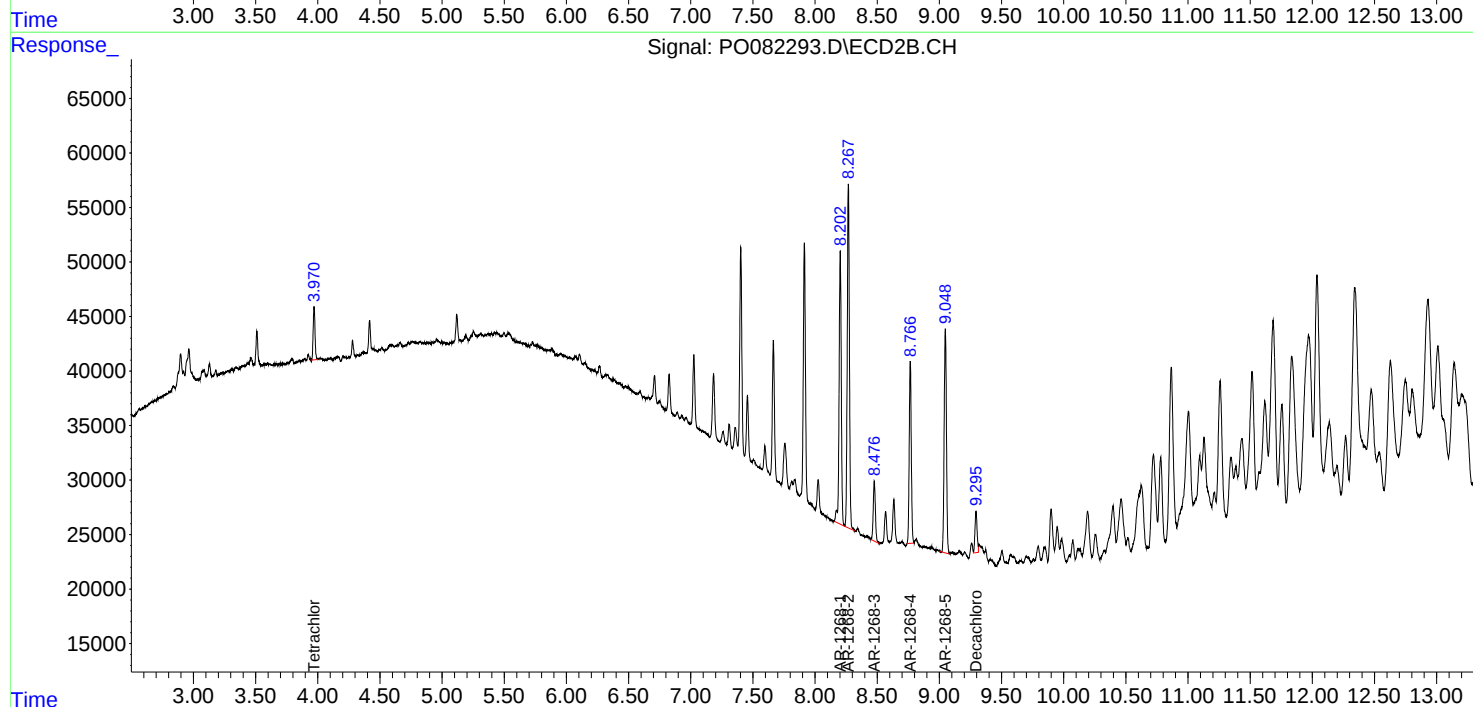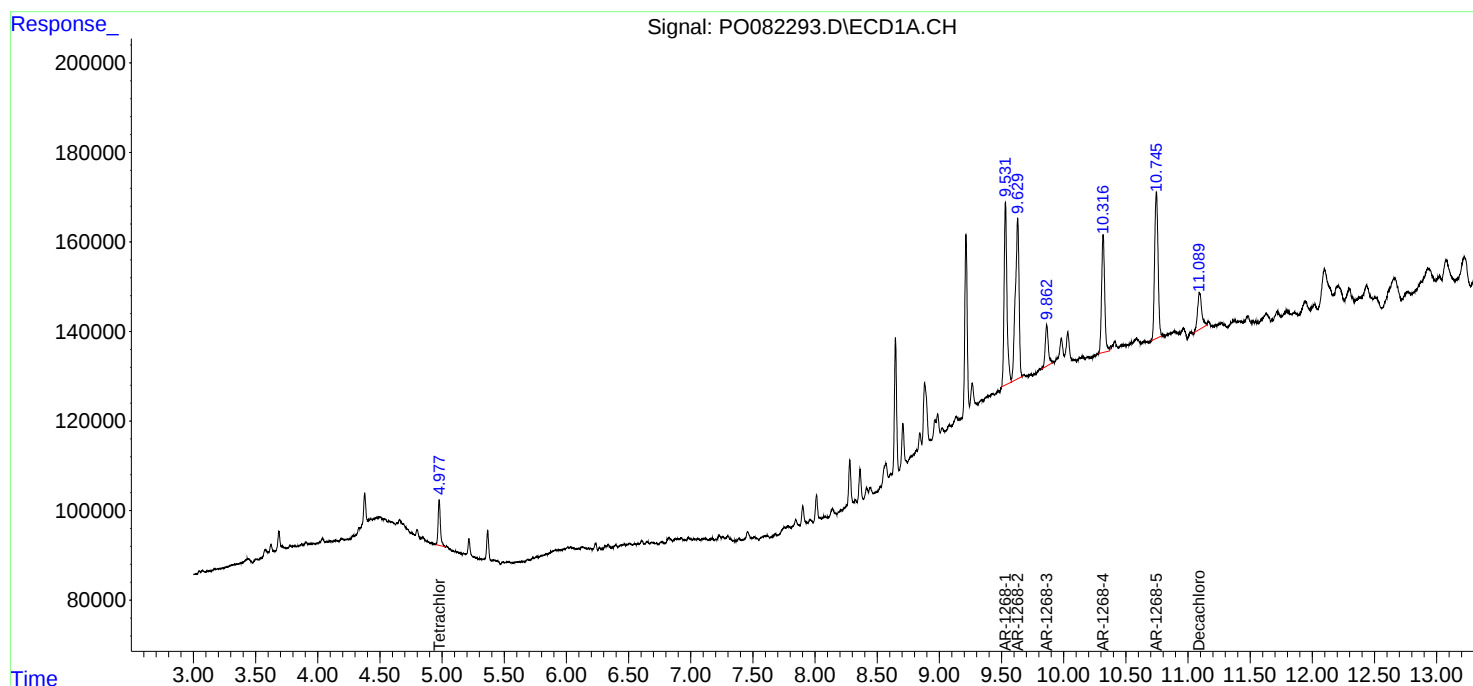


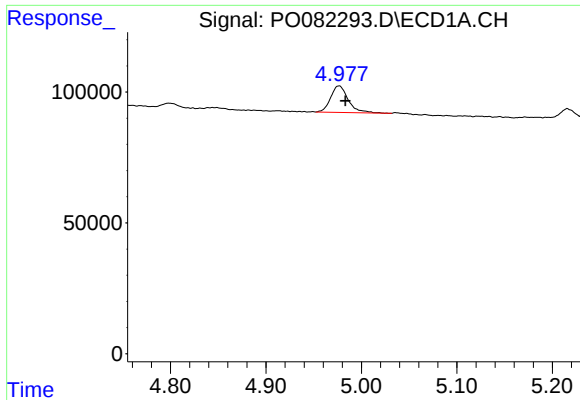

#1 Tetrachloro-m-xylene


R.T.: 4.977 min
Delta R.T.: -0.006 min
Response: 130088
Conc: 1.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-5-A

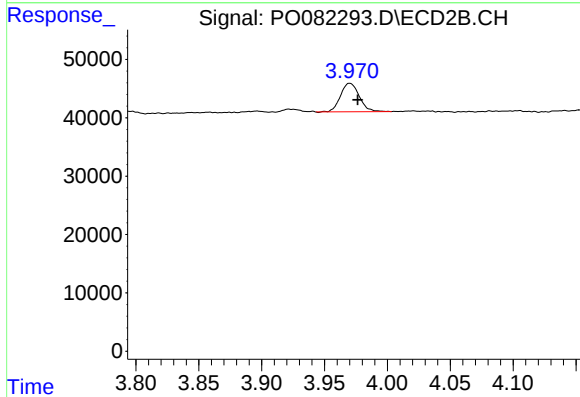


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: -0.006 min
Response: 50833
Conc: 1.72 ng/ml

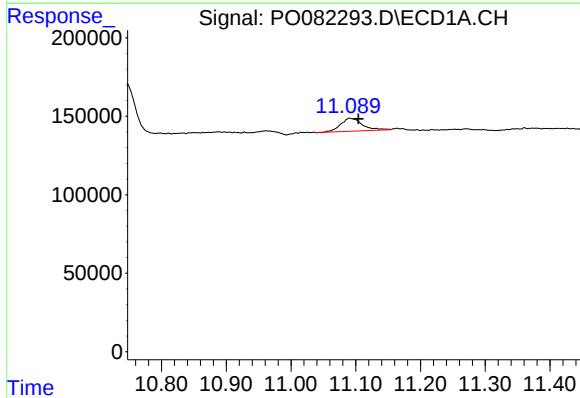


#2 Decachlorobiphenyl

R.T.: 11.091 min
Delta R.T.: -0.013 min
Response: 194156
Conc: 3.49 ng/ml

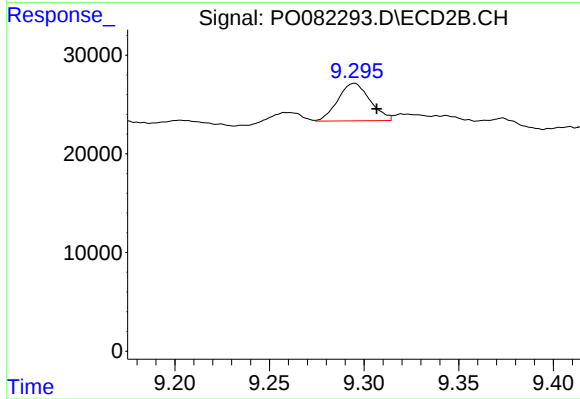

#2 Decachlorobiphenyl


R.T.: 9.295 min
Delta R.T.: -0.012 min
Response: 45431
Conc: 1.78 ng/ml m

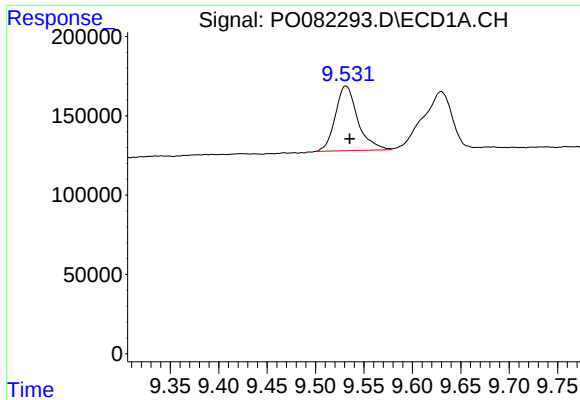

#41 AR-1268-1


R.T.: 9.531 min
Delta R.T.: -0.004 min
Response: 653630
Conc: 87.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-5-A

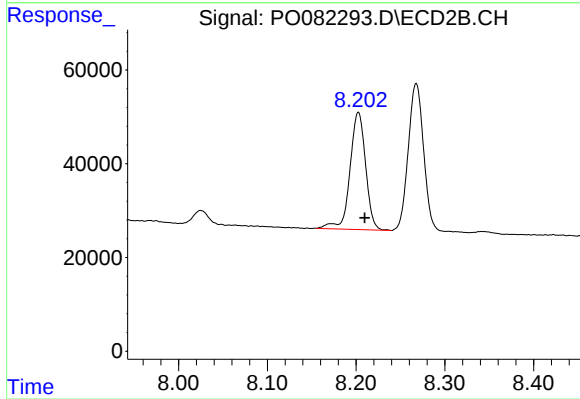


#41 AR-1268-1

R.T.: 8.203 min
Delta R.T.: -0.007 min
Response: 306543
Conc: 72.75 ng/ml

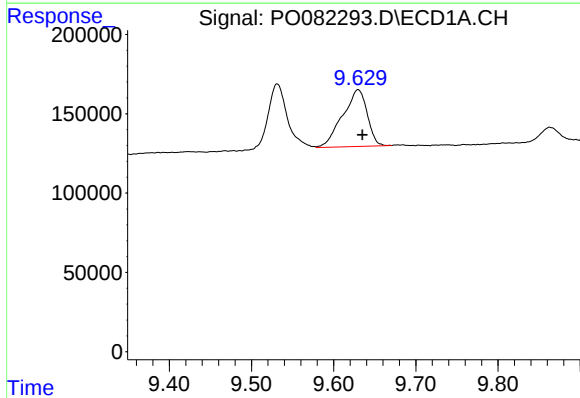


#42 AR-1268-2

R.T.: 9.630 min
Delta R.T.: -0.005 min
Response: 744393
Conc: 110.03 ng/ml

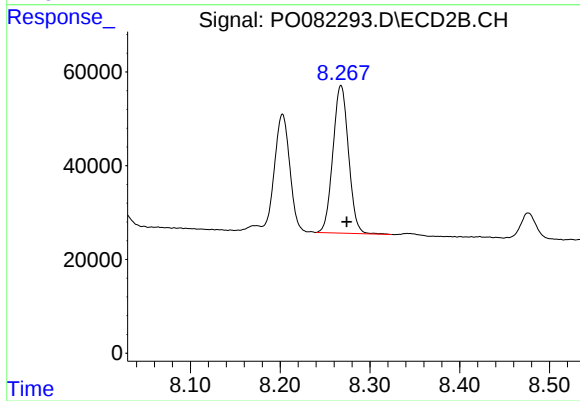

#42 AR-1268-2


R.T.: 8.268 min
Delta R.T.: -0.006 min
Response: 380877
Conc: 100.27 ng/ml

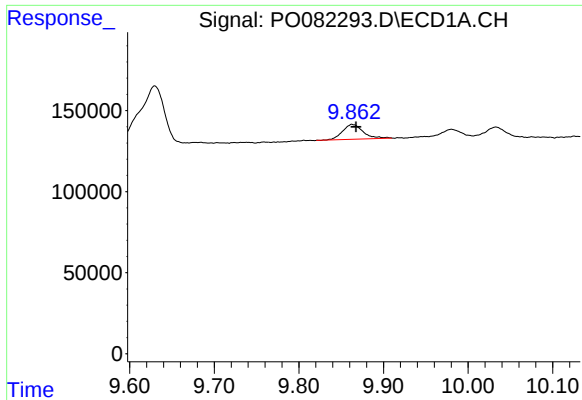

#43 AR-1268-3


R.T.: 9.863 min
Delta R.T.: -0.005 min
Response: 157152
Conc: 26.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-5-A

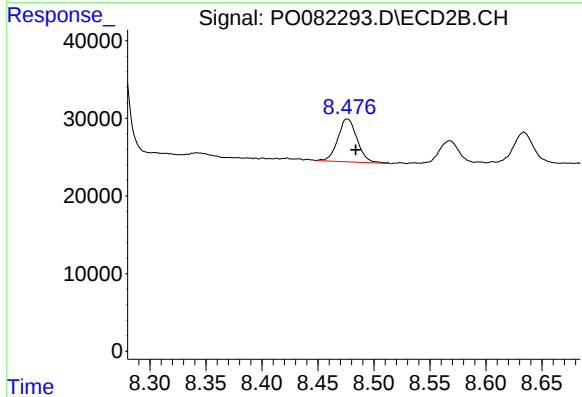


#43 AR-1268-3

R.T.: 8.476 min
Delta R.T.: -0.007 min
Response: 66402
Conc: 20.48 ng/ml

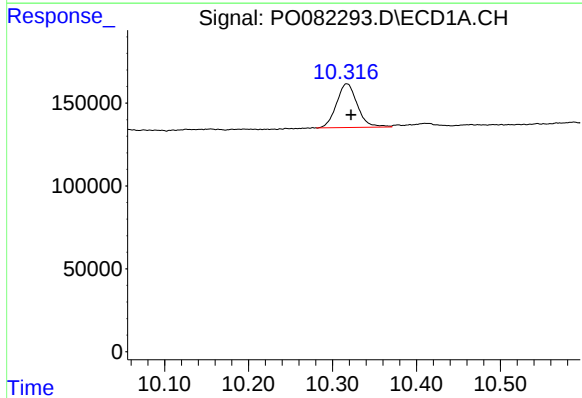


#44 AR-1268-4

R.T.: 10.317 min
Delta R.T.: -0.005 min
Response: 452541
Conc: 178.83 ng/ml

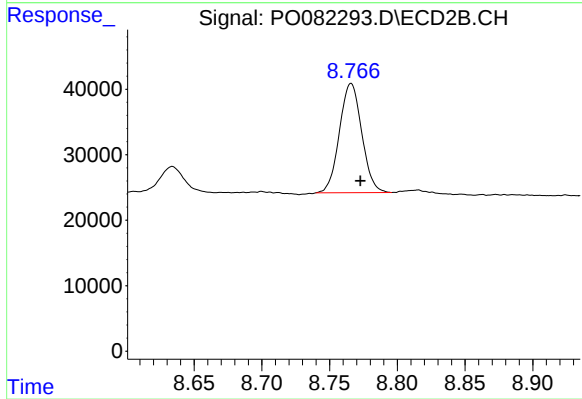

#44 AR-1268-4


R.T.: 8.766 min
Delta R.T.: -0.007 min
Response: 191794
Conc: 138.07 ng/ml

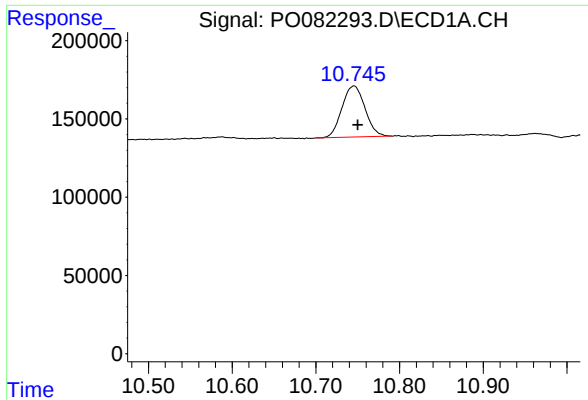

#45 AR-1268-5

R.T.: 10.746 min
Delta R.T.: -0.004 min
Response: 623995
Conc: 31.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-5-A

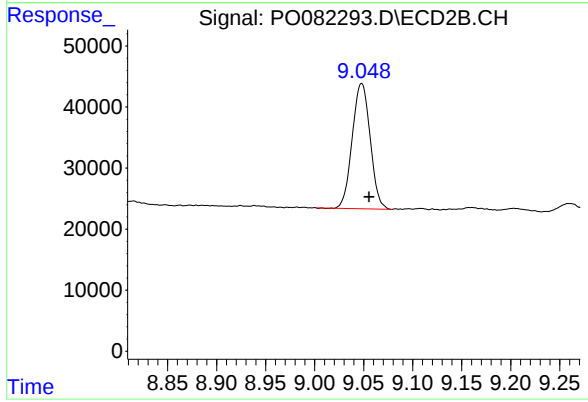

#45 AR-1268-5

R.T.: 9.048 min
Delta R.T.: -0.007 min
Response: 261784
Conc: 27.04 ng/ml