

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
 Data File : PO082300.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 15:38
 Operator : AJ\MA
 Sample : M4342-10 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-7-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 04:43:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.977	3.971	138621	51133	1.716	1.733
2) SA Decachlor...	11.094	9.294	129069	35337	2.322	1.387 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
Data File : PO082300.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 15:38
Operator : AJ\MA
Sample : M4342-10 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-7-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 04:43:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

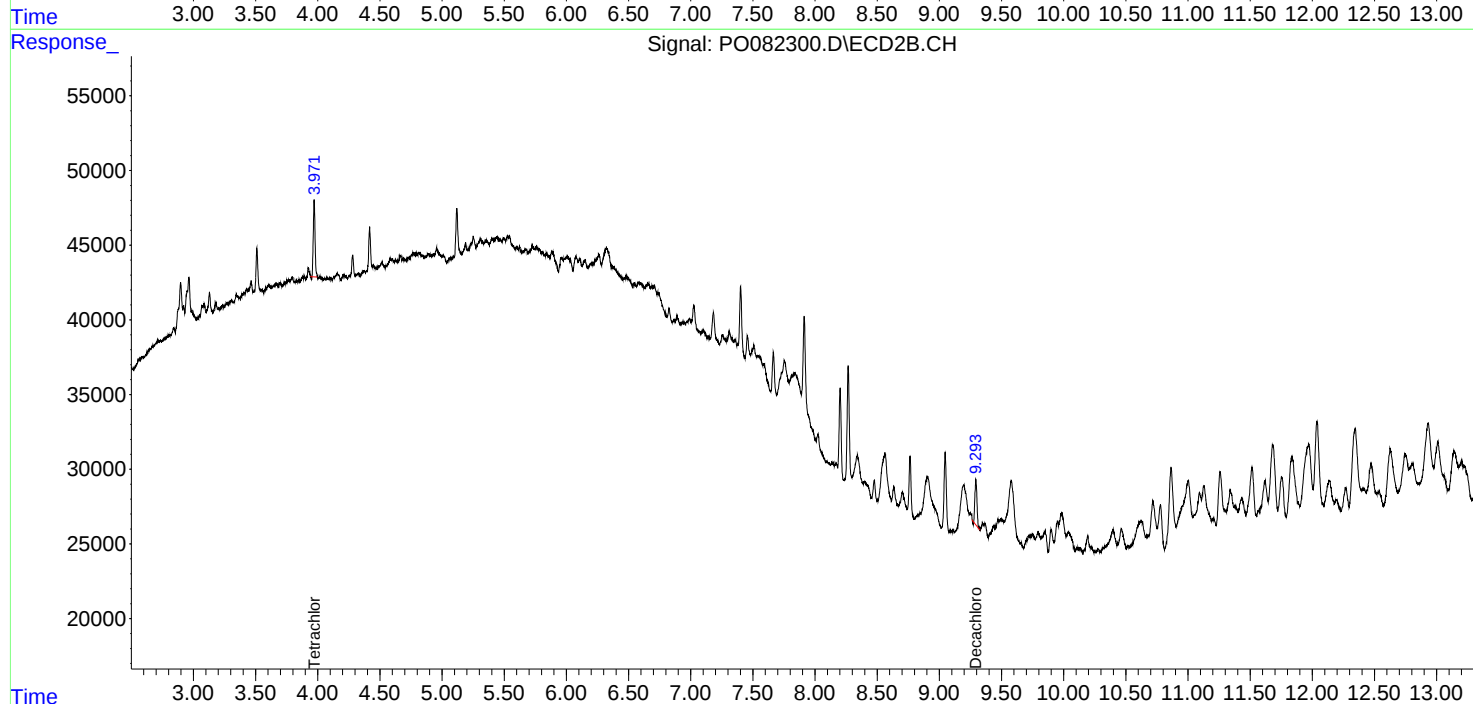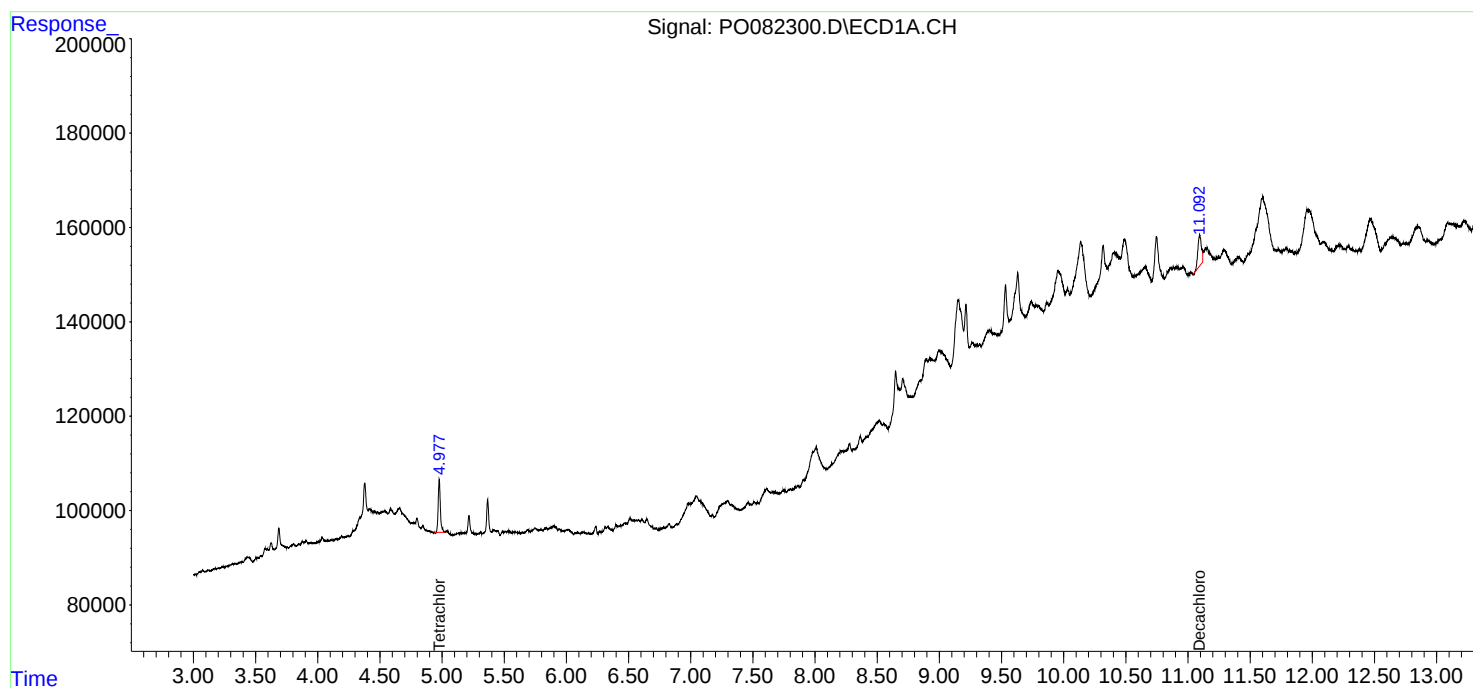


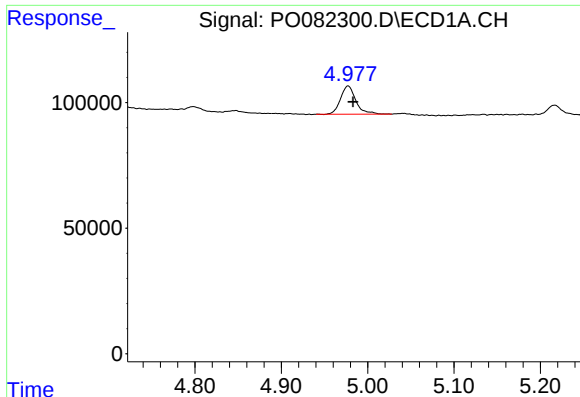

#1 Tetrachloro-m-xylene


R.T.: 4.977 min
Delta R.T.: -0.006 min
Response: 138621
Conc: 1.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-7-A

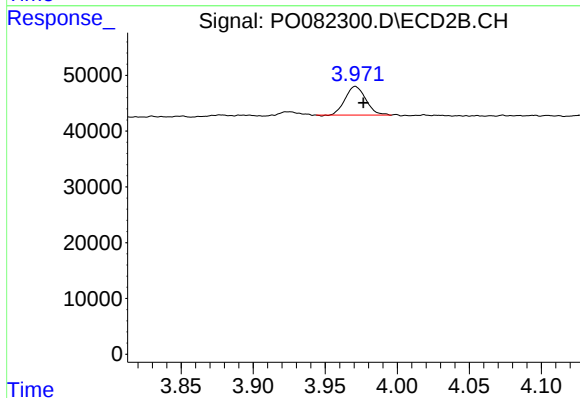


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: -0.006 min
Response: 51133
Conc: 1.73 ng/ml

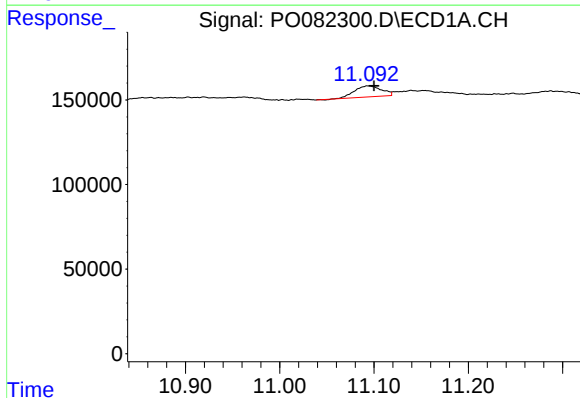

#2 Decachlorobiphenyl

R.T.: 11.094 min
Delta R.T.: -0.006 min
Response: 129069
Conc: 2.32 ng/ml

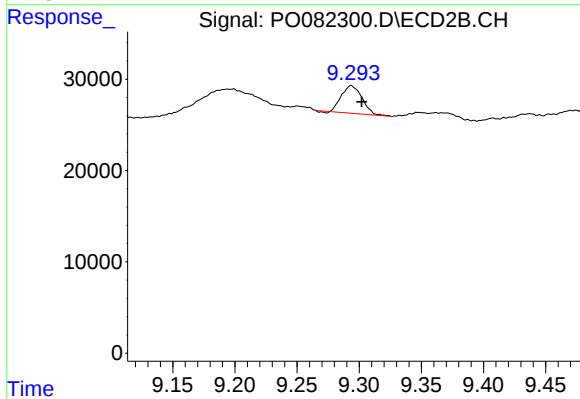

#2 Decachlorobiphenyl

R.T.: 9.294 min
Delta R.T.: -0.008 min
Response: 35337
Conc: 1.39 ng/ml