

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
 Data File : PO082313.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Oct 2021 19:57
 Operator : AJ\MA
 Sample : M4389-02 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IRV-2021-2A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 04:12:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 19 04:37:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.975	3.970	158755	54205	1.965	1.837
2) SA Decachlor...	11.091	9.291	115675	37554	2.081	1.474 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102821\
Data File : P0082313.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Oct 2021 19:57
Operator : AJ\MA
Sample : M4389-02 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IRV-2021-2A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 04:12:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 19 04:37:47 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

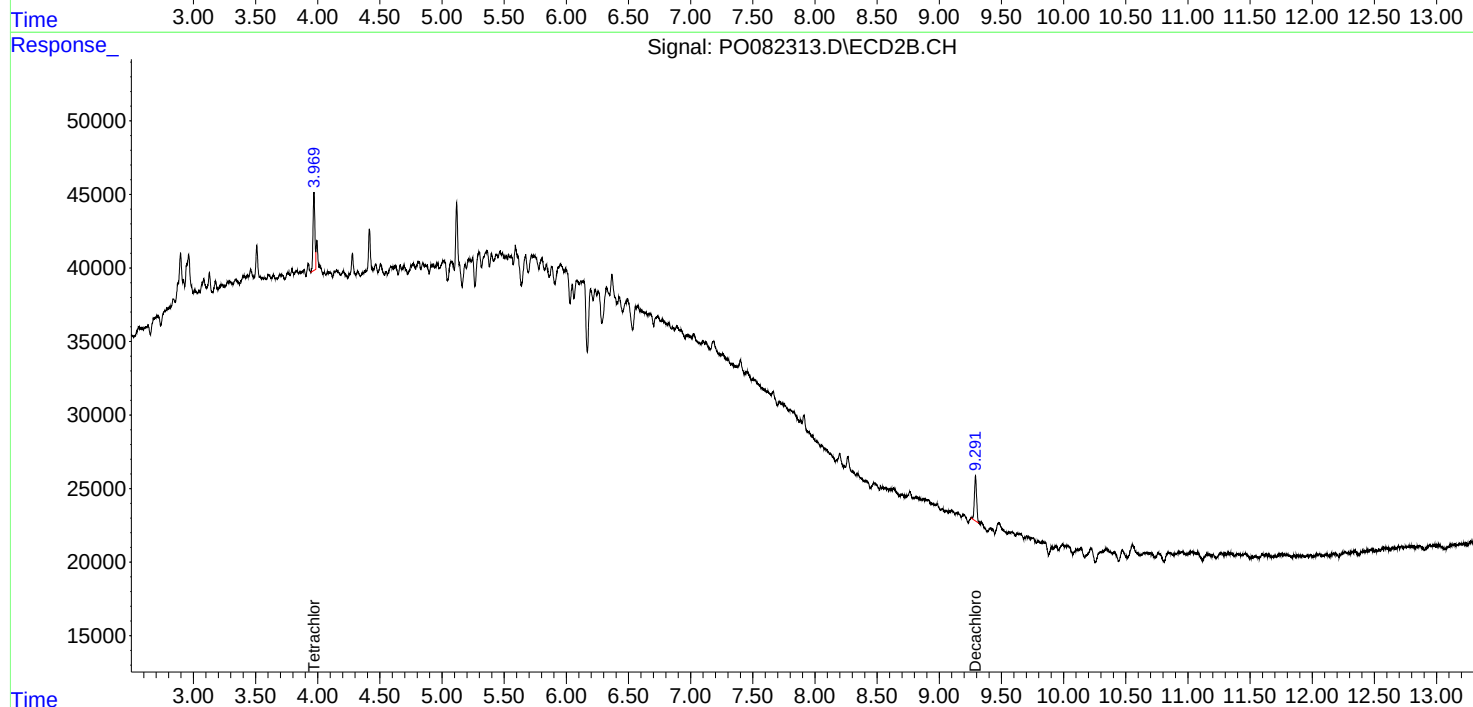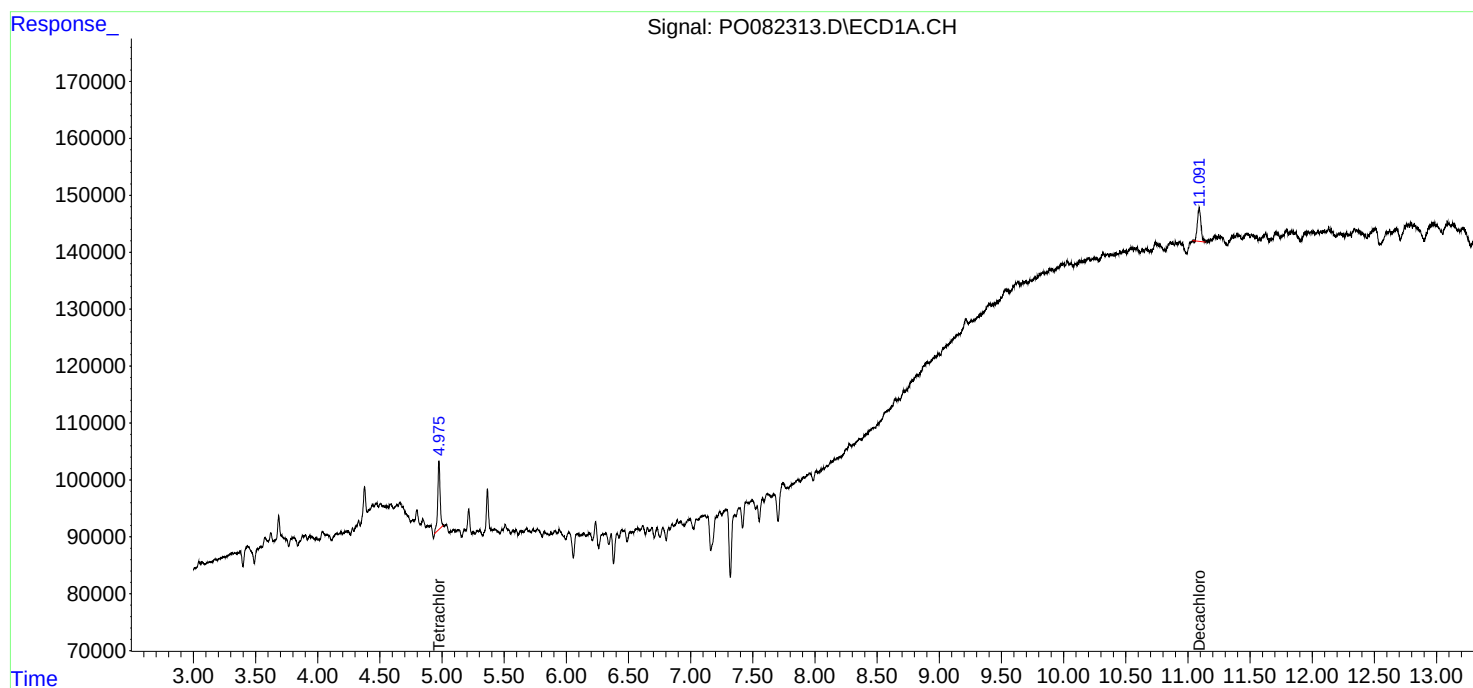


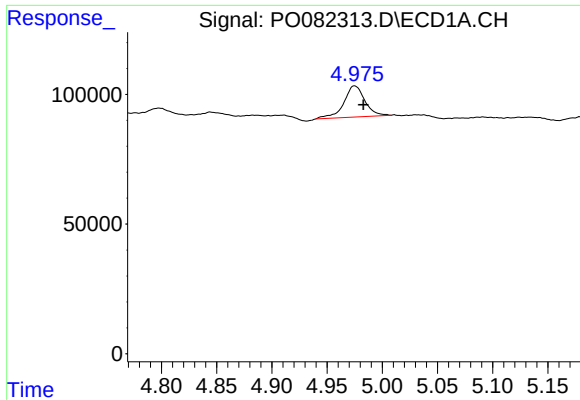

#1 Tetrachloro-m-xylene


R.T.: 4.975 min
Delta R.T.: -0.008 min
Response: 158755
Conc: 1.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
IRV-2021-2A

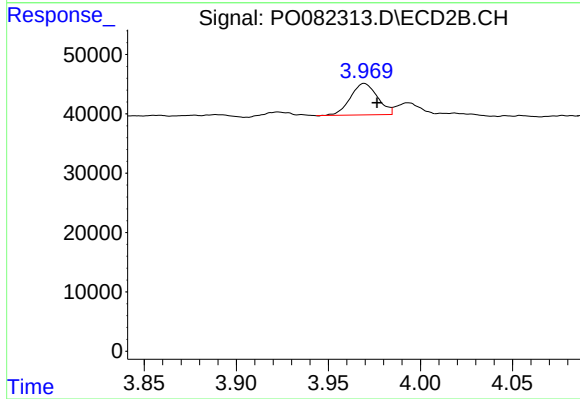


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: -0.007 min
Response: 54205
Conc: 1.84 ng/ml

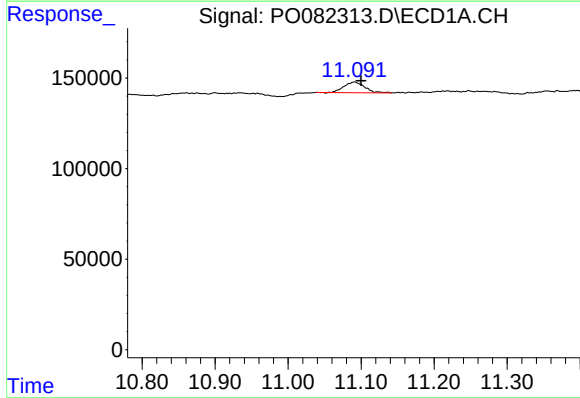

#2 Decachlorobiphenyl

R.T.: 11.091 min
Delta R.T.: -0.009 min
Response: 115675
Conc: 2.08 ng/ml

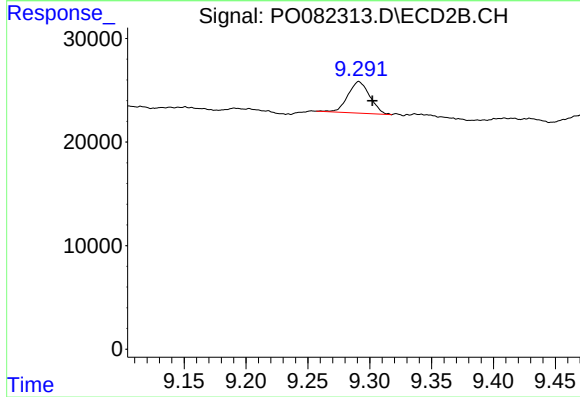

#2 Decachlorobiphenyl

R.T.: 9.291 min
Delta R.T.: -0.011 min
Response: 37554
Conc: 1.47 ng/ml