

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO102821\  
 Data File : PO082315.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 28 Oct 2021 20:31  
 Operator : AJ\MA  
 Sample : M4389-04 10X  
 Misc :  
 ALS Vial : 28 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 IRV-2021-3B

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 29 04:07:28 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO101821.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Oct 19 04:37:47 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml  |
|-----------------------------|--------|-------|--------|--------|-------|--------|
| -----                       |        |       |        |        |       |        |
| System Monitoring Compounds |        |       |        |        |       |        |
| 1) SA Tetrachlo...          | 4.976  | 3.971 | 107694 | 42407  | 1.333 | 1.437  |
| 2) SA Decachlor...          | 11.091 | 9.291 | 119387 | 52858  | 2.148 | 2.075m |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO102821\  
Data File : P0082315.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 28 Oct 2021 20:31  
Operator : AJ\MA  
Sample : M4389-04 10X  
Misc :  
ALS Vial : 28 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
IRV-2021-3B

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 29 04:07:28 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO101821.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Oct 19 04:37:47 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

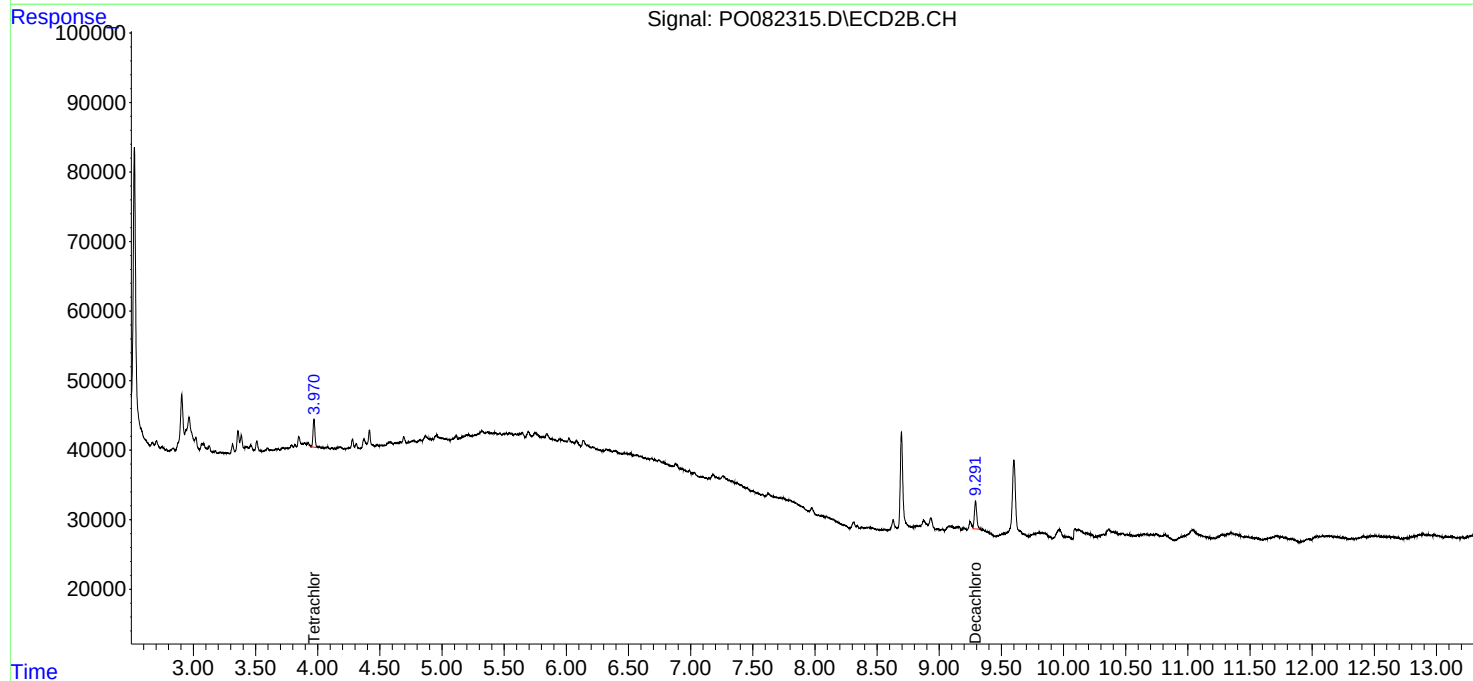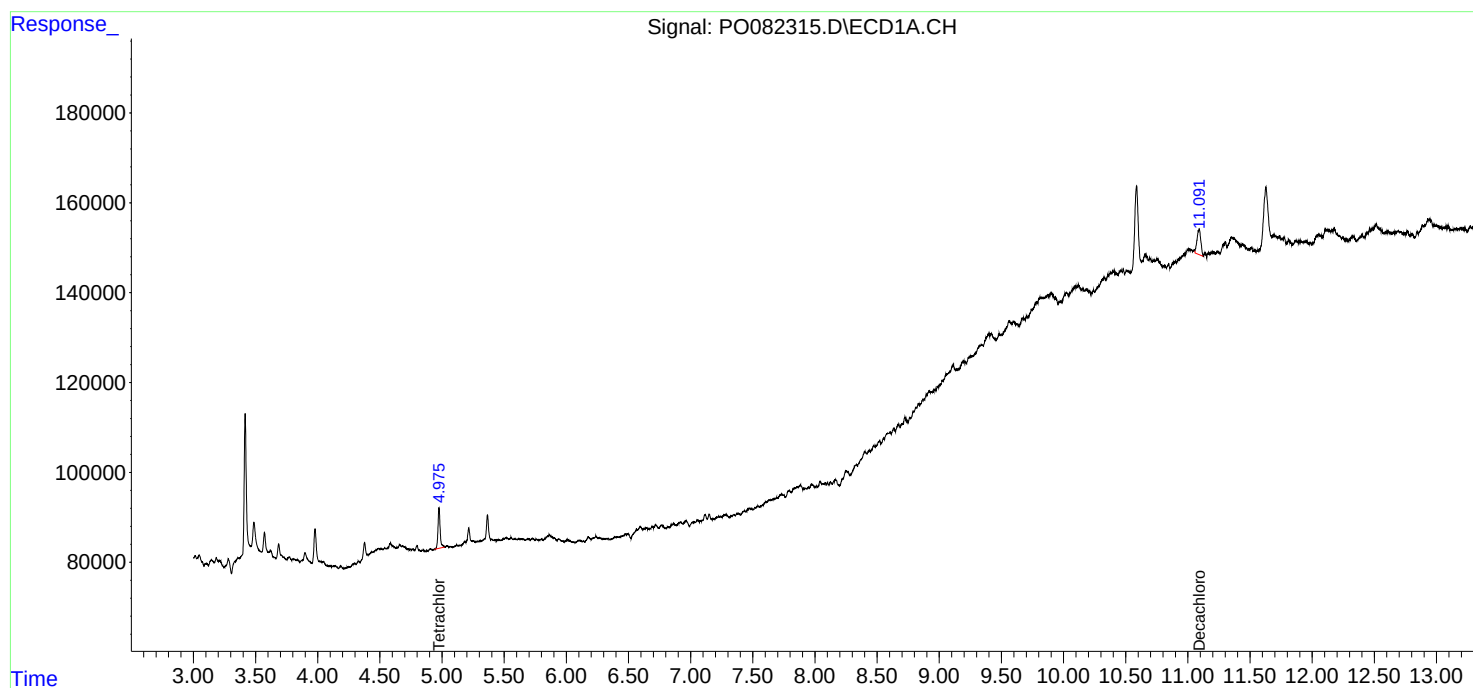


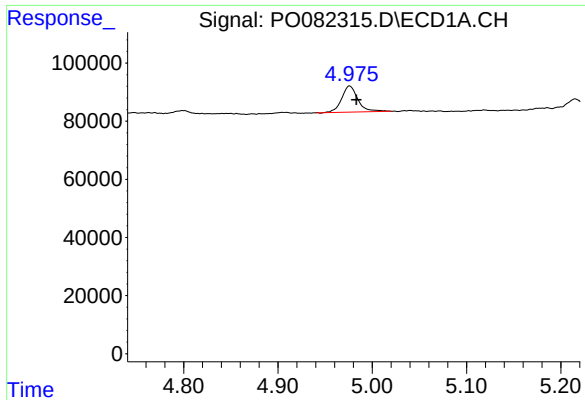

#1 Tetrachloro-m-xylene


R.T.: 4.976 min  
Delta R.T.: -0.007 min  
Response: 107694  
Conc: 1.33 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
IRV-2021-3B

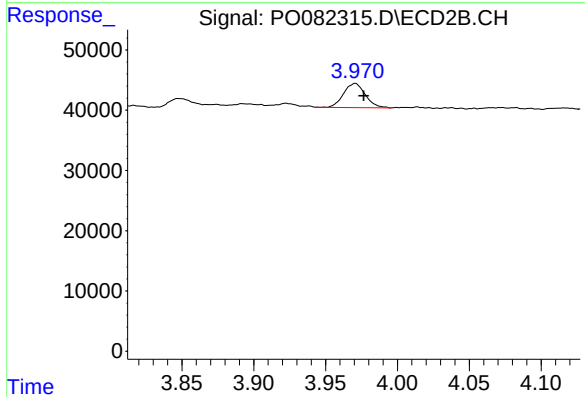


#1 Tetrachloro-m-xylene

R.T.: 3.971 min  
Delta R.T.: -0.006 min  
Response: 42407  
Conc: 1.44 ng/ml

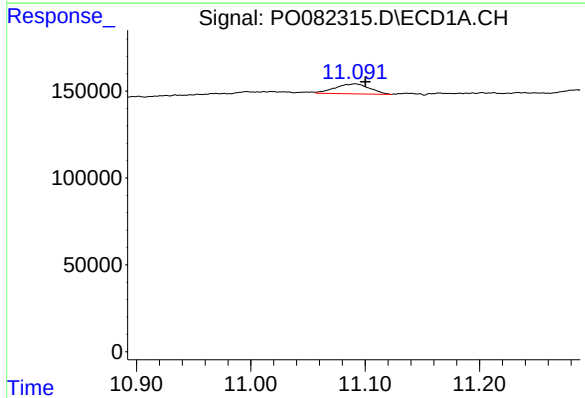

#2 Decachlorobiphenyl

R.T.: 11.091 min  
Delta R.T.: -0.009 min  
Response: 119387  
Conc: 2.15 ng/ml

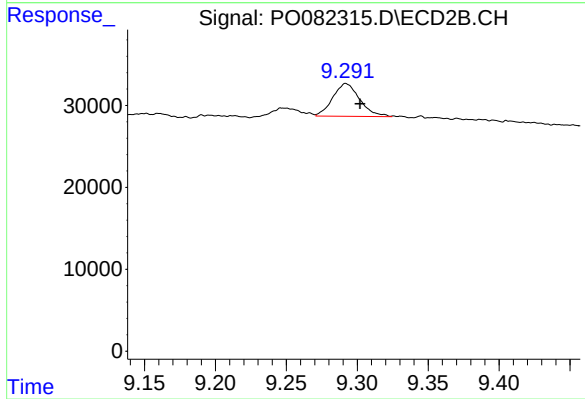

#2 Decachlorobiphenyl

R.T.: 9.291 min  
Delta R.T.: -0.011 min  
Response: 52858  
Conc: 2.08 ng/ml m