

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102822\
 Data File : PO090026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 19:52
 Operator : YP/AJ
 Sample : N4955-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:02:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.304	3.484	62971933	20694816	19.594	19.472
2) SA Decachlor...	10.045	8.489	54989358	21435992	22.440	20.813
Target Compounds						
11) L3 AR-1232-1	4.677	3.860	1939196	664051	29.613	27.912
12) L3 AR-1232-2	5.209	4.588	988922	543736	25.725	22.690
13) L3 AR-1232-3	5.501	4.765	1632705	255987	24.365	20.158
14) L3 AR-1232-4	5.662	4.849	682572	251418	20.673	20.621
15) L3 AR-1232-5	5.755	5.019	709187	228936	26.769	17.146 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102822\
Data File : PO090026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 19:52
Operator : YP/AJ
Sample : N4955-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:02:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

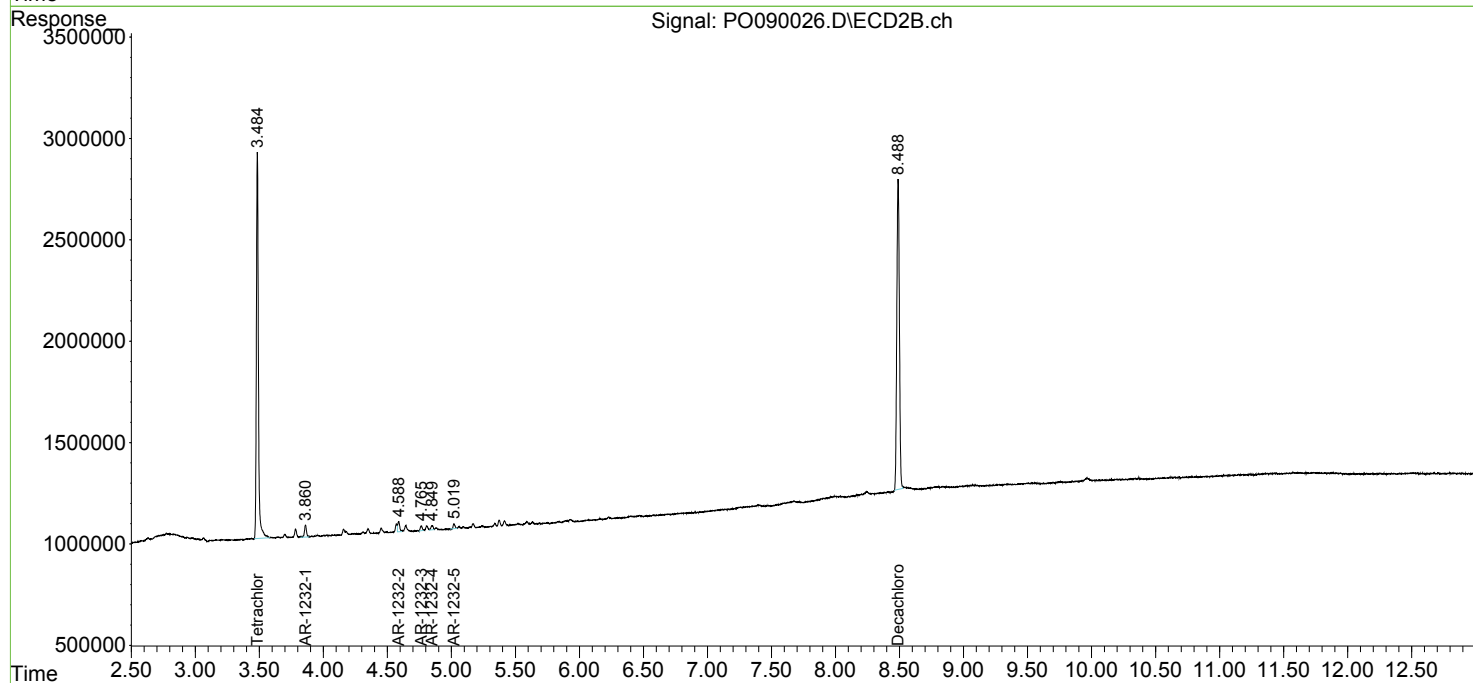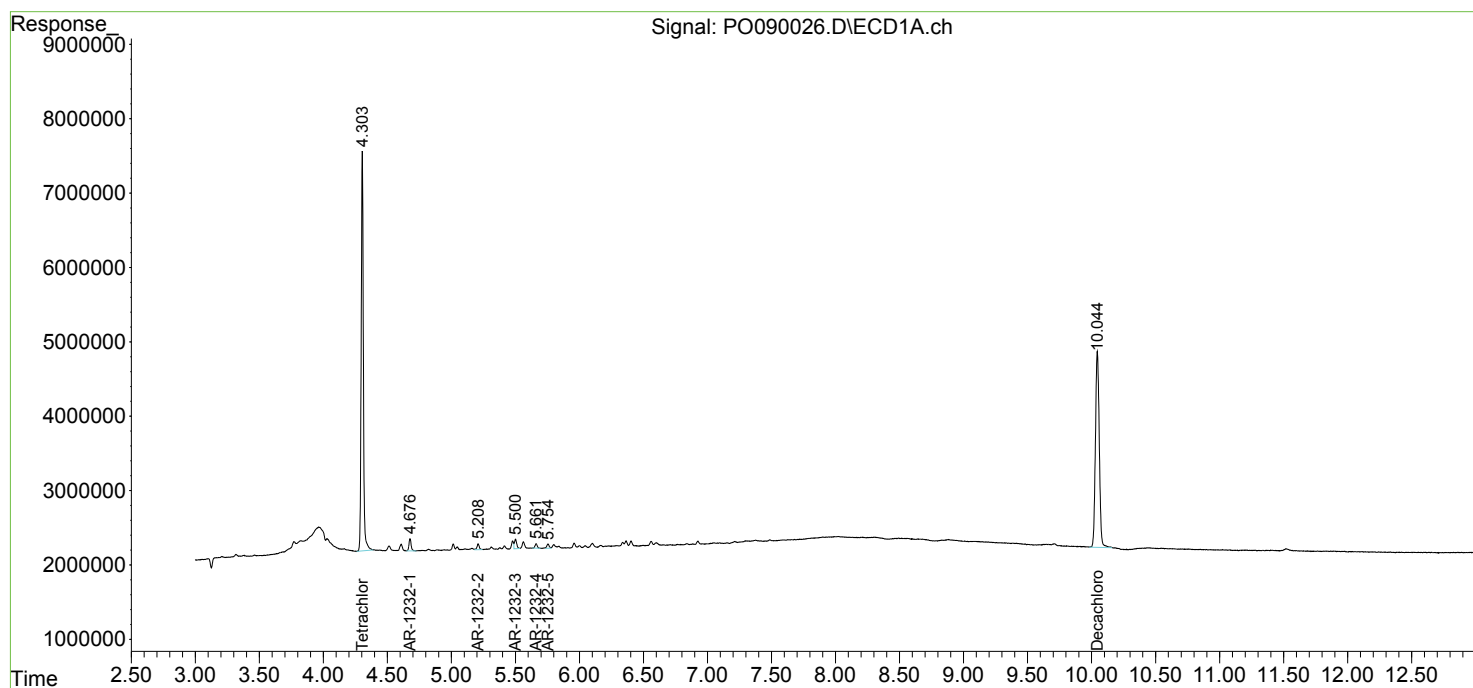


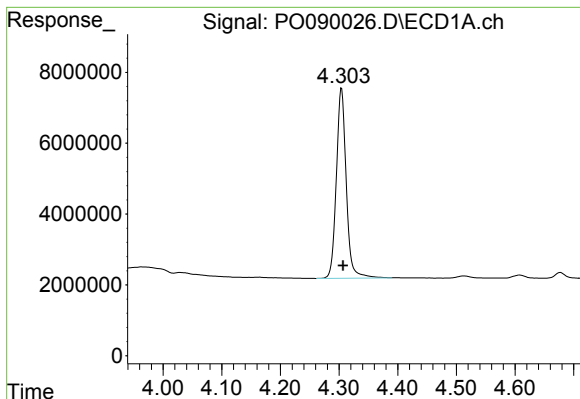

#1 Tetrachloro-m-xylene


R.T.: 4.304 min
Delta R.T.: -0.003 min
Response: 62971933
Conc: 19.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

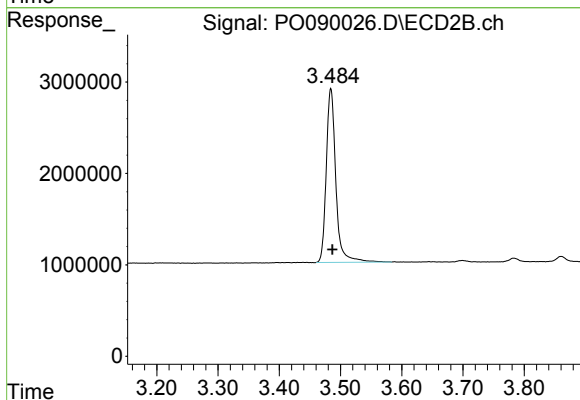


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 20694816
Conc: 19.47 ng/ml

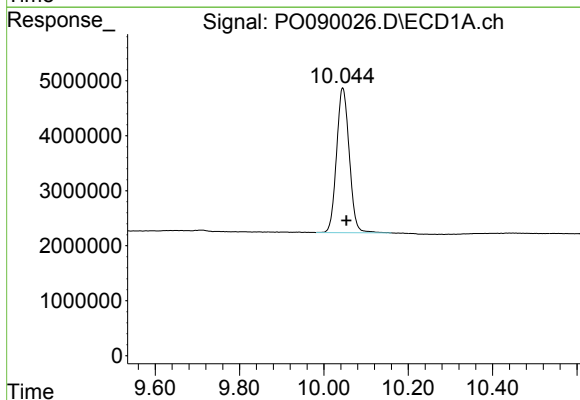


#2 Decachlorobiphenyl

R.T.: 10.045 min
Delta R.T.: -0.009 min
Response: 54989358
Conc: 22.44 ng/ml

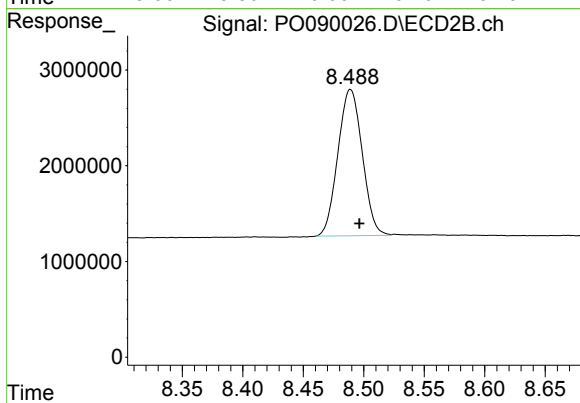

#2 Decachlorobiphenyl


R.T.: 8.489 min
Delta R.T.: -0.007 min
Response: 21435992
Conc: 20.81 ng/ml

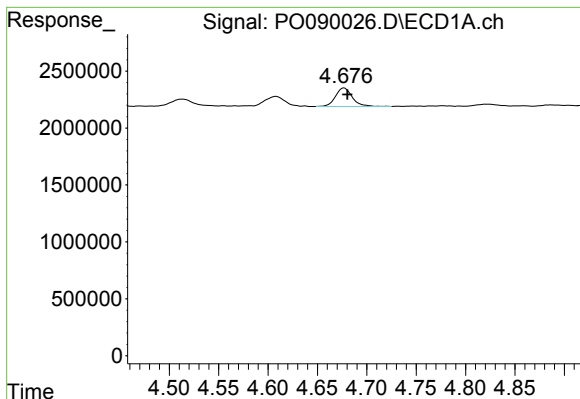

#11 AR-1232-1


R.T.: 4.677 min
Delta R.T.: -0.003 min
Response: 1939196
Conc: 29.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

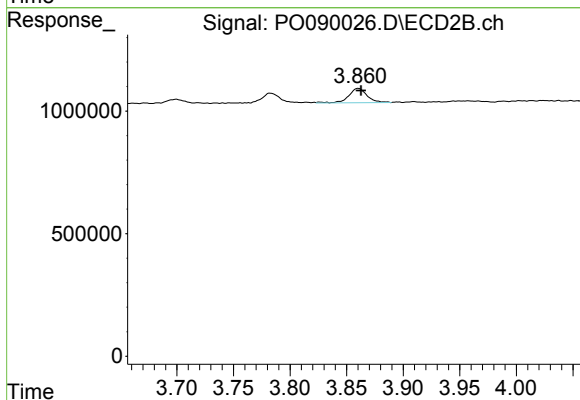


#11 AR-1232-1

R.T.: 3.860 min
Delta R.T.: -0.002 min
Response: 664051
Conc: 27.91 ng/ml

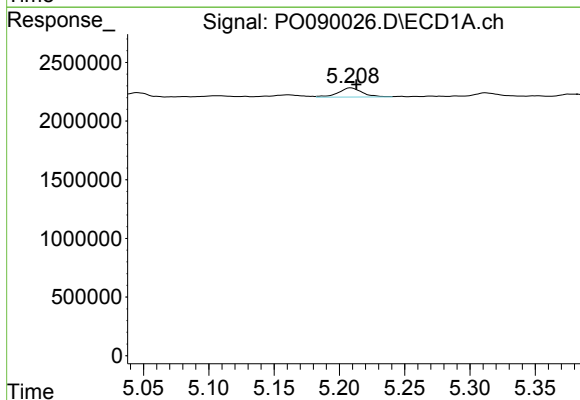


#12 AR-1232-2

R.T.: 5.209 min
Delta R.T.: -0.004 min
Response: 988922
Conc: 25.73 ng/ml

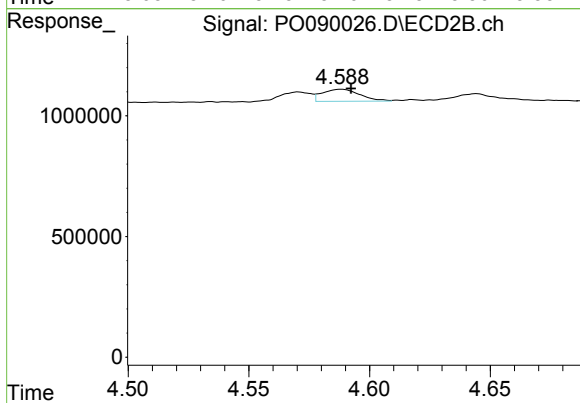

#12 AR-1232-2


R.T.: 4.588 min
Delta R.T.: -0.004 min
Response: 543736
Conc: 22.69 ng/ml

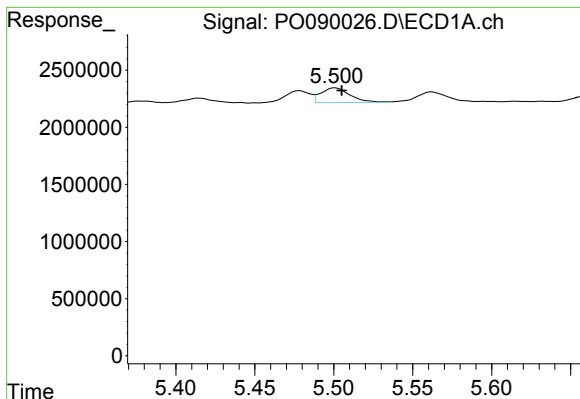

#13 AR-1232-3


R.T.: 5.501 min
Delta R.T.: -0.004 min
Response: 1632705
Conc: 24.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

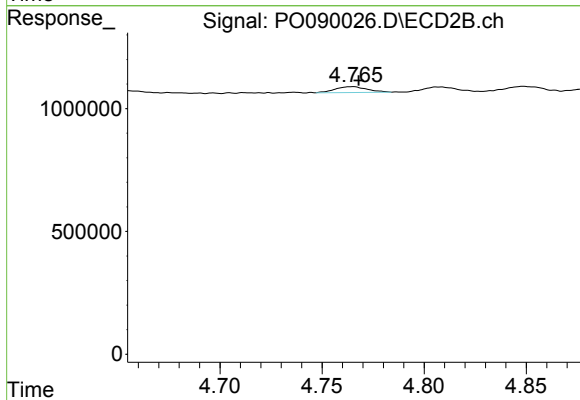


#13 AR-1232-3

R.T.: 4.765 min
Delta R.T.: -0.003 min
Response: 255987
Conc: 20.16 ng/ml

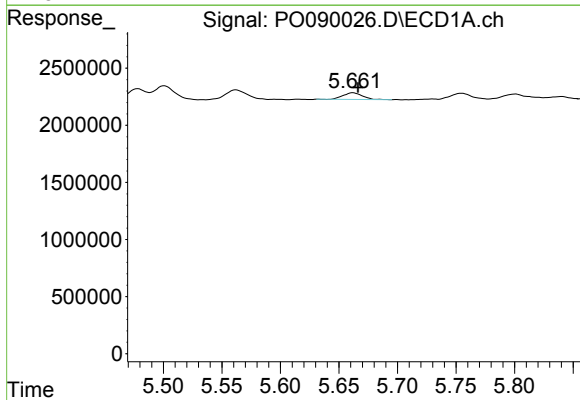


#14 AR-1232-4

R.T.: 5.662 min
Delta R.T.: -0.004 min
Response: 682572
Conc: 20.67 ng/ml

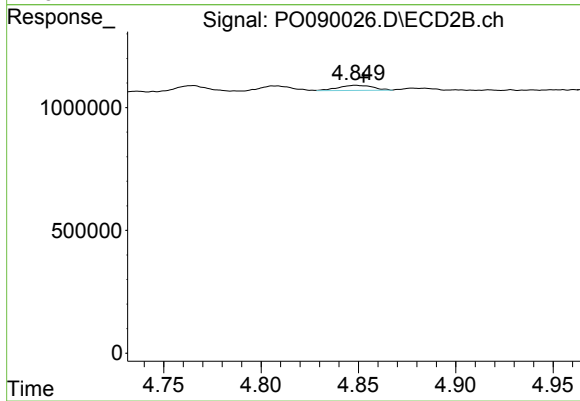

#14 AR-1232-4


R.T.: 4.849 min
Delta R.T.: -0.004 min
Response: 251418
Conc: 20.62 ng/ml

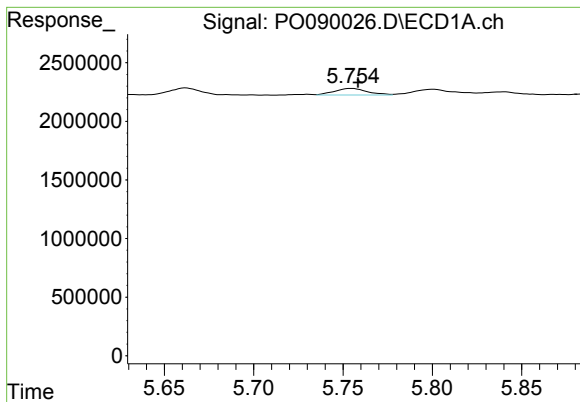

#15 AR-1232-5

R.T.: 5.755 min
Delta R.T.: -0.004 min
Response: 709187
Conc: 26.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

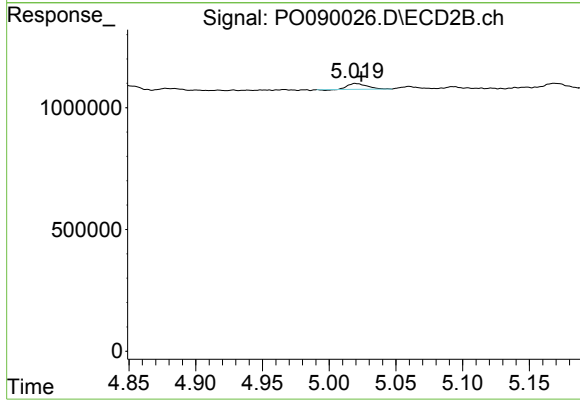

#15 AR-1232-5

R.T.: 5.019 min
Delta R.T.: -0.005 min
Response: 228936
Conc: 17.15 ng/ml