

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102822\
 Data File : PO090031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2022 21:17
 Operator : YP/AJ
 Sample : N4955-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:05:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.305	3.484	63944125	20878304	19.896	19.645
2) SA Decachlor...	10.047	8.490	59633046	23309636	24.334	22.632
Target Compounds						
41) L9 AR-1268-1	8.561	7.404	7868261	3533769	22.569	22.429
42) L9 AR-1268-2	8.653	7.468	7030417	2924366	22.536	20.843
43) L9 AR-1268-3	8.879	7.676	6157342	2665376	22.913	22.210
44) L9 AR-1268-4	9.300	7.964	2371943	1037615	20.356	19.106
45) L9 AR-1268-5	9.710	8.244	18633164	7972611	21.731	22.775



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102822\
Data File : PO090031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2022 21:17
Operator : YP/AJ
Sample : N4955-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:05:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

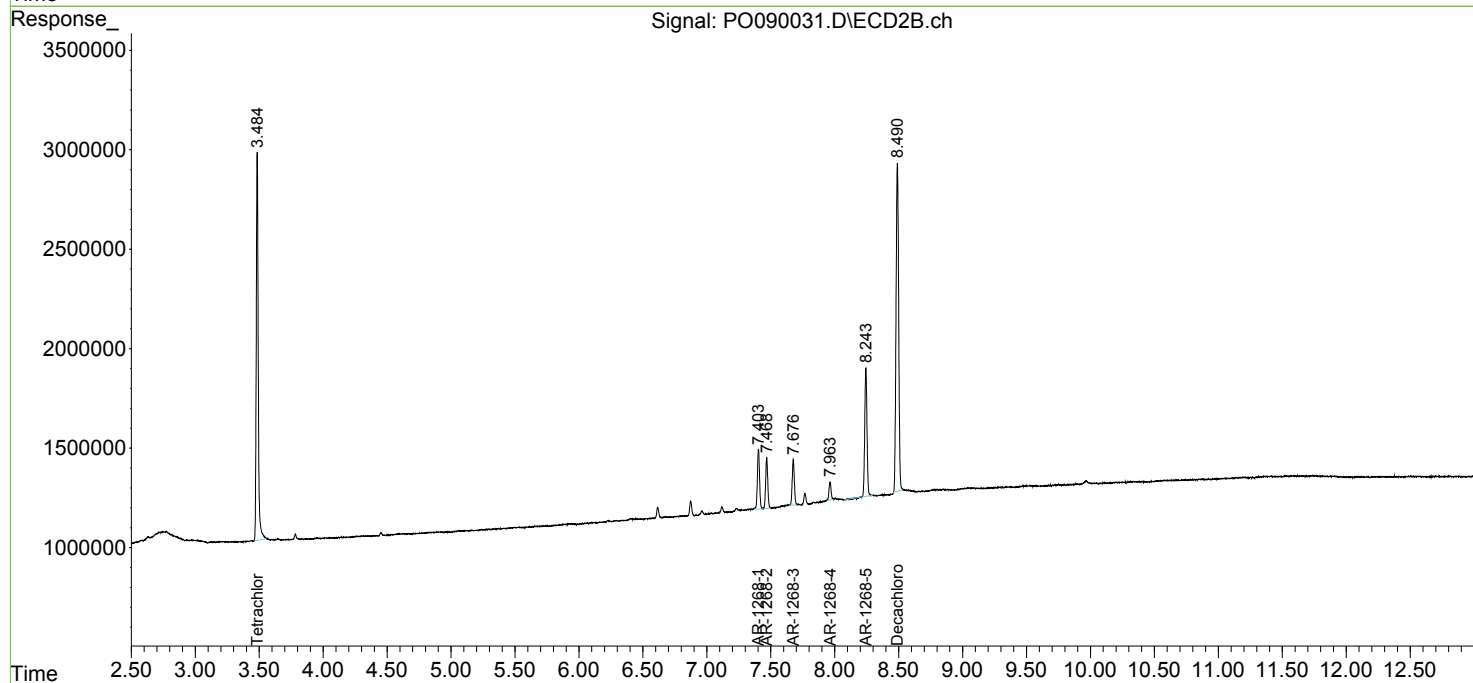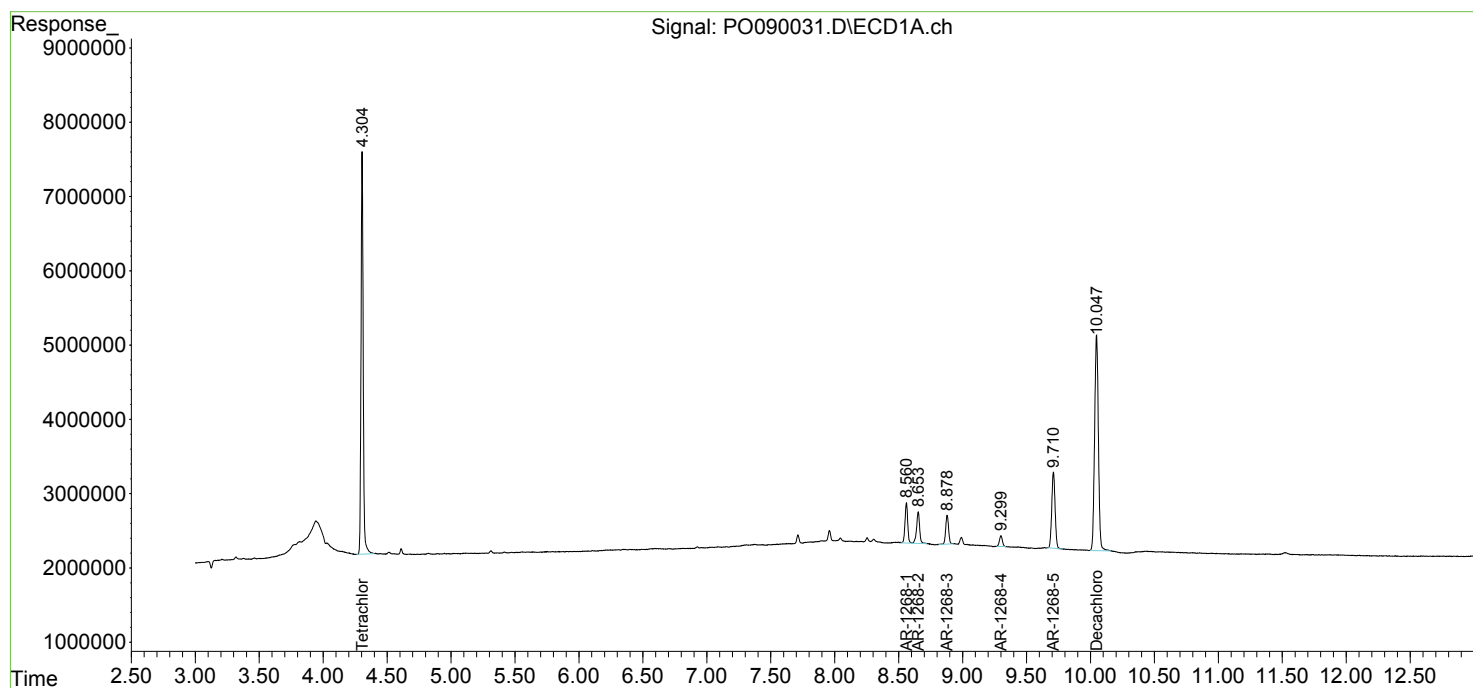


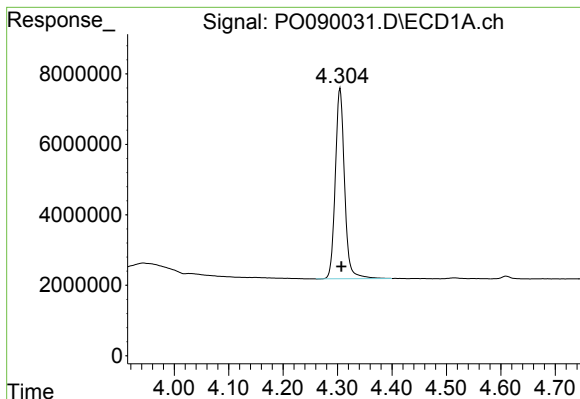

#1 Tetrachloro-m-xylene


R.T.: 4.305 min
Delta R.T.: -0.002 min
Response: 63944125
Conc: 19.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

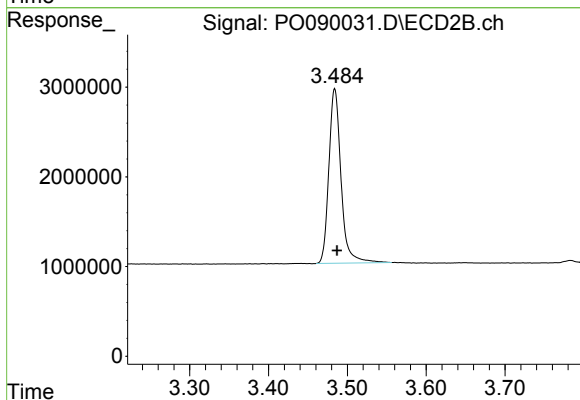


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.003 min
Response: 20878304
Conc: 19.64 ng/ml

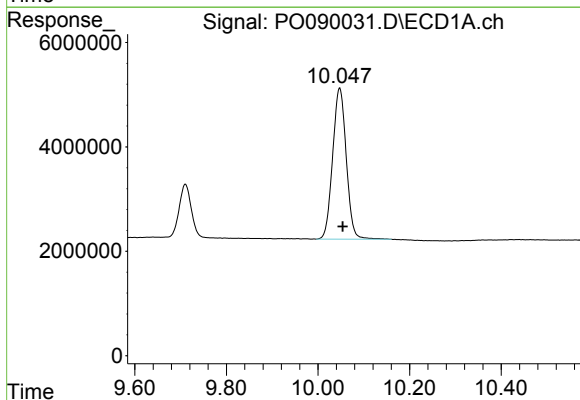


#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: -0.006 min
Response: 59633046
Conc: 24.33 ng/ml

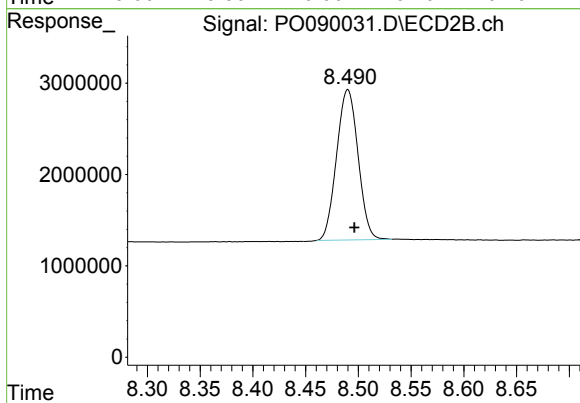

#2 Decachlorobiphenyl


R.T.: 8.490 min
Delta R.T.: -0.006 min
Response: 23309636
Conc: 22.63 ng/ml

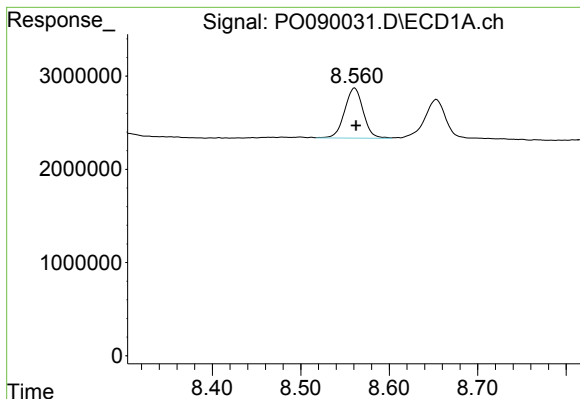

#41 AR-1268-1


R.T.: 8.561 min
Delta R.T.: -0.002 min
Response: 7868261
Conc: 22.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

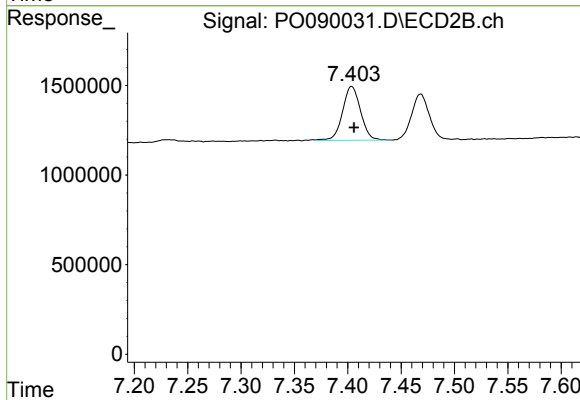


#41 AR-1268-1

R.T.: 7.404 min
Delta R.T.: -0.002 min
Response: 3533769
Conc: 22.43 ng/ml

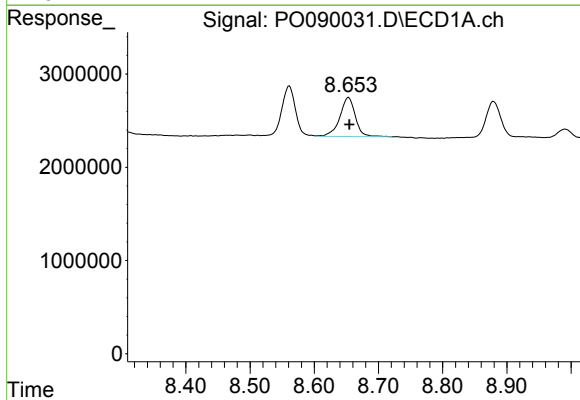


#42 AR-1268-2

R.T.: 8.653 min
Delta R.T.: -0.002 min
Response: 7030417
Conc: 22.54 ng/ml

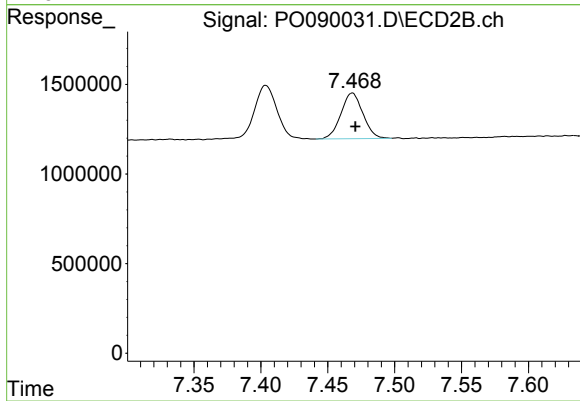

#42 AR-1268-2


R.T.: 7.468 min
Delta R.T.: -0.002 min
Response: 2924366
Conc: 20.84 ng/ml

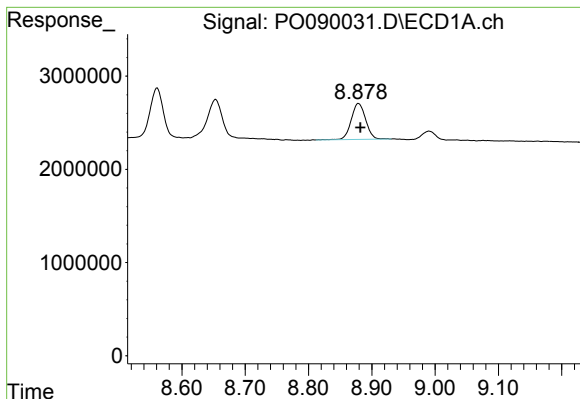

#43 AR-1268-3


R.T.: 8.879 min
Delta R.T.: -0.003 min
Response: 6157342
Conc: 22.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

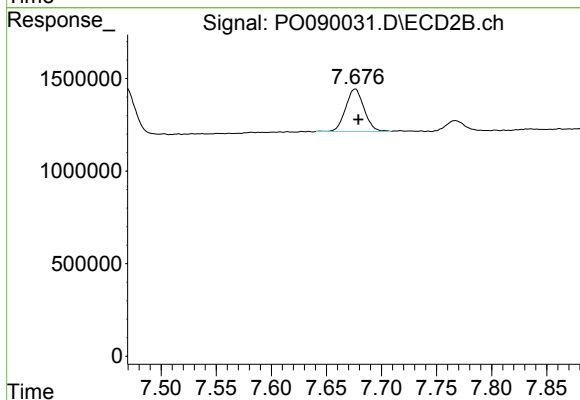


#43 AR-1268-3

R.T.: 7.676 min
Delta R.T.: -0.003 min
Response: 2665376
Conc: 22.21 ng/ml

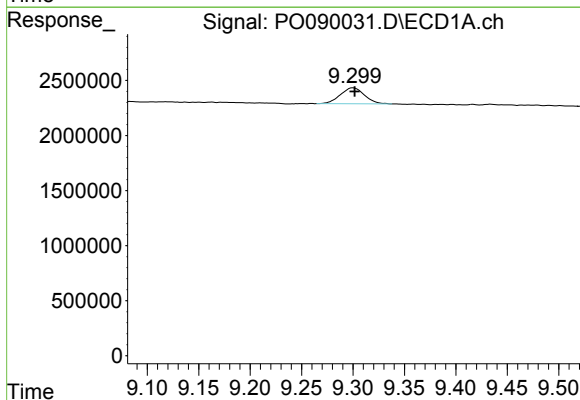


#44 AR-1268-4

R.T.: 9.300 min
Delta R.T.: -0.002 min
Response: 2371943
Conc: 20.36 ng/ml

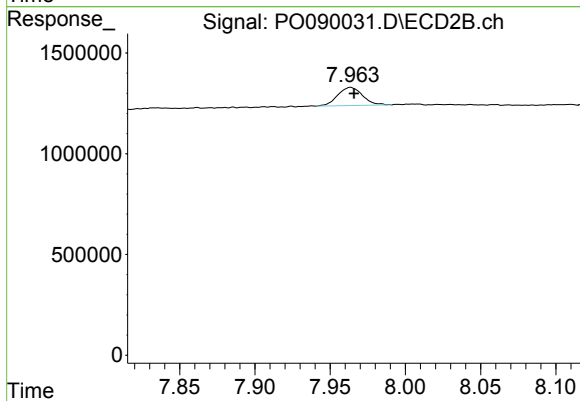

#44 AR-1268-4


R.T.: 7.964 min
Delta R.T.: -0.002 min
Response: 1037615
Conc: 19.11 ng/ml

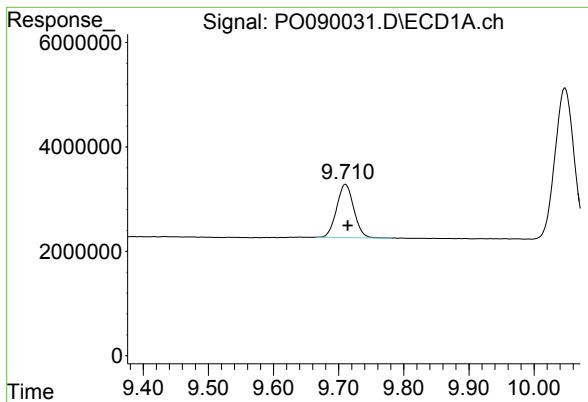

#45 AR-1268-5

R.T.: 9.710 min
Delta R.T.: -0.003 min
Response: 18633164
Conc: 21.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT4-2022

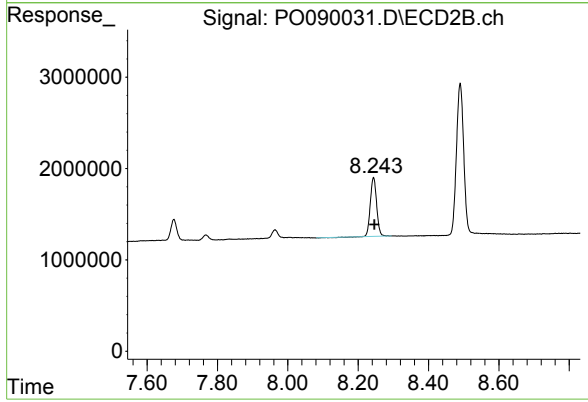

#45 AR-1268-5

R.T.: 8.244 min
Delta R.T.: -0.002 min
Response: 7972611
Conc: 22.77 ng/ml