



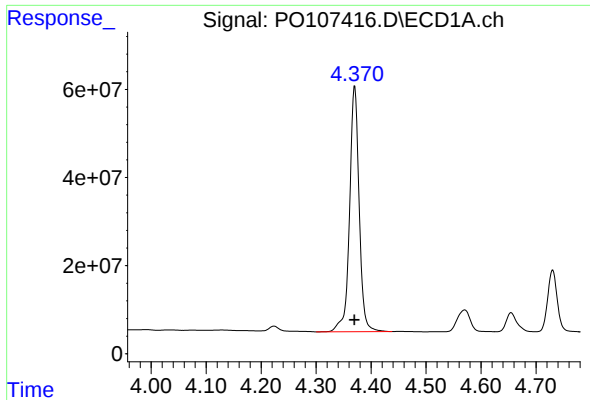

#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 676870891
Conc: 74.50 ng/ml

Instrument :
ECD_O
ClientSampleId :

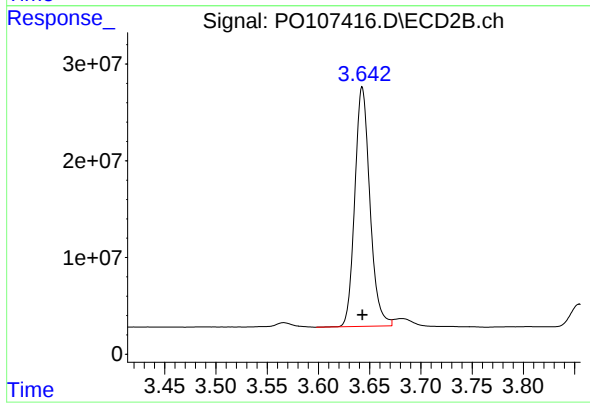

#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: 0.000 min
Response: 253954857
Conc: 75.05 ng/ml