

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102825\
 Data File : PO114713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 16:41
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/29/2025
 Supervised By :Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 01:42:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.654	109.9E6	72551592	20.234	18.128
2) SA Decachlor...	9.933	8.648	72939419	67240355	20.032	20.173m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO102825\
Data File : PO114713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 16:41
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 01:42:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

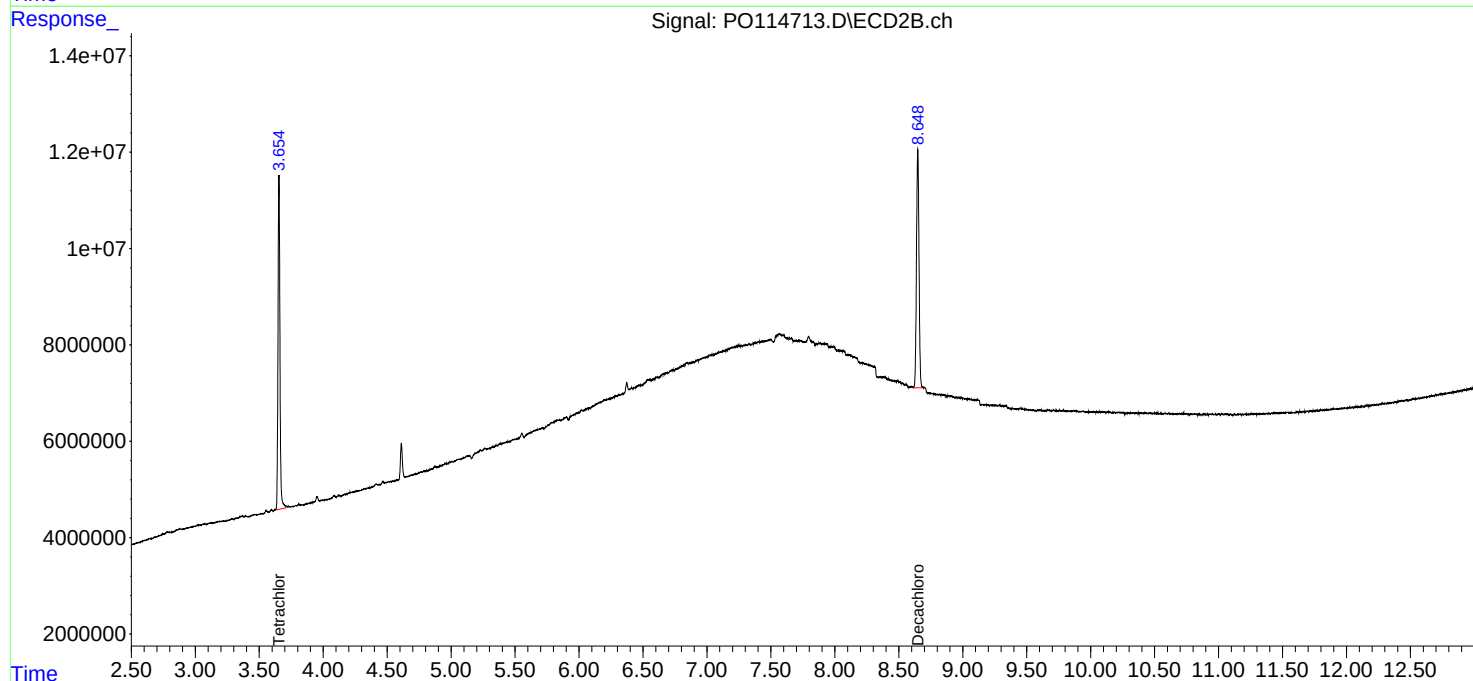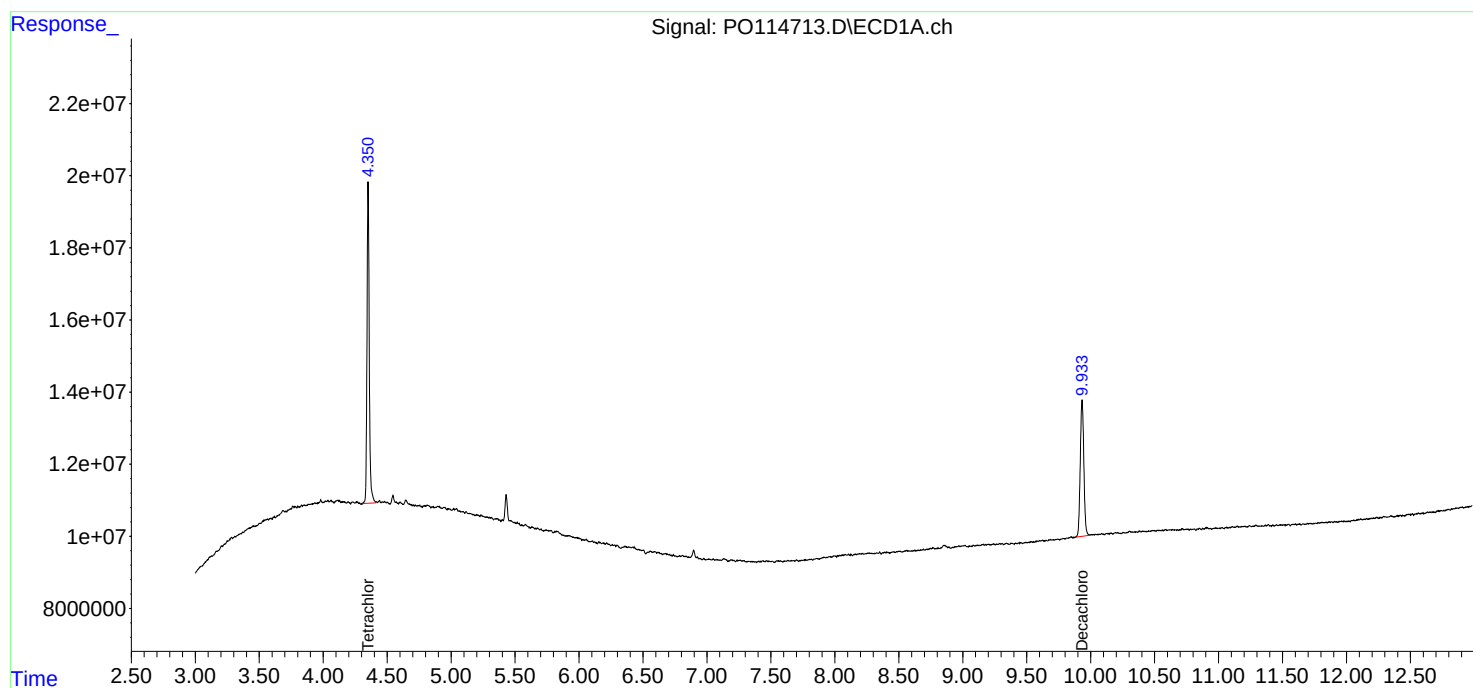

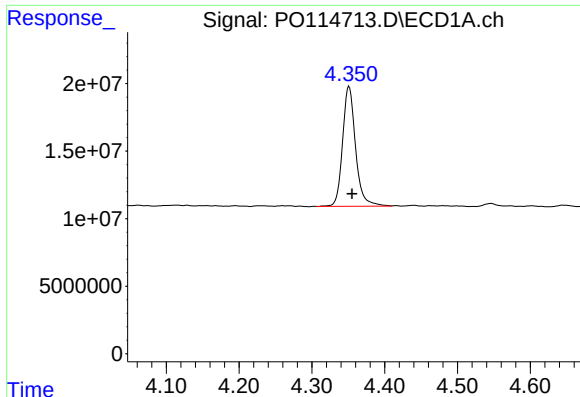

#1 Tetrachloro-m-xylene

R.T.: 4.351 min
Delta R.T.: -0.004 min
Response: 109851552
Conc: 20.23 ng/ml

Instrument :


ECD_O

ClientSampleId :

I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/29/2025
Supervised By :Sohil Jodhani 10/29/2025

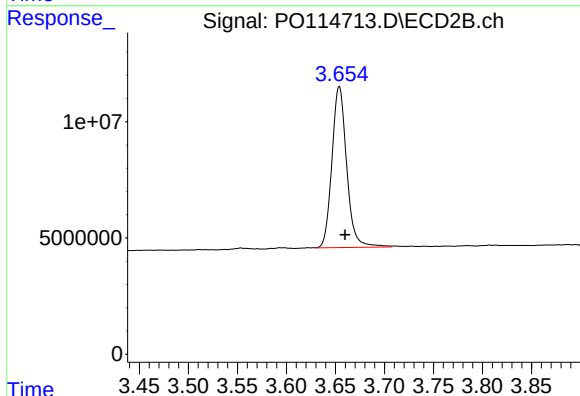


#1 Tetrachloro-m-xylene

R.T.: 3.654 min
Delta R.T.: -0.006 min
Response: 72551592
Conc: 18.13 ng/ml

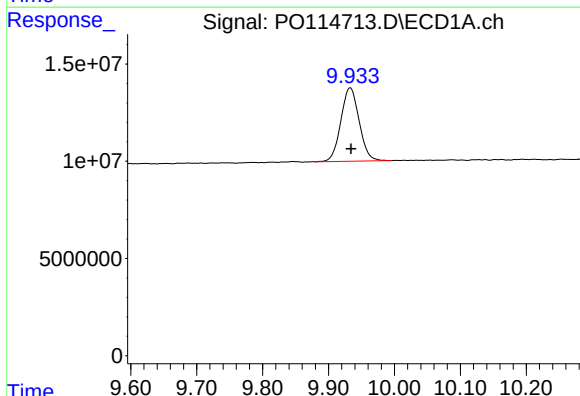

#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.001 min
Response: 72939419
Conc: 20.03 ng/ml

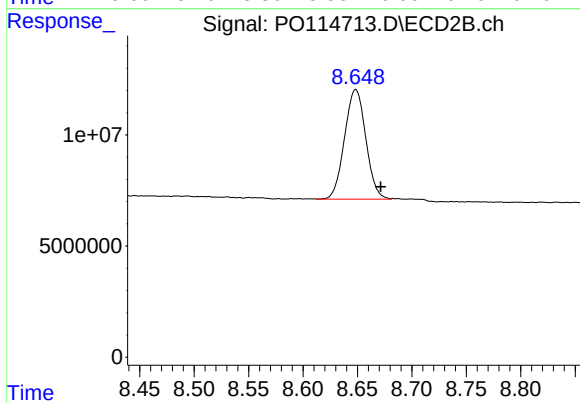

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.023 min
Response: 67240355
Conc: 20.17 ng/ml m