

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102920\
Data File : PO072897.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2020 14:15
Operator : DD\AJ
Sample : 20 PPB SURRPGATE TEST
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20 PPB SURRPGATE TEST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 17:52:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 27 16:48:42 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.949	4.023	1078289	738626	23.387	21.075
2) SA Decachlor...	10.986	9.310	1082767	978975	29.307	29.356

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102920\
Data File : PO072897.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2020 14:15
Operator : DD\AJ
Sample : 20 PPB SURRPGATE TEST
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20 PPB SURRPGATE TEST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 17:52:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 27 16:48:42 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

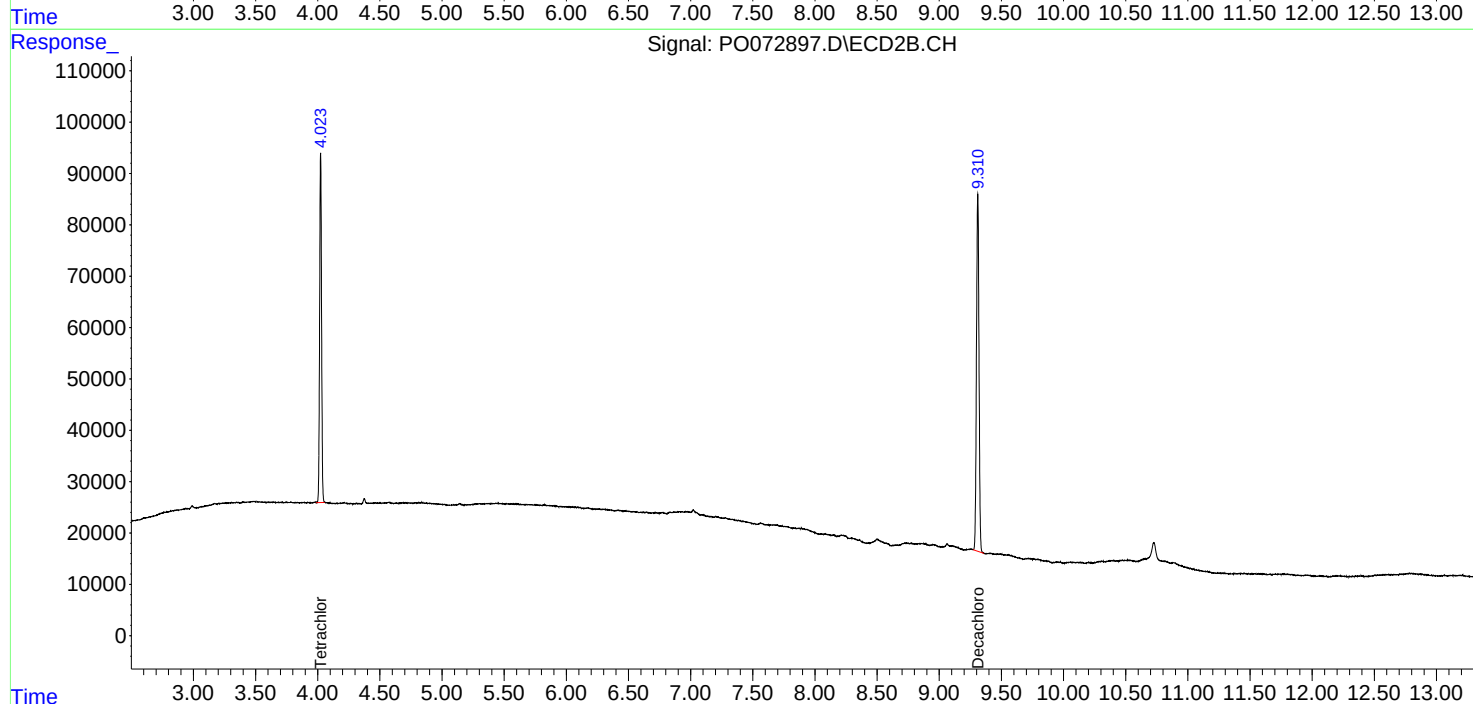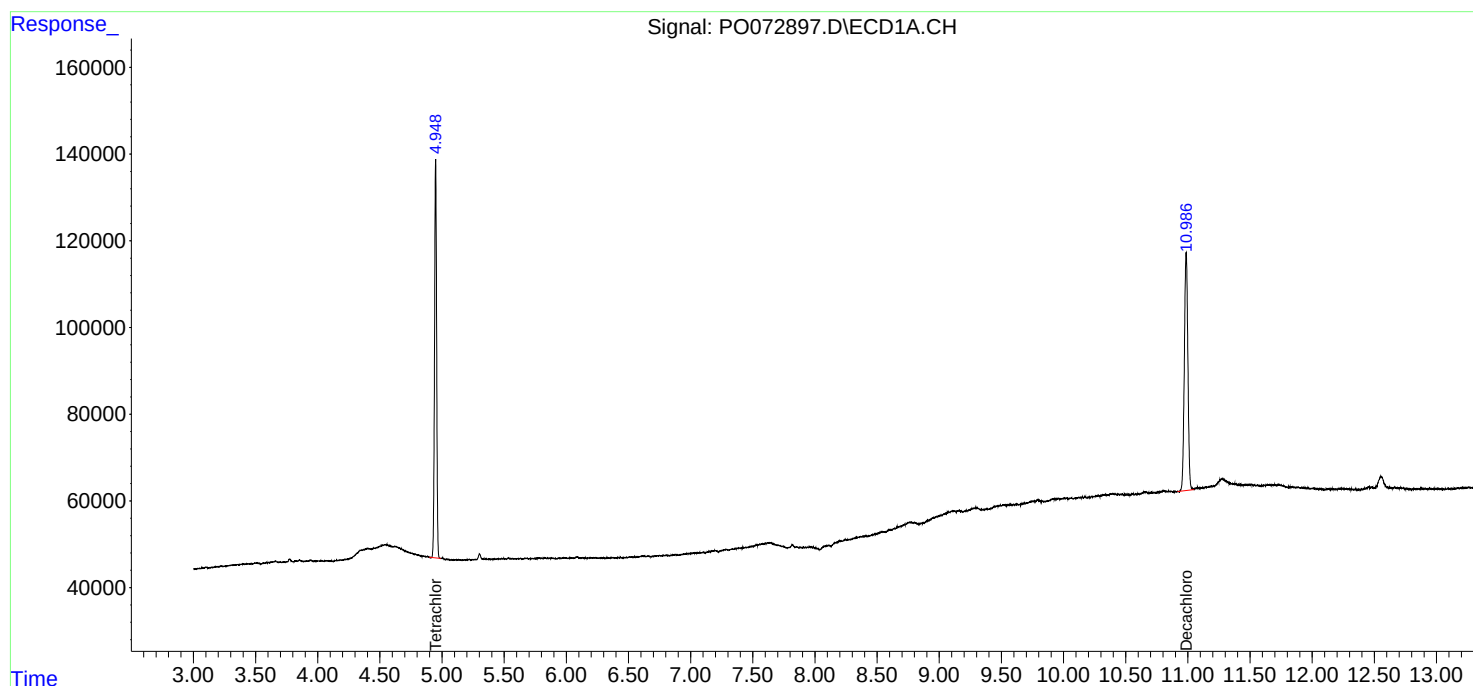


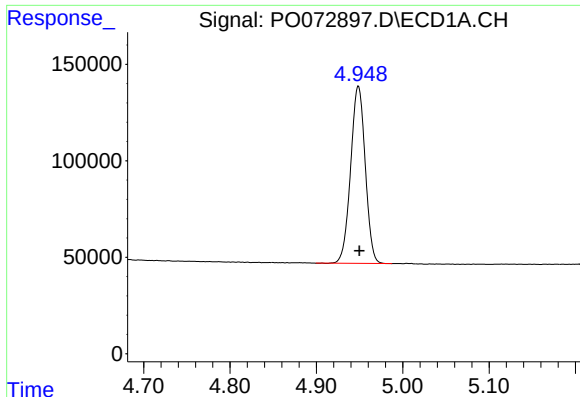

#1 Tetrachloro-m-xylene


R.T.: 4.949 min
Delta R.T.: -0.001 min
Response: 1078289
Conc: 23.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
20 PPB SURRGATE TEST

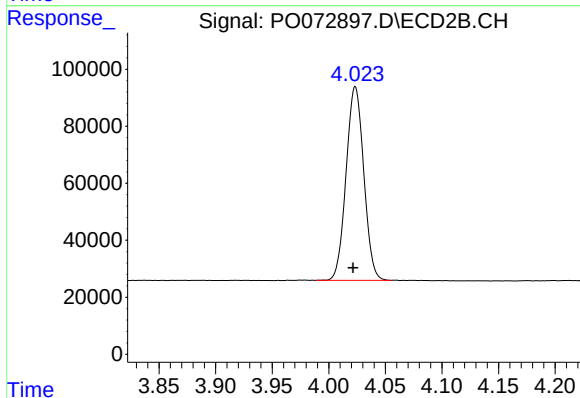


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.002 min
Response: 738626
Conc: 21.08 ng/ml

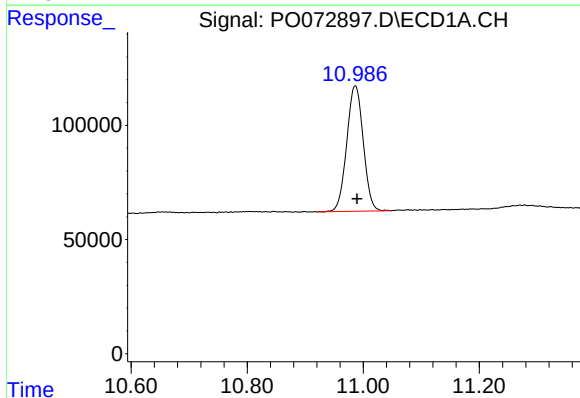

#2 Decachlorobiphenyl

R.T.: 10.986 min
Delta R.T.: -0.003 min
Response: 1082767
Conc: 29.31 ng/ml

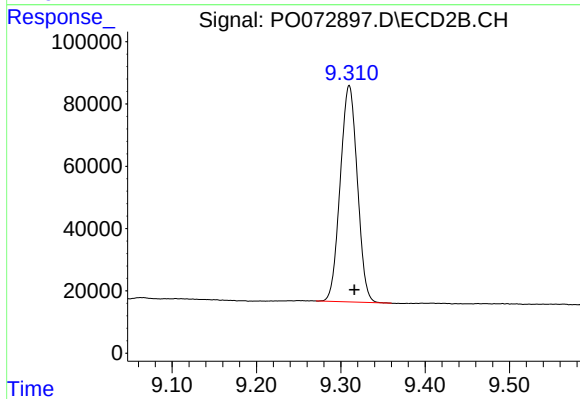

#2 Decachlorobiphenyl

R.T.: 9.310 min
Delta R.T.: -0.006 min
Response: 978975
Conc: 29.36 ng/ml