

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102921\
 Data File : P0082337.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2021 12:48
 Operator : AJ\MA
 Sample : M4342-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2021-6-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 15:24:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 29 11:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.979	3.973	1477309	571939	18.283	19.385
2) SA Decachlor...	11.100	9.299	1309424	441047	23.560	17.316 #
Target Compounds						
41) L9 AR-1268-1	9.536	8.205	1887703	805552	222.374	161.302 #
42) L9 AR-1268-2	9.635	8.270	1974050	1005625	253.926	224.605
43) L9 AR-1268-3	9.867	8.479	396899	190331	58.496	49.998
44) L9 AR-1268-4	10.322	8.769	1323755	565617	457.910	361.190
45) L9 AR-1268-5	10.751	9.053	1841734	796005	80.330	72.111



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102921\
Data File : P0082337.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 12:48
Operator : AJ\MA
Sample : M4342-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2021-6-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 15:24:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

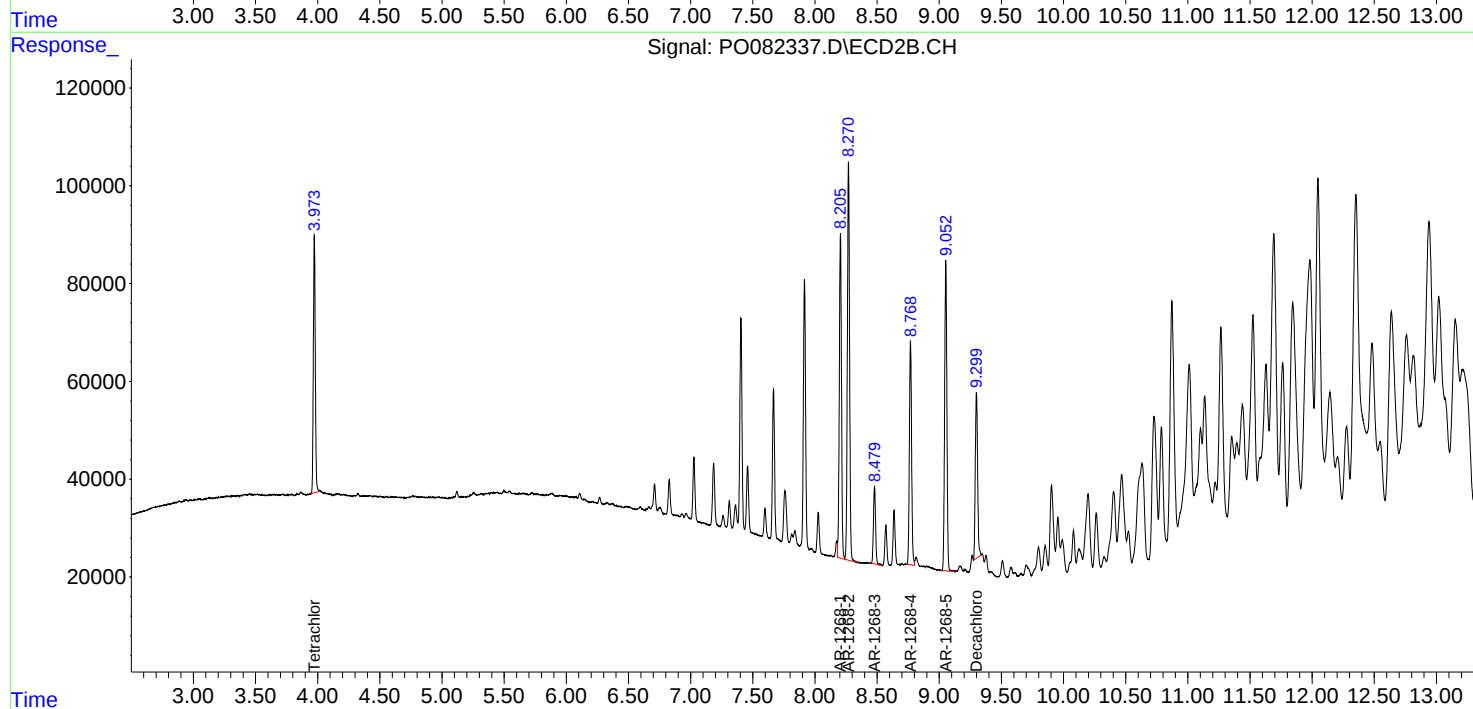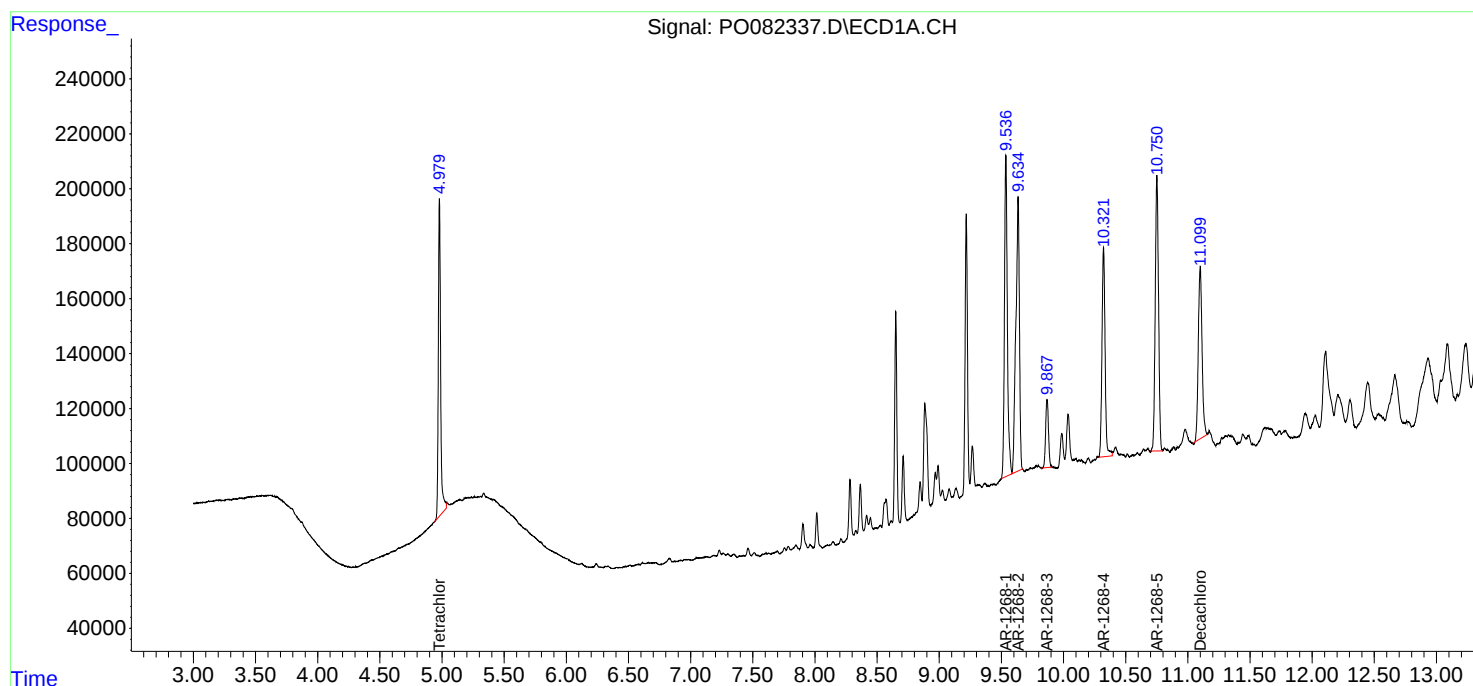


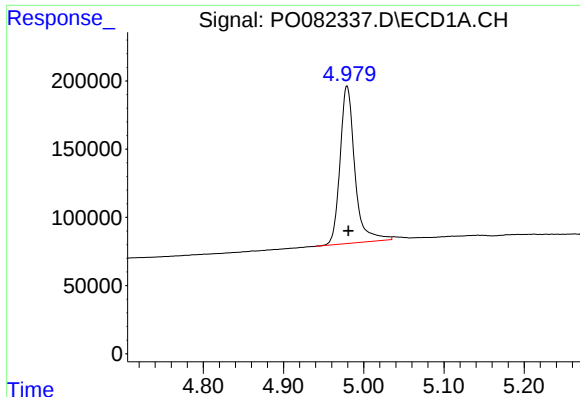

#1 Tetrachloro-m-xylene


R.T.: 4.979 min
Delta R.T.: -0.002 min
Response: 1477309
Conc: 18.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-6-A

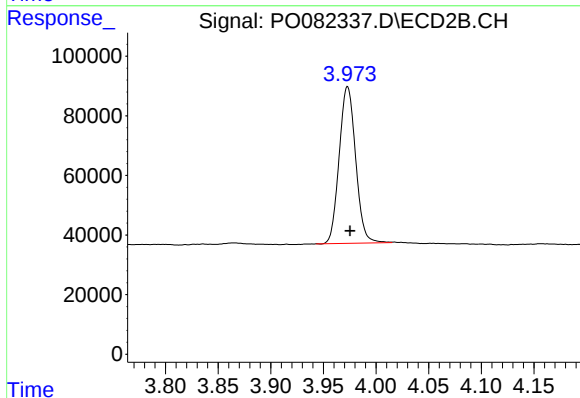


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: -0.002 min
Response: 571939
Conc: 19.38 ng/ml

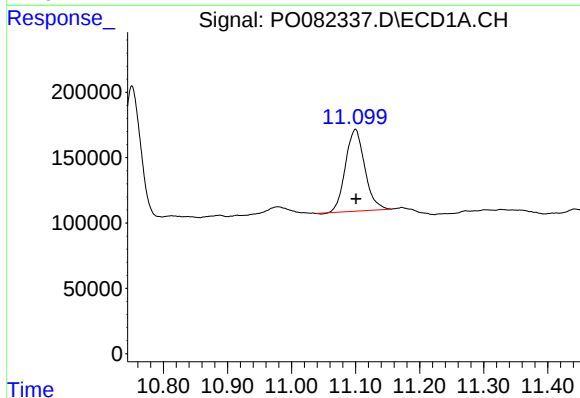


#2 Decachlorobiphenyl

R.T.: 11.100 min
Delta R.T.: 0.000 min
Response: 1309424
Conc: 23.56 ng/ml

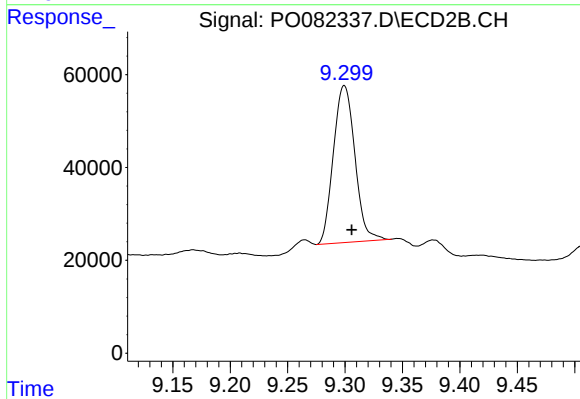

#2 Decachlorobiphenyl


R.T.: 9.299 min
Delta R.T.: -0.006 min
Response: 441047
Conc: 17.32 ng/ml

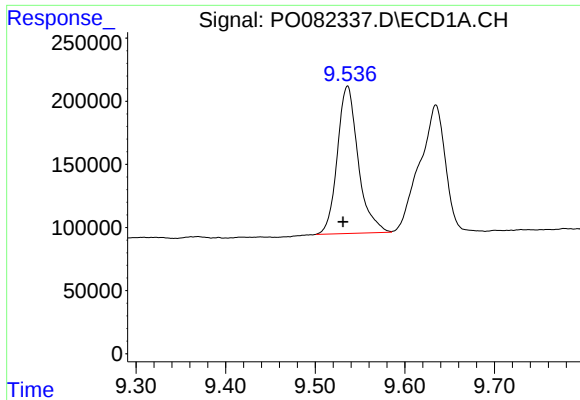

#41 AR-1268-1


R.T.: 9.536 min
Delta R.T.: 0.005 min
Response: 1887703
Conc: 222.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-6-A

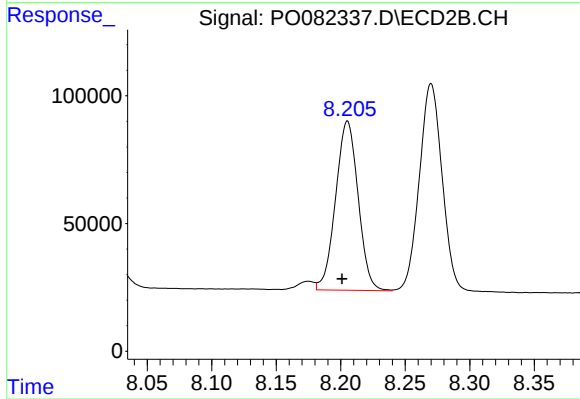


#41 AR-1268-1

R.T.: 8.205 min
Delta R.T.: 0.004 min
Response: 805552
Conc: 161.30 ng/ml

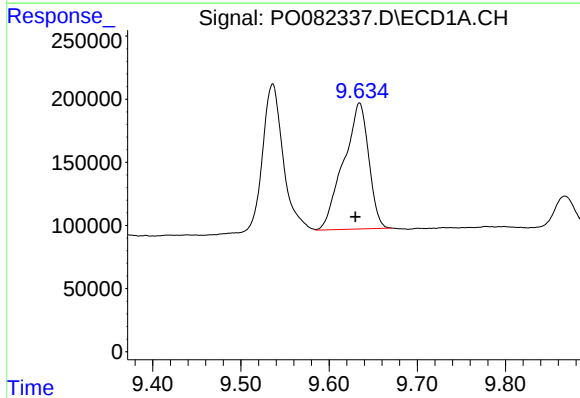


#42 AR-1268-2

R.T.: 9.635 min
Delta R.T.: 0.005 min
Response: 1974050
Conc: 253.93 ng/ml

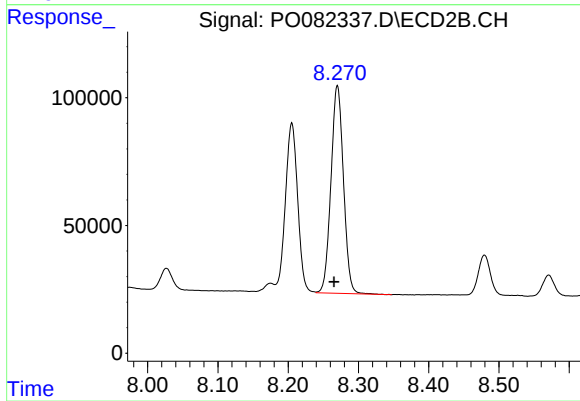

#42 AR-1268-2


R.T.: 8.270 min
Delta R.T.: 0.005 min
Response: 1005625
Conc: 224.60 ng/ml

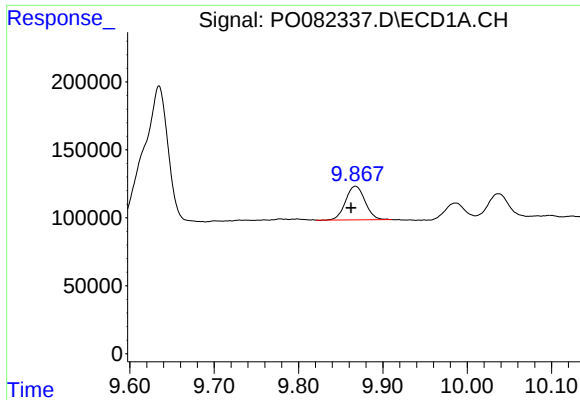

#43 AR-1268-3


R.T.: 9.867 min
Delta R.T.: 0.005 min
Response: 396899
Conc: 58.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-6-A

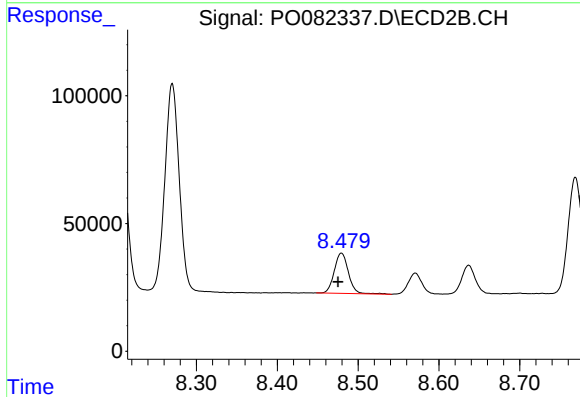


#43 AR-1268-3

R.T.: 8.479 min
Delta R.T.: 0.004 min
Response: 190331
Conc: 50.00 ng/ml

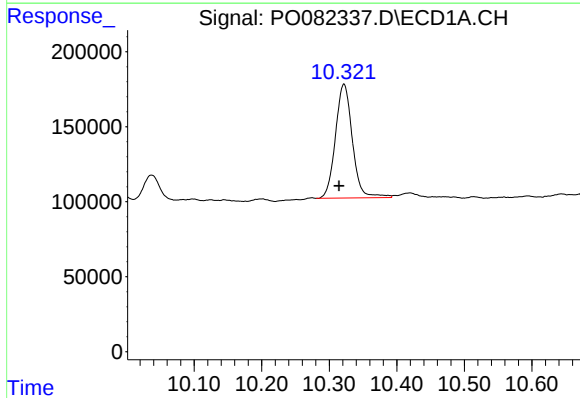


#44 AR-1268-4

R.T.: 10.322 min
Delta R.T.: 0.008 min
Response: 1323755
Conc: 457.91 ng/ml

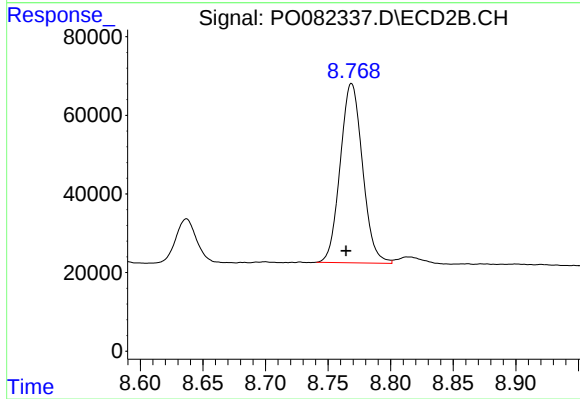

#44 AR-1268-4


R.T.: 8.769 min
Delta R.T.: 0.004 min
Response: 565617
Conc: 361.19 ng/ml

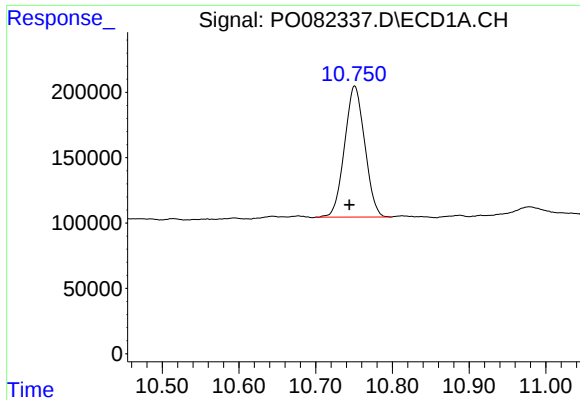

#45 AR-1268-5

R.T.: 10.751 min
Delta R.T.: 0.007 min
Response: 1841734
Conc: 80.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2021-6-A

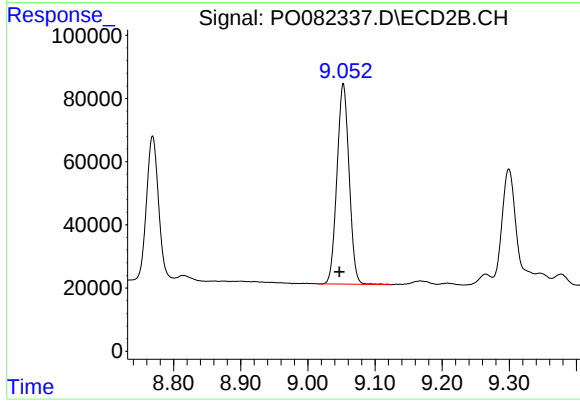

#45 AR-1268-5

R.T.: 9.053 min
Delta R.T.: 0.006 min
Response: 796005
Conc: 72.11 ng/ml