

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO102921\  
 Data File : PO082340.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 29 Oct 2021 14:33  
 Operator : AJ\MA  
 Sample : M4404-02 10X  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 MOO-2021-1B

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 29 15:25:23 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO101821.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Oct 29 11:08:21 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml  |
|-----------------------------|--------|-------|--------|--------|-------|--------|
| -----                       |        |       |        |        |       |        |
| System Monitoring Compounds |        |       |        |        |       |        |
| 1) SA Tetrachlo...          | 4.975  | 3.970 | 97811  | 37458  | 1.210 | 1.270m |
| 2) SA Decachlor...          | 11.094 | 9.293 | 68881  | 30686  | 1.239 | 1.205  |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO102921\  
Data File : PO082340.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 29 Oct 2021 14:33  
Operator : AJ\MA  
Sample : M4404-02 10X  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
MOO-2021-1B

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 29 15:25:23 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO101821.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Oct 29 11:08:21 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

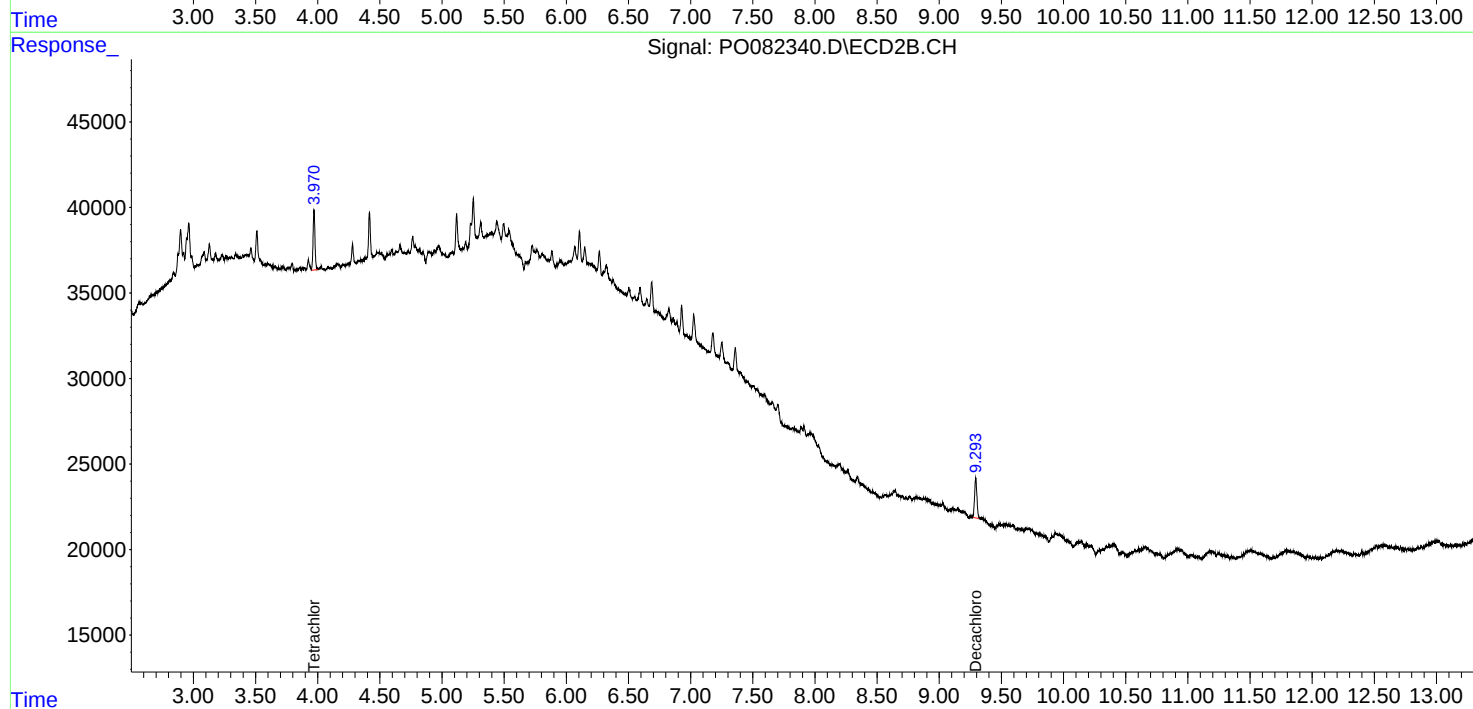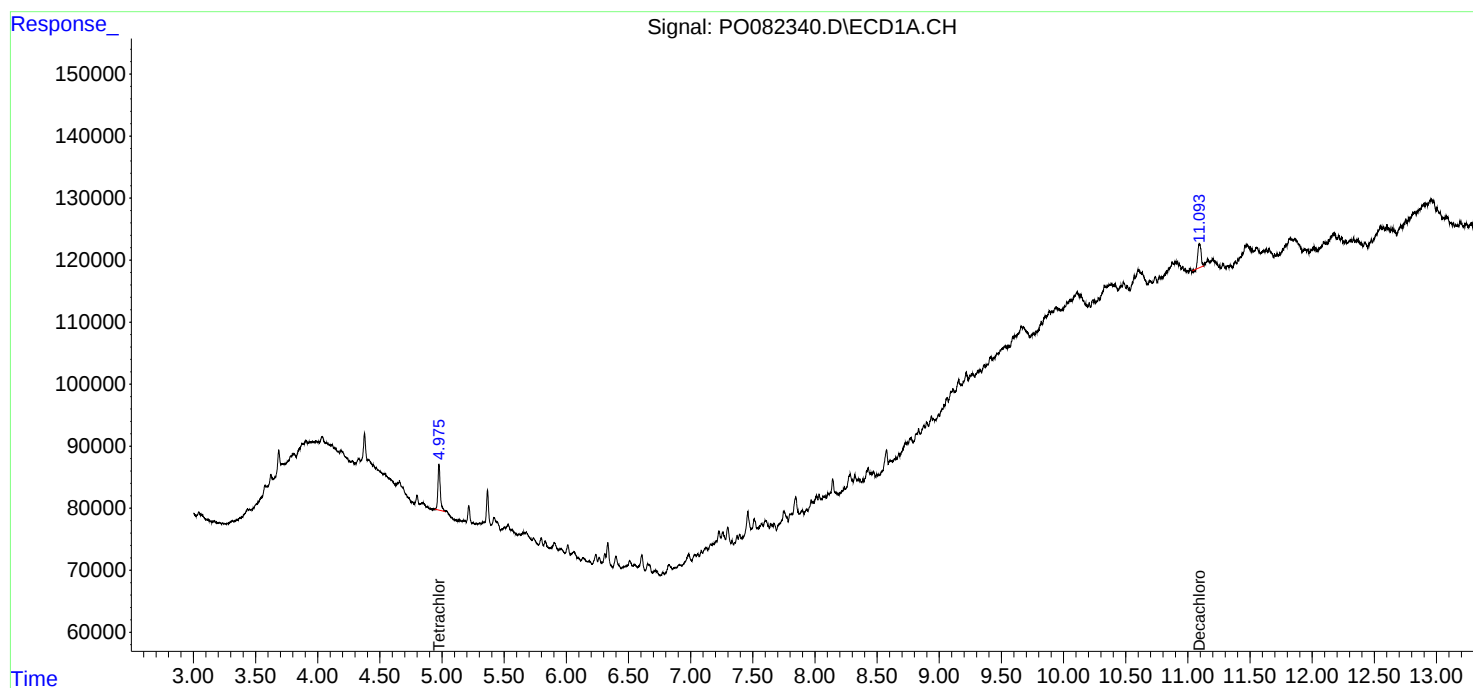


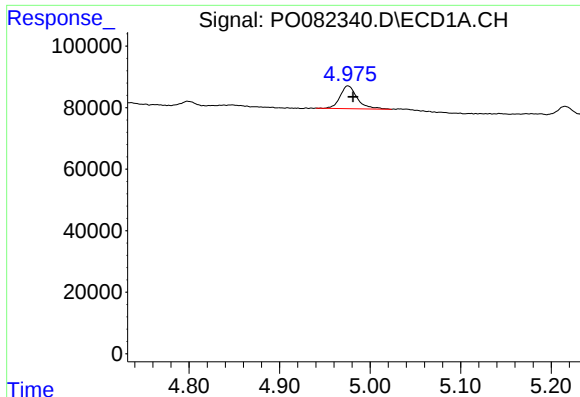

#1 Tetrachloro-m-xylene


R.T.: 4.975 min  
Delta R.T.: -0.006 min  
Response: 97811  
Conc: 1.21 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
MOO-2021-1B

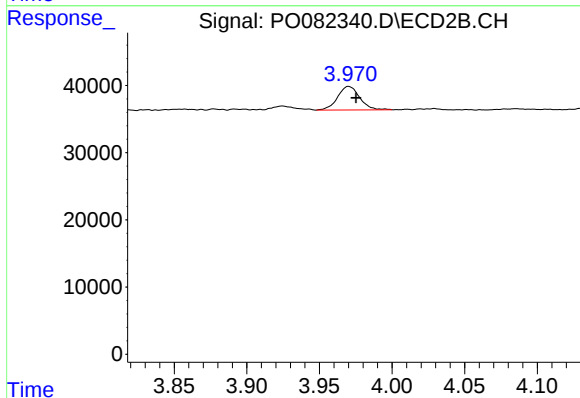


#1 Tetrachloro-m-xylene

R.T.: 3.970 min  
Delta R.T.: -0.006 min  
Response: 37458  
Conc: 1.27 ng/ml m

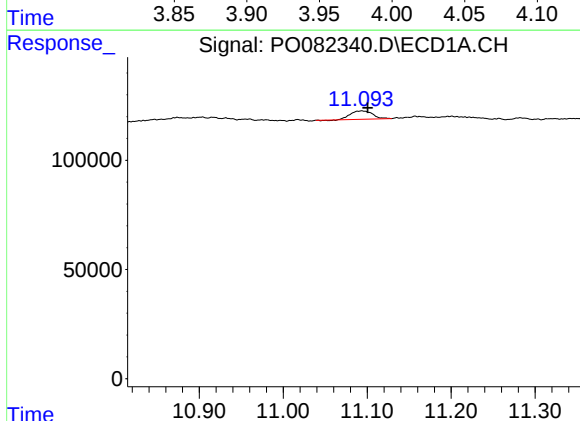

#2 Decachlorobiphenyl

R.T.: 11.094 min  
Delta R.T.: -0.007 min  
Response: 68881  
Conc: 1.24 ng/ml

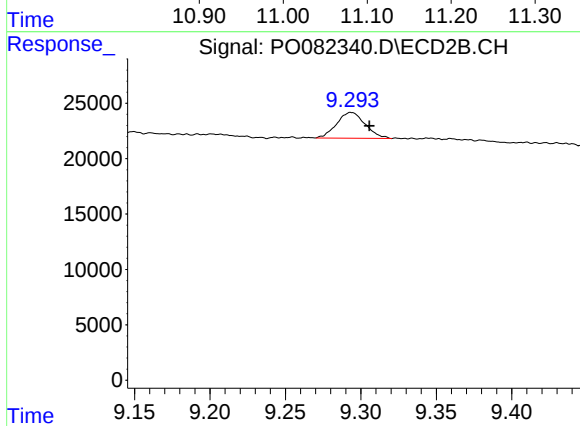

#2 Decachlorobiphenyl

R.T.: 9.293 min  
Delta R.T.: -0.012 min  
Response: 30686  
Conc: 1.20 ng/ml