

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102921\
 Data File : PO082352.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2021 18:29
 Operator : AJ\MA
 Sample : M4404-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-2021-2A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 04:13:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 29 11:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.980	3.974	1069925	411563	13.241	13.949
2) SA Decachlor...	11.120f	9.321f	984023	390899	17.705	15.347m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102921\
Data File : PO082352.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 18:29
Operator : AJ\MA
Sample : M4404-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MOO-2021-2A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 04:13:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

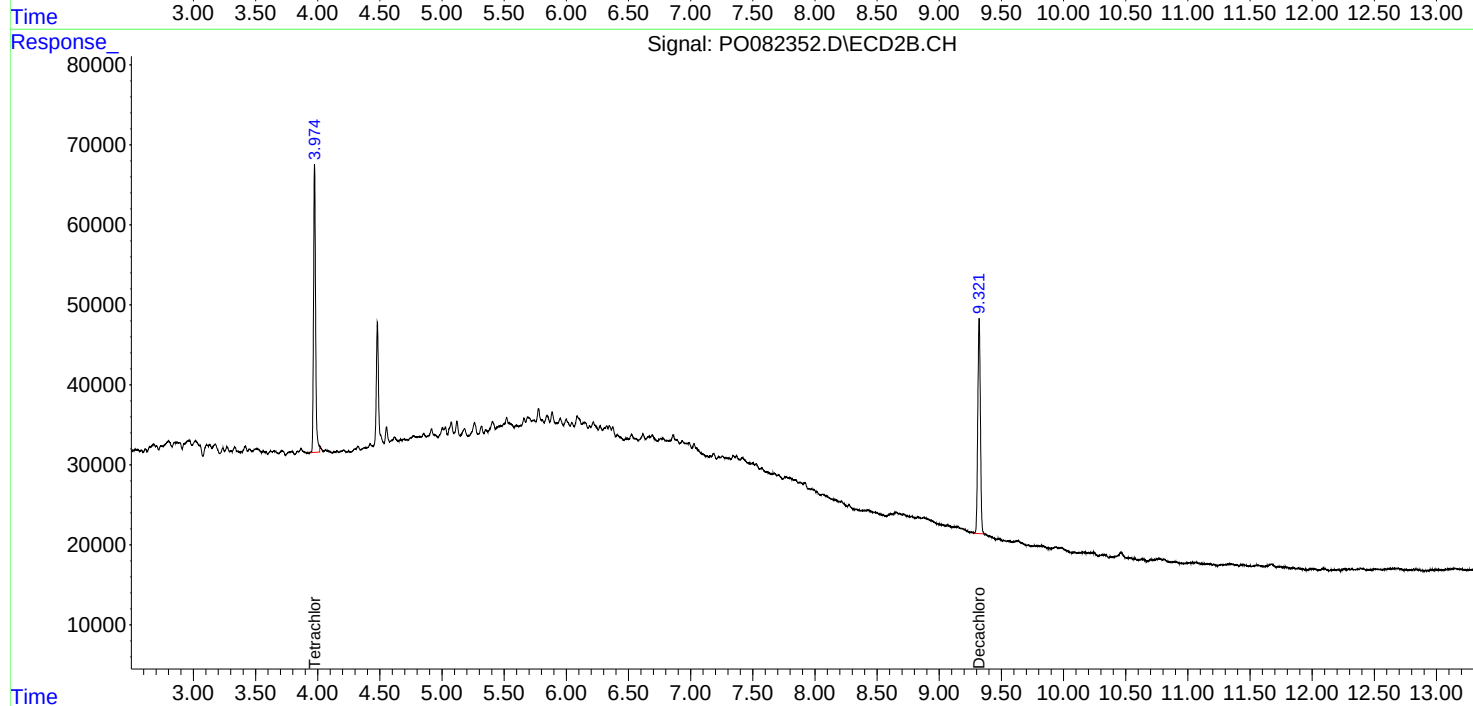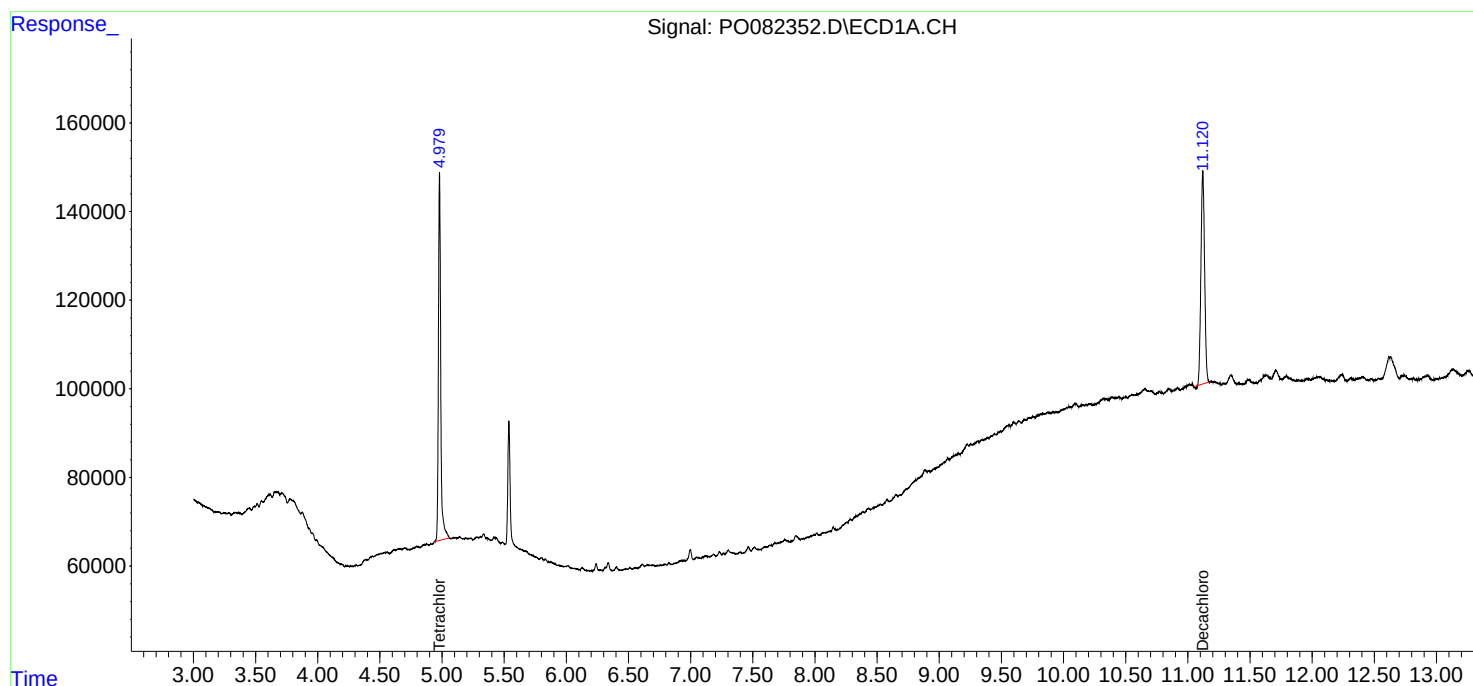


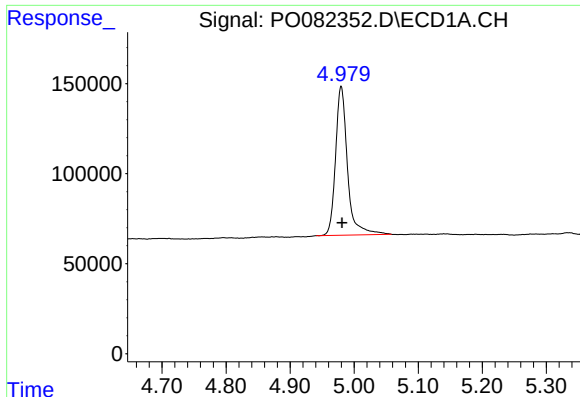

#1 Tetrachloro-m-xylene


R.T.: 4.980 min
Delta R.T.: -0.001 min
Response: 1069925
Conc: 13.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2021-2A

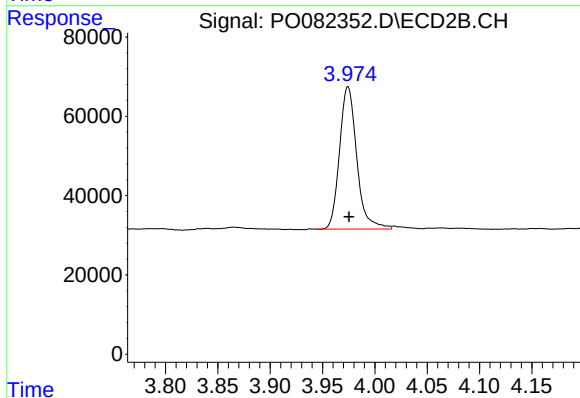


#1 Tetrachloro-m-xylene

R.T.: 3.974 min
Delta R.T.: 0.000 min
Response: 411563
Conc: 13.95 ng/ml

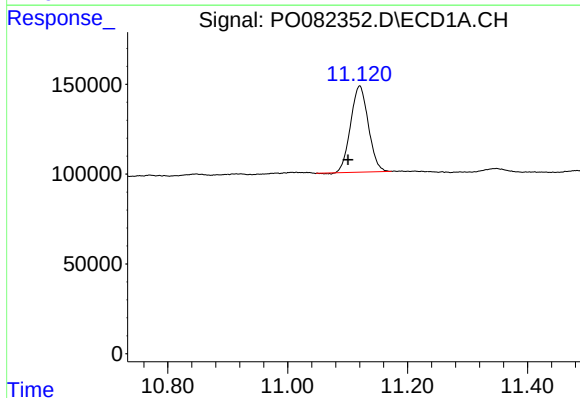

#2 Decachlorobiphenyl

R.T.: 11.120 min
Delta R.T.: 0.019 min
Response: 984023
Conc: 17.70 ng/ml

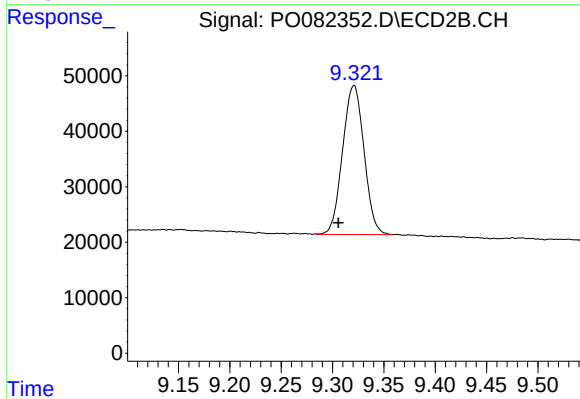

#2 Decachlorobiphenyl

R.T.: 9.321 min
Delta R.T.: 0.015 min
Response: 390899
Conc: 15.35 ng/ml m