

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102921\
 Data File : PO082353.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2021 18:47
 Operator : AJ\MA
 Sample : M4404-04 20X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-2021-3A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 04:14:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 29 11:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.982	3.973	25730	8912	0.318	0.302
2)	SA Decachlor...	11.104	9.299	30678	11982	0.552	0.470

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102921\
Data File : P0082353.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 18:47
Operator : AJ\MA
Sample : M4404-04 20X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MOO-2021-3A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 04:14:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

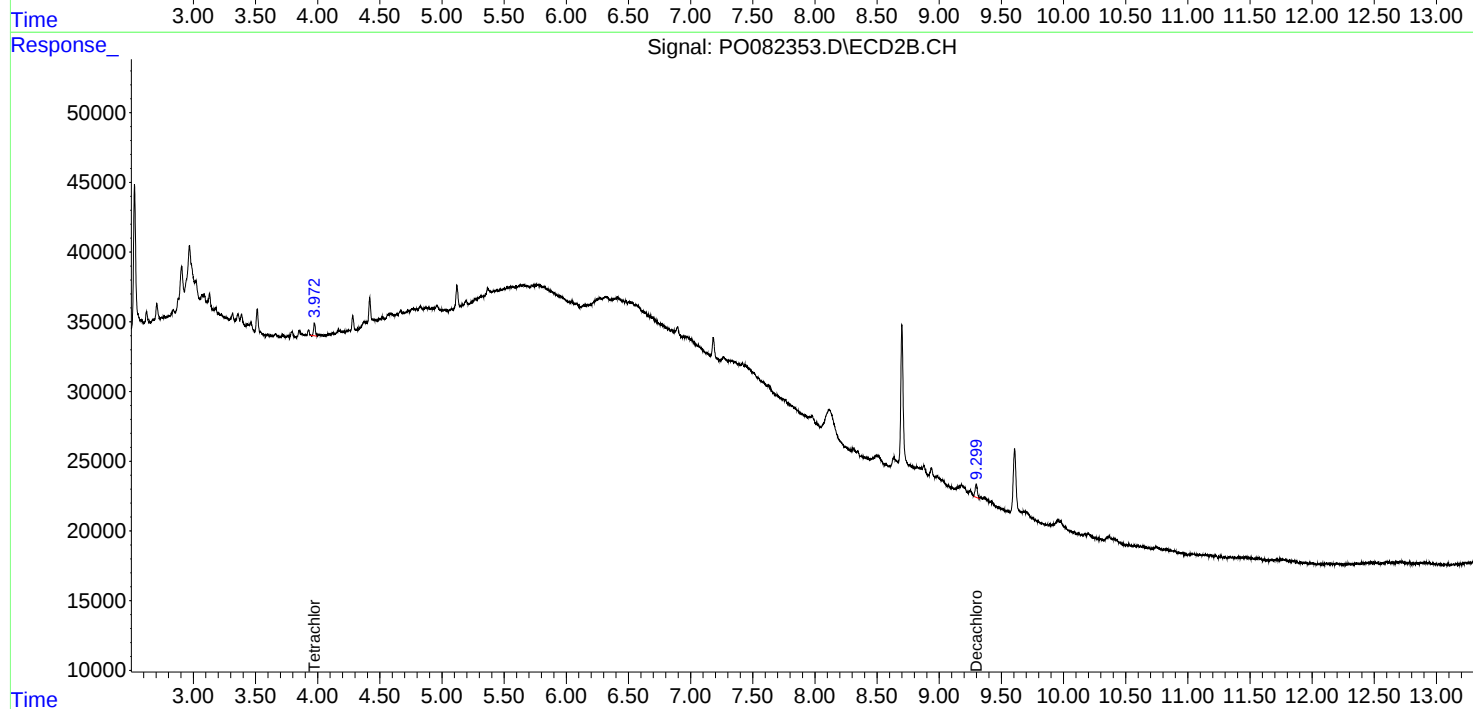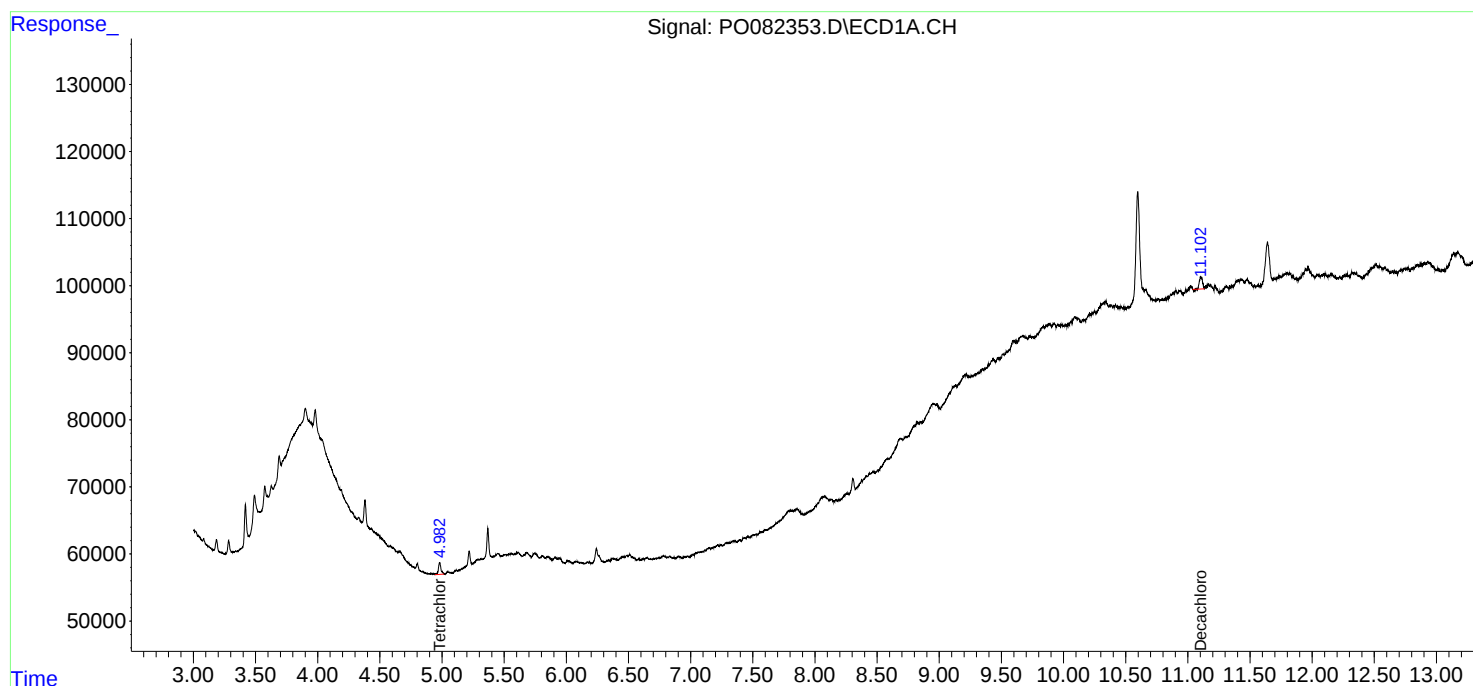


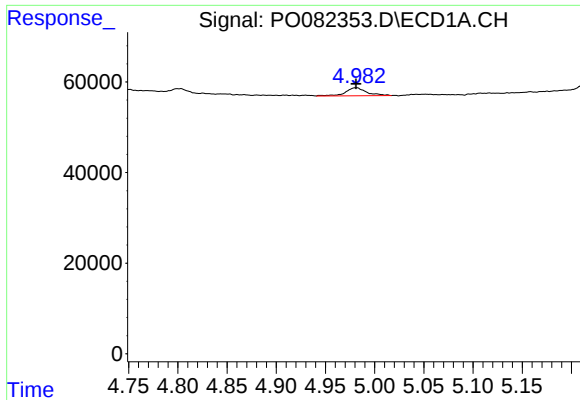

#1 Tetrachloro-m-xylene


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 25730
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2021-3A

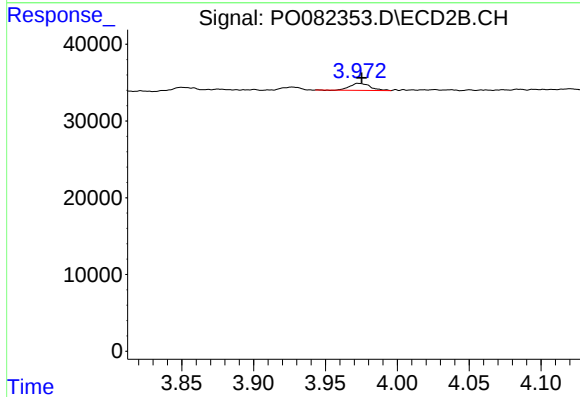


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: -0.002 min
Response: 8912
Conc: 0.30 ng/ml

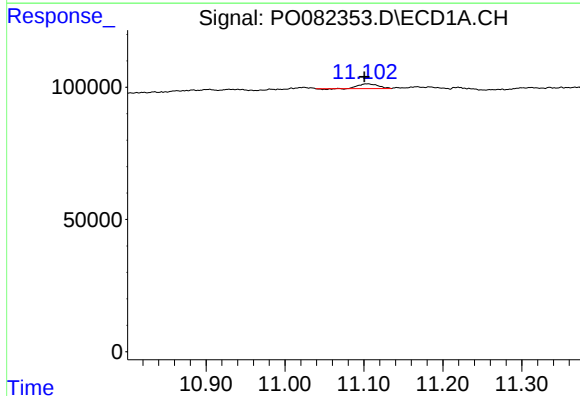

#2 Decachlorobiphenyl

R.T.: 11.104 min
Delta R.T.: 0.003 min
Response: 30678
Conc: 0.55 ng/ml

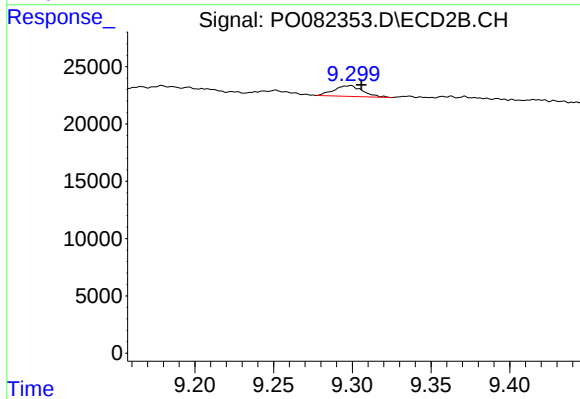

#2 Decachlorobiphenyl

R.T.: 9.299 min
Delta R.T.: -0.006 min
Response: 11982
Conc: 0.47 ng/ml