

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102921\
 Data File : P0082354.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Oct 2021 19:04
 Operator : AJ\MA
 Sample : M4404-05 20X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-2021-3B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 04:15:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 29 11:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.977	3.971	47294	22514	0.585	0.763 #
2) SA Decachlor...	11.098	9.294	44360	15660	0.798	0.615

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102921\
Data File : PO082354.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Oct 2021 19:04
Operator : AJ\MA
Sample : M4404-05 20X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MOO-2021-3B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 04:15:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

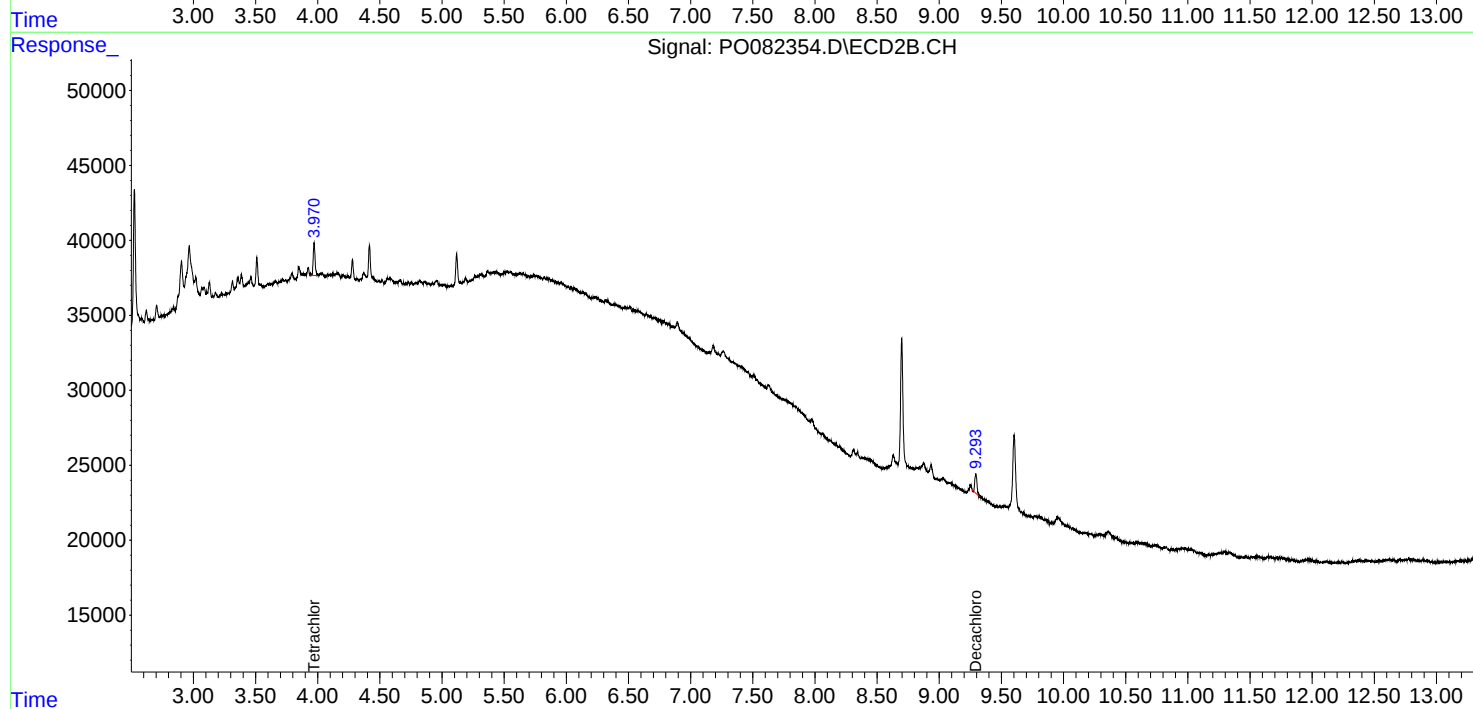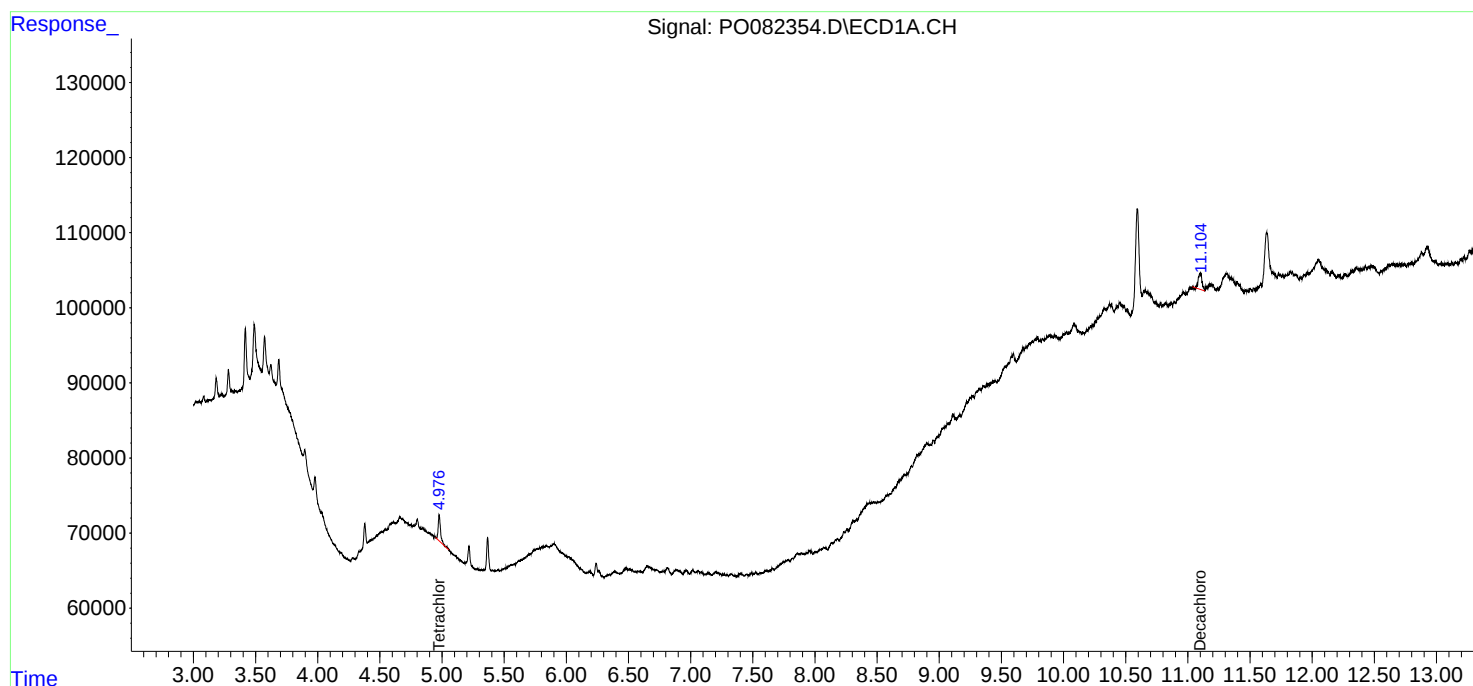


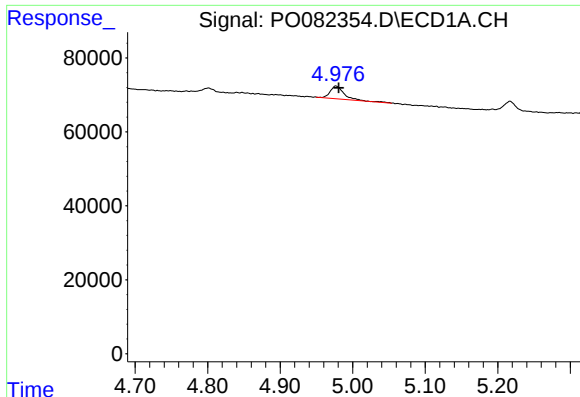

#1 Tetrachloro-m-xylene


R.T.: 4.977 min
Delta R.T.: -0.004 min
Response: 47294
Conc: 0.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2021-3B

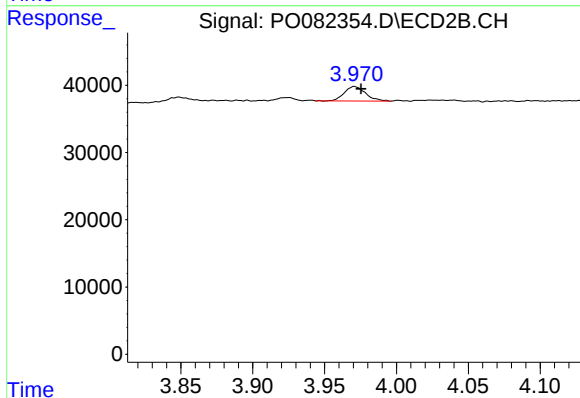


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: -0.005 min
Response: 22514
Conc: 0.76 ng/ml

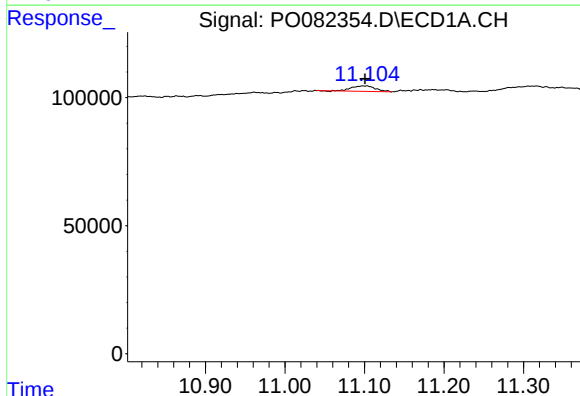

#2 Decachlorobiphenyl

R.T.: 11.098 min
Delta R.T.: -0.003 min
Response: 44360
Conc: 0.80 ng/ml

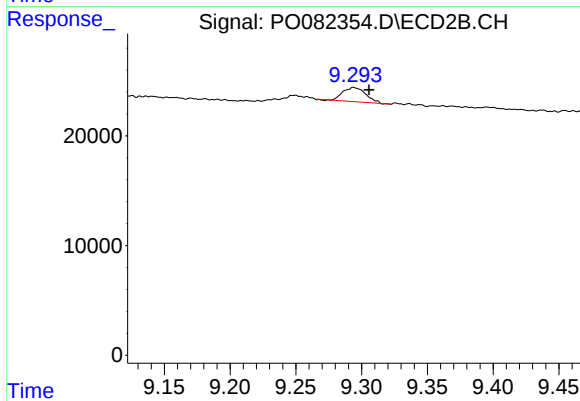

#2 Decachlorobiphenyl

R.T.: 9.294 min
Delta R.T.: -0.012 min
Response: 15660
Conc: 0.61 ng/ml