

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103019\
 Data File : P0063283.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2019 11:11
 Operator : HP/AJ
 Sample : K5569-02RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDW-DECON-WATER-102519RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 11:42:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.482	195995	193214	3.363	3.538
Target Compounds							
3)	L1 AR-1016-1	0.000	4.561	0	34826	N.D.	18.589 #
4)	L1 AR-1016-2	0.000	4.561	0	34826	N.D.	12.768 #
7)	L1 AR-1016-5	0.000	4.971	0	468	N.D.	0.311 #
12)	L3 AR-1232-2	5.244	4.561	196176	34826	198.175	17.705 #
15)	L3 AR-1232-5	0.000	4.971	0	468	N.D.	0.500 #
16)	L4 AR-1242-1	0.000	4.561	0	34826	N.D.	25.202 #
17)	L4 AR-1242-2	0.000	4.561	0	34826	N.D.	16.974 #
20)	L4 AR-1242-5	0.000	5.263	0	34382	N.D.	24.611 #
21)	L5 AR-1248-1	0.000	4.561	0	34826	N.D.	31.863 #
24)	L5 AR-1248-4	0.000	4.971	0	468	N.D.	0.260 #
26)	L6 AR-1254-1	0.000	5.263	0	34382	N.D.	11.414 #
29)	L6 AR-1254-4	0.000	6.092	0	152028	N.D.	53.350 #
32)	L7 AR-1260-2	0.000	6.170	0	67243	N.D.	17.526 #
33)	L7 AR-1260-3	0.000	6.299	0	68825	N.D.	21.935 #
34)	L7 AR-1260-4	0.000	6.750	0	138698	N.D.	54.780 #
36)	L8 AR-1262-1	0.000	6.573	0	311209	N.D.	171.035 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
Data File : P0063283.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 11:11
Operator : HP/AJ
Sample : K5569-02RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 11:42:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

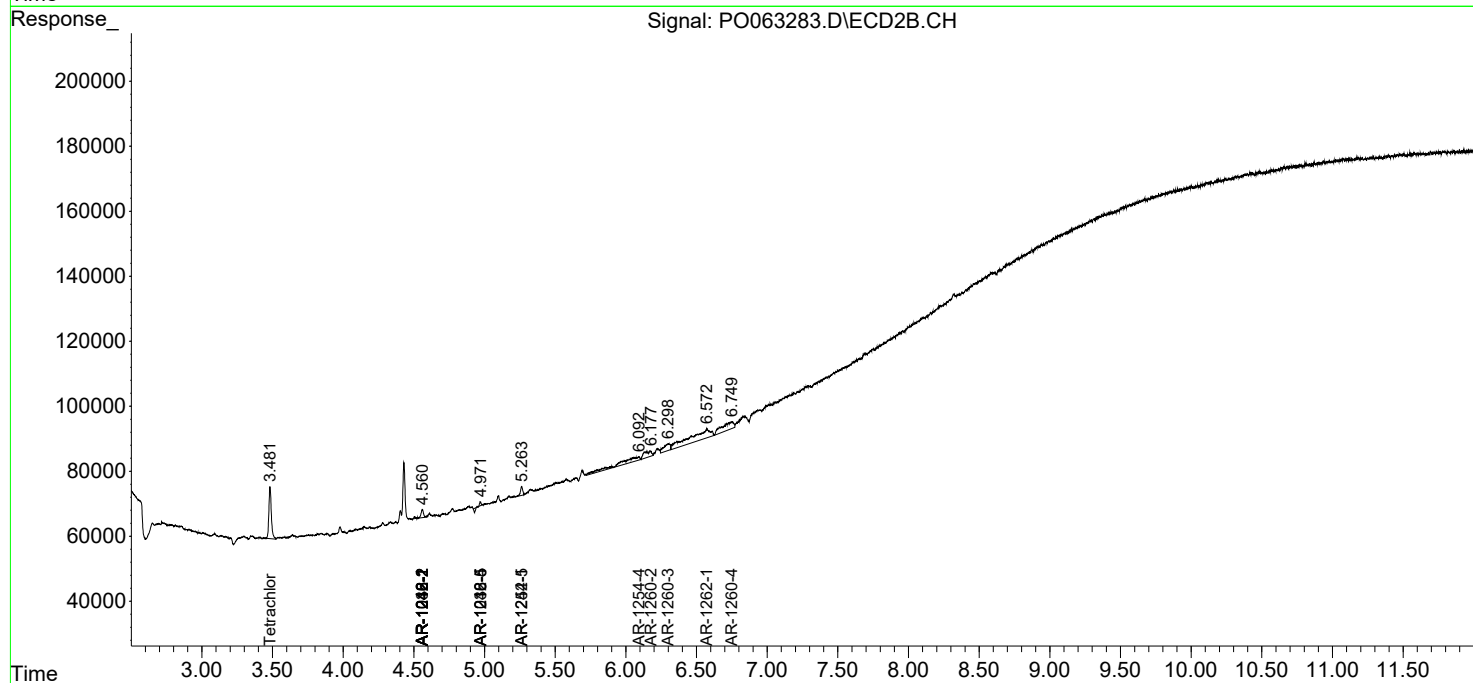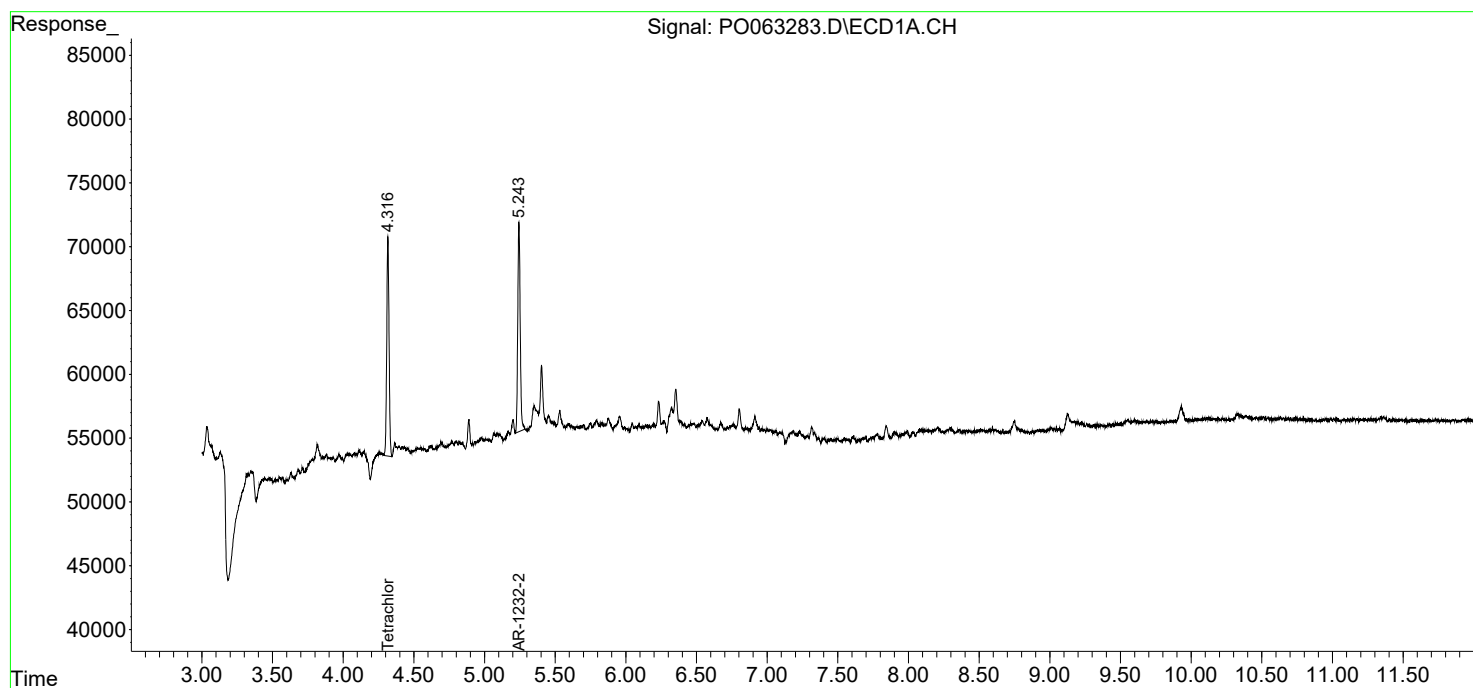


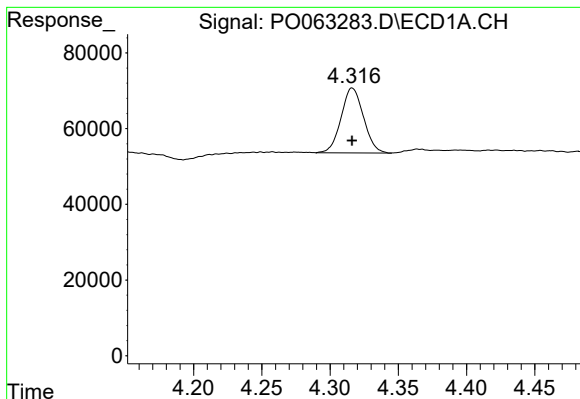

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 195995
Conc: 3.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

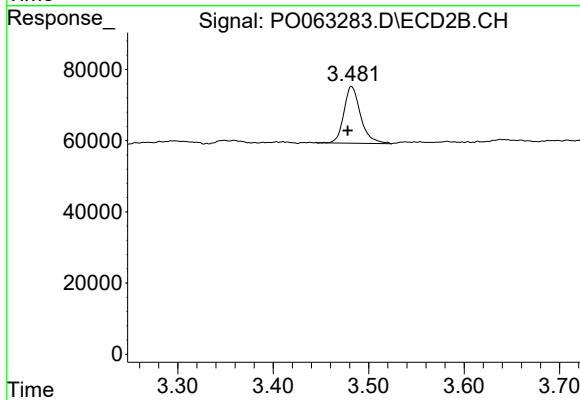


#1 Tetrachloro-m-xylene

R.T.: 3.482 min
Delta R.T.: 0.004 min
Response: 193214
Conc: 3.54 ng/ml

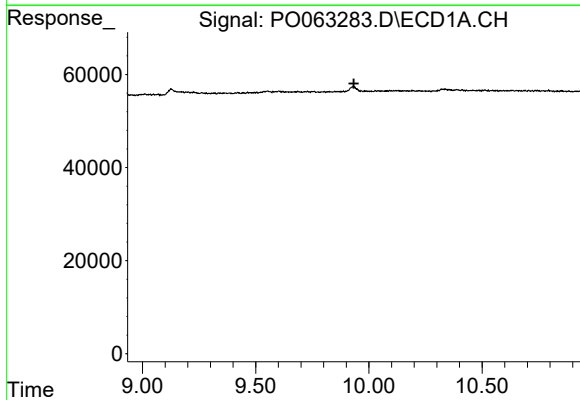


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.934 min
Response: 0
Conc: N.D.

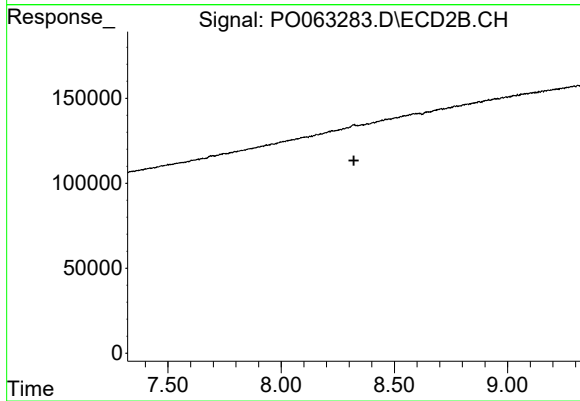

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.321 min
Response: 0
Conc: N.D.

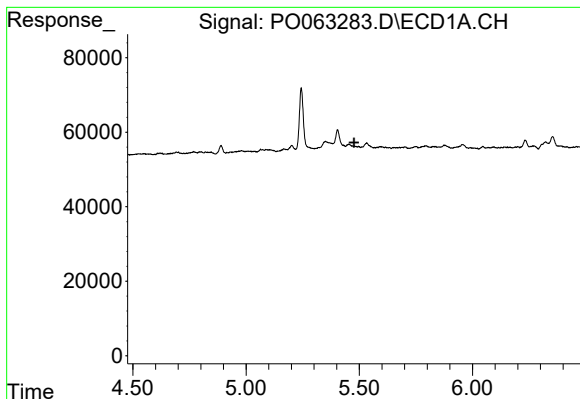

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T. : 5.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

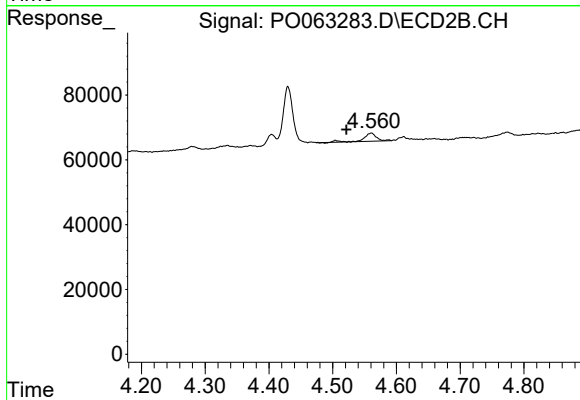


#3 AR-1016-1

R.T.: 4.561 min
Delta R.T.: 0.039 min
Response: 34826
Conc: 18.59 ng/ml

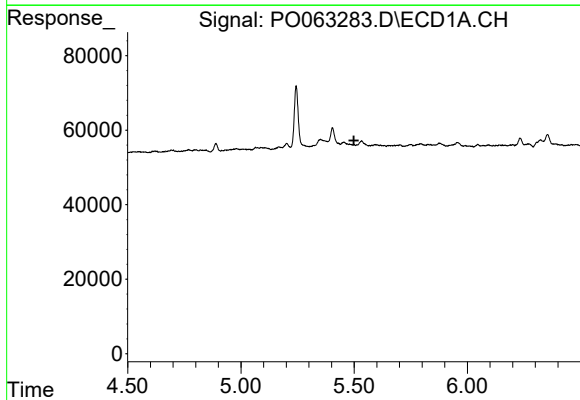


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.499 min
Response: 0
Conc: N.D.

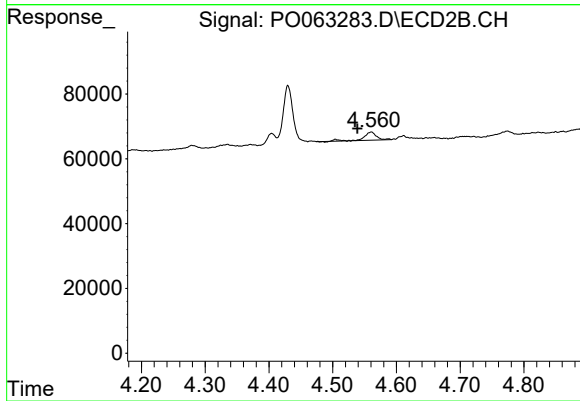

#4 AR-1016-2


R.T.: 4.561 min
Delta R.T.: 0.022 min
Response: 34826
Conc: 12.77 ng/ml

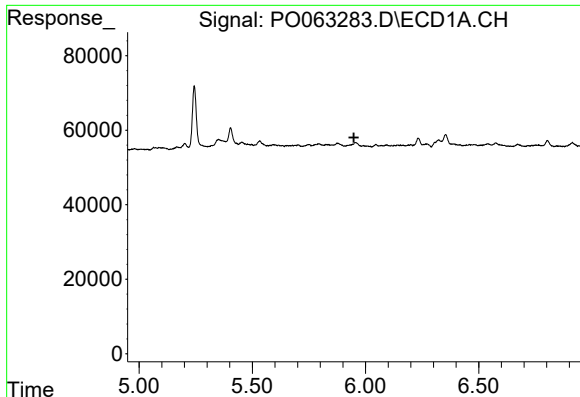

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

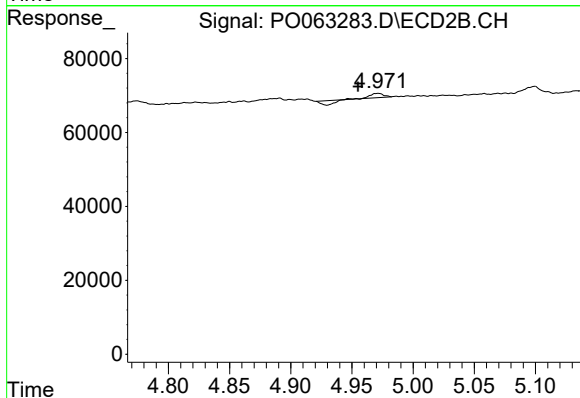


#7 AR-1016-5

R.T.: 4.971 min
Delta R.T.: 0.016 min
Response: 468
Conc: 0.31 ng/ml

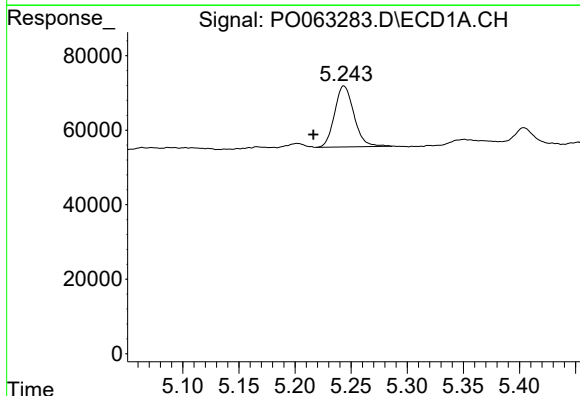


#12 AR-1232-2

R.T.: 5.244 min
Delta R.T.: 0.027 min
Response: 196176
Conc: 198.18 ng/ml

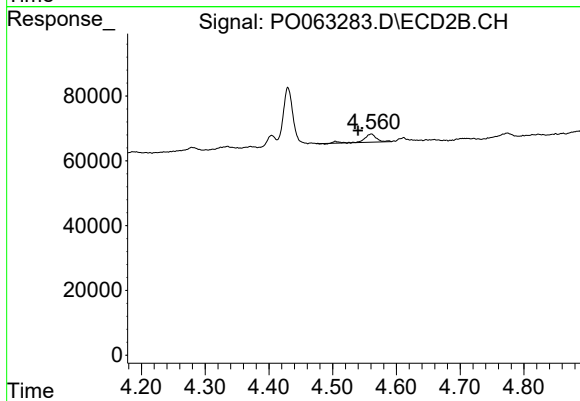

#12 AR-1232-2


R.T.: 4.561 min
Delta R.T.: 0.021 min
Response: 34826
Conc: 17.70 ng/ml

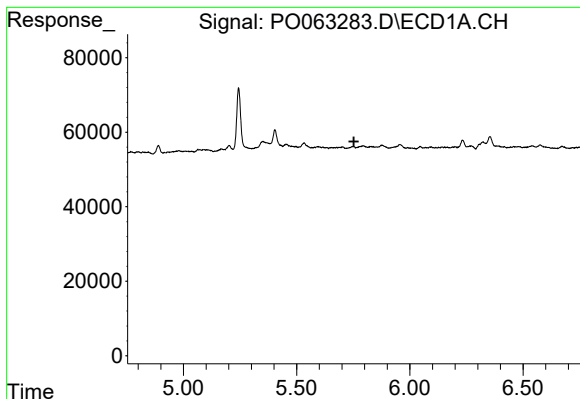

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.753 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

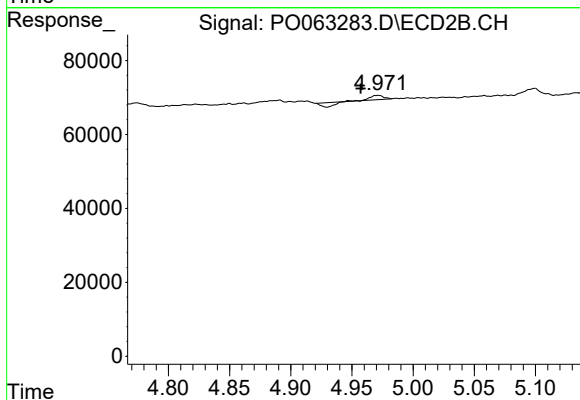


#15 AR-1232-5

R.T.: 4.971 min
Delta R.T.: 0.014 min
Response: 468
Conc: 0.50 ng/ml

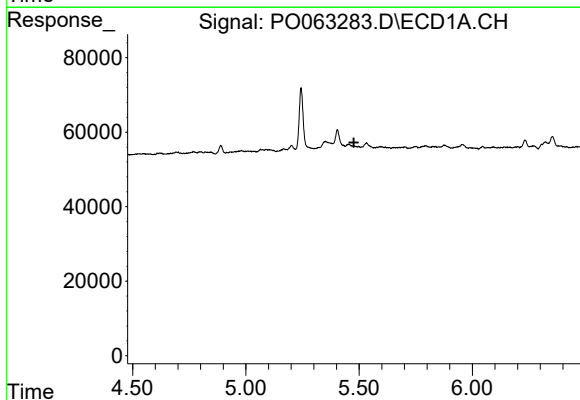


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.477 min
Response: 0
Conc: N.D.

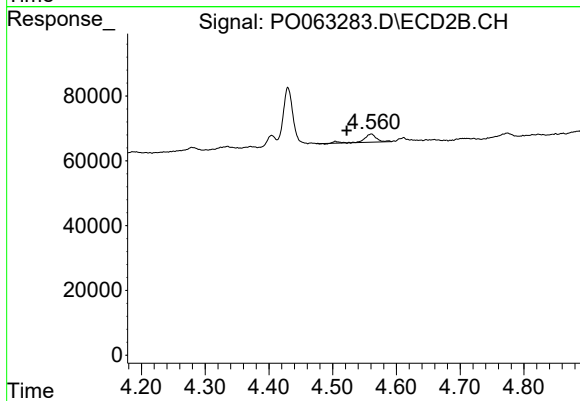

#16 AR-1242-1


R.T.: 4.561 min
Delta R.T.: 0.038 min
Response: 34826
Conc: 25.20 ng/ml

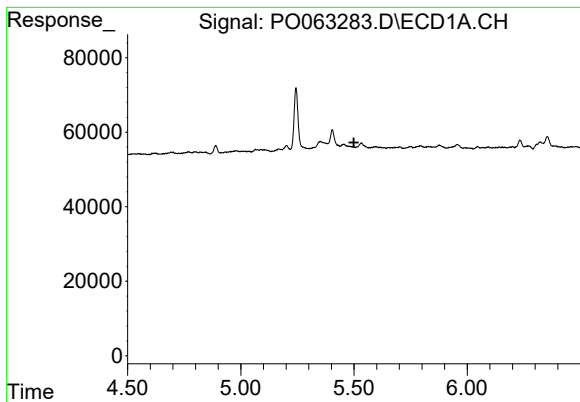

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

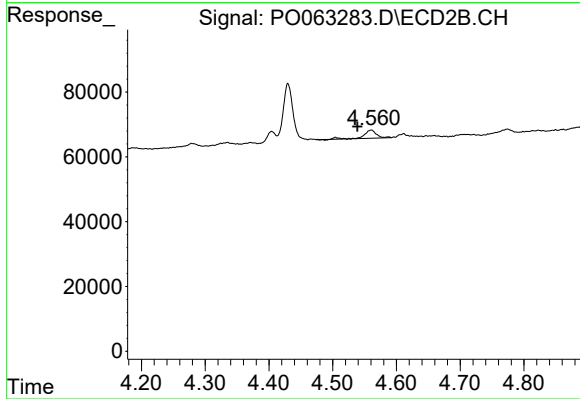


#17 AR-1242-2

R.T.: 4.561 min
Delta R.T.: 0.022 min
Response: 34826
Conc: 16.97 ng/ml

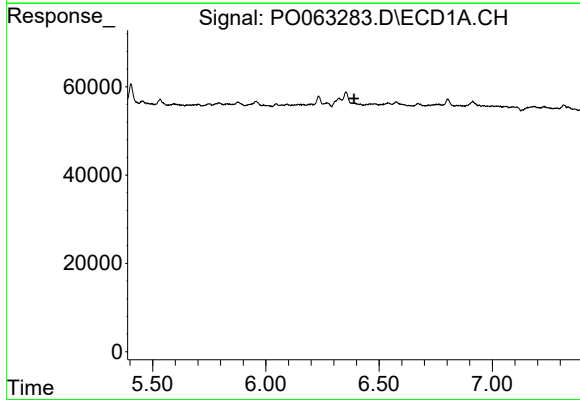


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

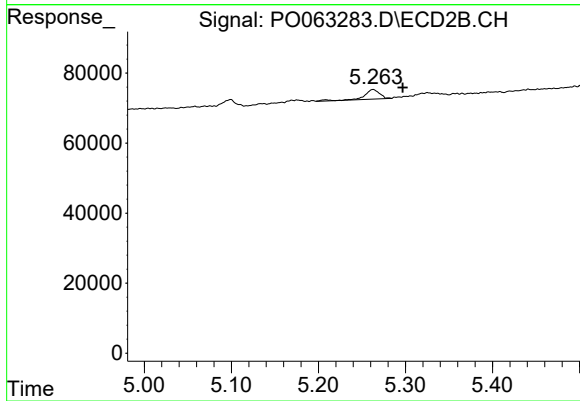

#20 AR-1242-5


R.T.: 5.263 min
Delta R.T.: -0.034 min
Response: 34382
Conc: 24.61 ng/ml

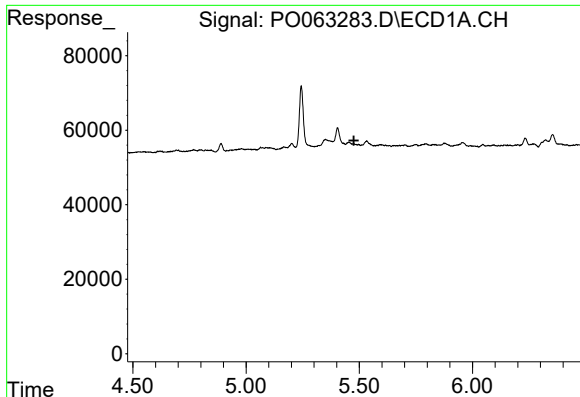

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

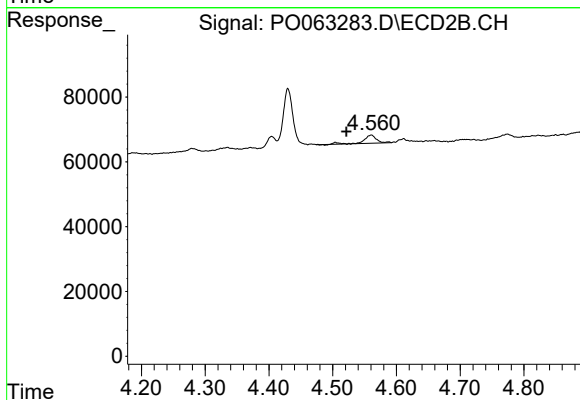


#21 AR-1248-1

R.T.: 4.561 min
Delta R.T.: 0.039 min
Response: 34826
Conc: 31.86 ng/ml

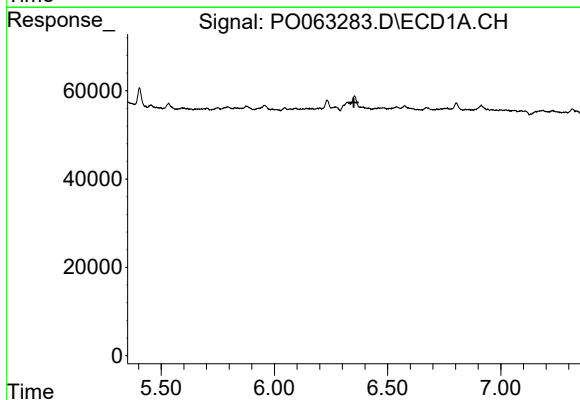


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.351 min
Response: 0
Conc: N.D.

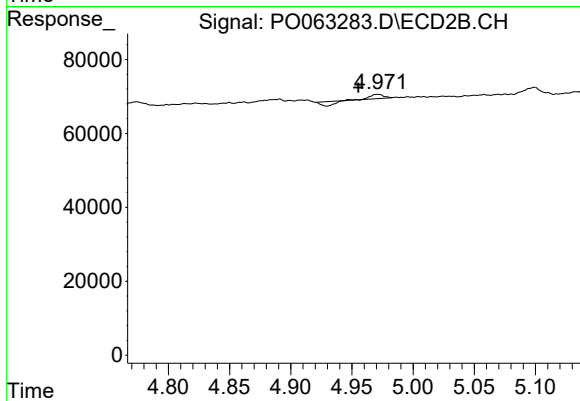

#24 AR-1248-4


R.T.: 4.971 min
Delta R.T.: 0.016 min
Response: 468
Conc: 0.26 ng/ml

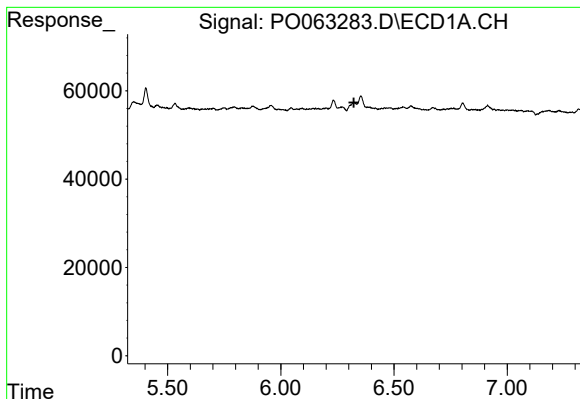

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

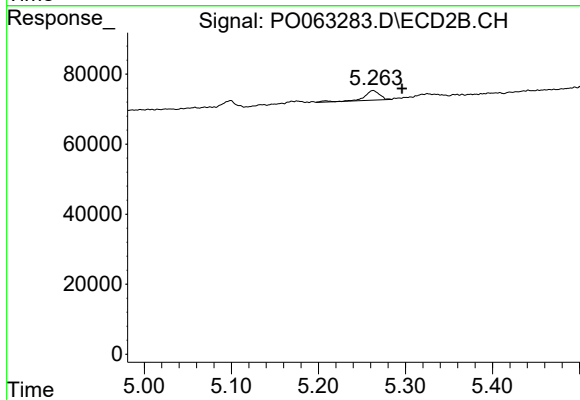


#26 AR-1254-1

R.T.: 5.263 min
Delta R.T.: -0.033 min
Response: 34382
Conc: 11.41 ng/ml

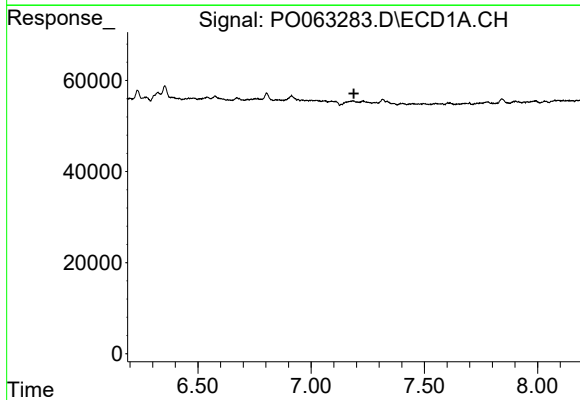


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 7.189 min
Response: 0
Conc: N.D.

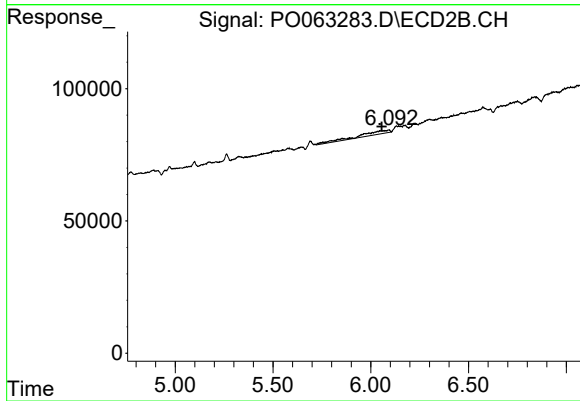

#29 AR-1254-4


R.T.: 6.092 min
Delta R.T.: 0.036 min
Response: 152028
Conc: 53.35 ng/ml

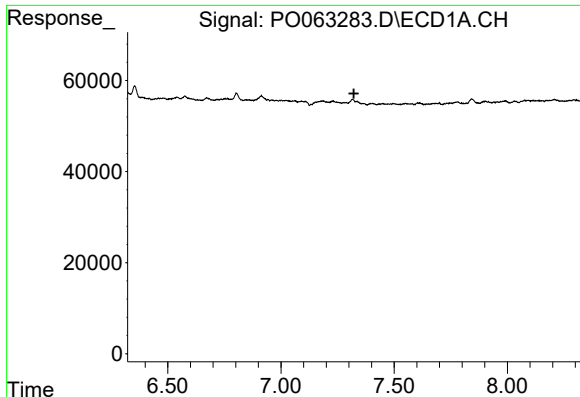

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.322 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

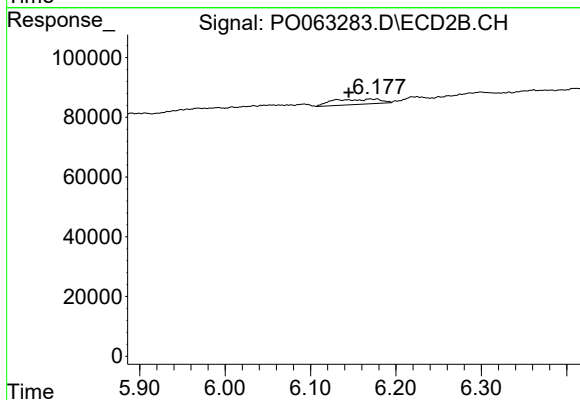


#32 AR-1260-2

R.T.: 6.170 min
Delta R.T.: 0.025 min
Response: 67243
Conc: 17.53 ng/ml

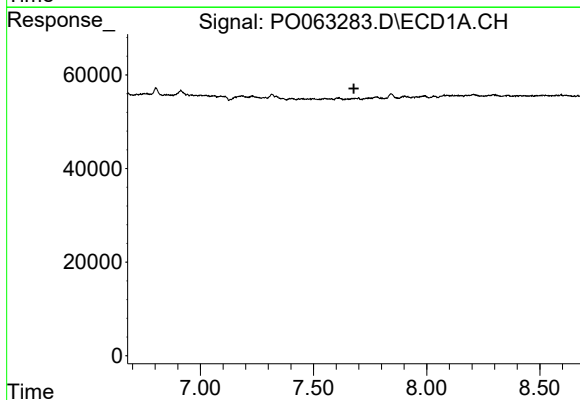


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.678 min
Response: 0
Conc: N.D.

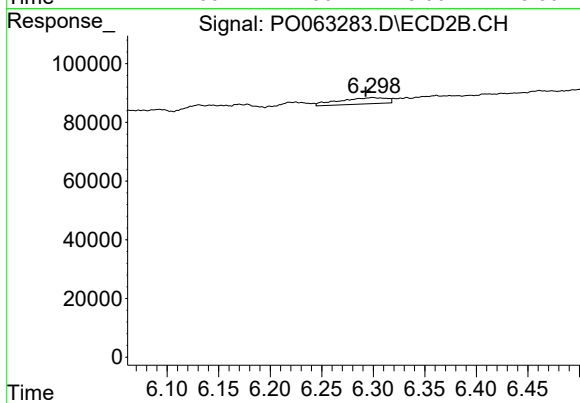

#33 AR-1260-3


R.T.: 6.299 min
Delta R.T.: 0.007 min
Response: 68825
Conc: 21.94 ng/ml

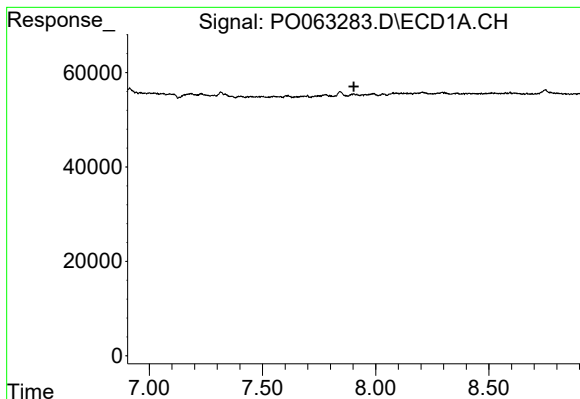

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
IDW-DECON-WATER-102519RE

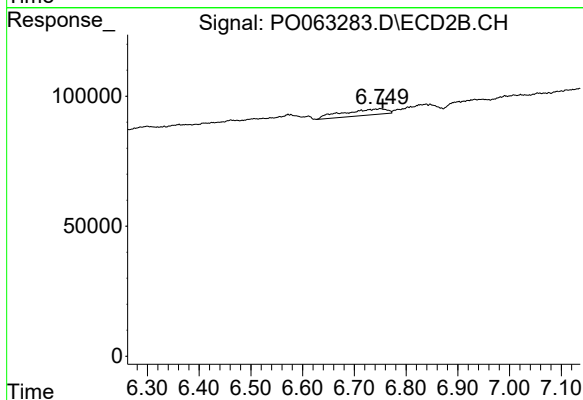


#34 AR-1260-4

R.T.: 6.750 min
Delta R.T.: -0.005 min
Response: 138698
Conc: 54.78 ng/ml

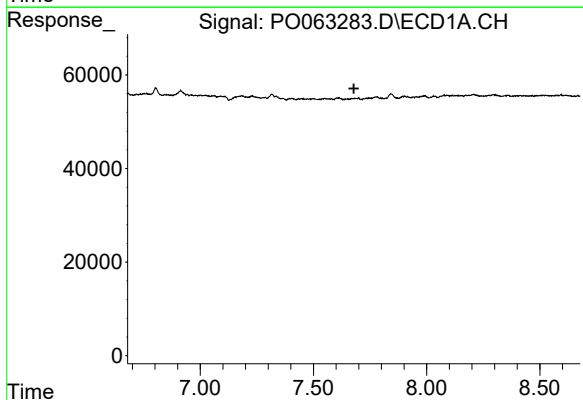

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.678 min
Response: 0
Conc: N.D.

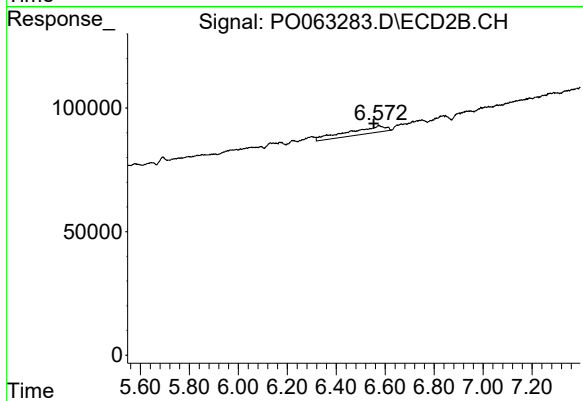

#36 AR-1262-1

R.T.: 6.573 min
Delta R.T.: 0.019 min
Response: 311209
Conc: 171.03 ng/ml