Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
Data File : PO063307.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 17:51
Operator : HP/AJ
Sample : K5599-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument : ECD_O
ClientSampleId : Z3-21A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:56:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	4.316	3.479	1170137	1154223	20.077	21.134
2)	SA Decachlor...	9.930	8.320	1013110	682901	17.412	15.973
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
Data File : PO063307.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 17:51
Operator : HP/AJ
Sample : K5599-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument : ECD_O
ClientSampleId : Z3-21A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:56:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

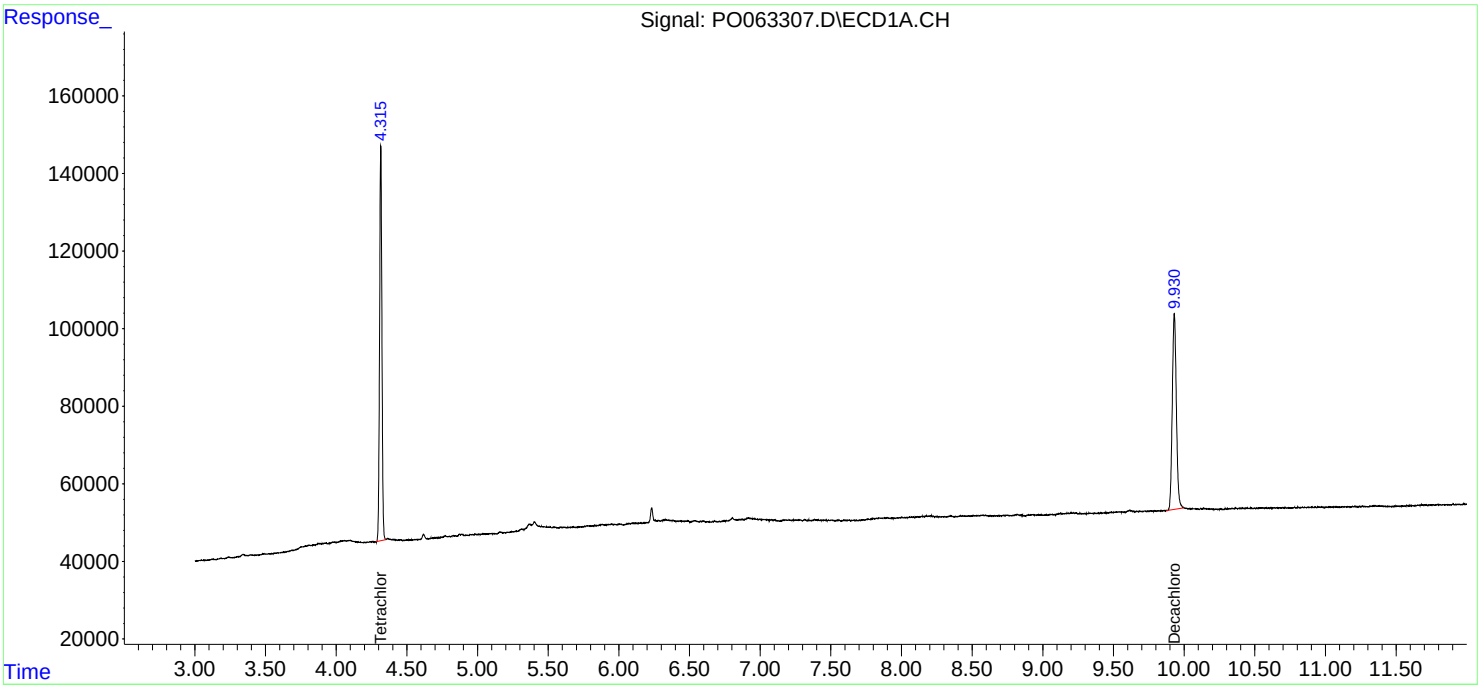

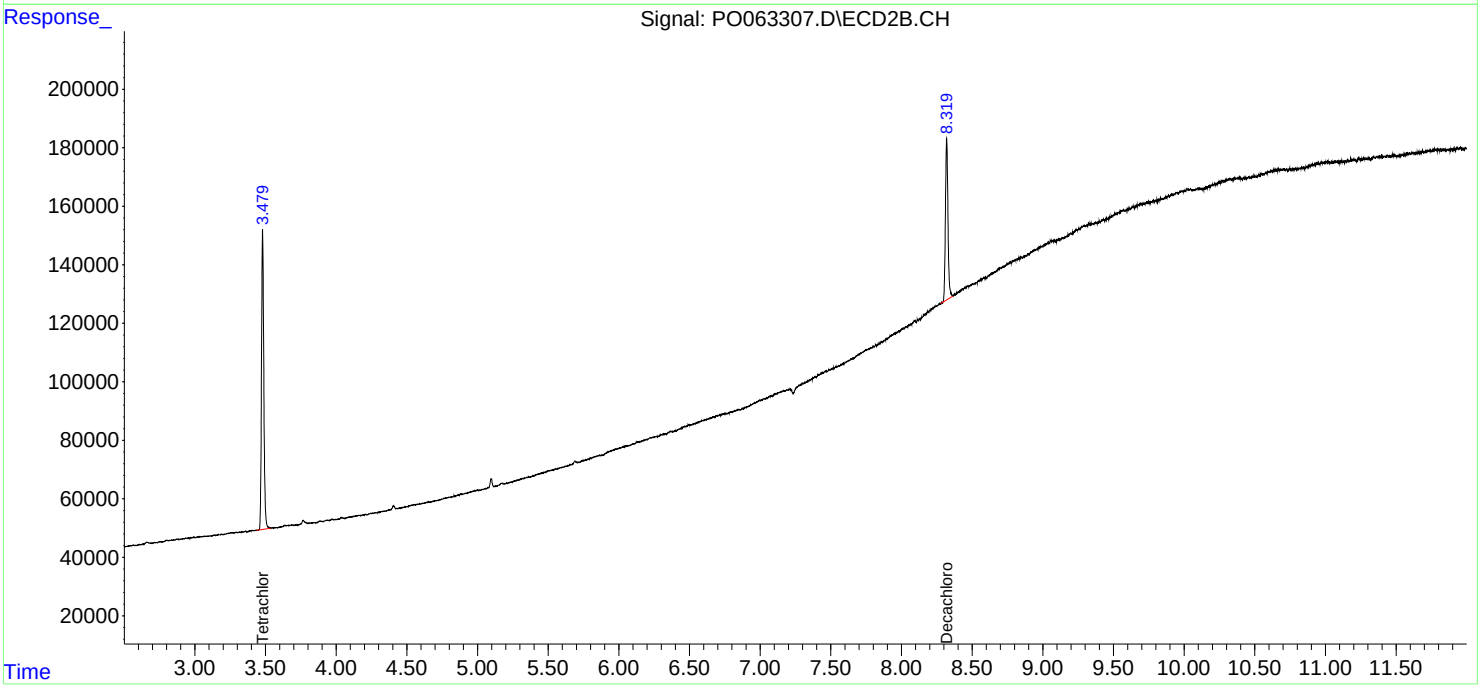

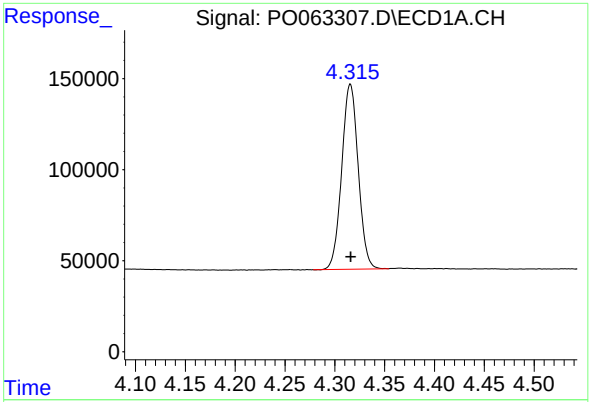

#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 1170137
Conc: 20.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
Z3-21A

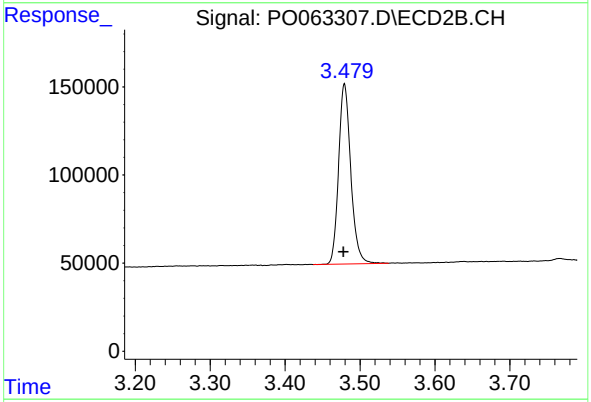

#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.001 min
Response: 1154223
Conc: 21.13 ng/ml

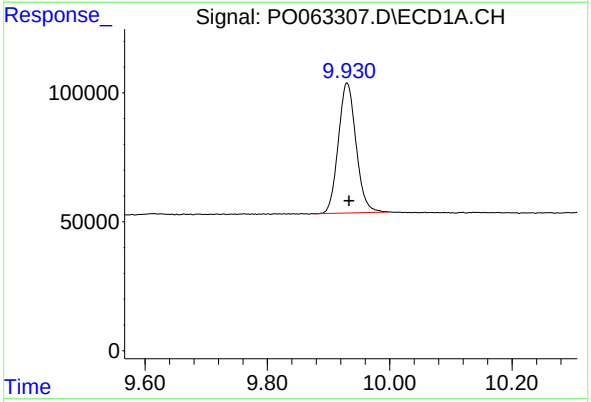

#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: -0.003 min
Response: 1013110
Conc: 17.41 ng/ml

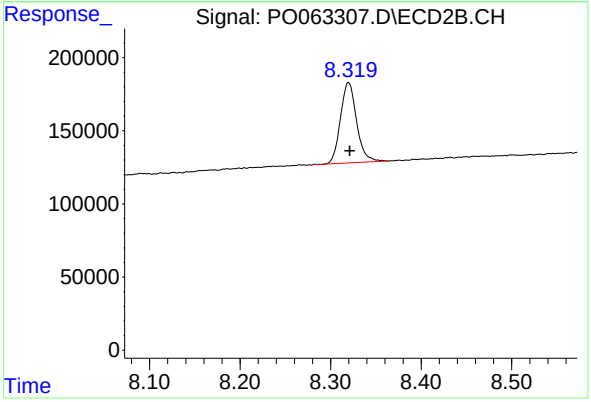

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.001 min
Response: 682901
Conc: 15.97 ng/ml