

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103019\
 Data File : P0063332.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Oct 2019 1:34
 Operator : HP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 04:12:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.480	1401226	1350132	24.042	24.721
2)	SA Decachlor...	9.931	8.318	1202886	884973	20.674	20.700
Target Compounds							
7)	L1 AR-1016-5	0.000	4.913	0	95700	N.D.	63.524 #
15)	L3 AR-1232-5	0.000	4.913	0	95700	N.D.	102.248 #
20)	L4 AR-1242-5	0.000	5.320	0	111945	N.D.	80.131 #
24)	L5 AR-1248-4	0.000	4.913	0	95700	N.D.	53.146 #
25)	L5 AR-1248-5	0.000	5.320	0	111945	N.D.	60.558 #
26)	L6 AR-1254-1	0.000	5.320	0	111945	N.D.	37.163 #
40)	L8 AR-1262-5	0.000	7.779	0	21319	N.D.	10.864 #
44)	L9 AR-1268-4	0.000	7.779	0	21319	N.D.	9.877 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
Data File : PO063332.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Oct 2019 1:34
Operator : HP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 04:12:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

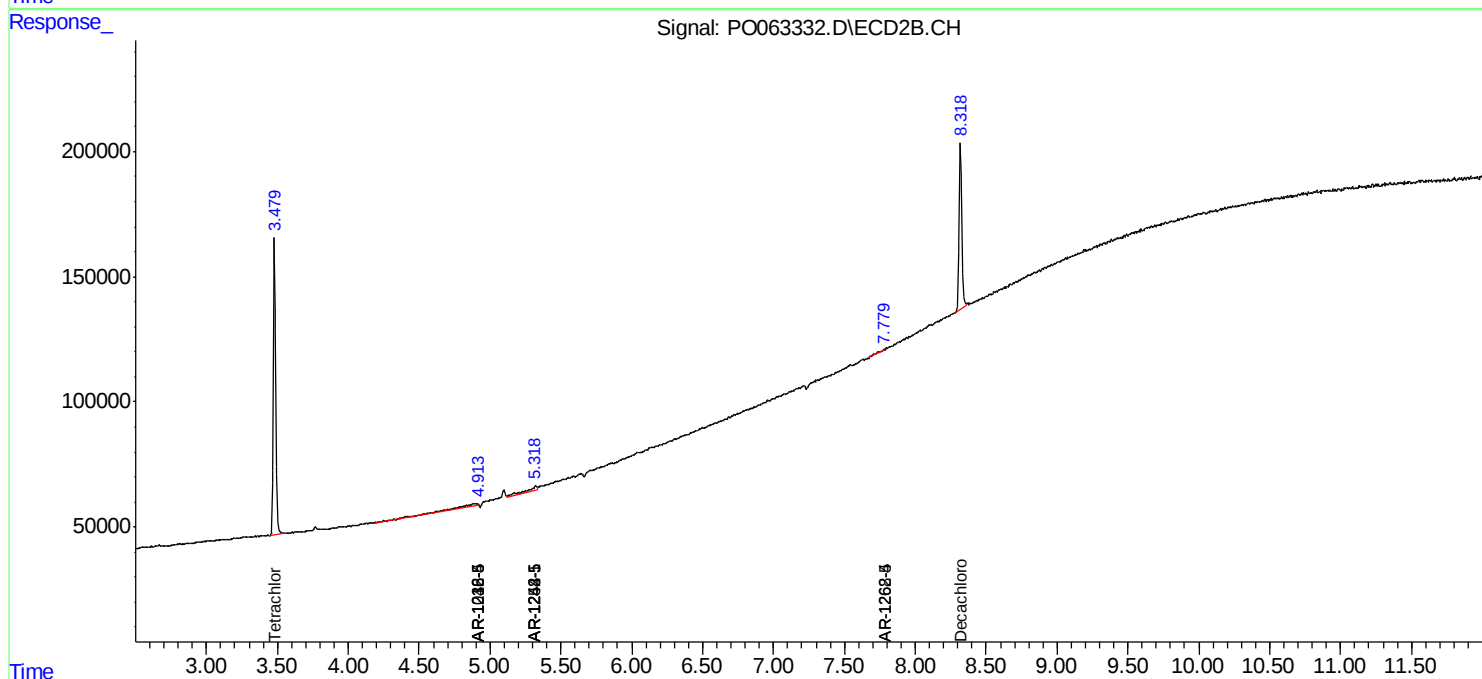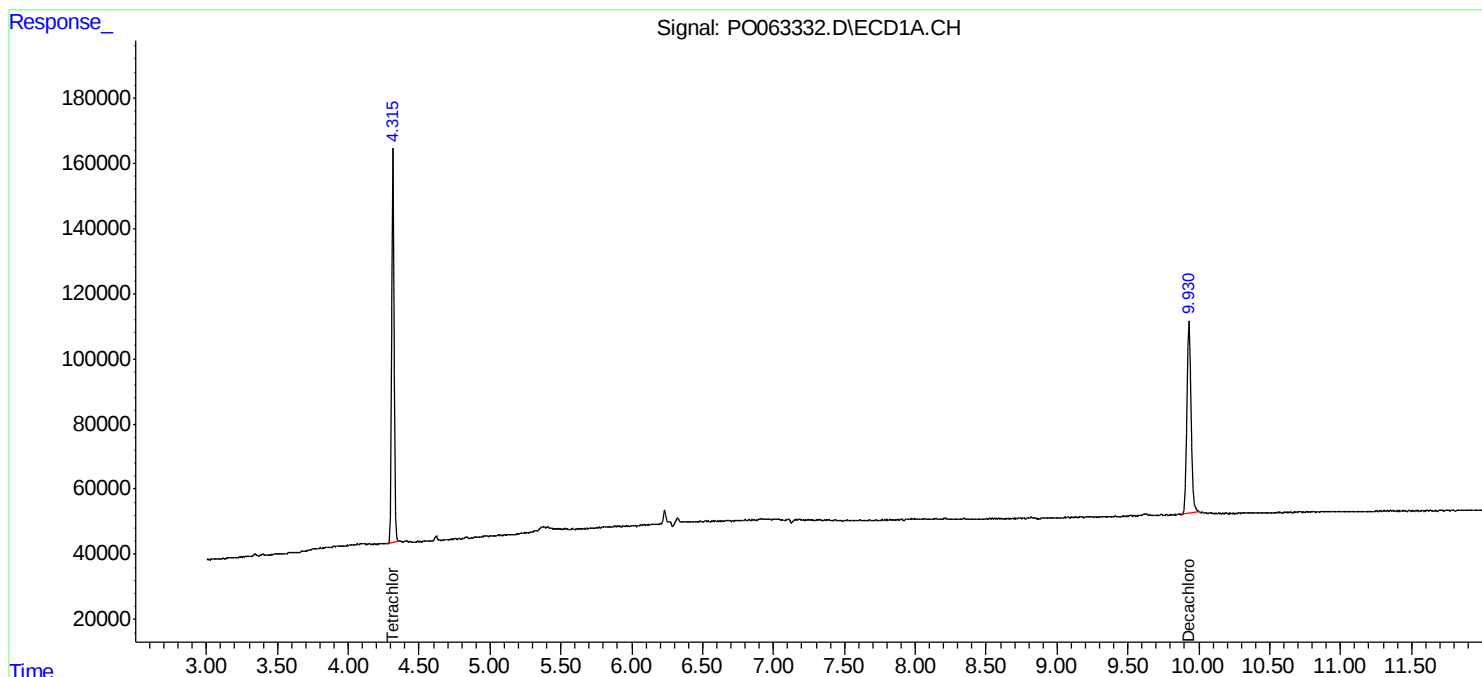


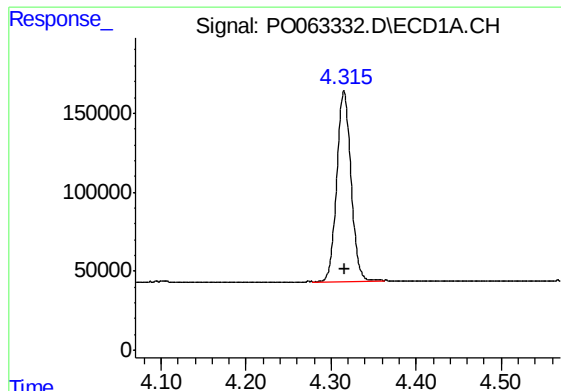

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: 0.000 min
Response: 1401226
Conc: 24.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

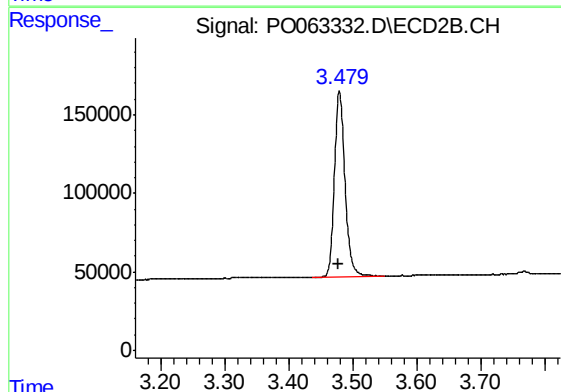


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 1350132
Conc: 24.72 ng/ml

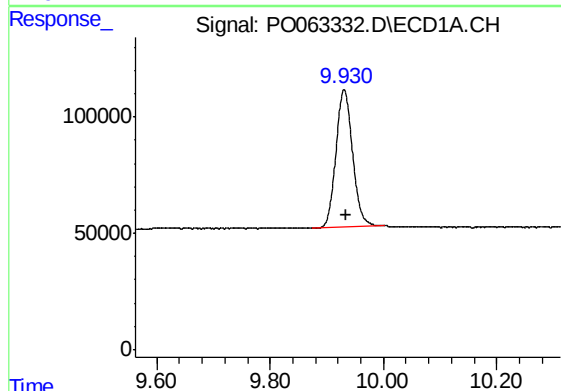


#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.003 min
Response: 1202886
Conc: 20.67 ng/ml

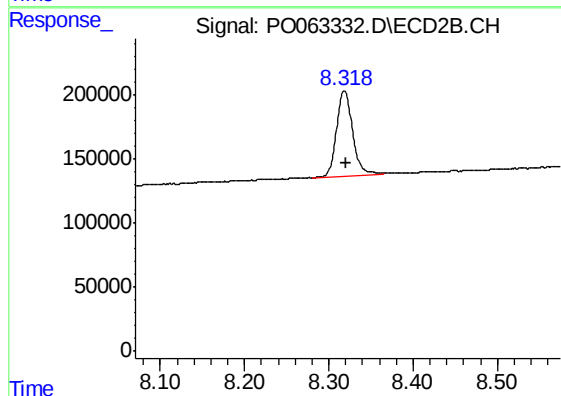

#2 Decachlorobiphenyl


R.T.: 8.318 min
Delta R.T.: -0.003 min
Response: 884973
Conc: 20.70 ng/ml

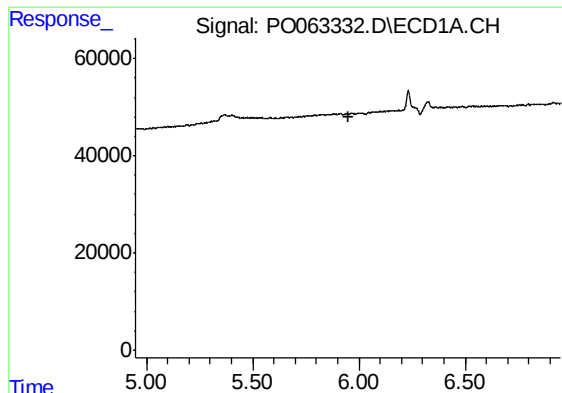

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

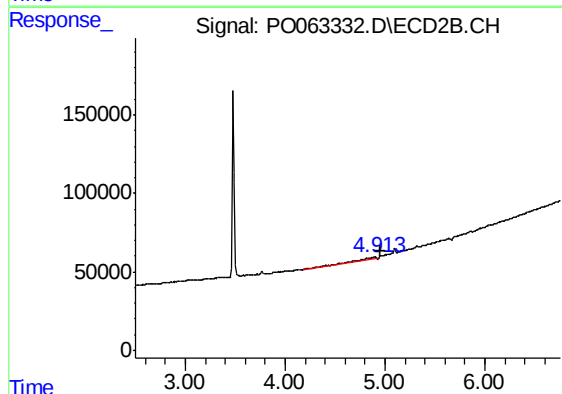


#7 AR-1016-5

R.T.: 4.913 min
Delta R.T.: -0.042 min
Response: 95700
Conc: 63.52 ng/ml

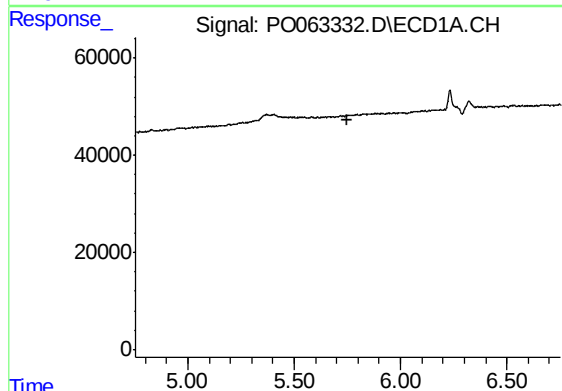


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.753 min
Response: 0
Conc: N.D.

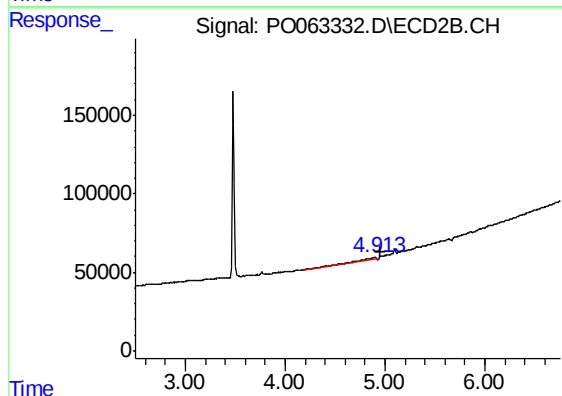

#15 AR-1232-5


R.T.: 4.913 min
Delta R.T.: -0.044 min
Response: 95700
Conc: 102.25 ng/ml

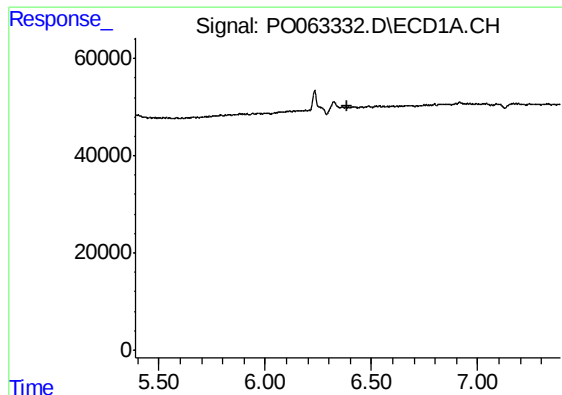

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

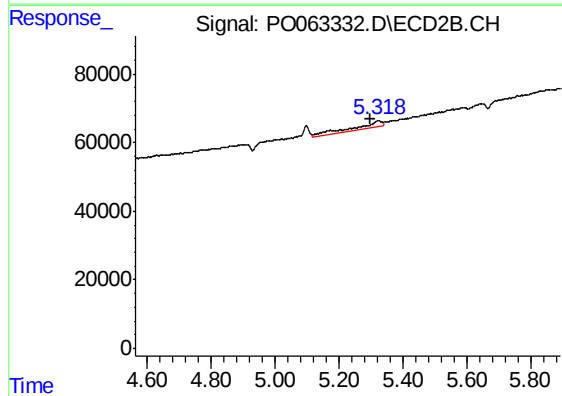


#20 AR-1242-5

R.T.: 5.320 min
Delta R.T.: 0.023 min
Response: 111945
Conc: 80.13 ng/ml

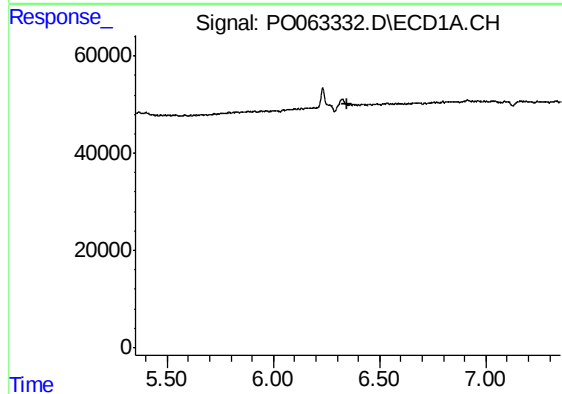


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.351 min
Response: 0
Conc: N.D.

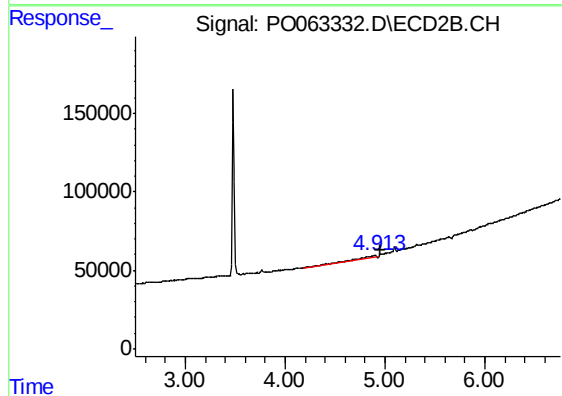

#24 AR-1248-4


R.T.: 4.913 min
Delta R.T.: -0.042 min
Response: 95700
Conc: 53.15 ng/ml

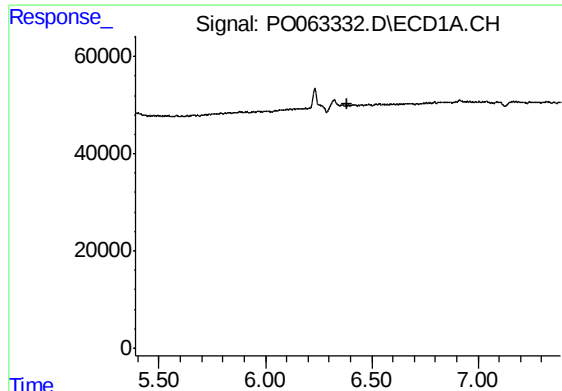

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.388 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

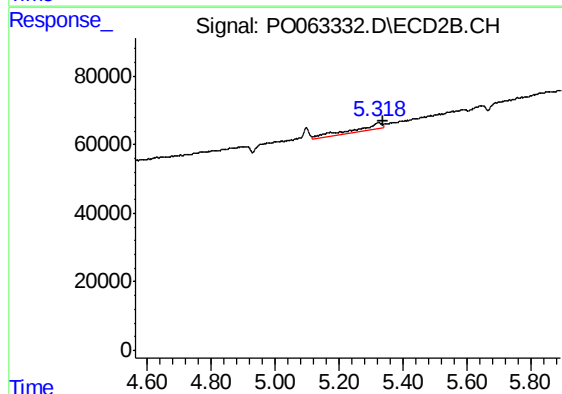


#25 AR-1248-5

R.T.: 5.320 min
Delta R.T.: -0.016 min
Response: 111945
Conc: 60.56 ng/ml

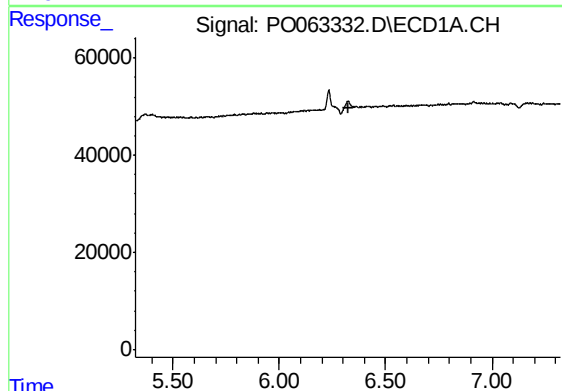


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.

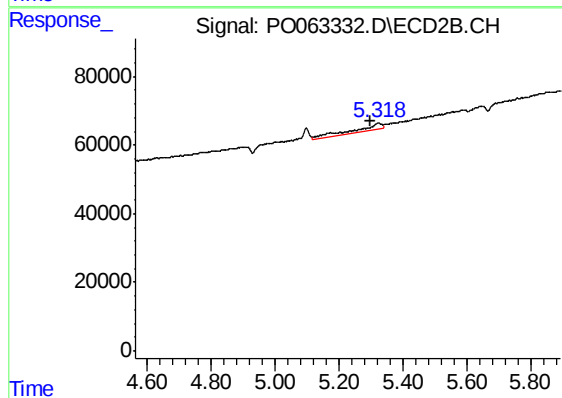

#26 AR-1254-1


R.T.: 5.320 min
Delta R.T.: 0.024 min
Response: 111945
Conc: 37.16 ng/ml

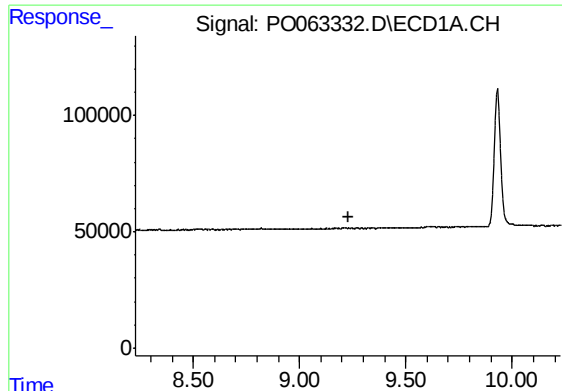

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

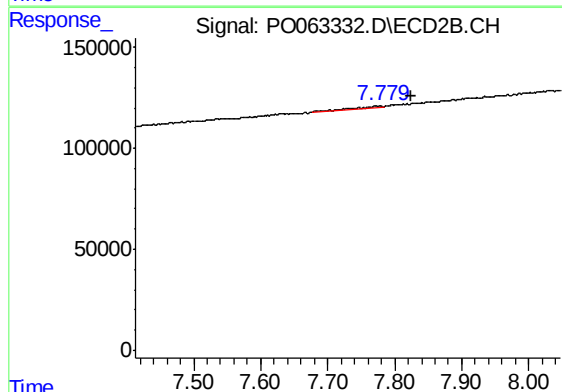


#40 AR-1262-5

R.T.: 7.779 min
Delta R.T.: -0.045 min
Response: 21319
Conc: 10.86 ng/ml

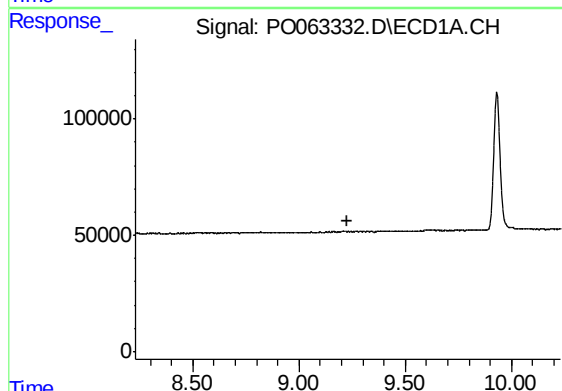

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.230 min
Response: 0
Conc: N.D.

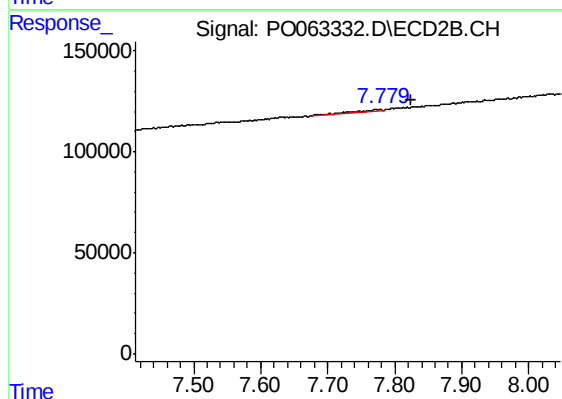

#44 AR-1268-4

R.T.: 7.779 min
Delta R.T.: -0.046 min
Response: 21319
Conc: 9.88 ng/ml