

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103019\
 Data File : P0063285.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2019 11:44
 Operator : HP/AJ
 Sample : K5584-01DL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-9A-(0-2)DL

Manual Integrations
 APPROVED

Ankita
 10/31/2019 9:53:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 01:49:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.480	120881	115213	2.074	2.110
2)	SA Decachlor...	9.932	8.320	93381	57326	1.605m	1.341
Target Compounds							
26)	L6 AR-1254-1	6.321	5.295	689032	698531	271.015	231.893
27)	L6 AR-1254-2	6.538	5.440	1398326	1057301	345.691	392.028
28)	L6 AR-1254-3	6.903	5.831	1868795	1944894	439.055	453.016
29)	L6 AR-1254-4	7.187	6.055	1345369	1208232	397.474	423.994
30)	L6 AR-1254-5	7.604	6.464	1817088	2450951	547.809	657.506

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
Data File : PO063285.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 11:44
Operator : HP/AJ
Sample : K5584-01DL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
445X-9A-(0-2)DL


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:49:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

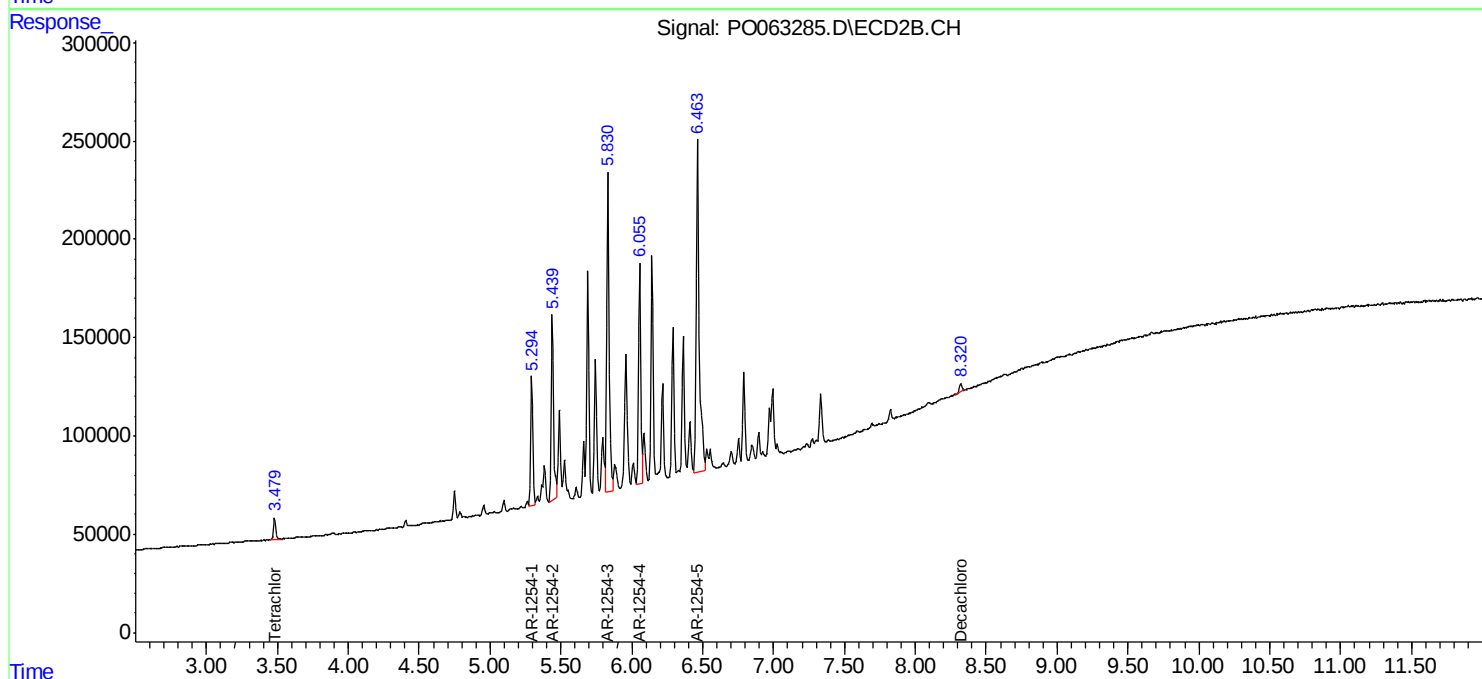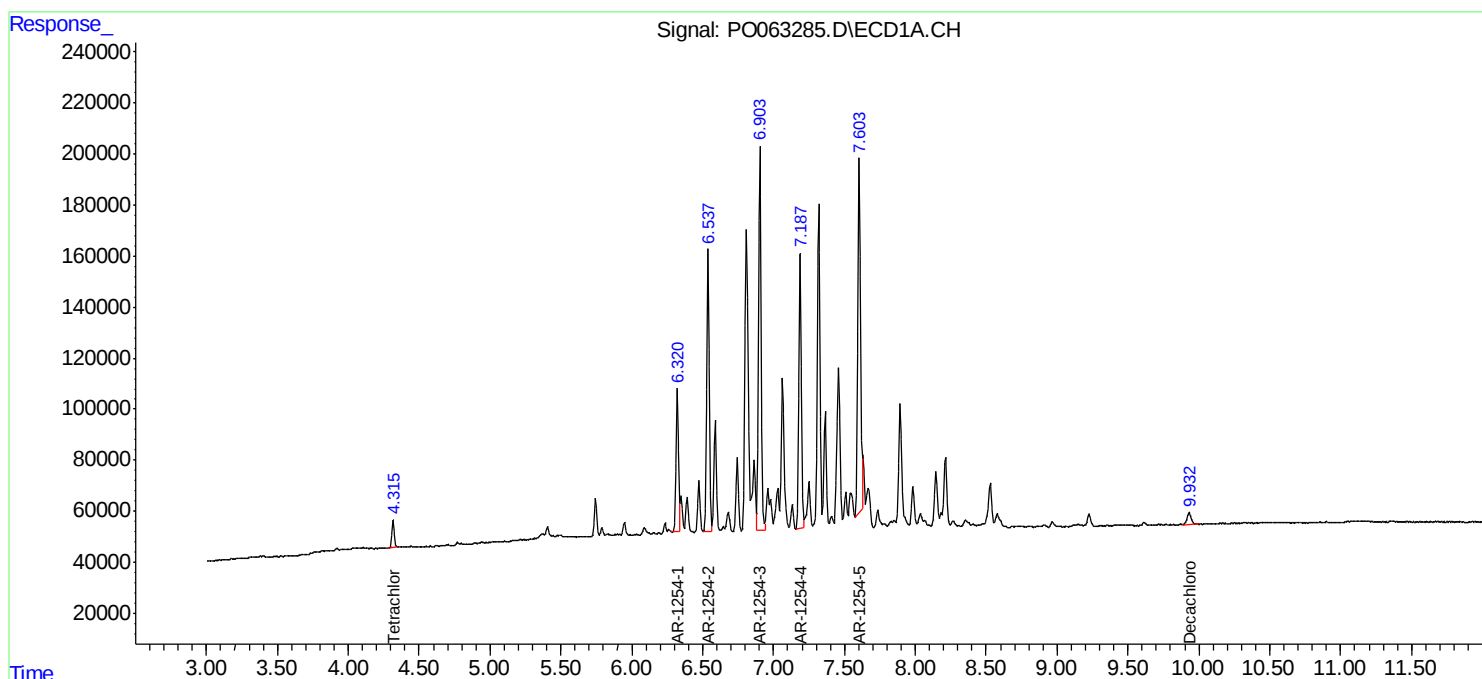

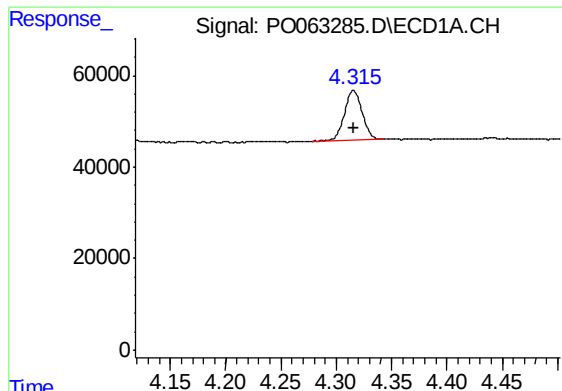


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 120881
Conc: 2.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(0-2)DL


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:16 AM

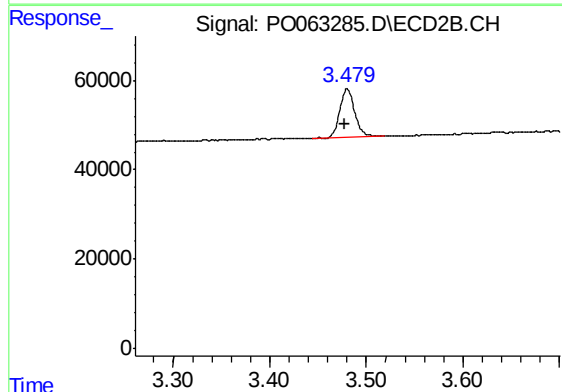


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 115213
Conc: 2.11 ng/ml

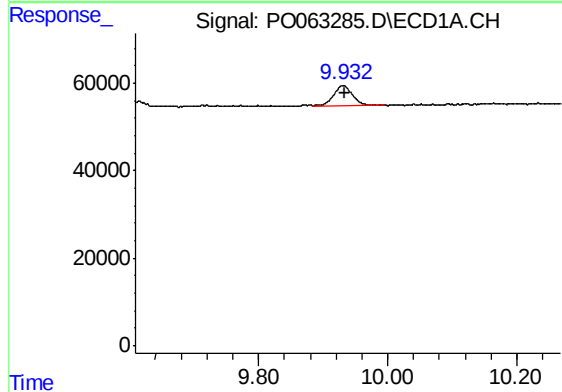


#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.002 min
Response: 93381
Conc: 1.60 ng/ml m

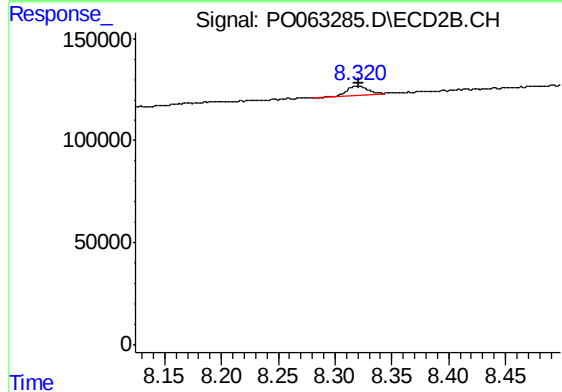

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 57326
Conc: 1.34 ng/ml

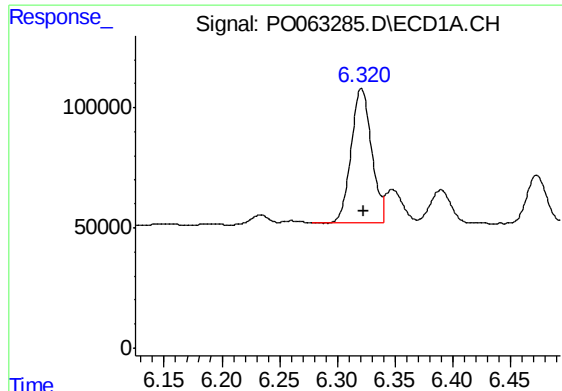


#26 AR-1254-1

R.T.: 6.321 min
Delta R.T.: -0.002 min
Response: 689032
Conc: 271.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(0-2)DL


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:16 AM

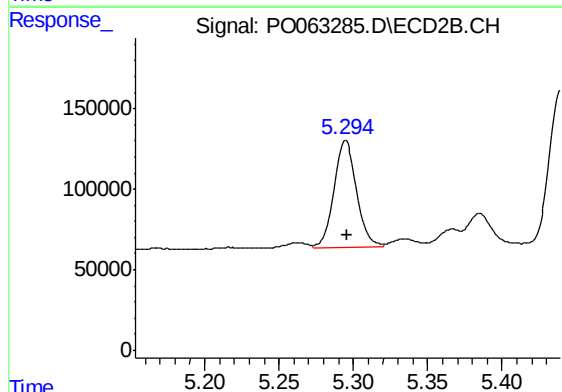


#26 AR-1254-1

R.T.: 5.295 min
Delta R.T.: -0.001 min
Response: 698531
Conc: 231.89 ng/ml

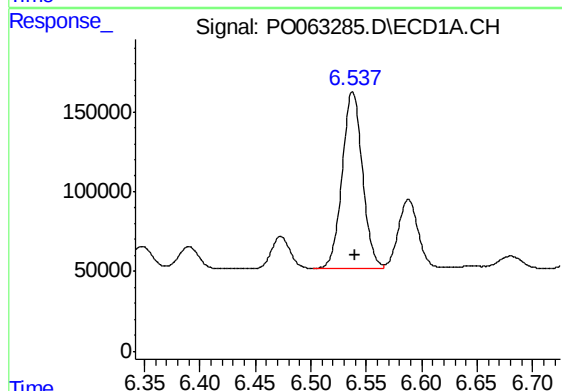


#27 AR-1254-2

R.T.: 6.538 min
Delta R.T.: -0.002 min
Response: 1398326
Conc: 345.69 ng/ml

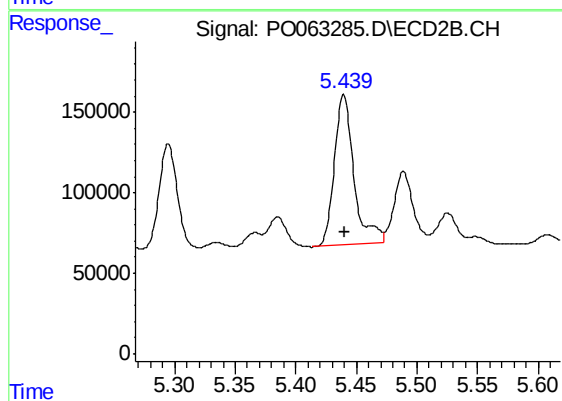

#27 AR-1254-2

R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 1057301
Conc: 392.03 ng/ml

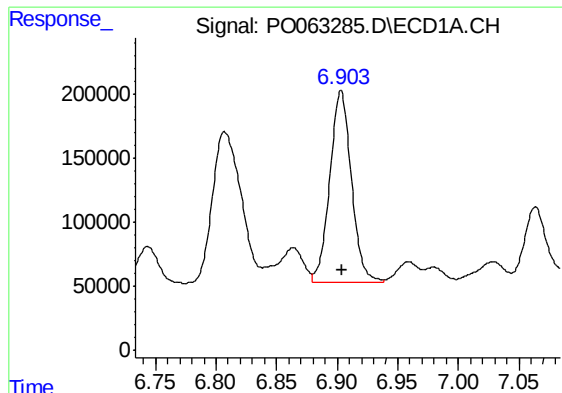


#28 AR-1254-3

R.T.: 6.903 min
Delta R.T.: -0.001 min
Response: 1868795
Conc: 439.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(0-2)DL


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:16 AM

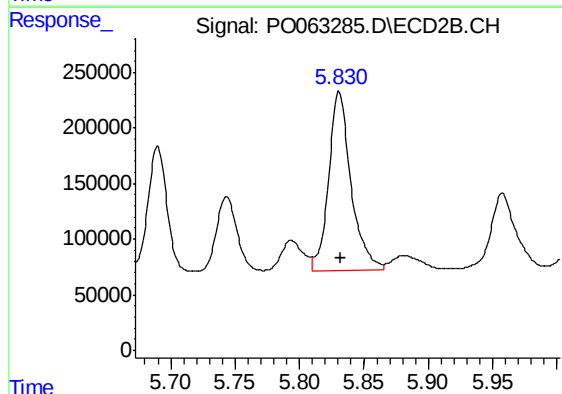


#28 AR-1254-3

R.T.: 5.831 min
Delta R.T.: -0.002 min
Response: 1944894
Conc: 453.02 ng/ml

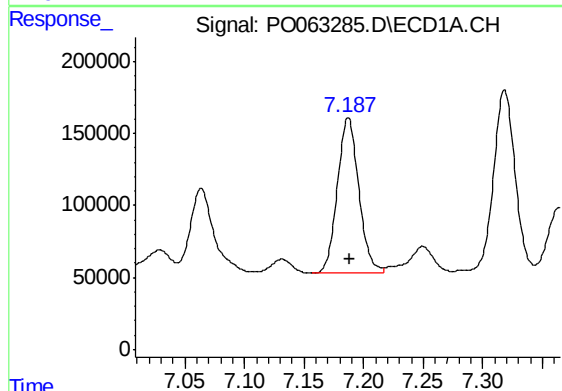


#29 AR-1254-4

R.T.: 7.187 min
Delta R.T.: -0.002 min
Response: 1345369
Conc: 397.47 ng/ml

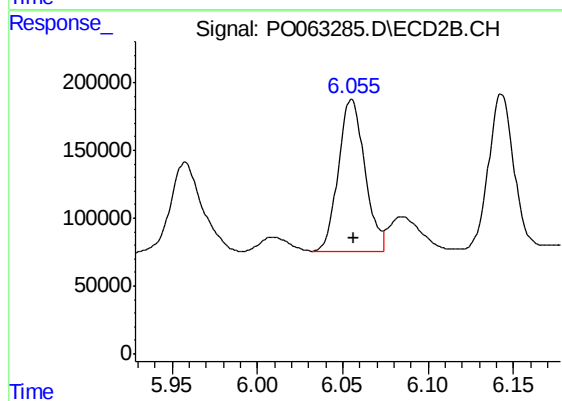

#29 AR-1254-4

R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 1208232
Conc: 423.99 ng/ml

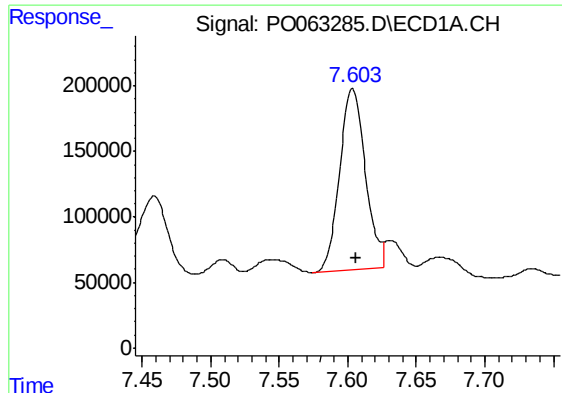


#30 AR-1254-5

R.T.: 7.604 min
Delta R.T.: -0.002 min
Response: 1817088
Conc: 547.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(0-2)DL

Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:16 AM

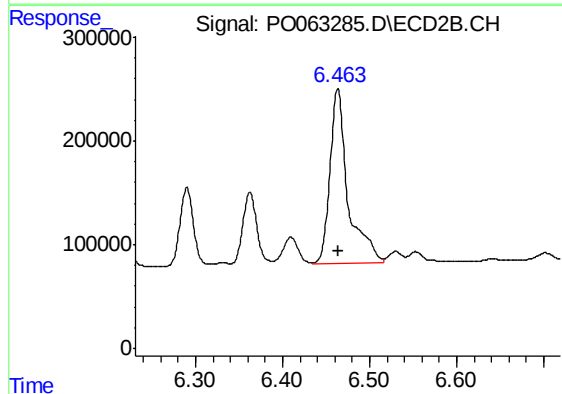

#30 AR-1254-5

R.T.: 6.464 min
Delta R.T.: 0.000 min
Response: 2450951
Conc: 657.51 ng/ml