

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103019\
 Data File : P0063286.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2019 12:01
 Operator : HP/AJ
 Sample : K5584-02DL 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 445X-9A-(2-4)DL

Manual Integrations
 APPROVED

Ankita
 10/31/2019 9:53:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 01:49:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.480	154711	150020	2.655	2.747
2)	SA Decachlor...	9.932	8.320	124706	79518	2.143m	1.860
Target Compounds							
26)	L6 AR-1254-1	6.320	5.295	752983	682140	296.168m	226.452
27)	L6 AR-1254-2	6.537	5.439	1489903	935813	368.330	346.983
28)	L6 AR-1254-3	6.902	5.831	1947500	1966350	457.545	458.014
29)	L6 AR-1254-4	7.187	6.055	1321514	1172648	390.427	411.506
30)	L6 AR-1254-5	7.603	6.463	2450103	2620684	738.648	703.040

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
Data File : PO063286.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 12:01
Operator : HP/AJ
Sample : K5584-02DL 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
445X-9A-(2-4)DL


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:49:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

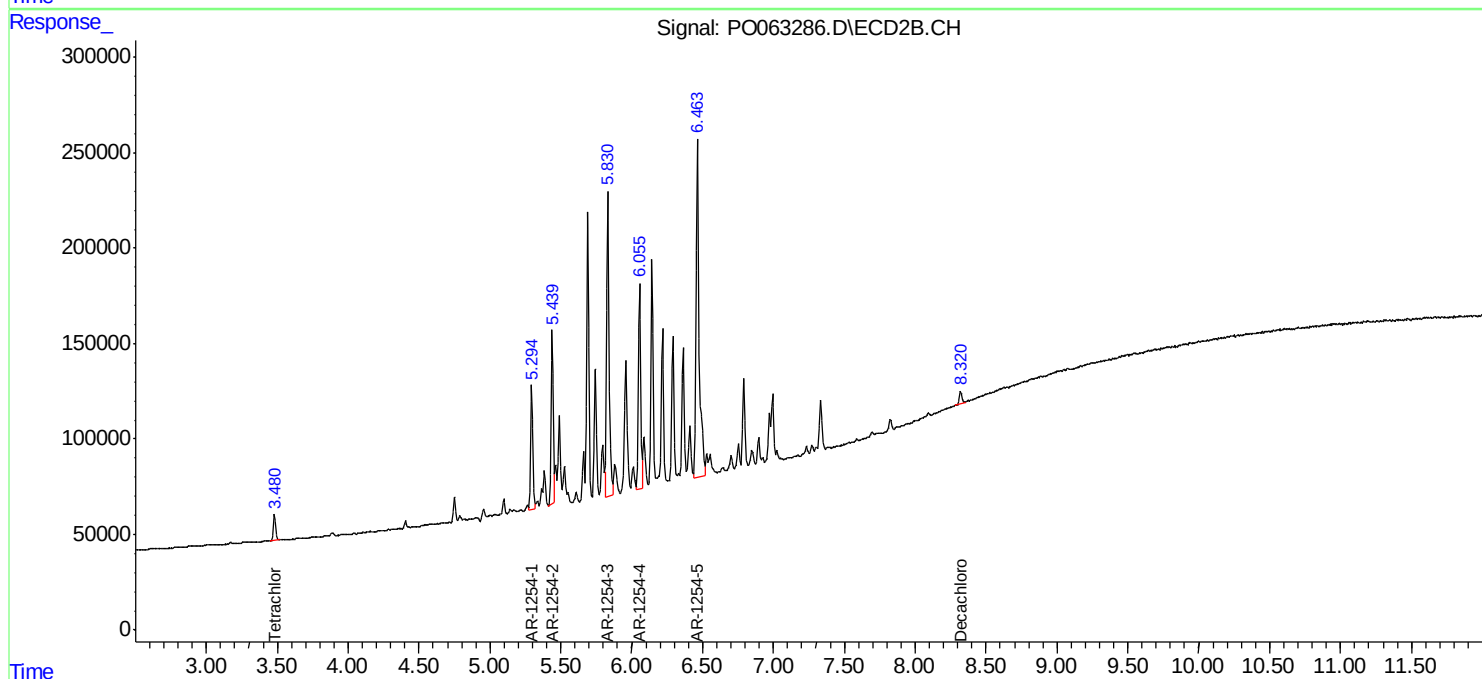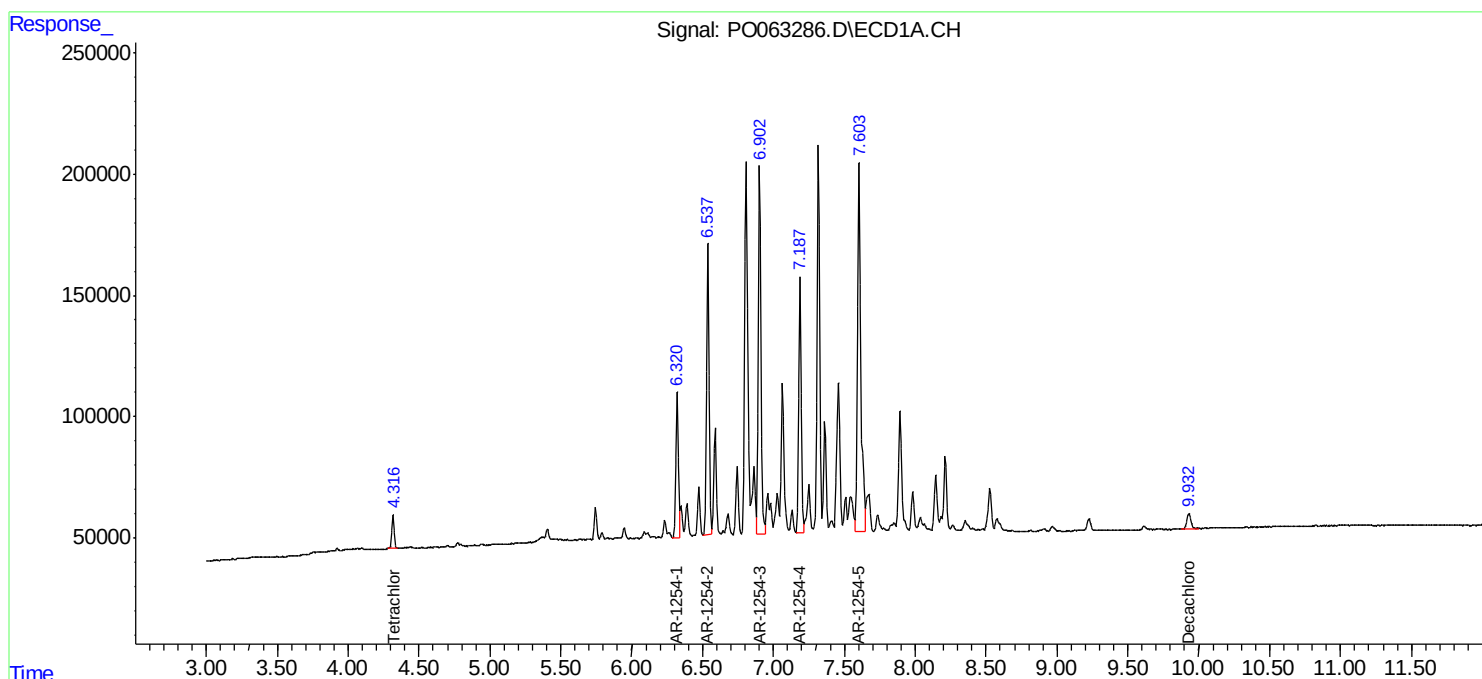

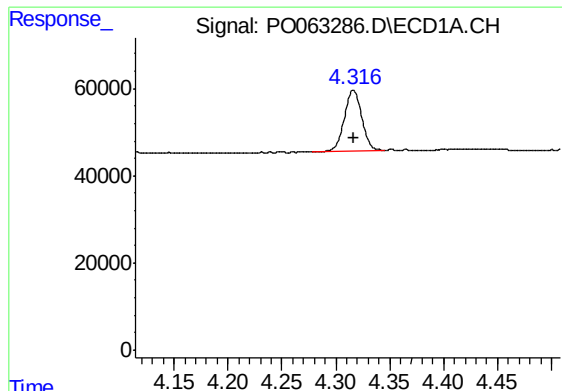


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 154711
Conc: 2.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(2-4)DL


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:18 AM

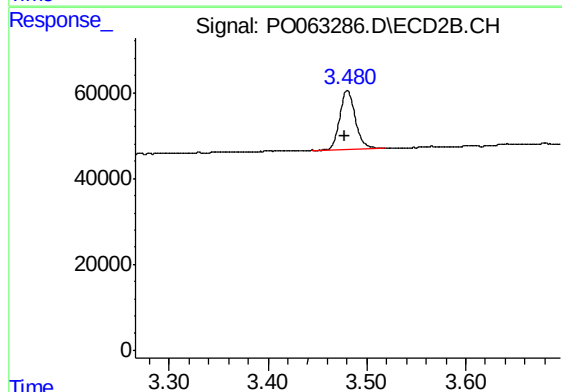


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 150020
Conc: 2.75 ng/ml

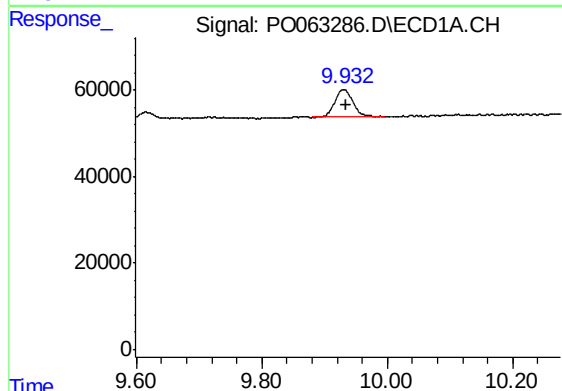


#2 Decachlorobiphenyl

R.T.: 9.932 min
Delta R.T.: -0.002 min
Response: 124706
Conc: 2.14 ng/ml m

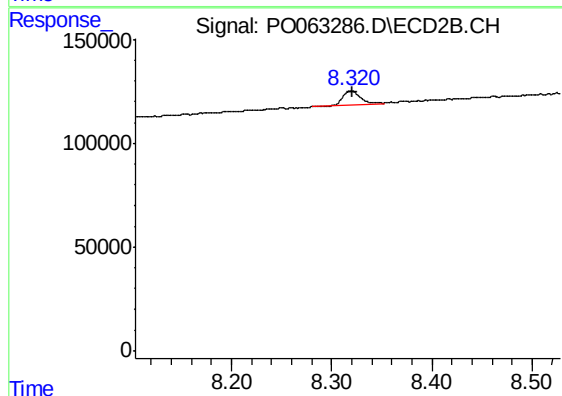

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.001 min
Response: 79518
Conc: 1.86 ng/ml

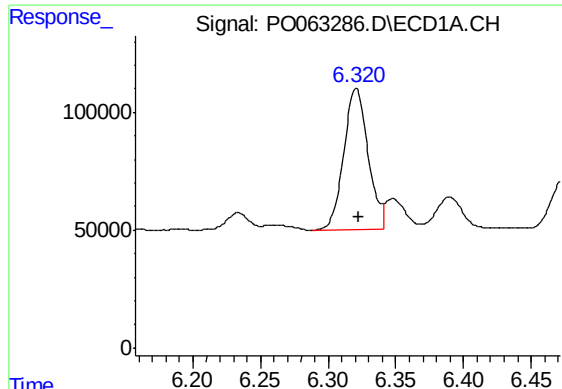


#26 AR-1254-1

R.T.: 6.320 min
Delta R.T.: -0.002 min
Response: 752983
Conc: 296.17 ng/ml m

Instrument :
ECD_O
ClientSampleId :
445X-9A-(2-4)DL


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:18 AM

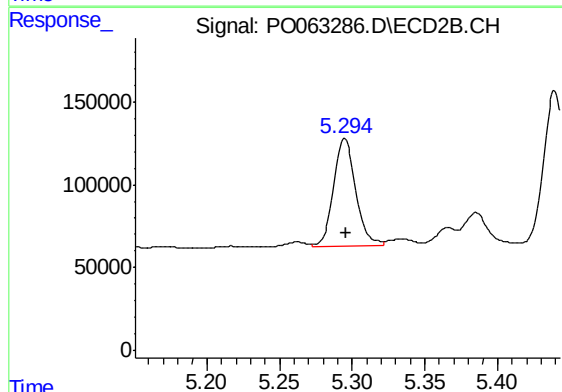


#26 AR-1254-1

R.T.: 5.295 min
Delta R.T.: -0.001 min
Response: 682140
Conc: 226.45 ng/ml

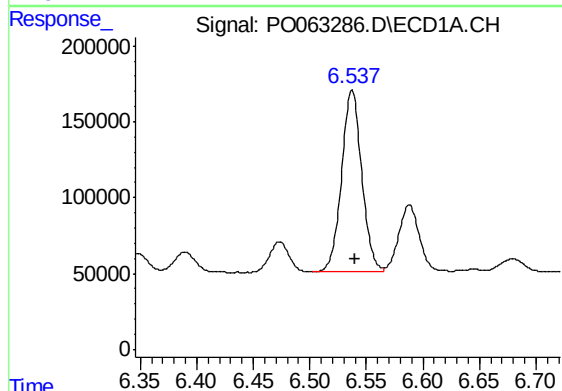


#27 AR-1254-2

R.T.: 6.537 min
Delta R.T.: -0.002 min
Response: 1489903
Conc: 368.33 ng/ml

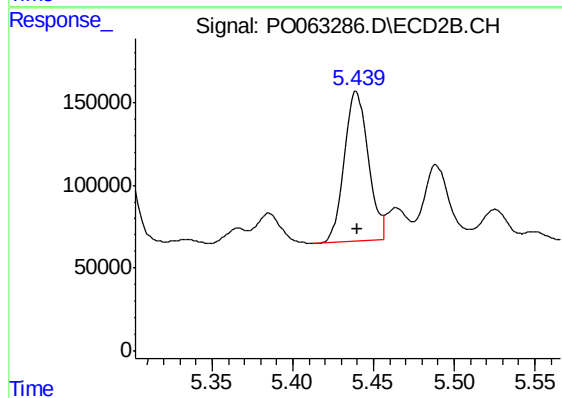

#27 AR-1254-2

R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 935813
Conc: 346.98 ng/ml

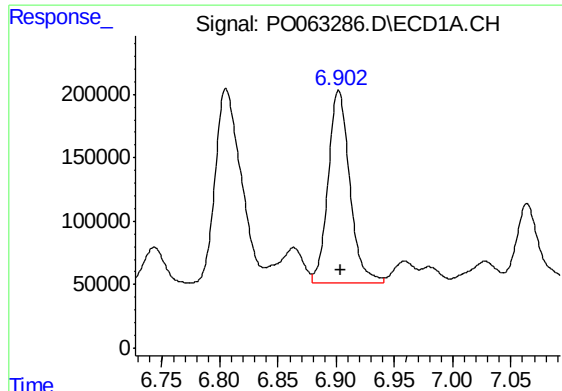


#28 AR-1254-3

R.T.: 6.902 min
Delta R.T.: -0.002 min
Response: 1947500
Conc: 457.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(2-4)DL


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:18 AM

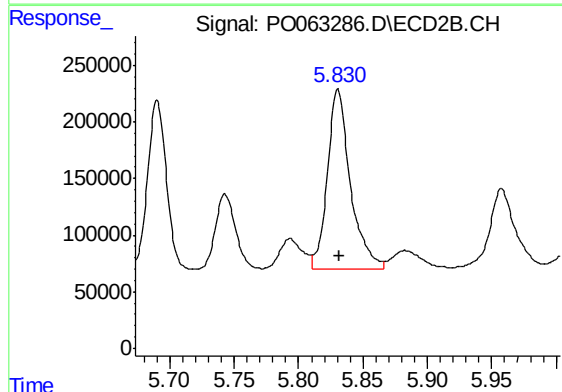


#28 AR-1254-3

R.T.: 5.831 min
Delta R.T.: -0.002 min
Response: 1966350
Conc: 458.01 ng/ml

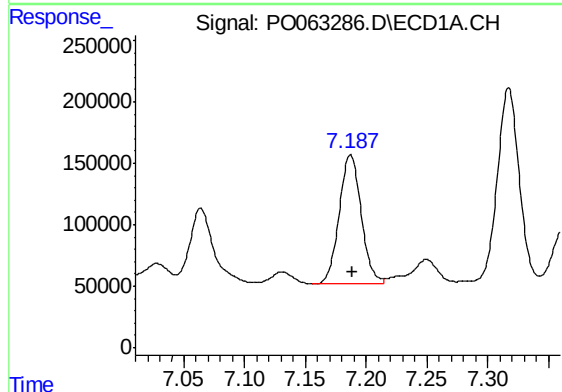


#29 AR-1254-4

R.T.: 7.187 min
Delta R.T.: -0.002 min
Response: 1321514
Conc: 390.43 ng/ml

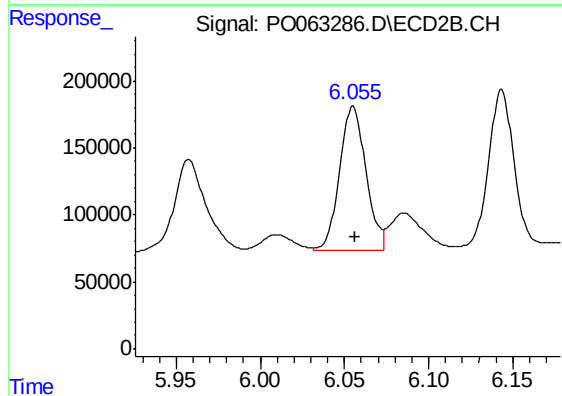

#29 AR-1254-4

R.T.: 6.055 min
Delta R.T.: -0.001 min
Response: 1172648
Conc: 411.51 ng/ml

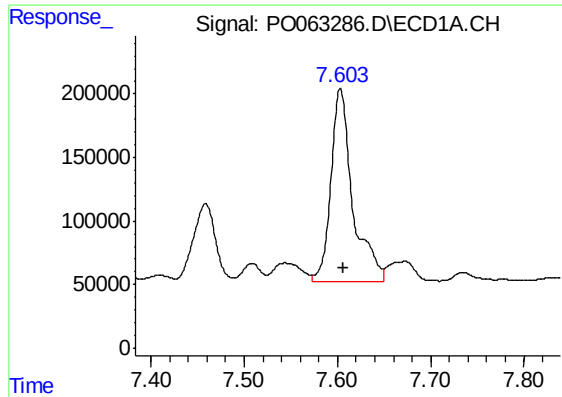


#30 AR-1254-5

R.T.: 7.603 min
Delta R.T.: -0.003 min
Response: 2450103
Conc: 738.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
445X-9A-(2-4)DL

Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:18 AM

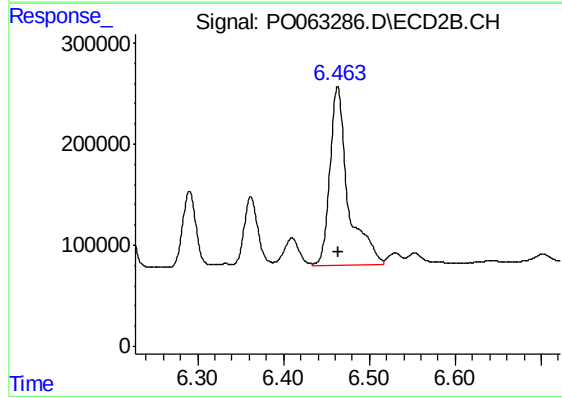

#30 AR-1254-5

R.T.: 6.463 min
Delta R.T.: -0.001 min
Response: 2620684
Conc: 703.04 ng/ml