

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103019\
 Data File : P0063290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2019 13:06
 Operator : HP/AJ
 Sample : K5563-10RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2RE

Manual Integrations
 APPROVED

Ankita
 11/6/2019 8:21:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 17:01:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.316	3.480	923125	909251	15.839m	16.649
2) SA Decachlor...	9.931	8.319	660392	429368	11.350m	10.043

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
Data File : PO063290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 13:06
Operator : HP/AJ
Sample : K5563-10RE
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-2RE


Manual Integrations
APPROVED

Ankita
11/6/2019 8:21:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 17:01:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

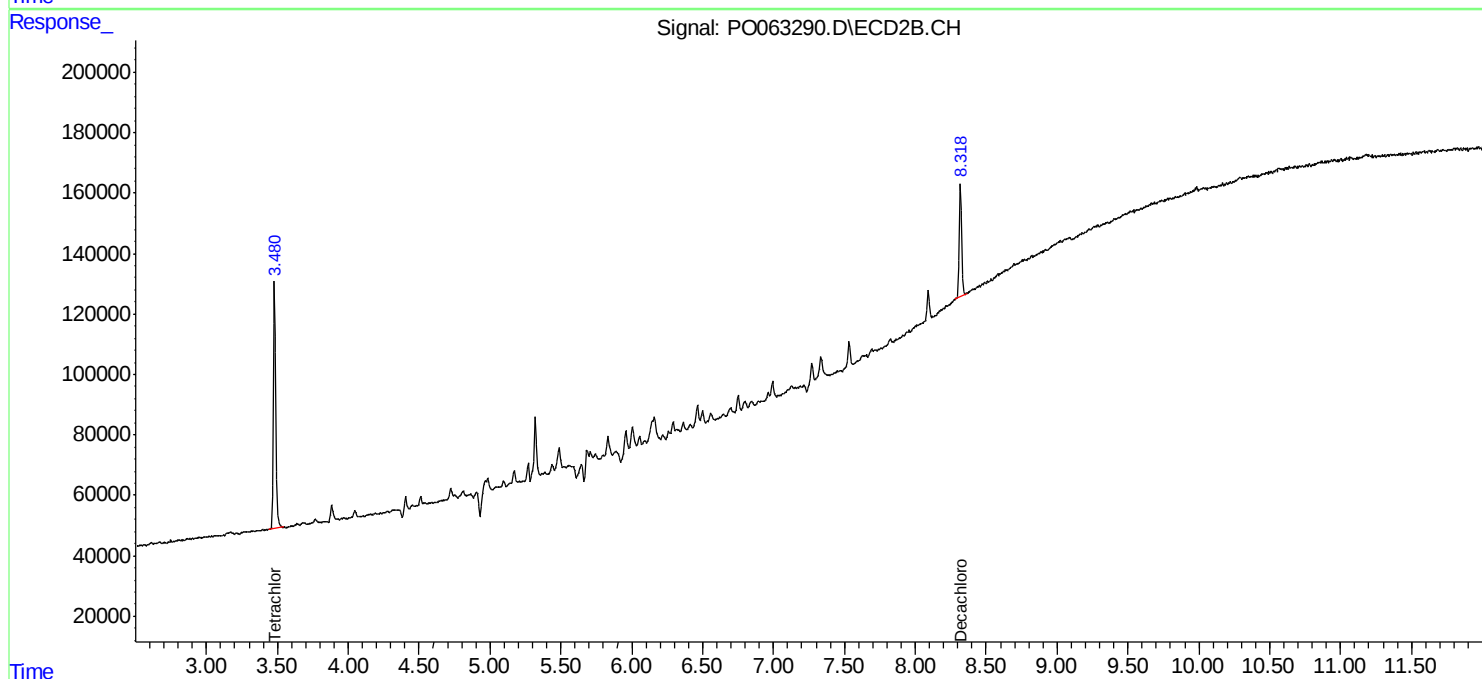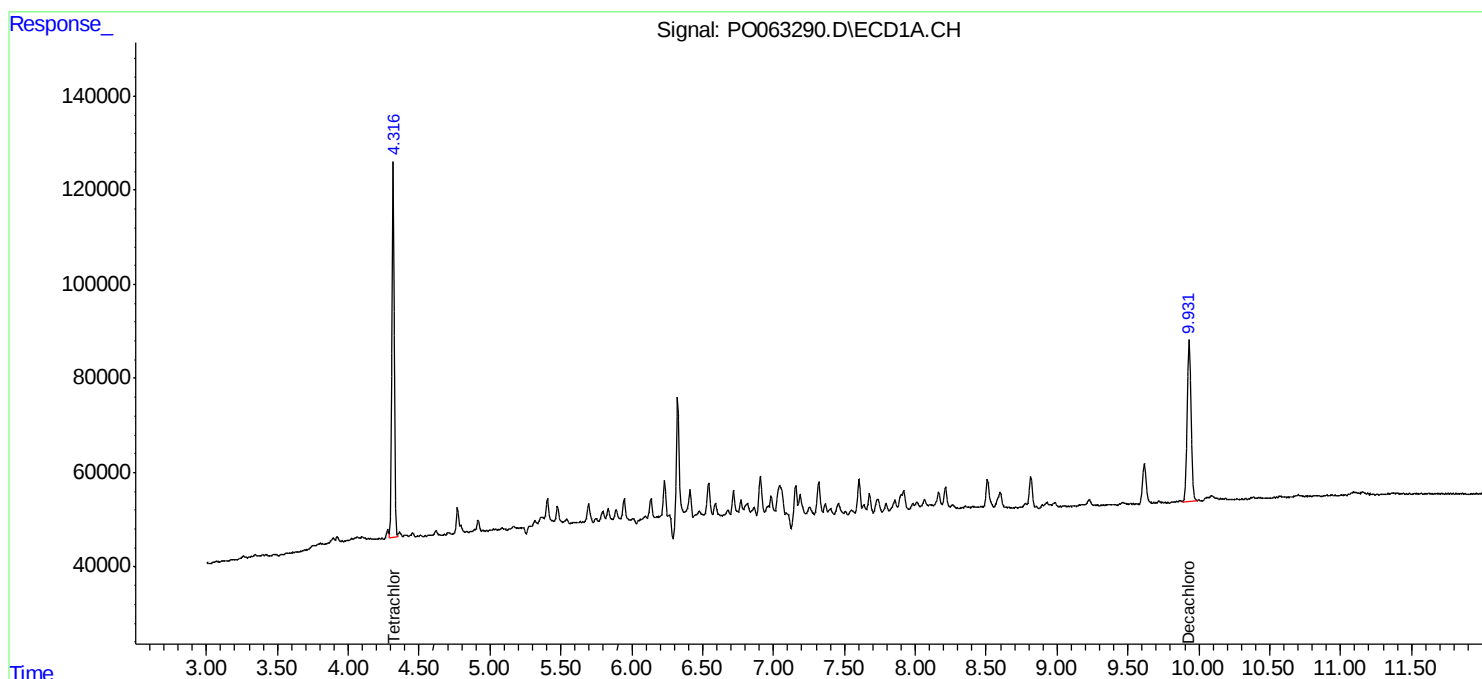

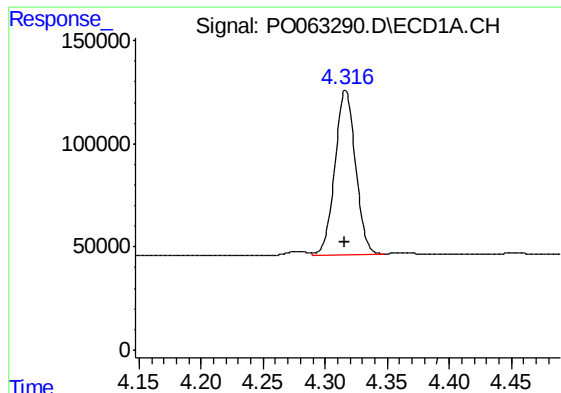


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 923125
Conc: 15.84 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2RE


Manual Integrations
APPROVED

Ankita
11/6/2019 8:21:37 AM

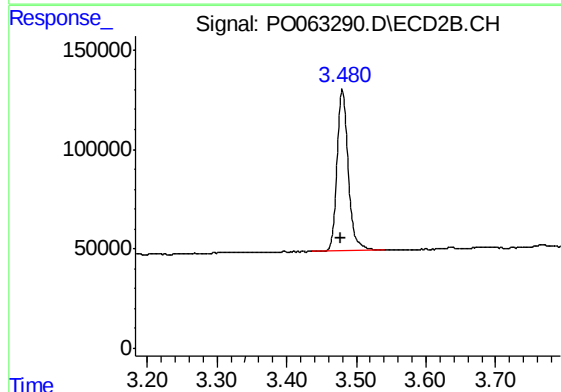


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 909251
Conc: 16.65 ng/ml

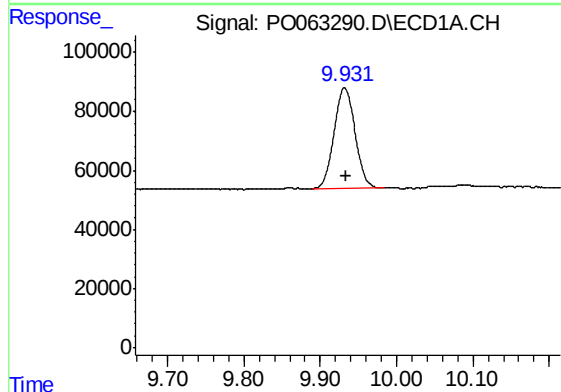

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.002 min
Response: 660392
Conc: 11.35 ng/ml m

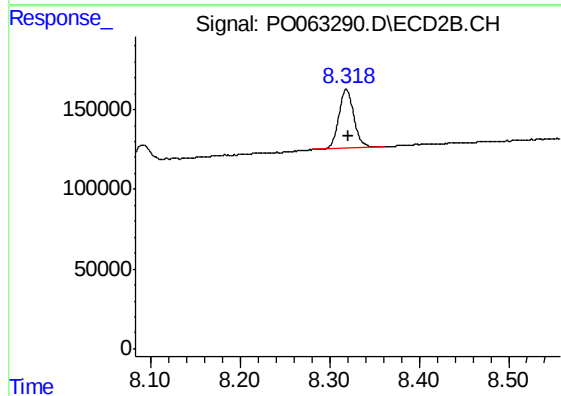

#2 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: -0.002 min
Response: 429368
Conc: 10.04 ng/ml