

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103019\
 Data File : P0063292.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2019 13:39
 Operator : HP/AJ
 Sample : K5573-03RE 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-A-03-B-03-CRE

Manual Integrations
 APPROVED

Ankita
 10/31/2019 9:53:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 01:51:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.480	364054	349004	6.246	6.390
2)	SA Decachlor...	9.931	8.320	352197	248771	6.053	5.819
Target Compounds							
26)	L6 AR-1254-1	6.321	5.294	637289	660632	250.663	219.312
27)	L6 AR-1254-2	6.538	5.439	827182	549197	204.494	203.632
28)	L6 AR-1254-3	6.903	5.830	584249	644357	137.263	150.088
29)	L6 AR-1254-4	7.187	6.055	311852	268871	92.133	94.353
30)	L6 AR-1254-5	7.602	6.463	228741	313157	68.960m	84.009

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
Data File : PO063292.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 13:39
Operator : HP/AJ
Sample : K5573-03RE 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 01:51:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

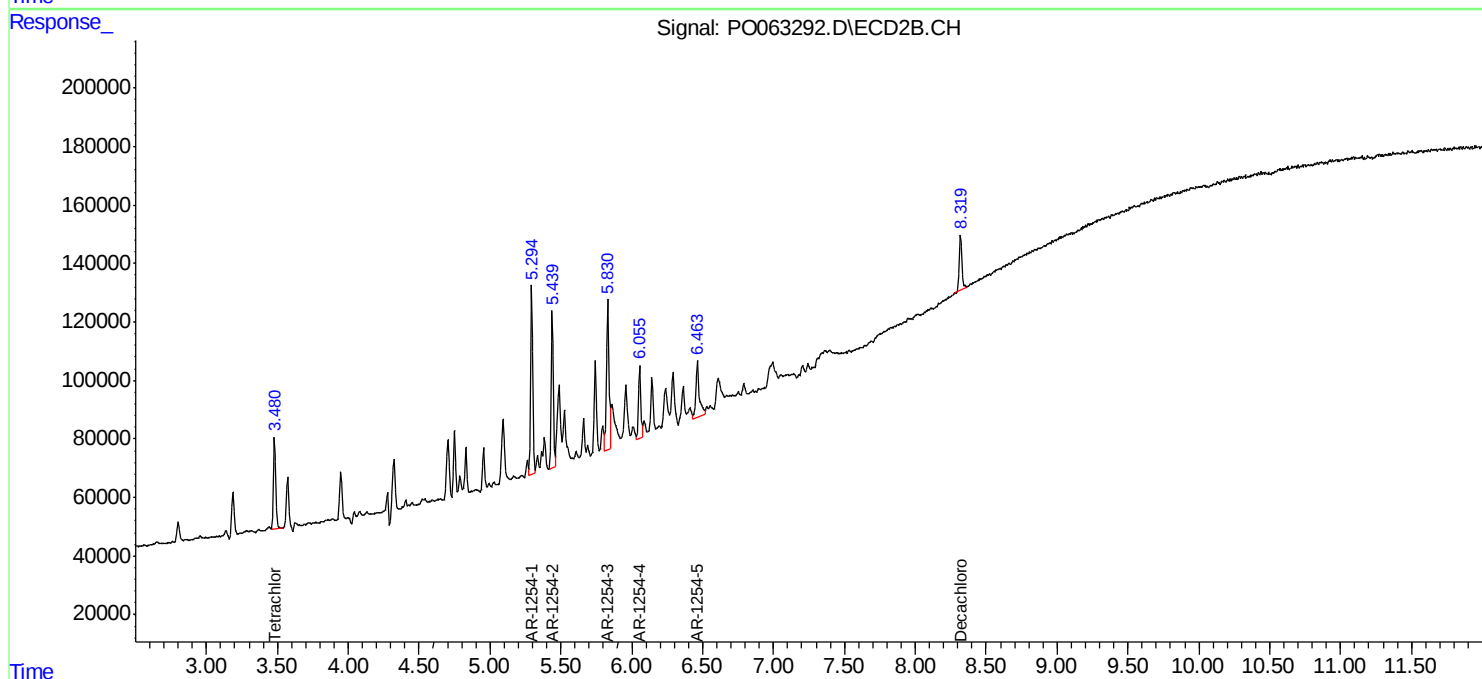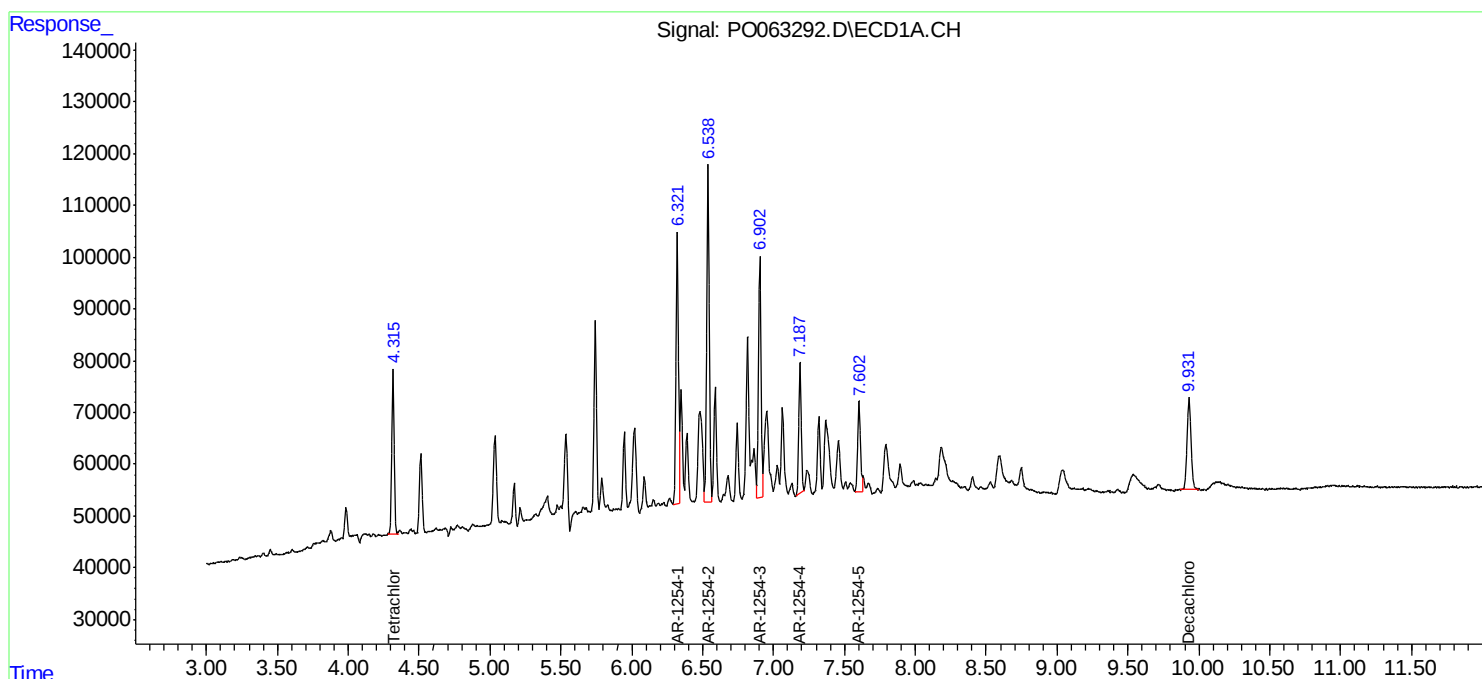

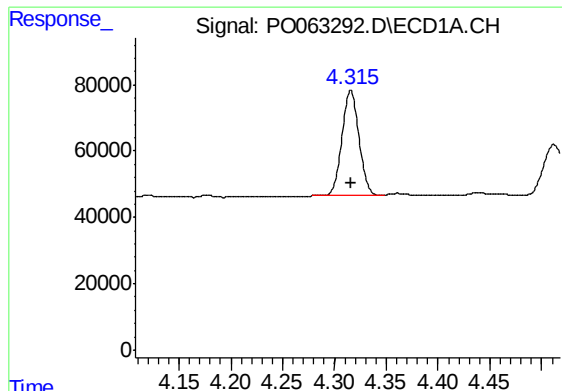


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 364054
Conc: 6.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:48 AM

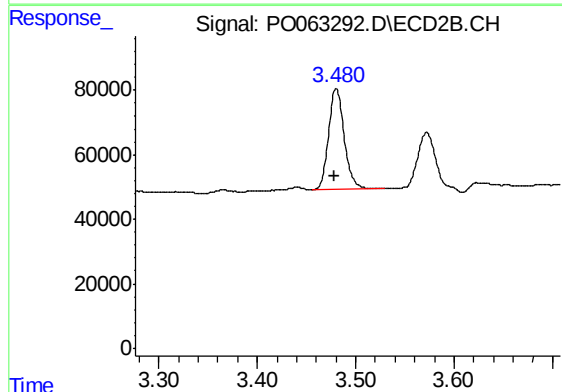


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 349004
Conc: 6.39 ng/ml

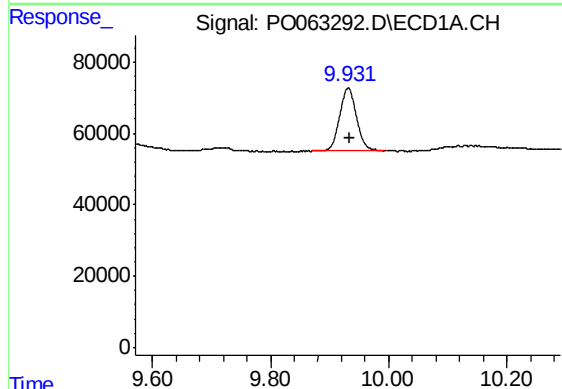


#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.002 min
Response: 352197
Conc: 6.05 ng/ml

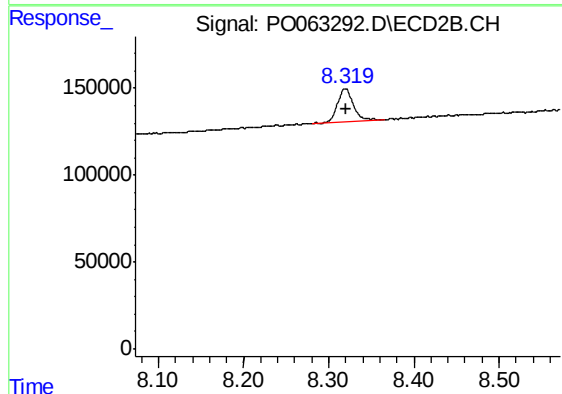

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.001 min
Response: 248771
Conc: 5.82 ng/ml

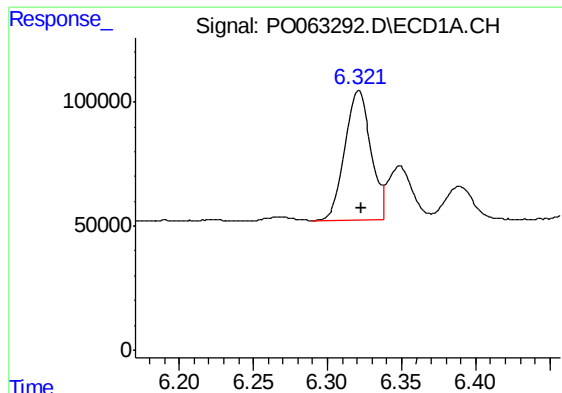


#26 AR-1254-1

R.T.: 6.321 min
Delta R.T.: -0.002 min
Response: 637289
Conc: 250.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:48 AM

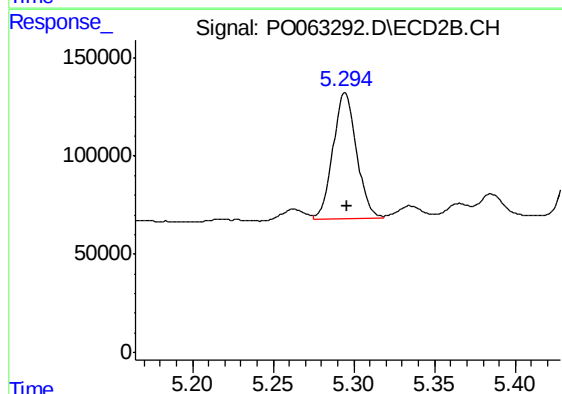


#26 AR-1254-1

R.T.: 5.294 min
Delta R.T.: -0.002 min
Response: 660632
Conc: 219.31 ng/ml

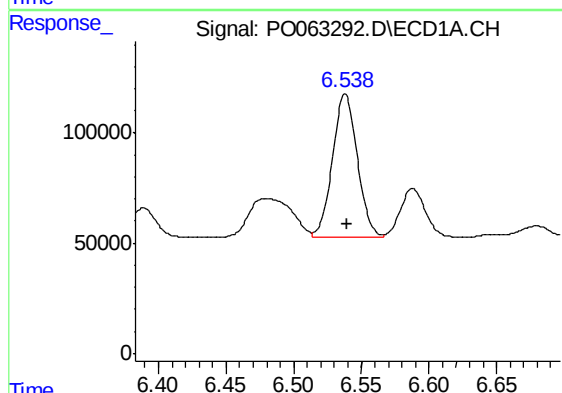


#27 AR-1254-2

R.T.: 6.538 min
Delta R.T.: -0.001 min
Response: 827182
Conc: 204.49 ng/ml

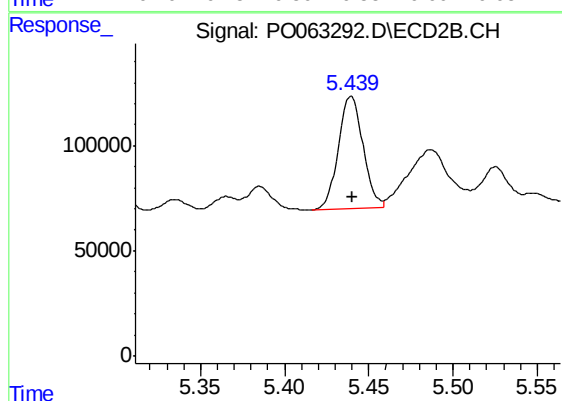

#27 AR-1254-2

R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 549197
Conc: 203.63 ng/ml

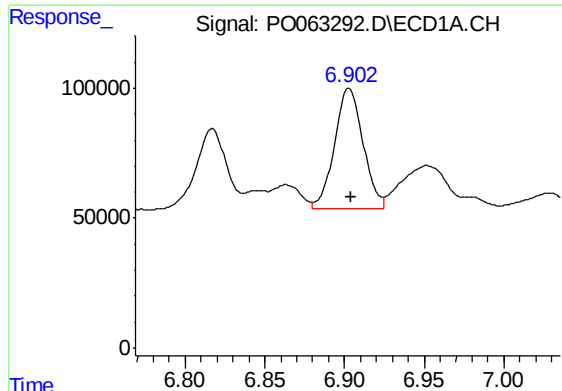


#28 AR-1254-3

R.T.: 6.903 min
Delta R.T.: -0.001 min
Response: 584249
Conc: 137.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:48 AM

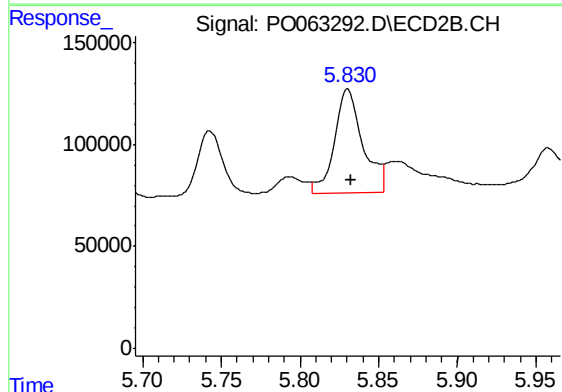


#28 AR-1254-3

R.T.: 5.830 min
Delta R.T.: -0.002 min
Response: 644357
Conc: 150.09 ng/ml

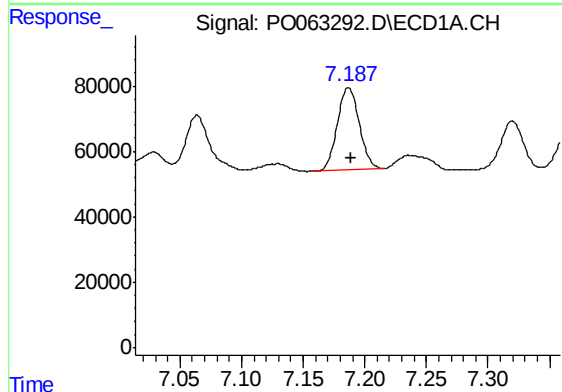


#29 AR-1254-4

R.T.: 7.187 min
Delta R.T.: -0.002 min
Response: 311852
Conc: 92.13 ng/ml

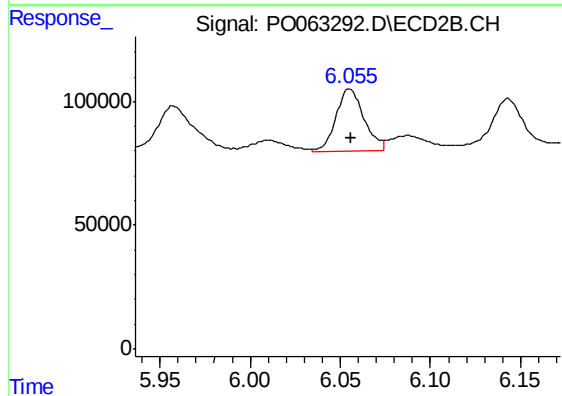

#29 AR-1254-4

R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 268871
Conc: 94.35 ng/ml

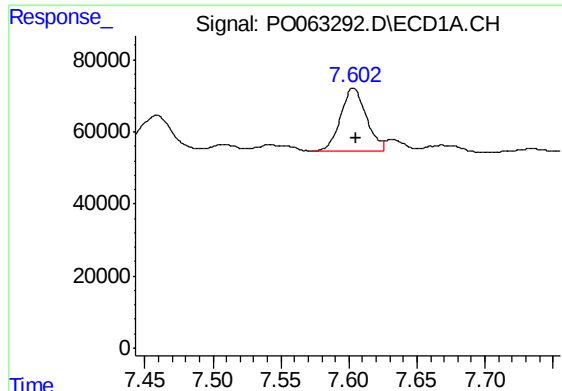


#30 AR-1254-5

R.T.: 7.602 min
Delta R.T.: -0.003 min
Response: 228741
Conc: 68.96 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE

Manual Integrations
APPROVED

Ankita
10/31/2019 9:53:48 AM

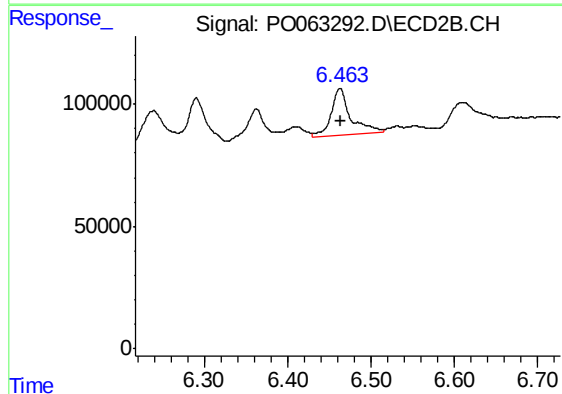

#30 AR-1254-5

R.T.: 6.463 min
Delta R.T.: -0.002 min
Response: 313157
Conc: 84.01 ng/ml