

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
 Data File : P0063321.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2019 21:42
 Operator : HP/AJ
 Sample : K5603-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20190949-AMENDED-COMPOSITE-

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 02:00:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.479	1004288	969483	17.232	17.752
2)	SA Decachlor...	9.931	8.320	638861	441815	10.980	10.334

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103019\
Data File : PO063321.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2019 21:42
Operator : HP/AJ
Sample : K5603-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20190949-AMENDED-COMPOSITE-

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 02:00:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

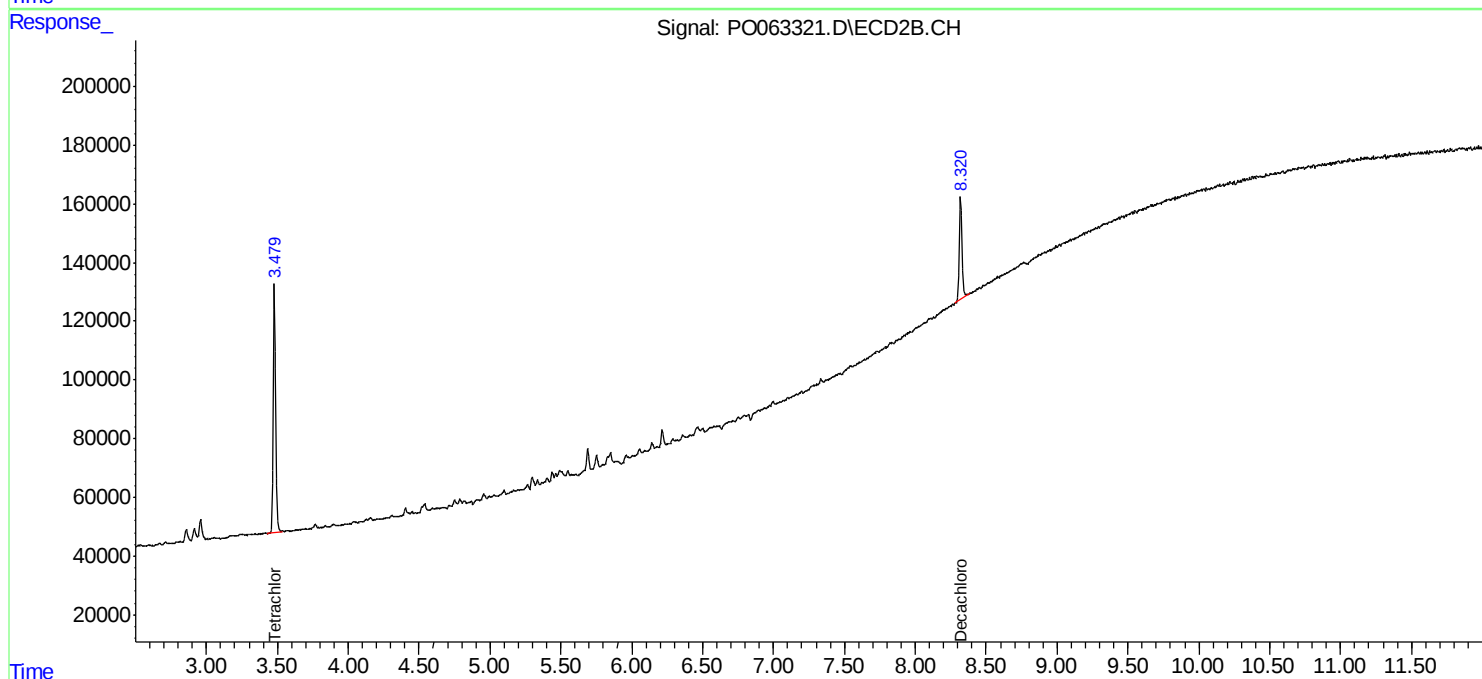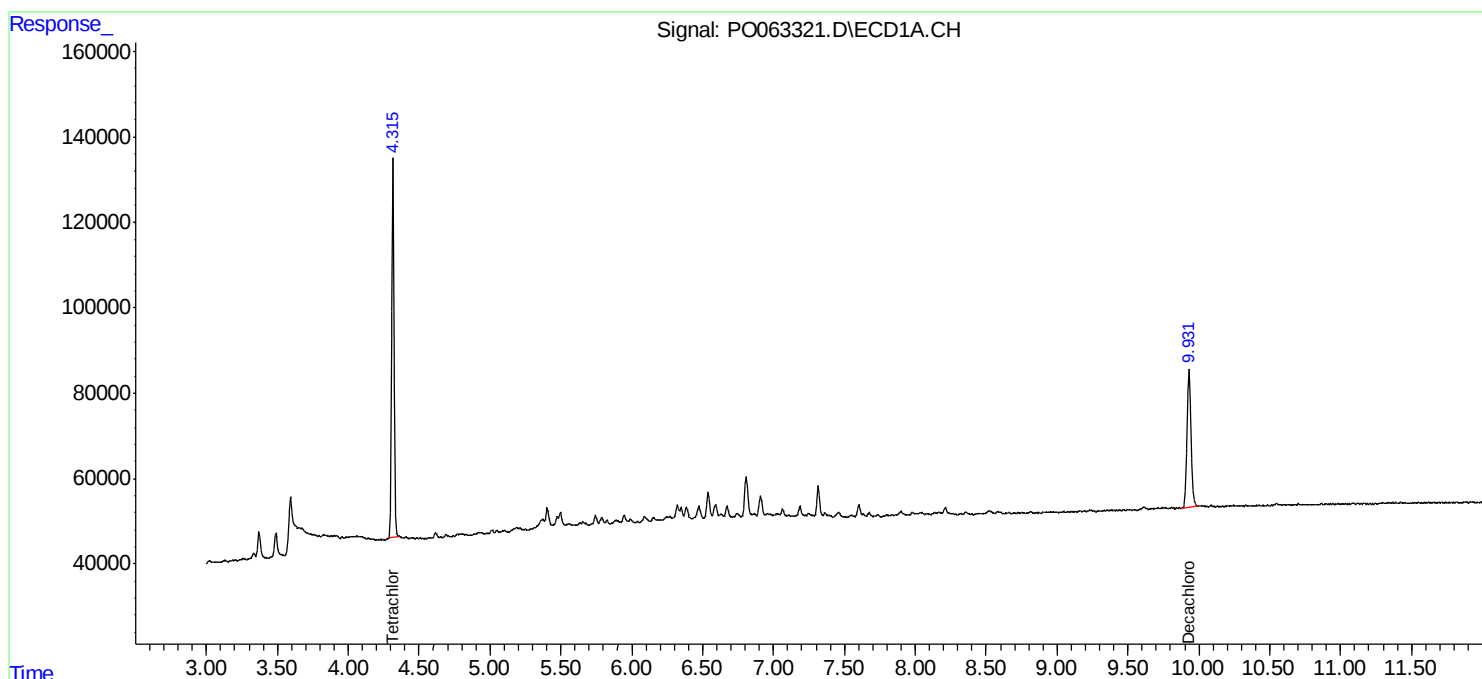


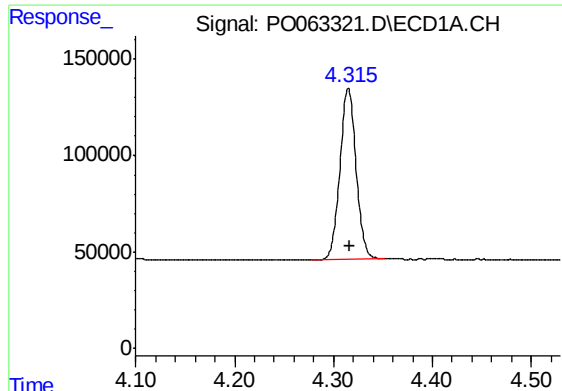

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: -0.001 min
Response: 1004288
Conc: 17.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
20190949-AMENDED-COMPOSITE-

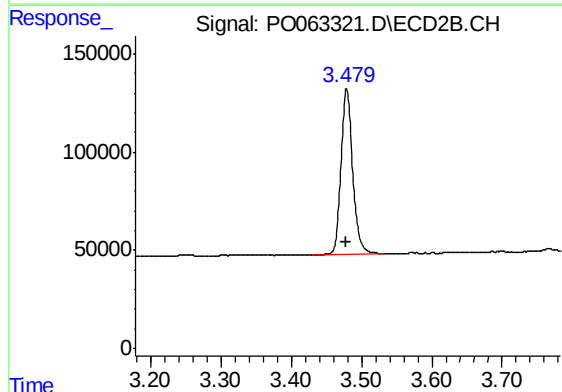


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.001 min
Response: 969483
Conc: 17.75 ng/ml

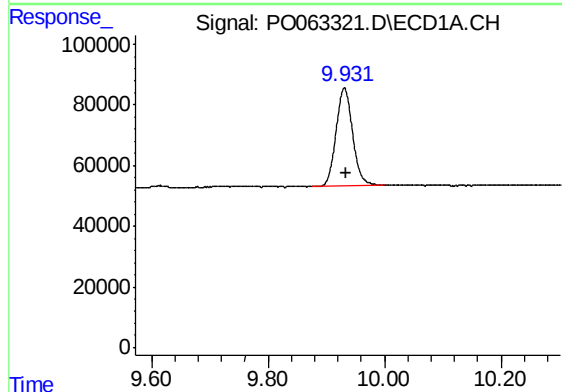

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.003 min
Response: 638861
Conc: 10.98 ng/ml

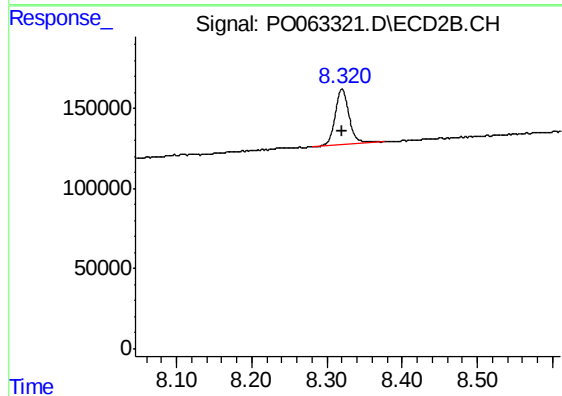

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.001 min
Response: 441815
Conc: 10.33 ng/ml