

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103025\
 Data File : PO114789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 00:52
 Operator : YP/AJ
 Sample : Q3487-07 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M3-A

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 10/31/2025
 Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 03:00:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.653	8817121	5528891	1.624m	1.381
2) SA Decachlor...	9.934	8.649	7299321	8272034	2.005m	2.482

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103025\
Data File : PO114789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 00:52
Operator : YP/AJ
Sample : Q3487-07 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
M3-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 03:00:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

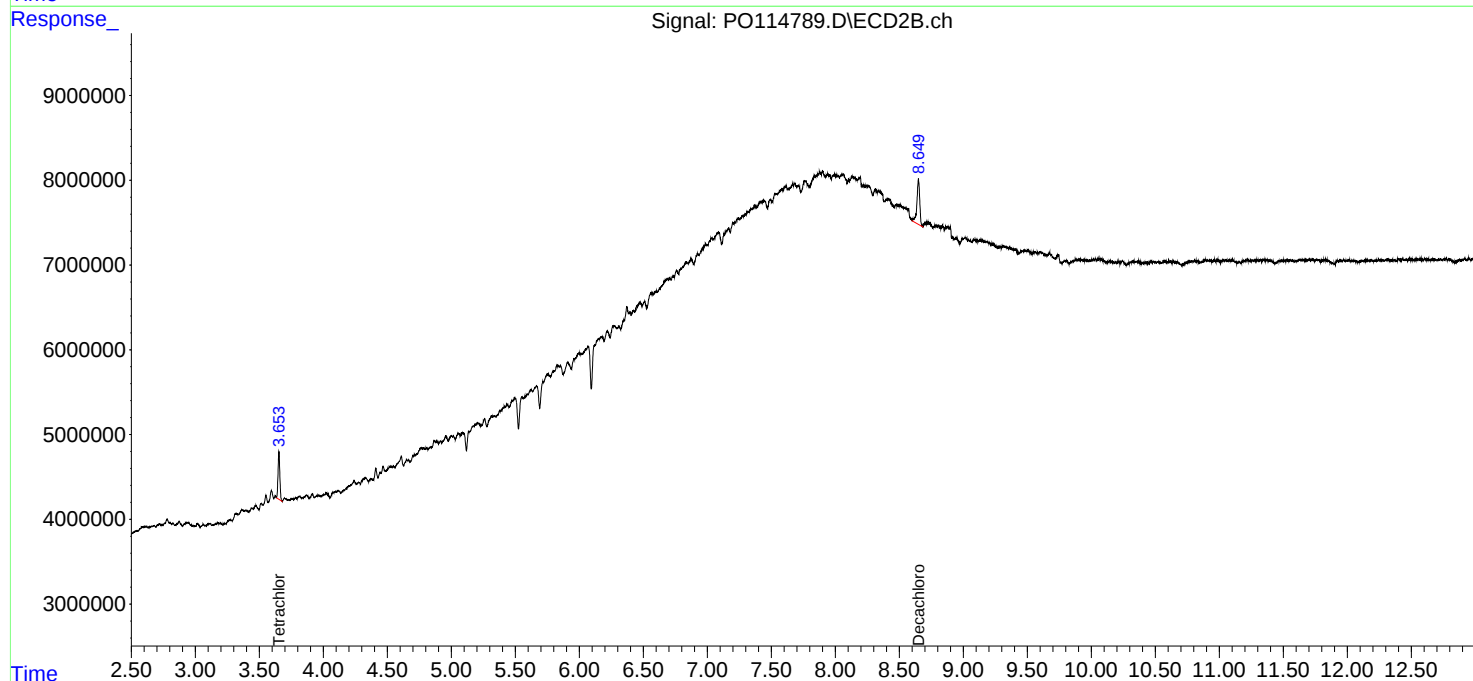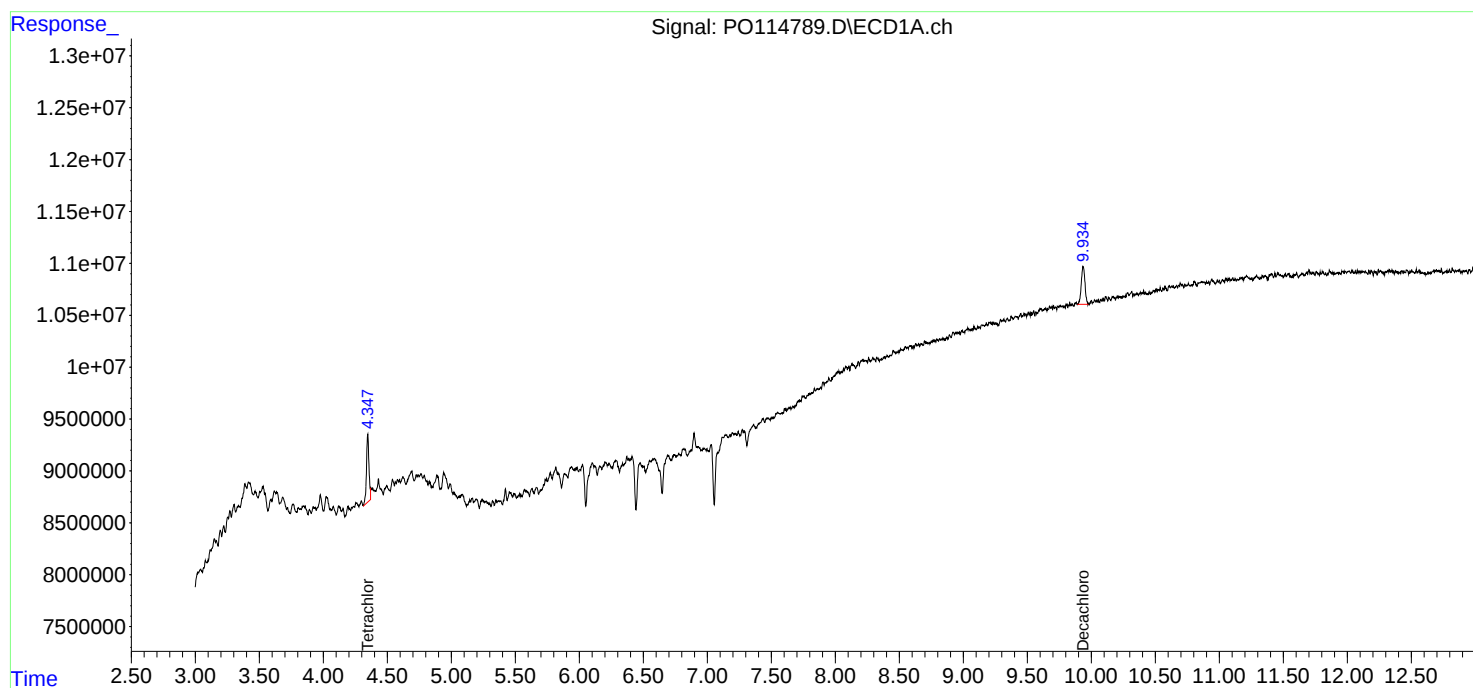

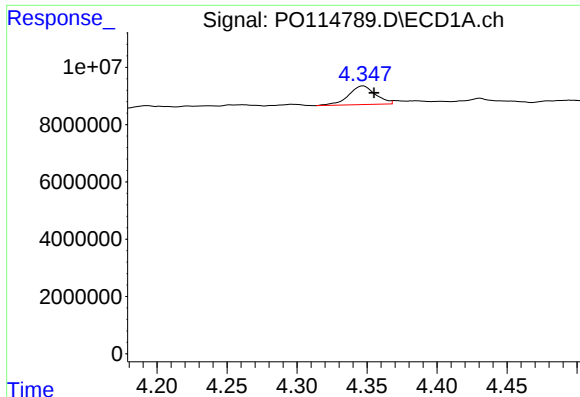


#1 Tetrachloro-m-xylene

R.T.: 4.347 min
Delta R.T.: -0.008 min
Response: 8817121
Conc: 1.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
M3-A


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 10/31/2025
Supervised By :Yogesh Patel 10/31/2025

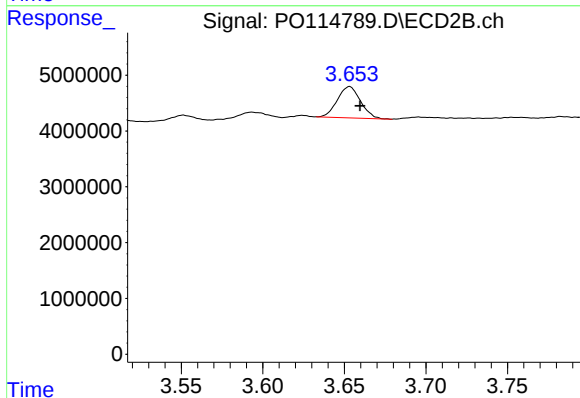


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.006 min
Response: 5528891
Conc: 1.38 ng/ml

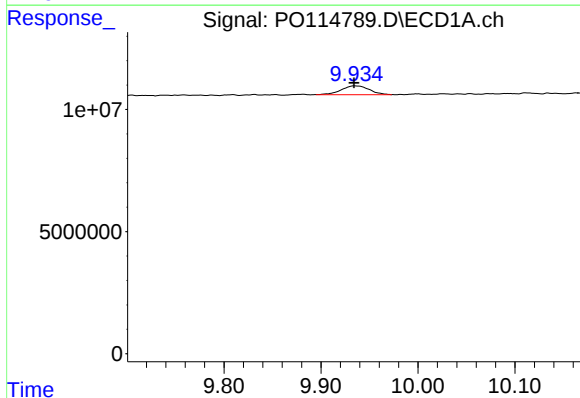

#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: 0.000 min
Response: 7299321
Conc: 2.00 ng/ml m

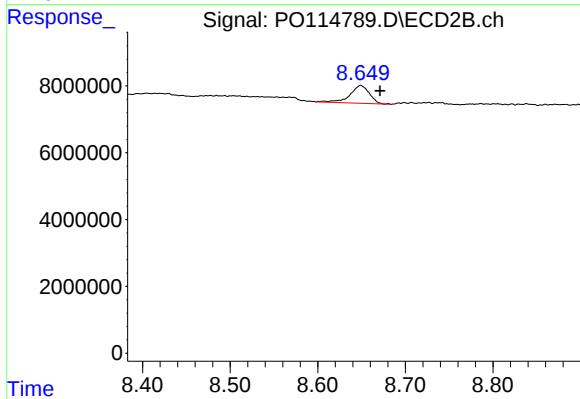

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.022 min
Response: 8272034
Conc: 2.48 ng/ml