

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103118\
Data File : P0050821.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Oct 2018 17:07
Operator : SM/SJ
Sample : J5719-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:44:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.354	3.348	2997856	1039975	5.997	4.785
2)	SA Decachlor...	10.012	8.093	2530302	2024385	8.141	7.914

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103118\
Data File : PO050821.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Oct 2018 17:07
Operator : SM/SJ
Sample : J5719-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:44:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

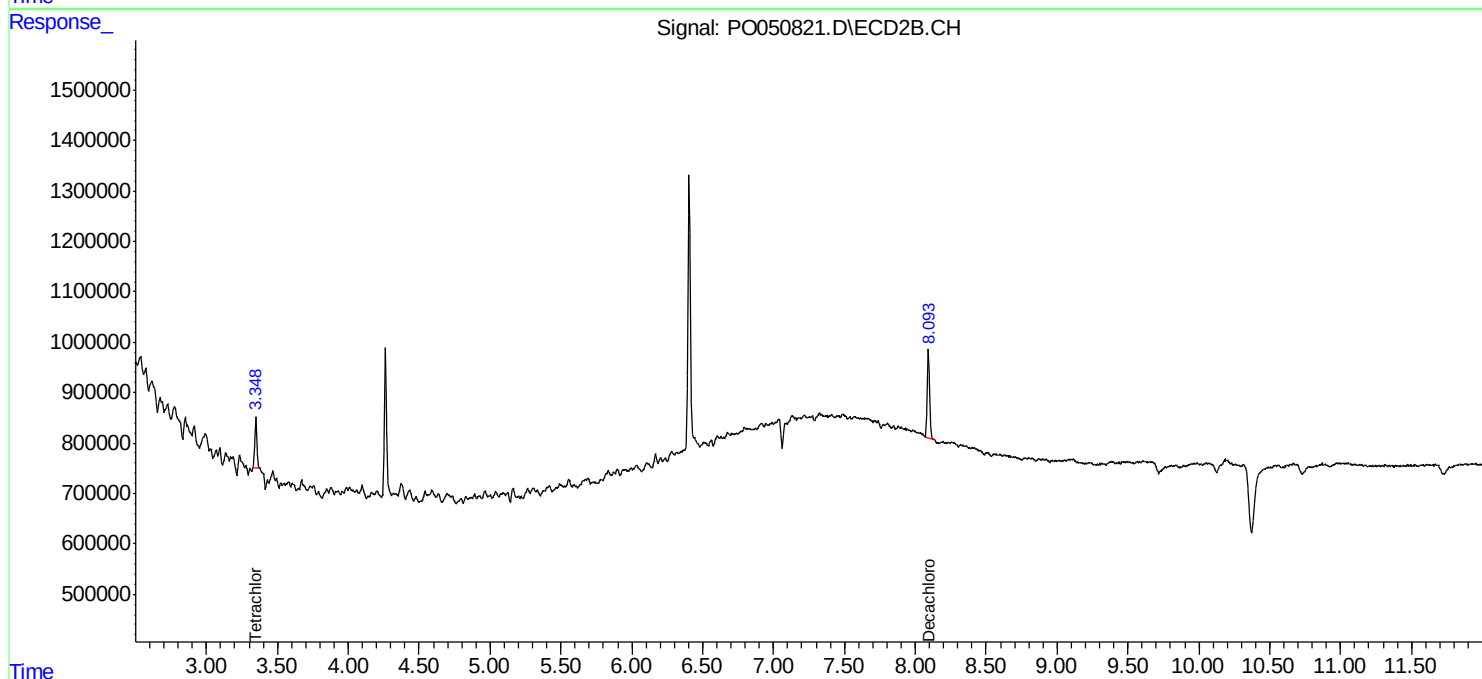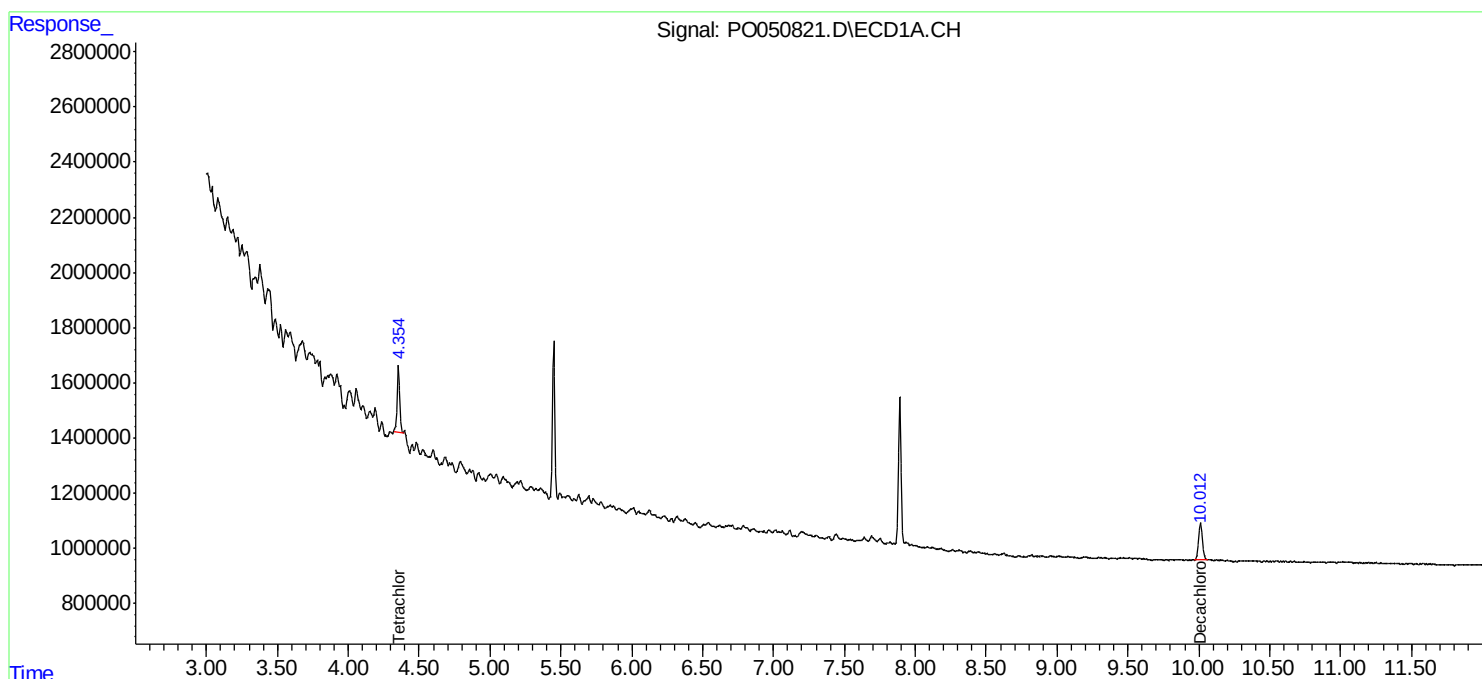


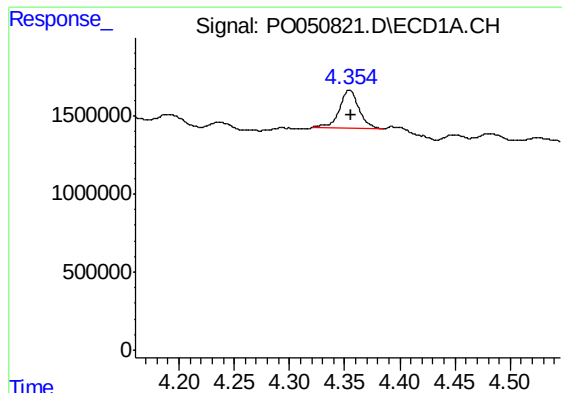

#1 Tetrachloro-m-xylene


R.T.: 4.354 min
Delta R.T.: -0.002 min
Response: 2997856
Conc: 6.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1

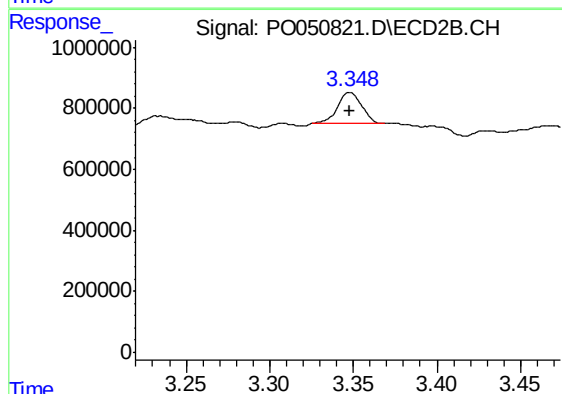


#1 Tetrachloro-m-xylene

R.T.: 3.348 min
Delta R.T.: 0.000 min
Response: 1039975
Conc: 4.78 ng/ml

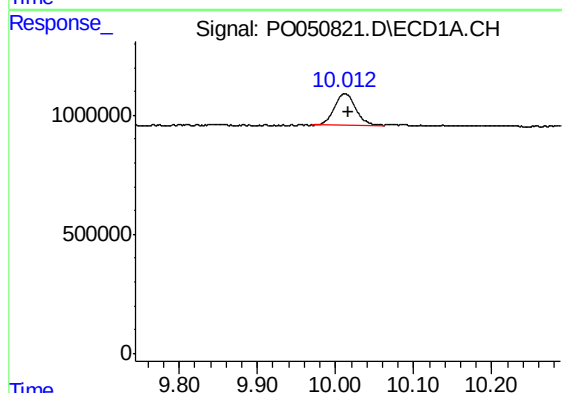

#2 Decachlorobiphenyl

R.T.: 10.012 min
Delta R.T.: -0.006 min
Response: 2530302
Conc: 8.14 ng/ml

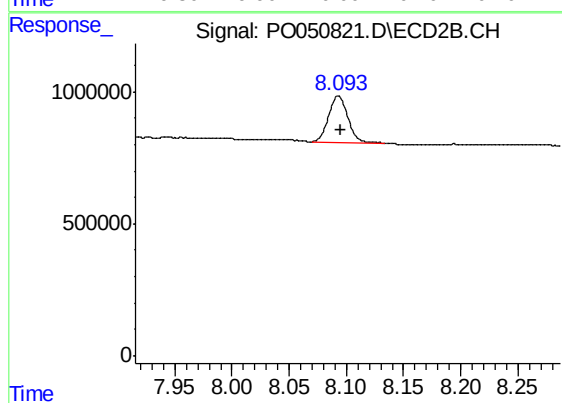

#2 Decachlorobiphenyl

R.T.: 8.093 min
Delta R.T.: -0.003 min
Response: 2024385
Conc: 7.91 ng/ml