

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103118\
Data File : P0050854.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 2:27
Operator : SM/SJ
Sample : J5737-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 03:23:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.353	3.347	10311704	4679653	20.629	21.530
2)	SA Decachlor...	10.013	8.093	4453938	3394820	14.329	13.272

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103118\
Data File : PO050854.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 2:27
Operator : SM/SJ
Sample : J5737-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 03:23:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

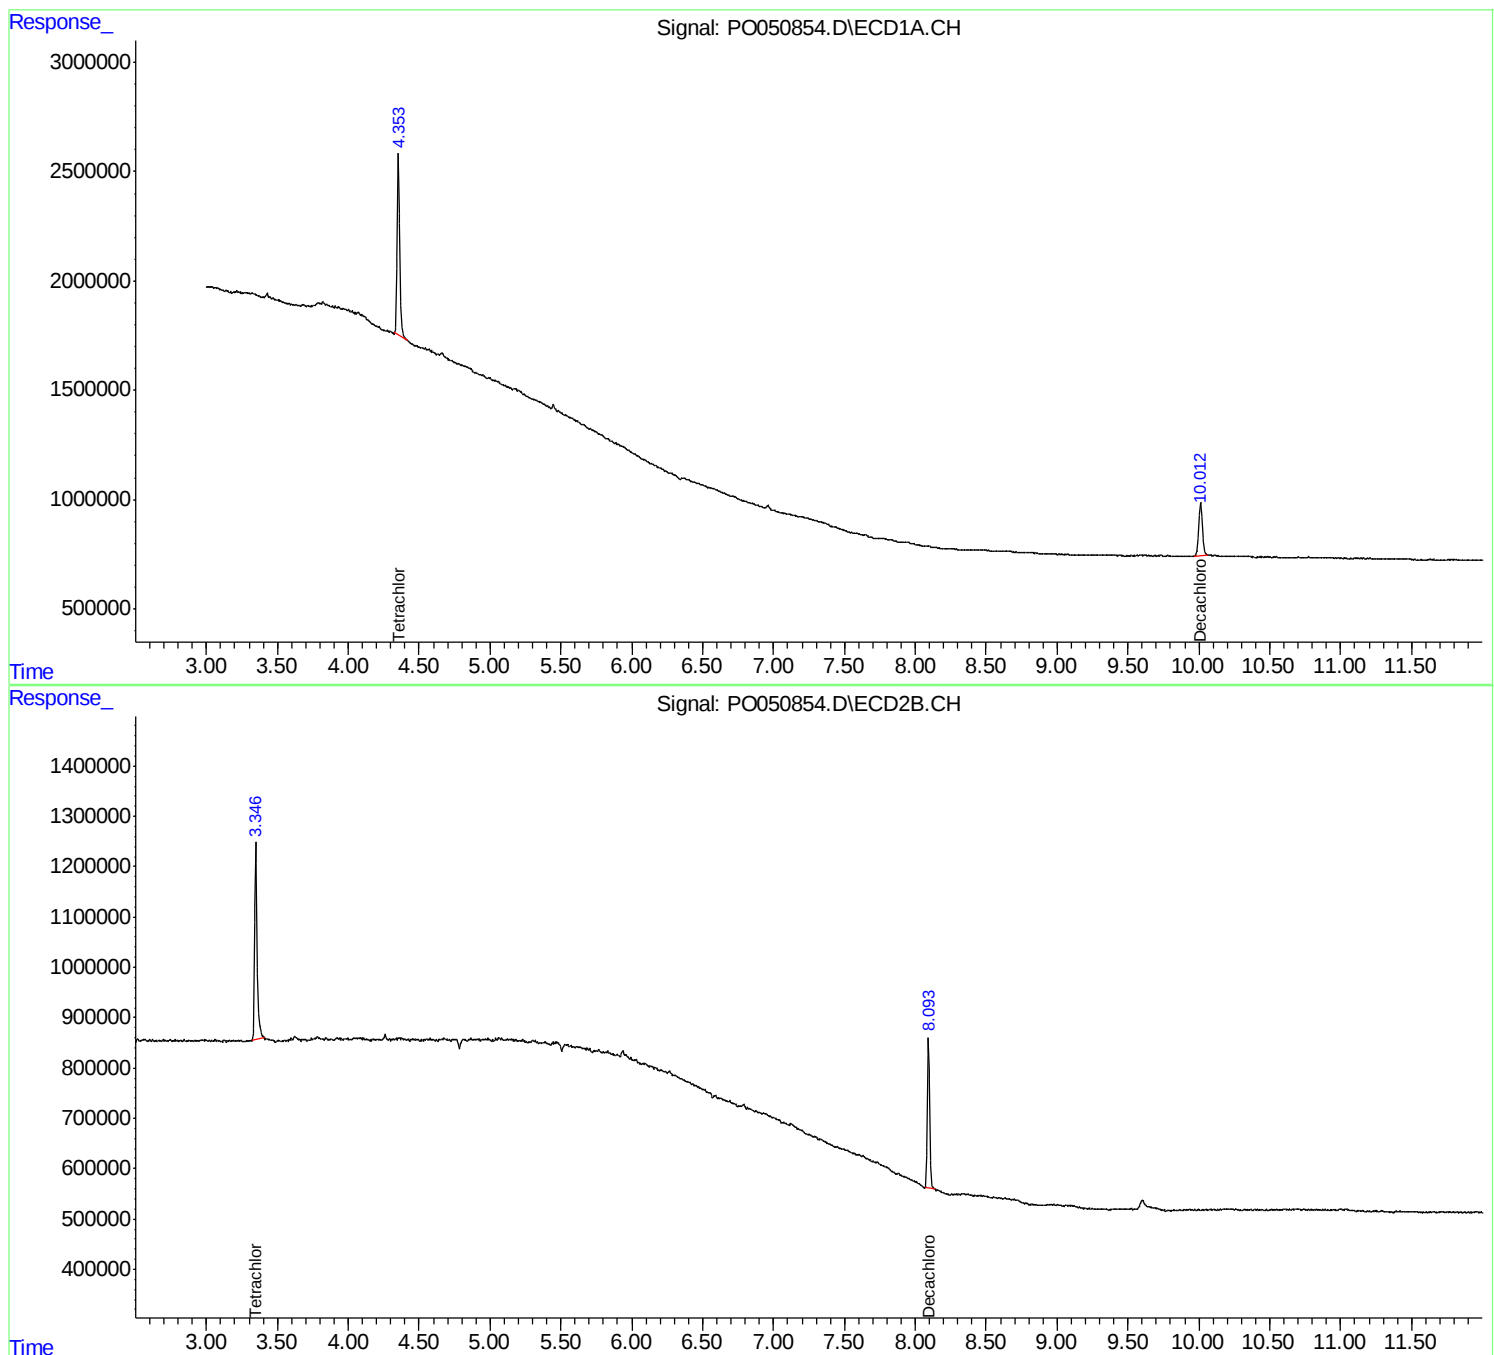


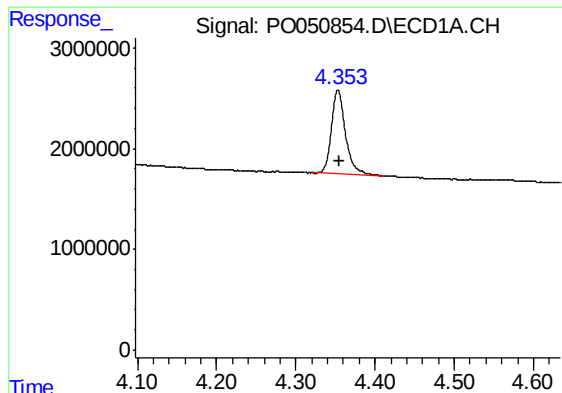

#1 Tetrachloro-m-xylene


R.T.: 4.353 min
Delta R.T.: -0.003 min
Response: 10311704
Conc: 20.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-A

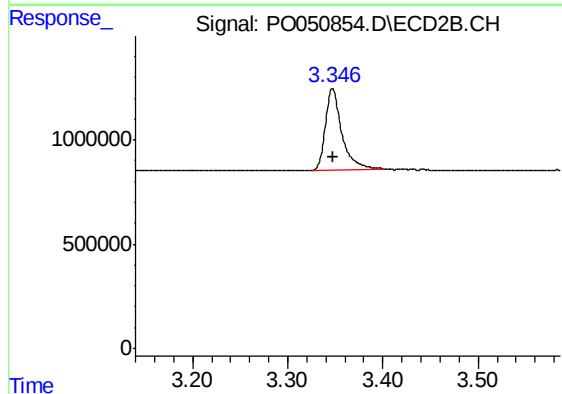


#1 Tetrachloro-m-xylene

R.T.: 3.347 min
Delta R.T.: -0.001 min
Response: 4679653
Conc: 21.53 ng/ml

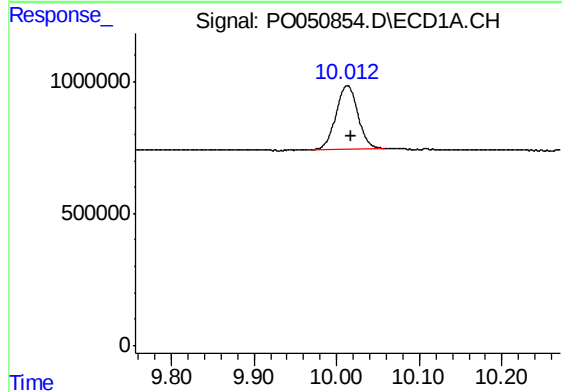

#2 Decachlorobiphenyl

R.T.: 10.013 min
Delta R.T.: -0.004 min
Response: 4453938
Conc: 14.33 ng/ml

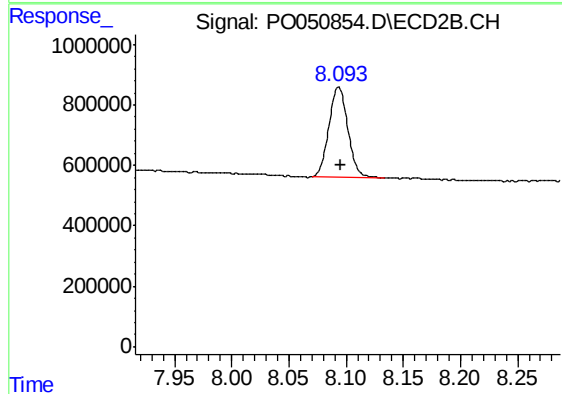

#2 Decachlorobiphenyl

R.T.: 8.093 min
Delta R.T.: -0.002 min
Response: 3394820
Conc: 13.27 ng/ml