

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
 Data File : PO072918.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2020 15:35
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 07:18:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.950	4.024	1121161	783962	24.317	22.369
2)	SA Decachlor...	10.982	9.307	985245	855322	26.668	25.648
Target Compounds							
9)	L2 AR-1221-2	0.000	4.373	0	11612	N.D.	31.872 #
20)	L4 AR-1242-5	0.000	6.169f	0	20013	N.D.	18.650 #
25)	L5 AR-1248-5	0.000	6.169f	0	20013	N.D.	12.998 #
26)	L6 AR-1254-1	0.000	6.169f	0	20013	N.D.	8.891 #
38)	L8 AR-1262-3	0.000	8.216	0	1353	N.D.	0.739 #
41)	L9 AR-1268-1	0.000	8.216	0	1353	N.D.	0.227 #
43)	L9 AR-1268-3	0.000	8.502	0	6322	N.D.	1.297 #
45)	L9 AR-1268-5	0.000	9.061	0	6076	N.D.	0.422 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
Data File : PO072918.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2020 15:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:18:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

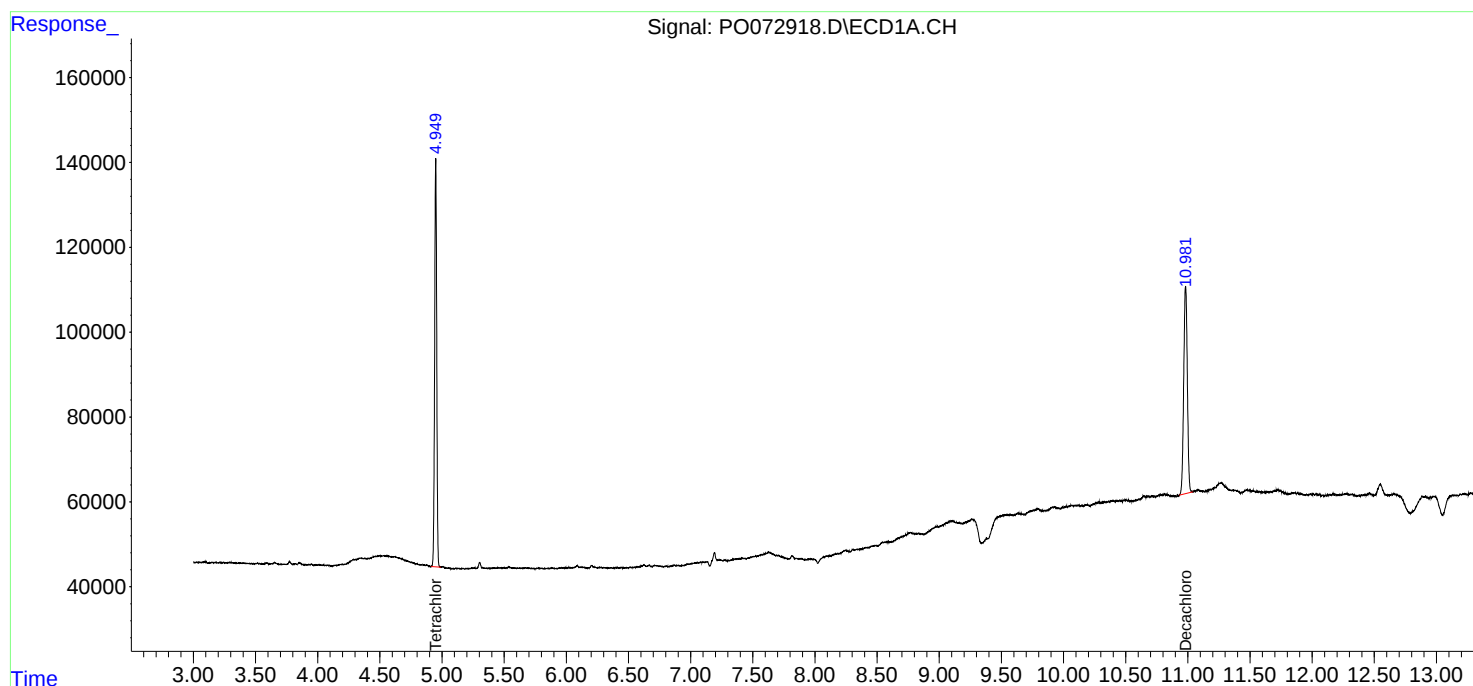


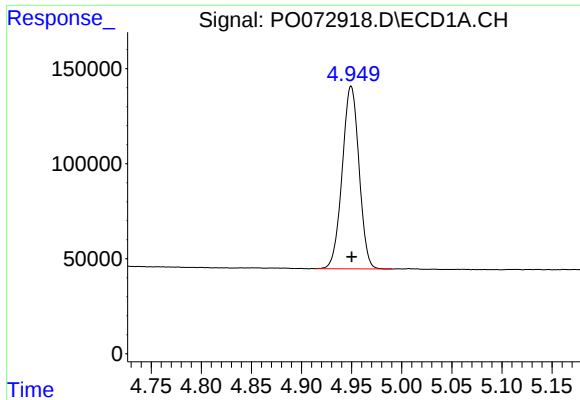

#1 Tetrachloro-m-xylene


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 1121161
Conc: 24.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

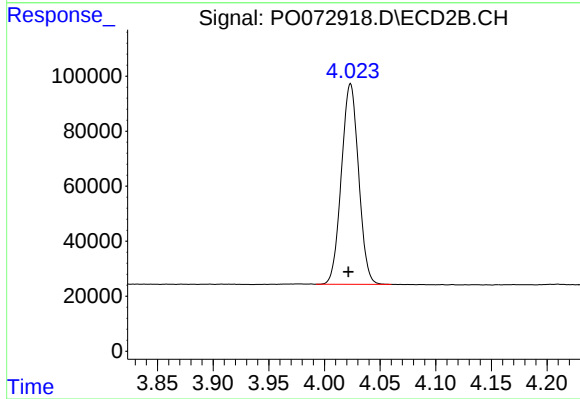


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.002 min
Response: 783962
Conc: 22.37 ng/ml

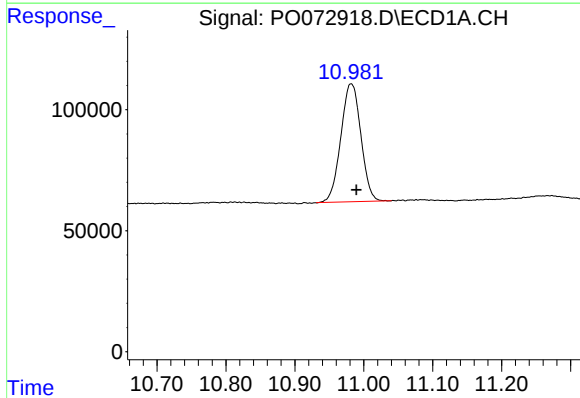


#2 Decachlorobiphenyl

R.T.: 10.982 min
Delta R.T.: -0.008 min
Response: 985245
Conc: 26.67 ng/ml

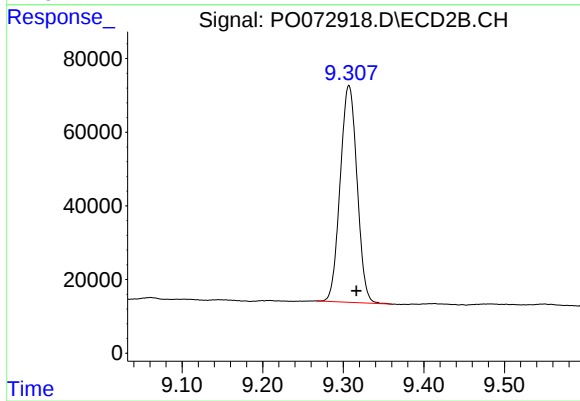

#2 Decachlorobiphenyl


R.T.: 9.307 min
Delta R.T.: -0.009 min
Response: 855322
Conc: 25.65 ng/ml

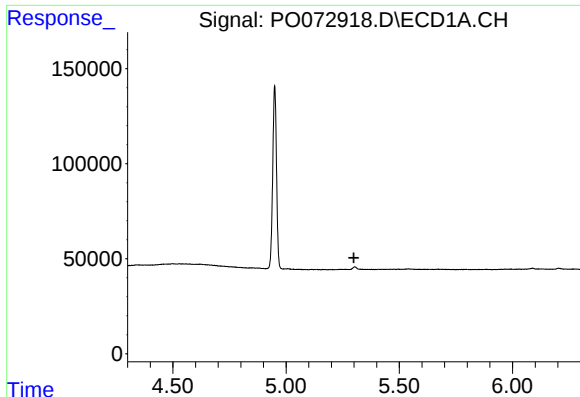

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

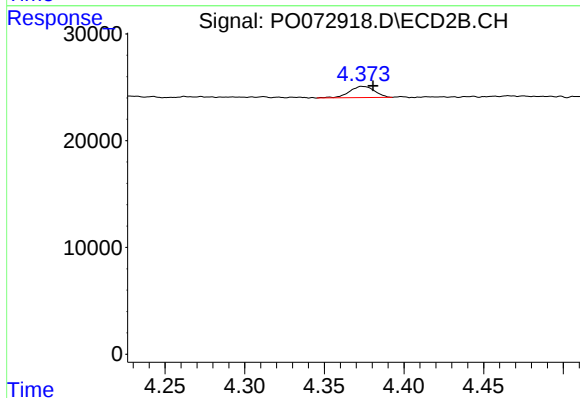


#9 AR-1221-2

R.T.: 4.373 min
Delta R.T.: -0.007 min
Response: 11612
Conc: 31.87 ng/ml

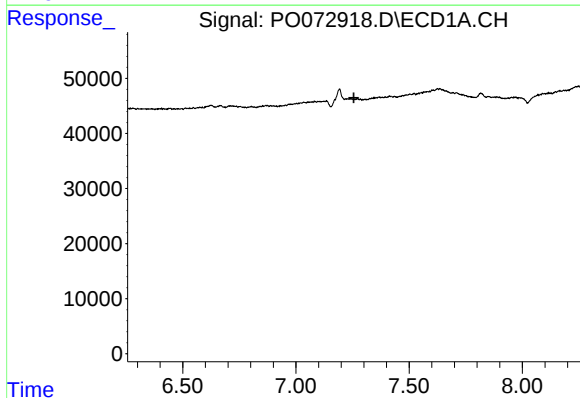


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.256 min
Response: 0
Conc: N.D.

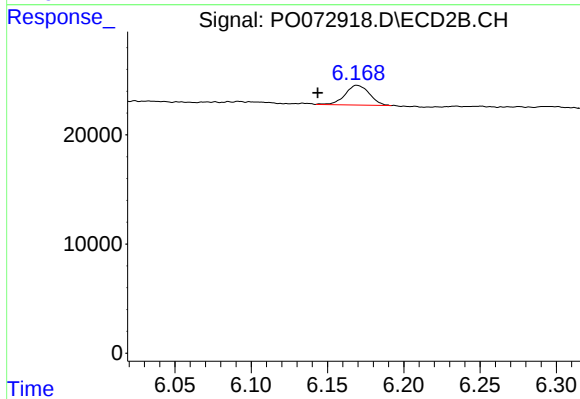

#20 AR-1242-5


R.T.: 6.169 min
Delta R.T.: 0.026 min
Response: 20013
Conc: 18.65 ng/ml

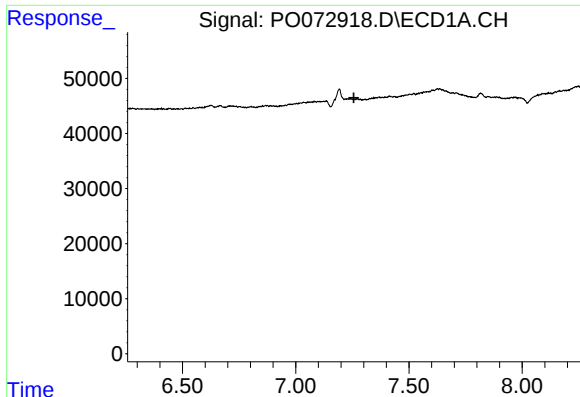

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

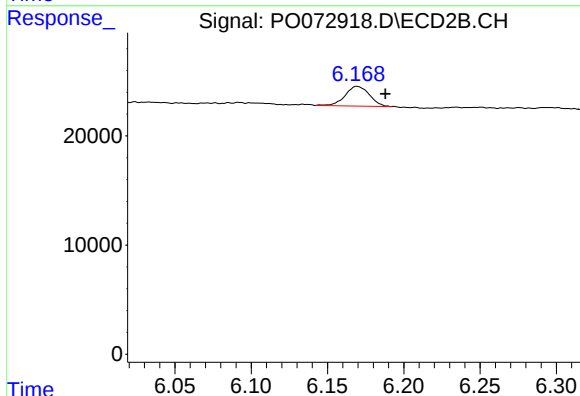


#25 AR-1248-5

R.T.: 6.169 min
Delta R.T.: -0.019 min
Response: 20013
Conc: 13.00 ng/ml

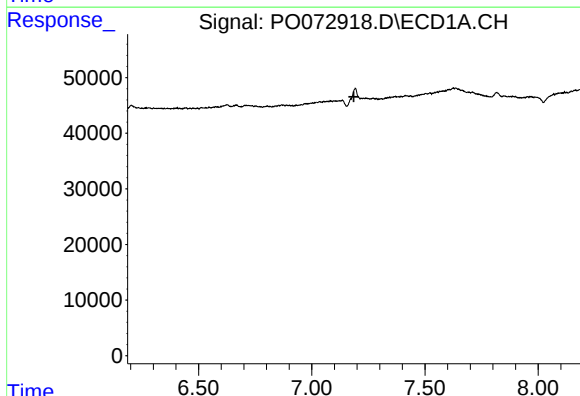


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.186 min
Response: 0
Conc: N.D.

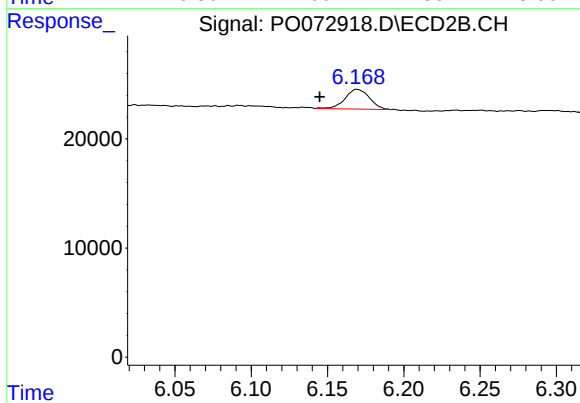

#26 AR-1254-1


R.T.: 6.169 min
Delta R.T.: 0.024 min
Response: 20013
Conc: 8.89 ng/ml

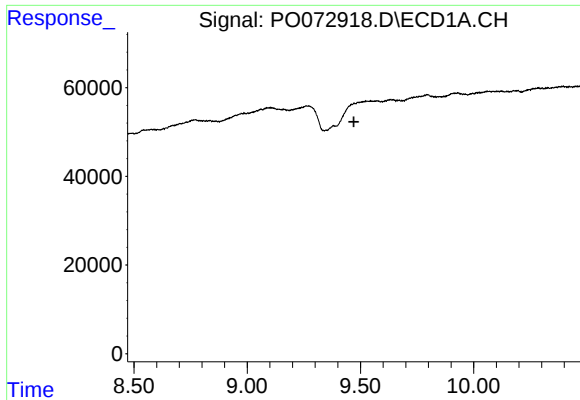

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

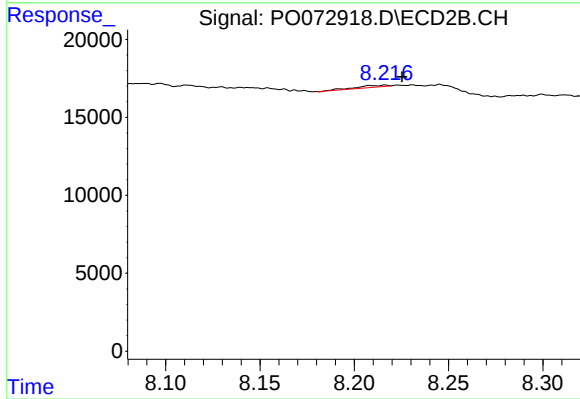


#38 AR-1262-3

R.T.: 8.216 min
Delta R.T.: -0.009 min
Response: 1353
Conc: 0.74 ng/ml

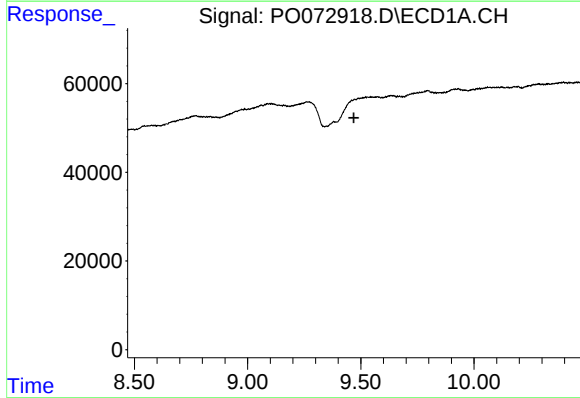


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.470 min
Response: 0
Conc: N.D.

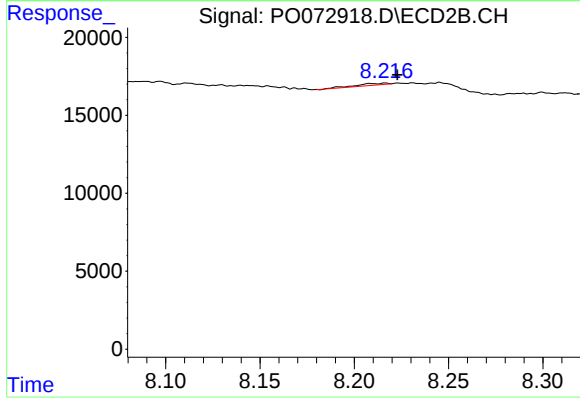

#41 AR-1268-1


R.T.: 8.216 min
Delta R.T.: -0.006 min
Response: 1353
Conc: 0.23 ng/ml

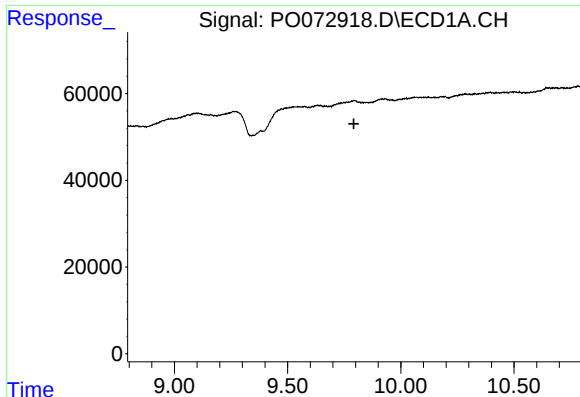

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

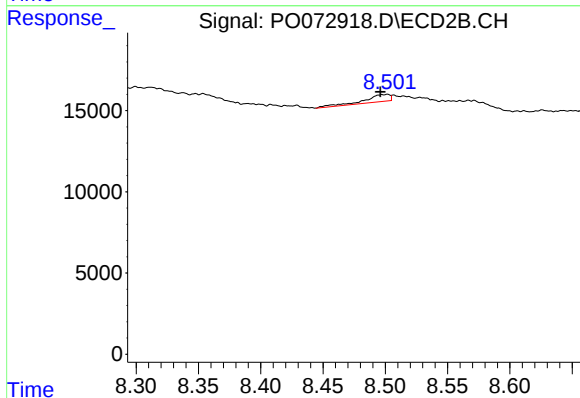


#43 AR-1268-3

R.T.: 8.502 min
Delta R.T.: 0.006 min
Response: 6322
Conc: 1.30 ng/ml

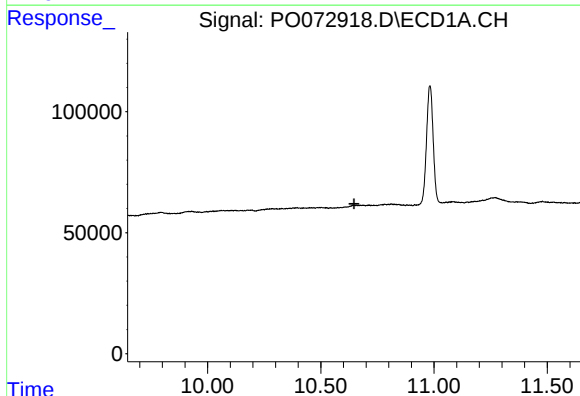

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.646 min
Response: 0
Conc: N.D.

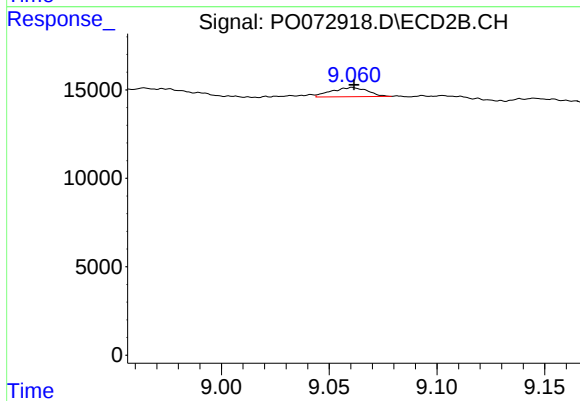

#45 AR-1268-5

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 6076
Conc: 0.42 ng/ml