

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
 Data File : PO072938.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2020 21:18
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 07:35:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.948	4.024	1170458	800056	25.386	22.828
2)	SA Decachlor...	10.979	9.305	1000043	870692	27.068	26.109
Target Compounds							
9)	L2 AR-1221-2	0.000	4.375	0	11011	N.D.	30.223 #
20)	L4 AR-1242-5	0.000	6.169f	0	25670	N.D.	23.922 #
24)	L5 AR-1248-4	7.189f	0.000	42937	0	23.776	N.D. #
25)	L5 AR-1248-5	0.000	6.169f	0	25670	N.D.	16.673 #
26)	L6 AR-1254-1	7.189	6.169f	42937	25670	24.776	11.405 #
31)	L7 AR-1260-1	0.000	6.862	0	1928	N.D.	0.970 #
33)	L7 AR-1260-3	0.000	7.203	0	9517	N.D.	4.318 #
35)	L7 AR-1260-5	0.000	7.965f	0	65062	N.D.	14.803 #
37)	L8 AR-1262-2	0.000	7.965f	0	65062	N.D.	14.262 #
38)	L8 AR-1262-3	0.000	8.216	0	531	N.D.	0.290 #
40)	L8 AR-1262-5	0.000	8.775	0	5428	N.D.	3.315 #
41)	L9 AR-1268-1	0.000	8.216	0	531	N.D.	0.089 #
43)	L9 AR-1268-3	0.000	8.497	0	10707	N.D.	2.196 #
44)	L9 AR-1268-4	0.000	8.775	0	5428	N.D.	2.486 #
45)	L9 AR-1268-5	0.000	9.060	0	6143	N.D.	0.427 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
Data File : PO072938.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2020 21:18
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:35:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

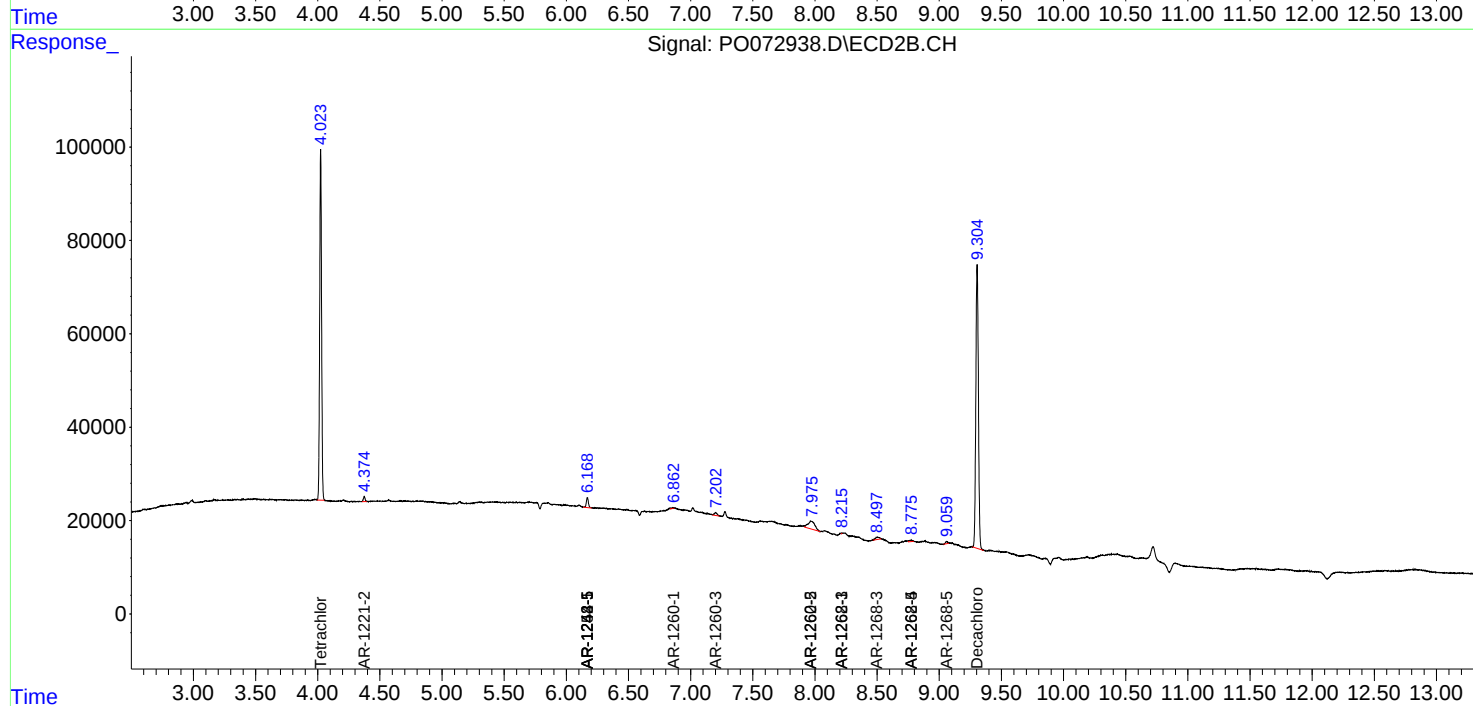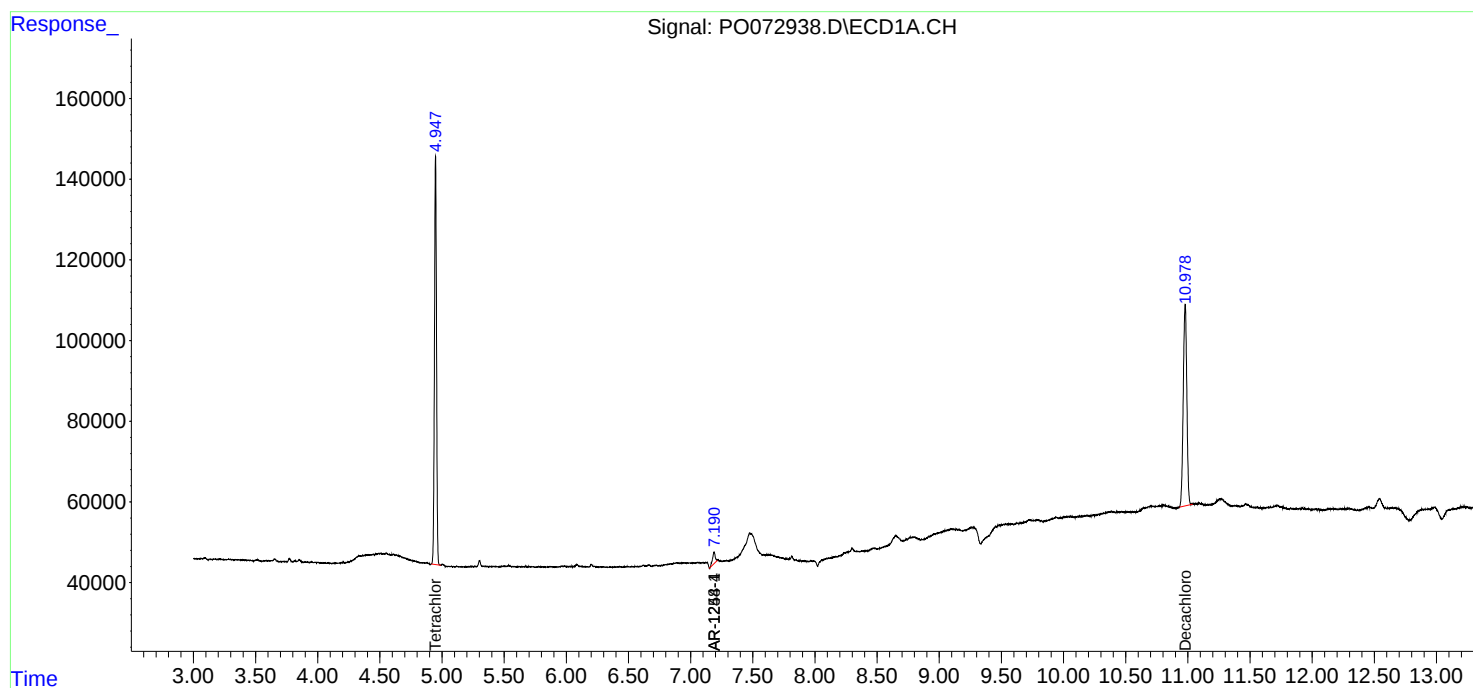


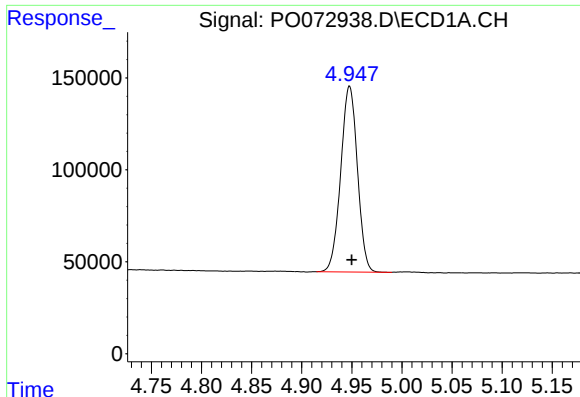

#1 Tetrachloro-m-xylene


R.T.: 4.948 min
Delta R.T.: -0.002 min
Response: 1170458
Conc: 25.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

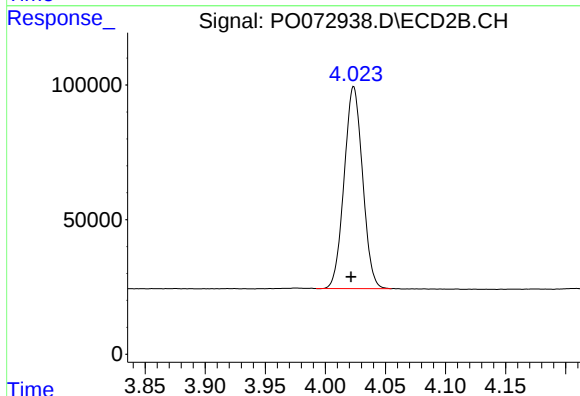


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.002 min
Response: 800056
Conc: 22.83 ng/ml

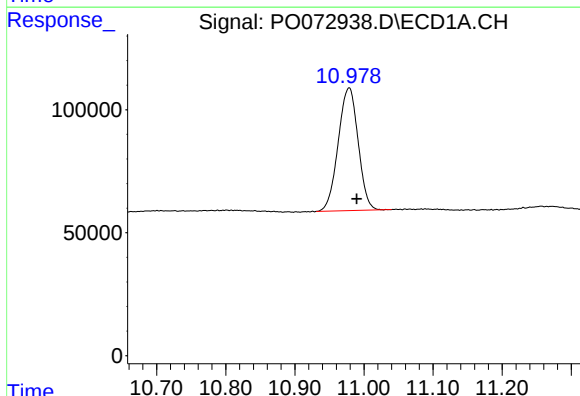


#2 Decachlorobiphenyl

R.T.: 10.979 min
Delta R.T.: -0.011 min
Response: 1000043
Conc: 27.07 ng/ml

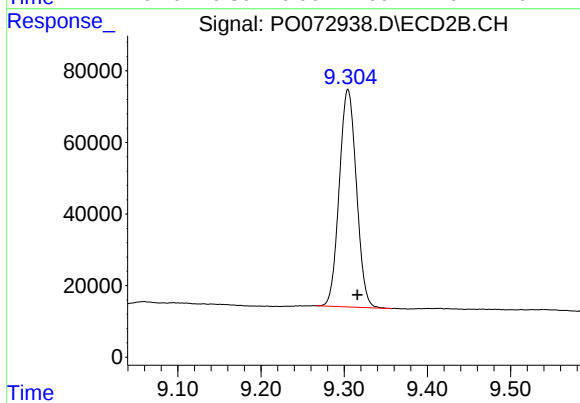

#2 Decachlorobiphenyl


R.T.: 9.305 min
Delta R.T.: -0.011 min
Response: 870692
Conc: 26.11 ng/ml

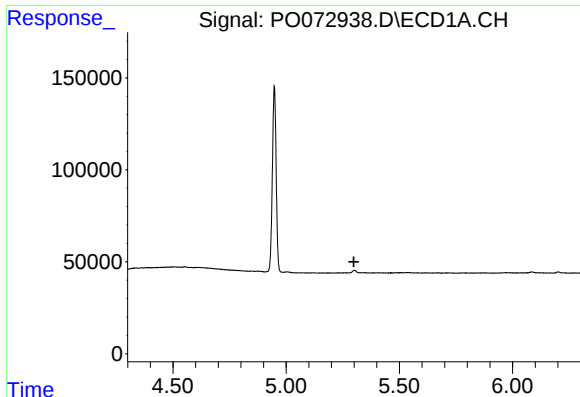

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

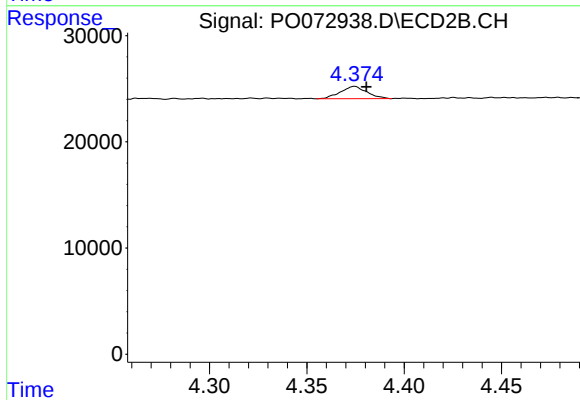


#9 AR-1221-2

R.T.: 4.375 min
Delta R.T.: -0.006 min
Response: 11011
Conc: 30.22 ng/ml

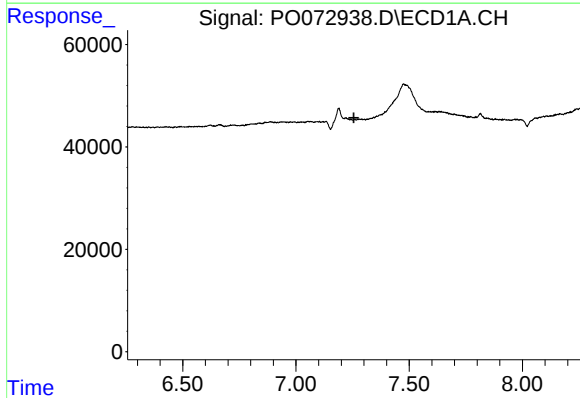


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.256 min
Response: 0
Conc: N.D.

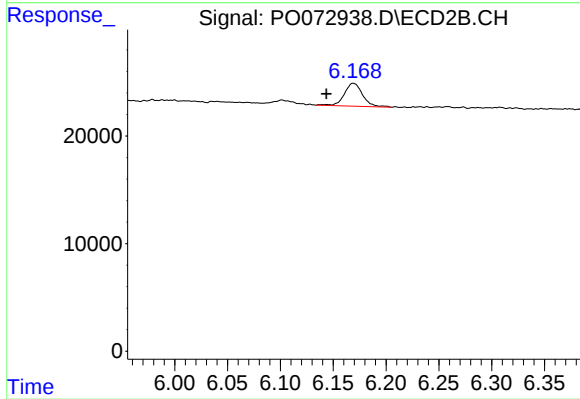

#20 AR-1242-5


R.T.: 6.169 min
Delta R.T.: 0.025 min
Response: 25670
Conc: 23.92 ng/ml

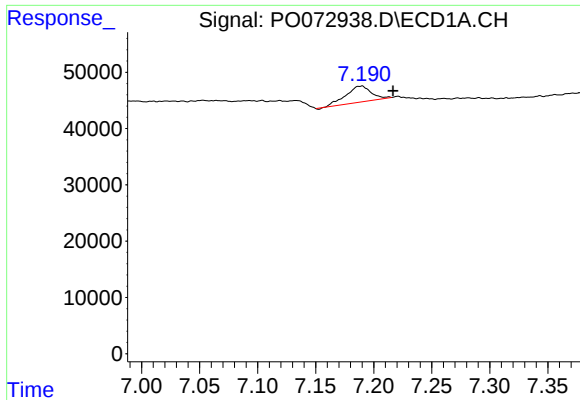

#24 AR-1248-4


R.T.: 7.189 min
Delta R.T.: -0.027 min
Response: 42937
Conc: 23.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

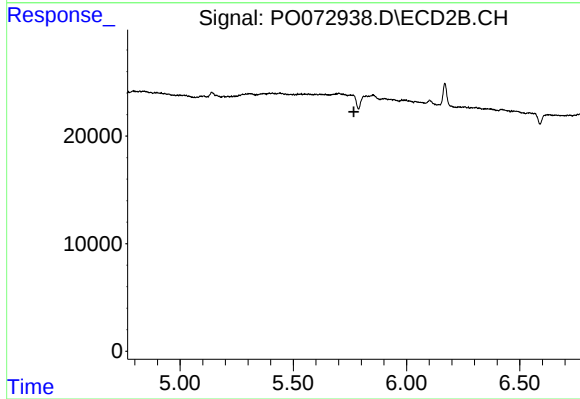


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.767 min
Response: 0
Conc: N.D.

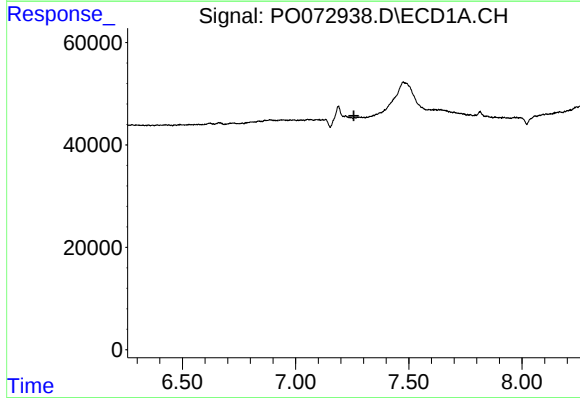


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 7.257 min
Response: 0
Conc: N.D.

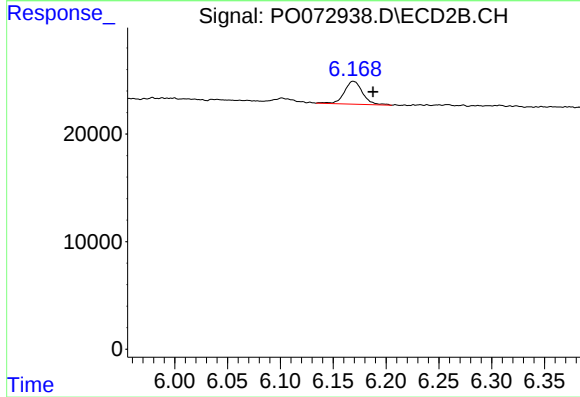

#25 AR-1248-5


R.T.: 6.169 min
Delta R.T.: -0.019 min
Response: 25670
Conc: 16.67 ng/ml

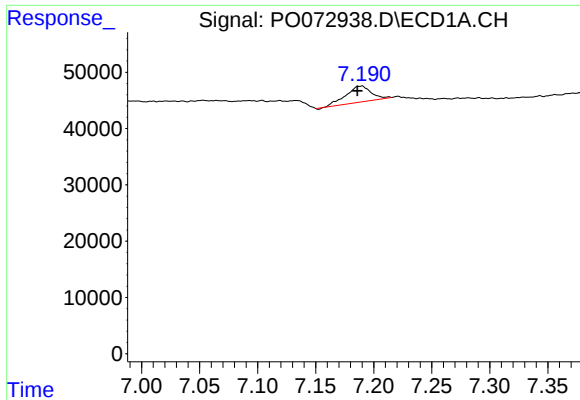

#26 AR-1254-1


R.T.: 7.189 min
Delta R.T.: 0.003 min
Response: 42937
Conc: 24.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

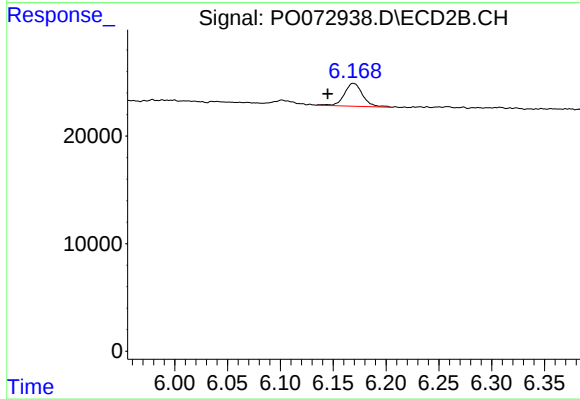


#26 AR-1254-1

R.T.: 6.169 min
Delta R.T.: 0.024 min
Response: 25670
Conc: 11.41 ng/ml

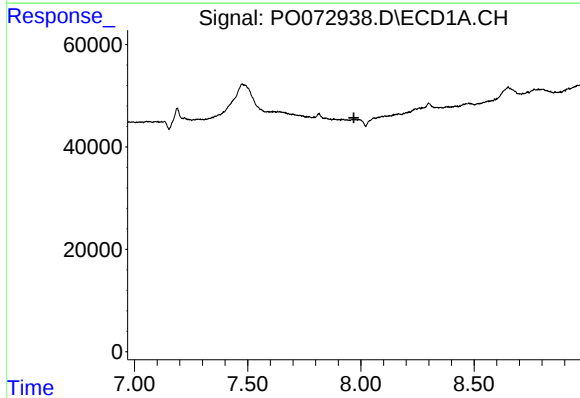


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.969 min
Response: 0
Conc: N.D.

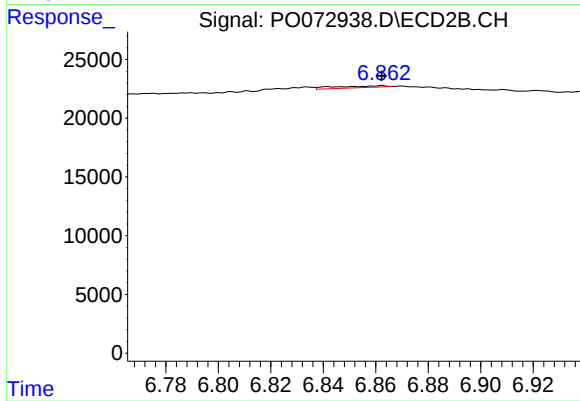

#31 AR-1260-1


R.T.: 6.862 min
Delta R.T.: 0.000 min
Response: 1928
Conc: 0.97 ng/ml

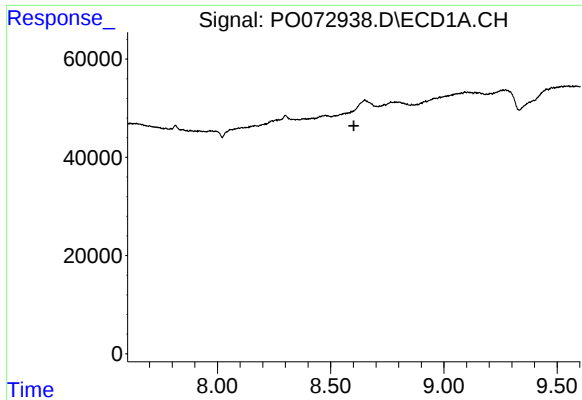

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

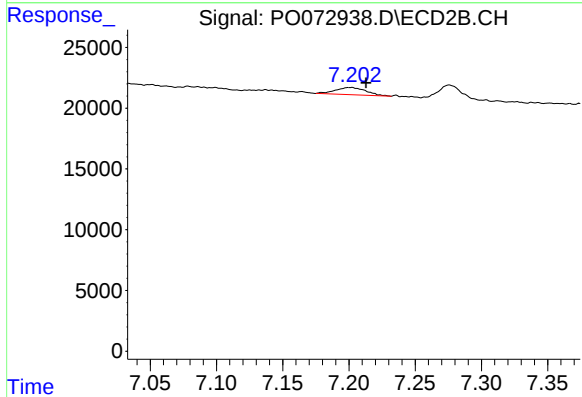


#33 AR-1260-3

R.T.: 7.203 min
Delta R.T.: -0.010 min
Response: 9517
Conc: 4.32 ng/ml

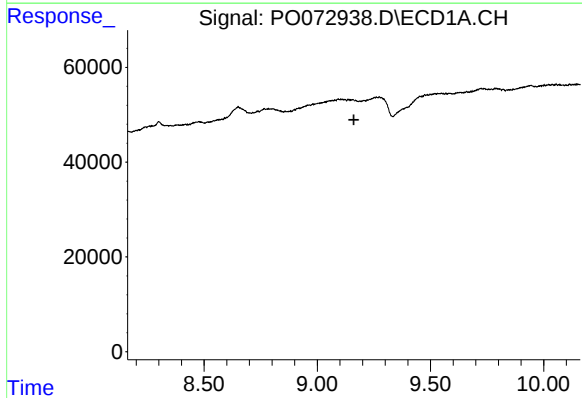


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 9.162 min
Response: 0
Conc: N.D.

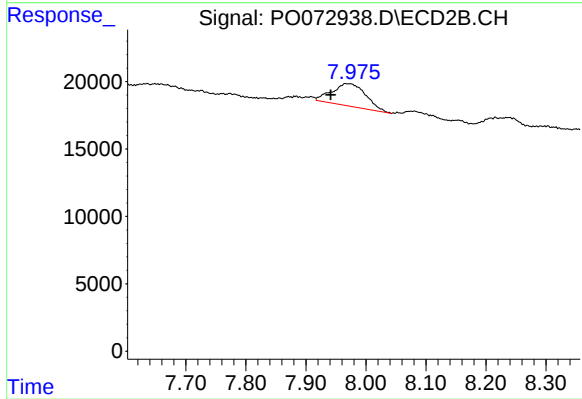

#35 AR-1260-5


R.T.: 7.965 min
Delta R.T.: 0.024 min
Response: 65062
Conc: 14.80 ng/ml

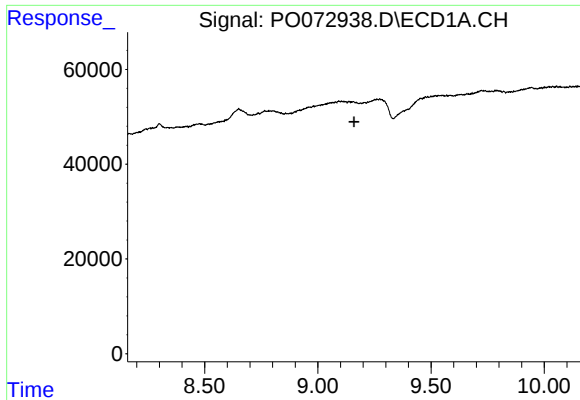

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 9.160 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

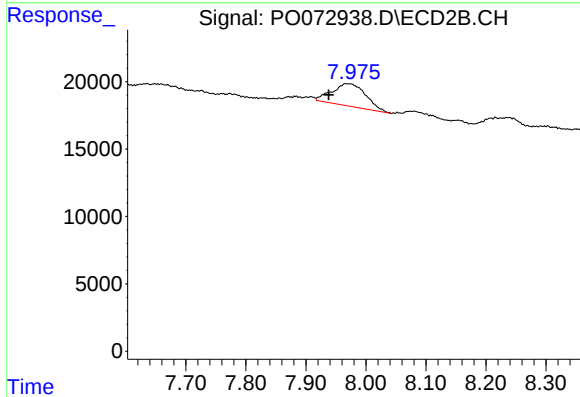


#37 AR-1262-2

R.T.: 7.965 min
Delta R.T.: 0.027 min
Response: 65062
Conc: 14.26 ng/ml

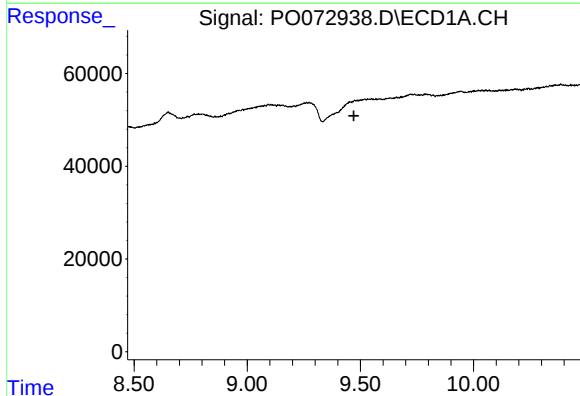


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.471 min
Response: 0
Conc: N.D.

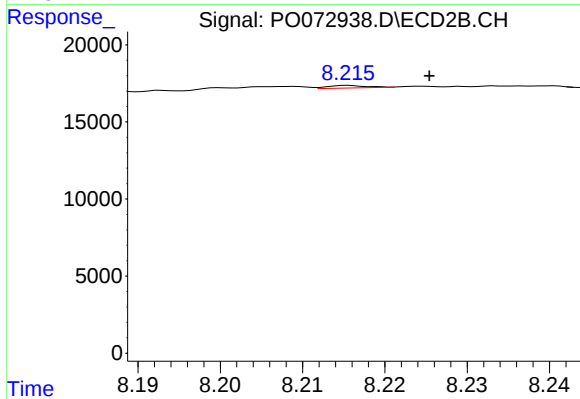

#38 AR-1262-3


R.T.: 8.216 min
Delta R.T.: -0.010 min
Response: 531
Conc: 0.29 ng/ml

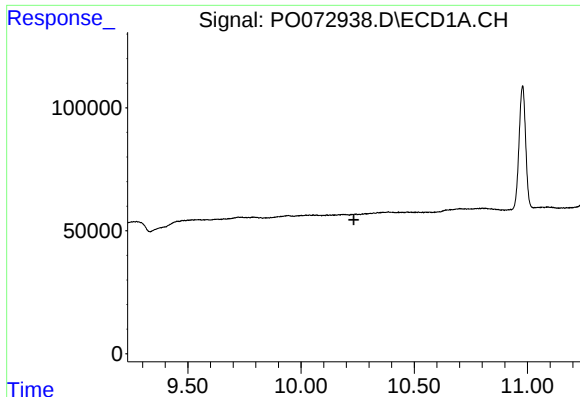

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 10.233 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

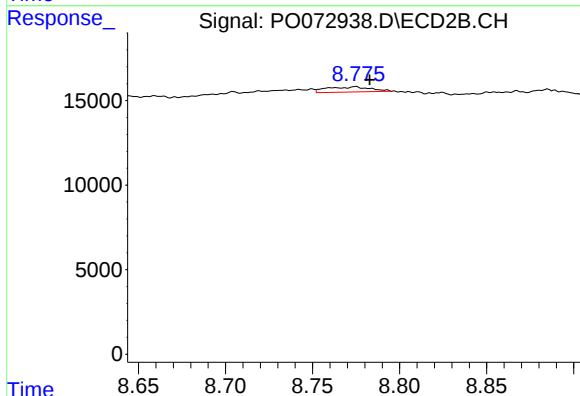


#40 AR-1262-5

R.T.: 8.775 min
Delta R.T.: -0.008 min
Response: 5428
Conc: 3.31 ng/ml

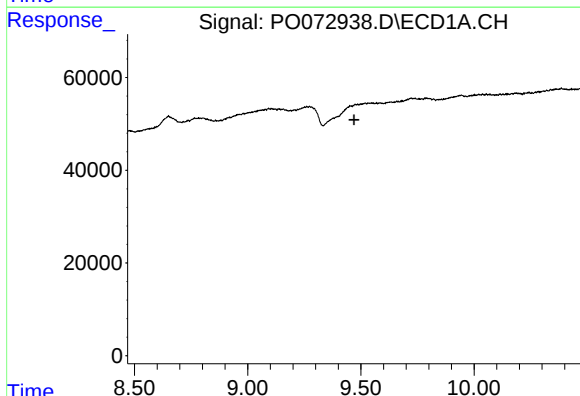


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.470 min
Response: 0
Conc: N.D.

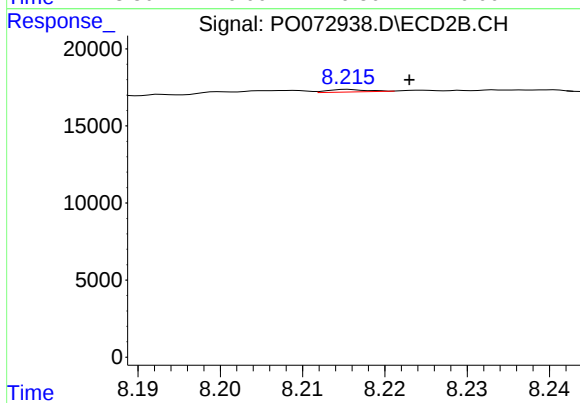

#41 AR-1268-1


R.T.: 8.216 min
Delta R.T.: -0.007 min
Response: 531
Conc: 0.09 ng/ml

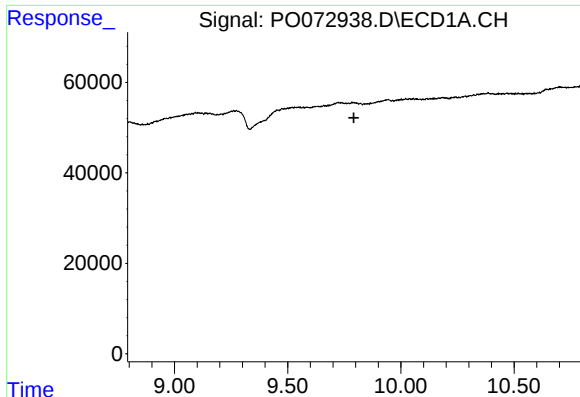

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 9.793 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

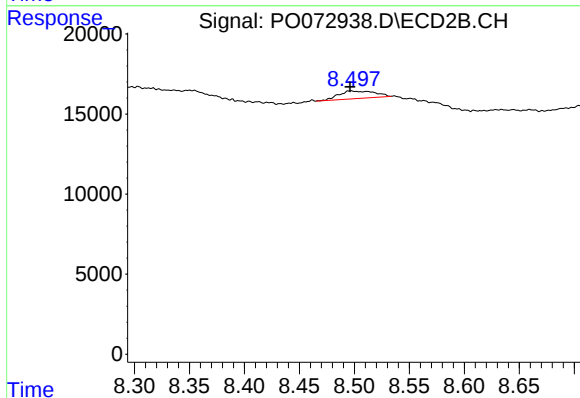


#43 AR-1268-3

R.T.: 8.497 min
Delta R.T.: 0.001 min
Response: 10707
Conc: 2.20 ng/ml

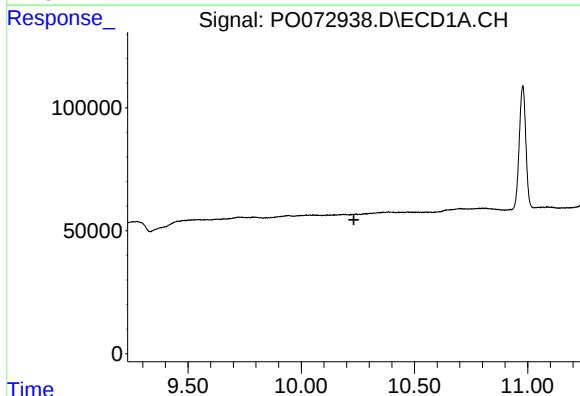


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 10.233 min
Response: 0
Conc: N.D.

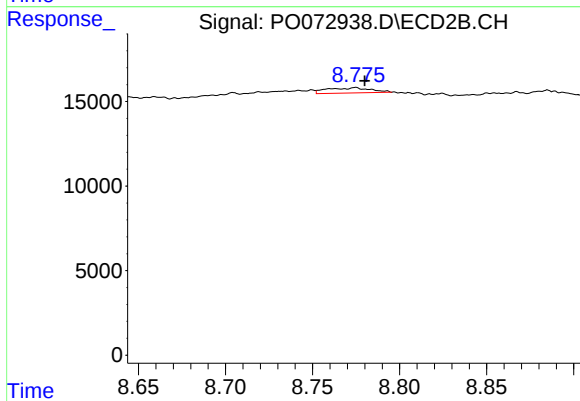

#44 AR-1268-4


R.T.: 8.775 min
Delta R.T.: -0.005 min
Response: 5428
Conc: 2.49 ng/ml

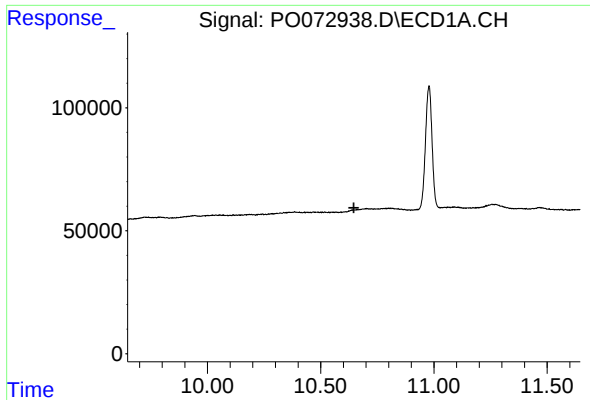

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

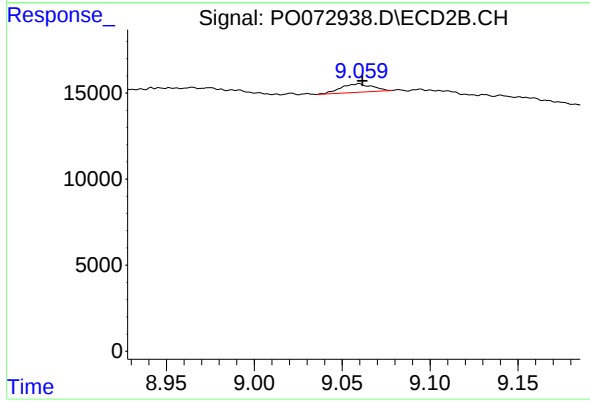

#45 AR-1268-5

R.T.: 9.060 min
Delta R.T.: -0.002 min
Response: 6143
Conc: 0.43 ng/ml