

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103120\
 Data File : P0072956.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Oct 2020 2:26
 Operator : DD\AJ
 Sample : L4541-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 07:54:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.948	4.025	1316323	912260	28.550	26.029
2)	SA Decachlor...	10.976	9.305	935405	779499	25.319	23.374
Target Compounds							
9)	L2 AR-1221-2	0.000	4.375	0	13327	N.D.	36.580 #
31)	L7 AR-1260-1	0.000	6.860	0	4077	N.D.	2.050 #
33)	L7 AR-1260-3	0.000	7.204	0	10917	N.D.	4.953 #
35)	L7 AR-1260-5	0.000	7.968f	0	22162	N.D.	5.042 #
37)	L8 AR-1262-2	0.000	7.968f	0	22162	N.D.	4.858 #
43)	L9 AR-1268-3	0.000	8.498	0	3931	N.D.	0.806 #
45)	L9 AR-1268-5	0.000	9.061	0	3194	N.D.	0.222 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
Data File : PO072956.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Oct 2020 2:26
Operator : DD\AJ
Sample : L4541-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:54:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

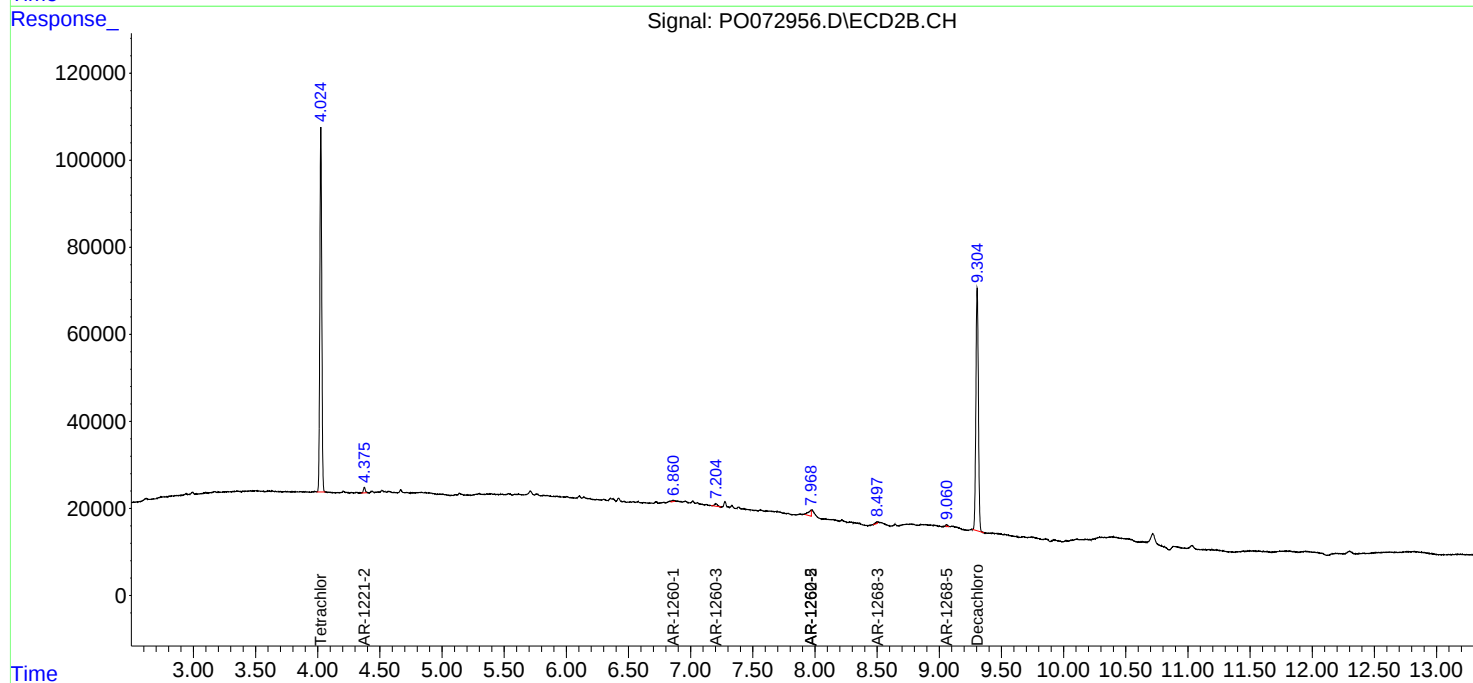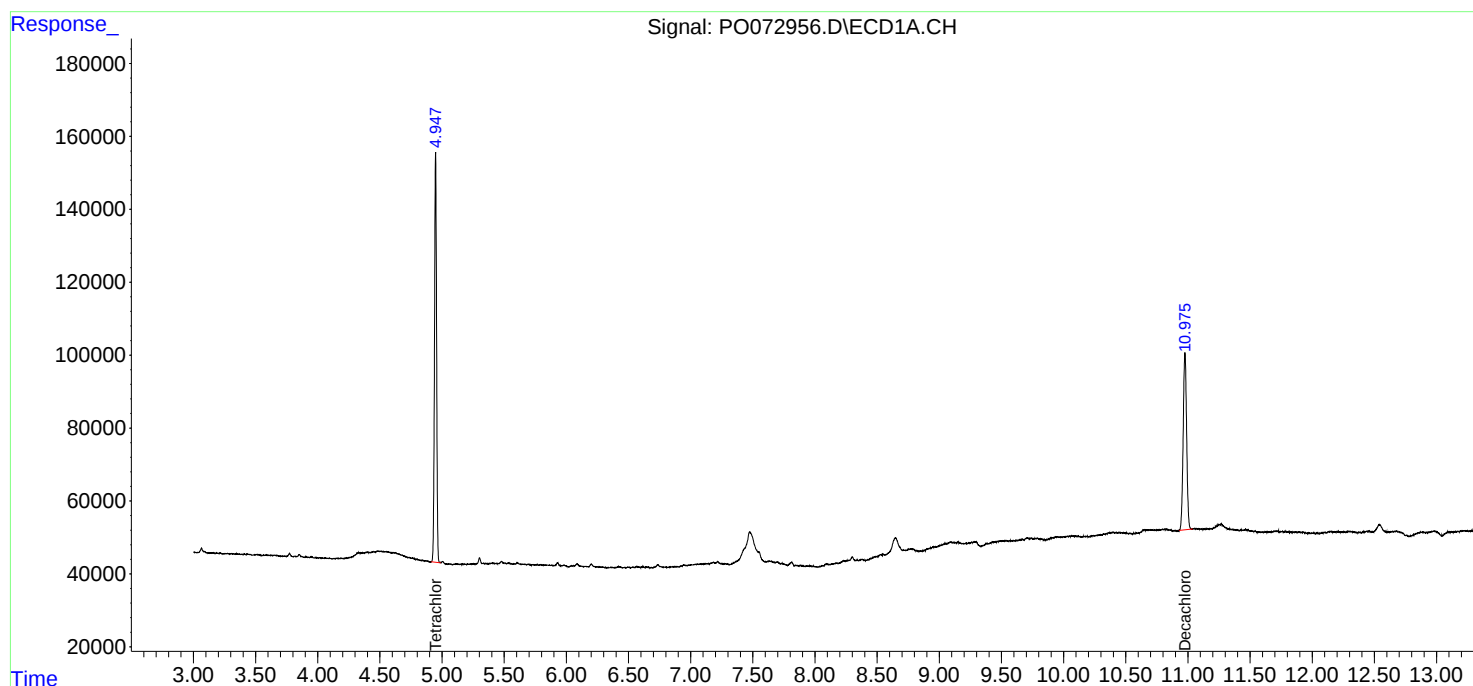


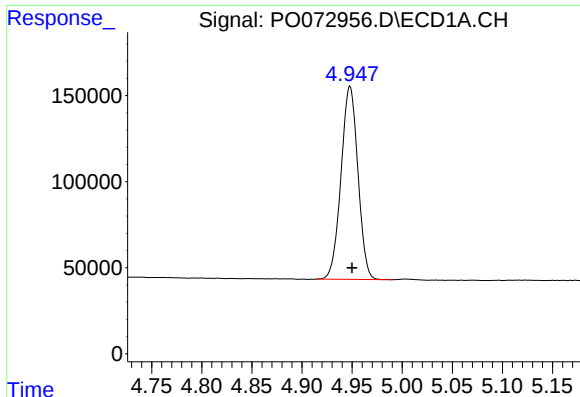

#1 Tetrachloro-m-xylene


R.T.: 4.948 min
Delta R.T.: -0.002 min
Response: 1316323
Conc: 28.55 ng/ml

Instrument :
ECD_O
ClientSampleId :

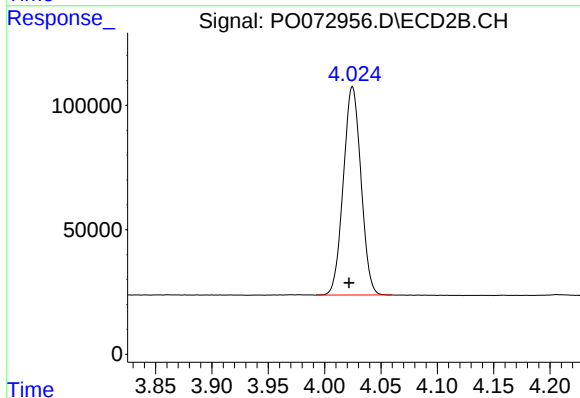


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.003 min
Response: 912260
Conc: 26.03 ng/ml

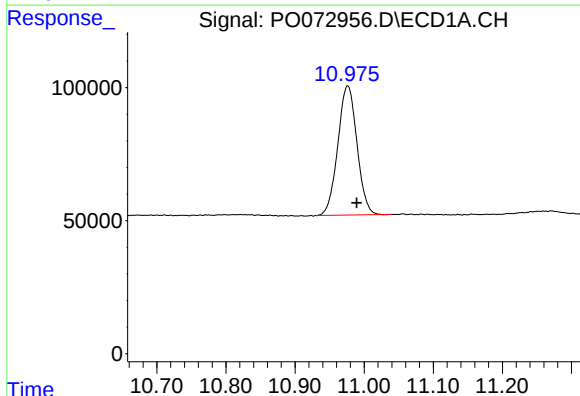


#2 Decachlorobiphenyl

R.T.: 10.976 min
Delta R.T.: -0.013 min
Response: 935405
Conc: 25.32 ng/ml

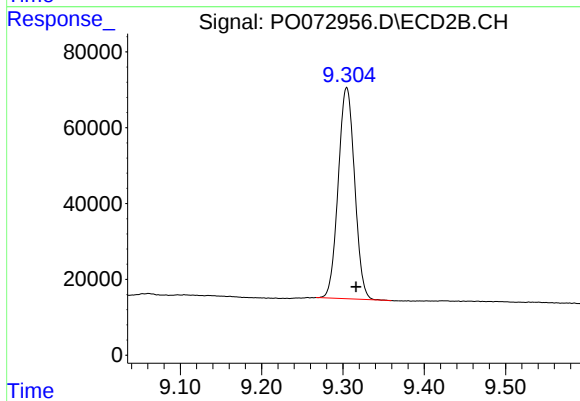

#2 Decachlorobiphenyl


R.T.: 9.305 min
Delta R.T.: -0.011 min
Response: 779499
Conc: 23.37 ng/ml

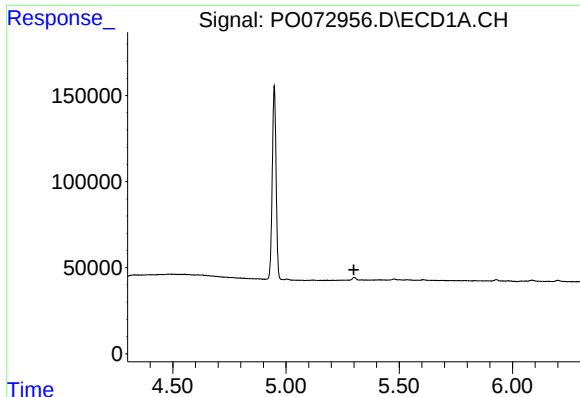

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

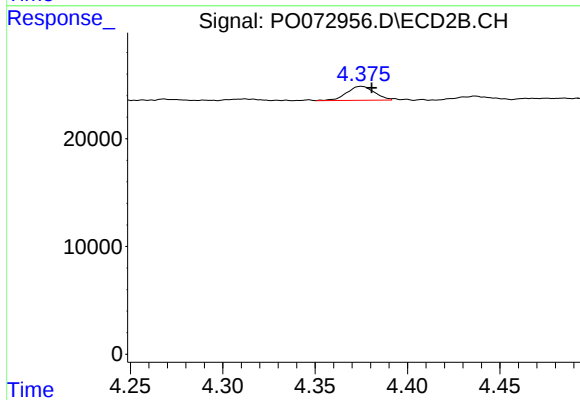


#9 AR-1221-2

R.T.: 4.375 min
Delta R.T.: -0.006 min
Response: 13327
Conc: 36.58 ng/ml

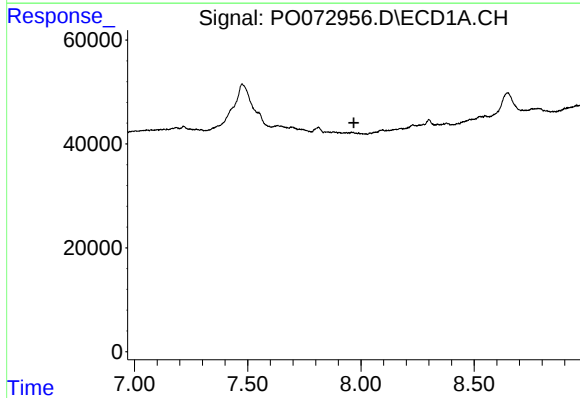


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.969 min
Response: 0
Conc: N.D.

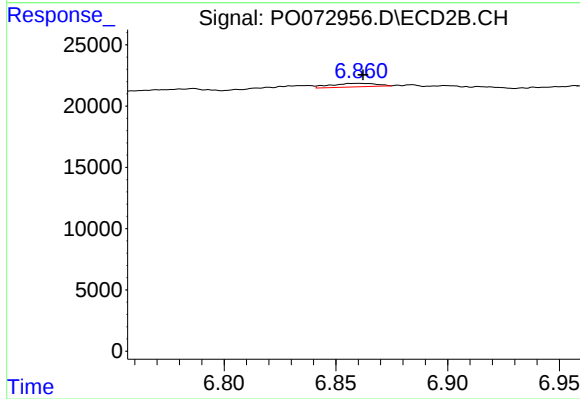

#31 AR-1260-1


R.T.: 6.860 min
Delta R.T.: -0.002 min
Response: 4077
Conc: 2.05 ng/ml

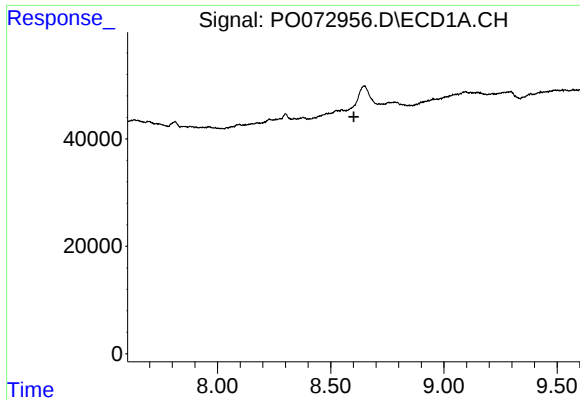

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

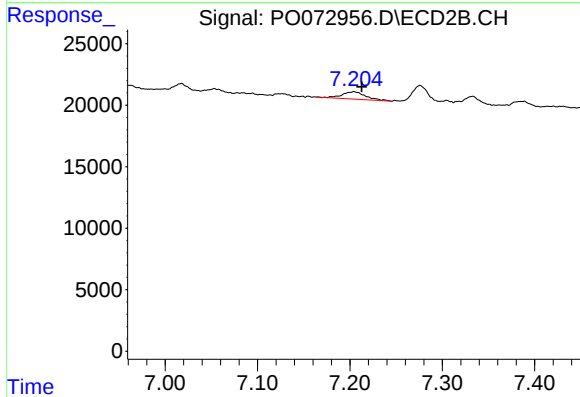


#33 AR-1260-3

R.T.: 7.204 min
Delta R.T.: -0.008 min
Response: 10917
Conc: 4.95 ng/ml

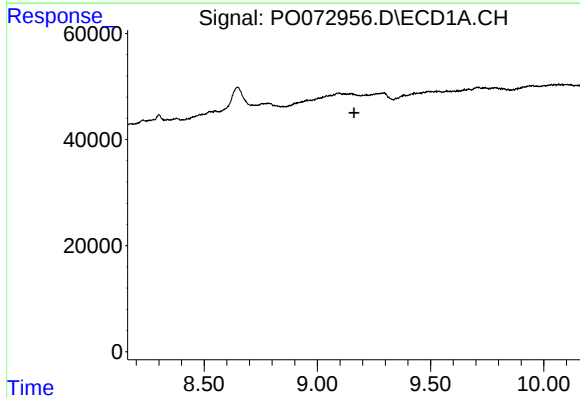


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 9.162 min
Response: 0
Conc: N.D.

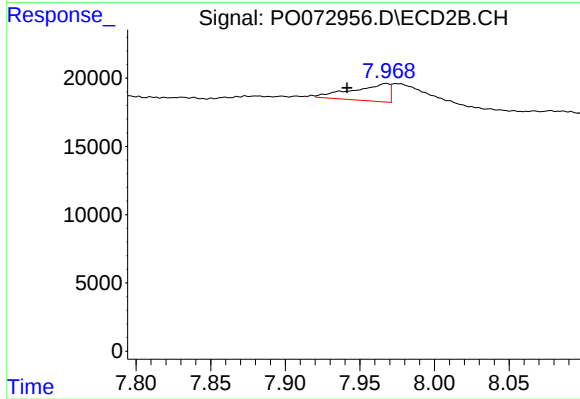

#35 AR-1260-5


R.T.: 7.968 min
Delta R.T.: 0.026 min
Response: 22162
Conc: 5.04 ng/ml

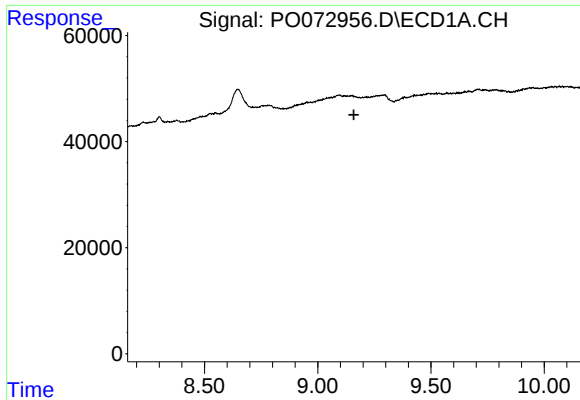

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 9.160 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

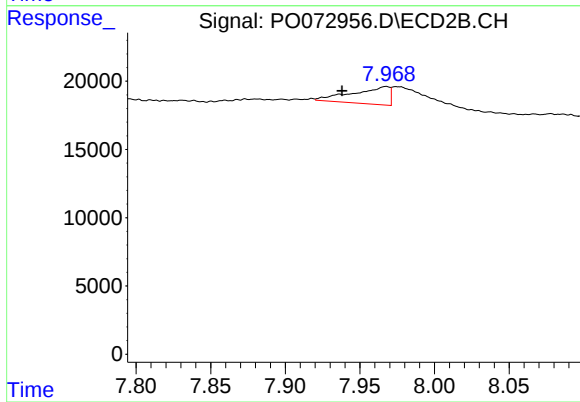


#37 AR-1262-2

R.T.: 7.968 min
Delta R.T.: 0.030 min
Response: 22162
Conc: 4.86 ng/ml

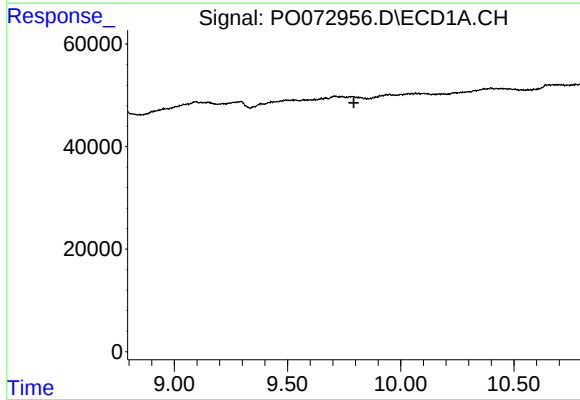


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.793 min
Response: 0
Conc: N.D.

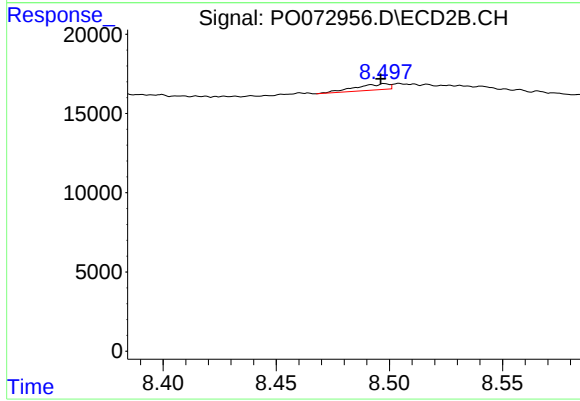

#43 AR-1268-3


R.T.: 8.498 min
Delta R.T.: 0.002 min
Response: 3931
Conc: 0.81 ng/ml

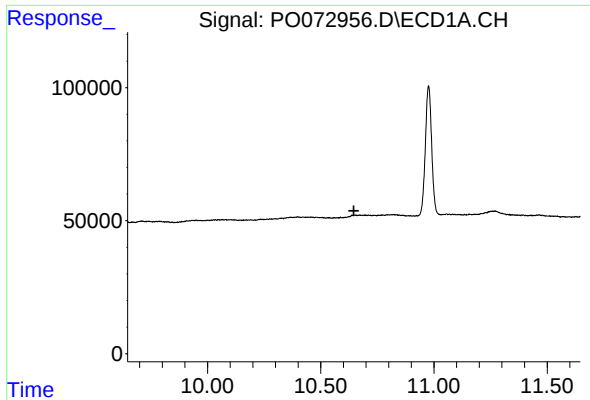

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

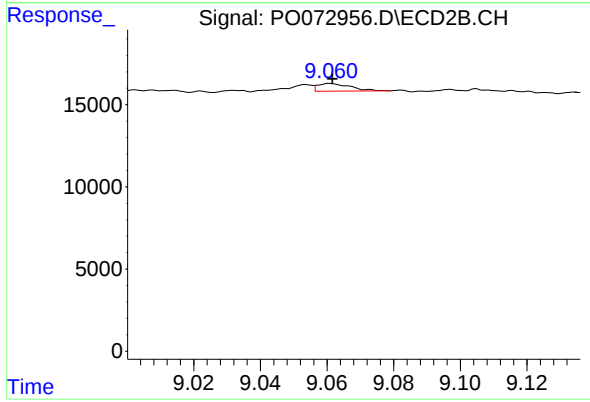

#45 AR-1268-5

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 3194
Conc: 0.22 ng/ml