

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
 Data File : PO072935.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2020 20:27
 Operator : DD\AJ
 Sample : L4559-18
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2020-10-27-EB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 07:32:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.948	4.024	1107074	751553	24.011	21.444
2)	SA Decachlor...	10.979	9.306	816936	727934	22.112	21.828

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
Data File : PO072935.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2020 20:27
Operator : DD\AJ
Sample : L4559-18
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2020-10-27-EB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:32:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

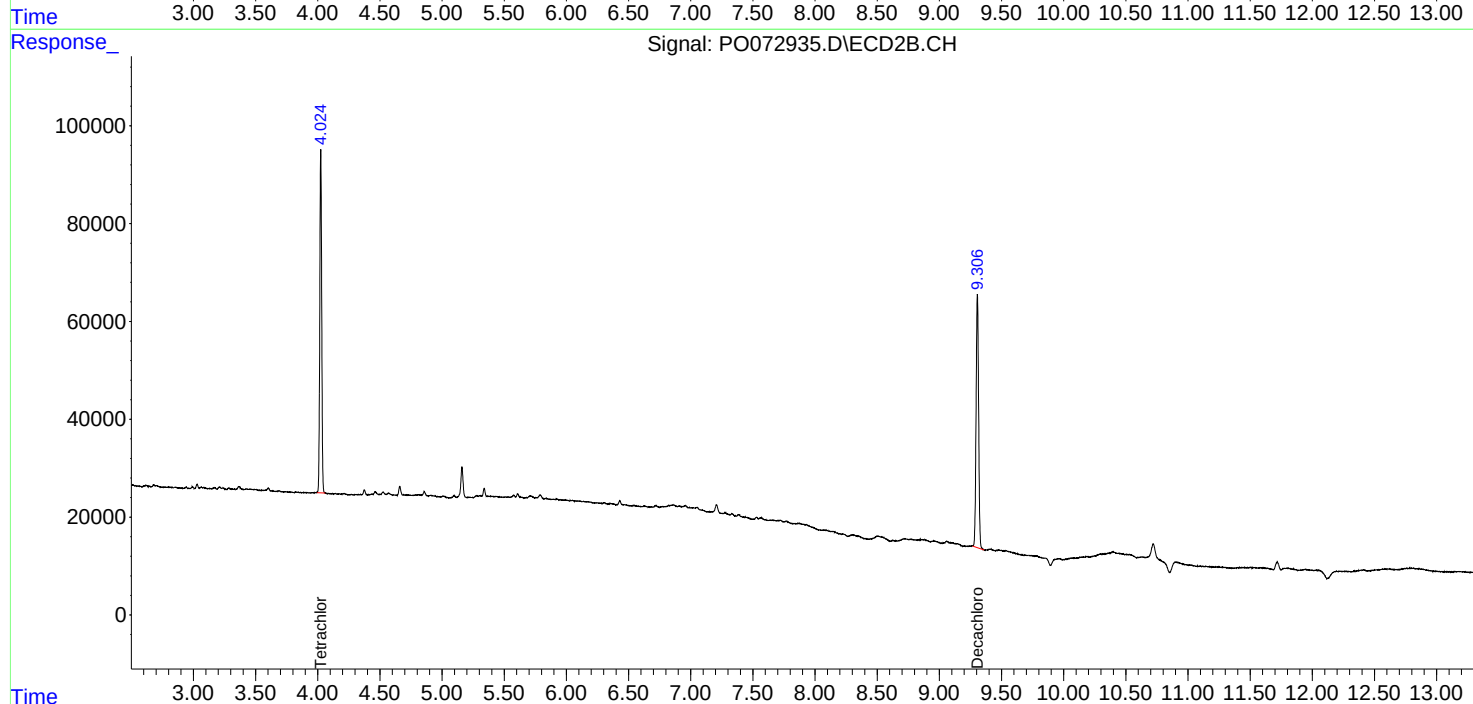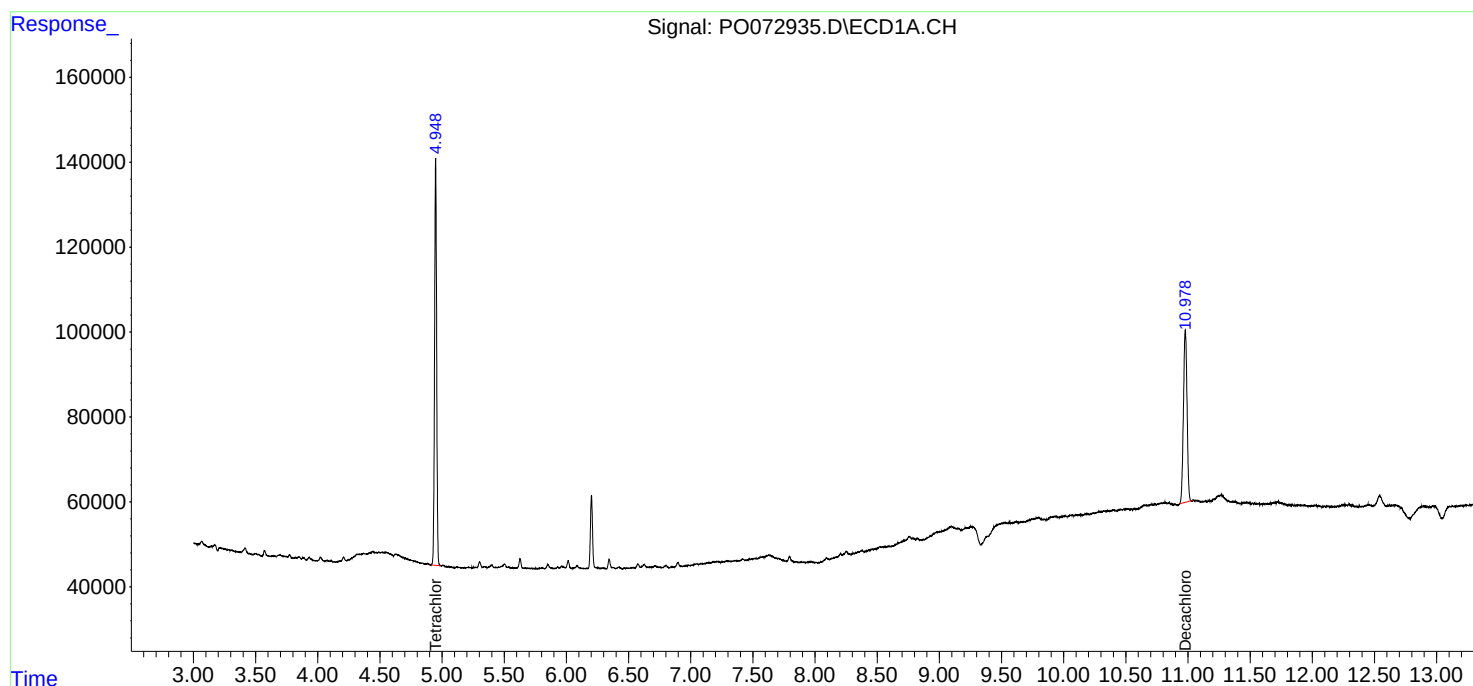


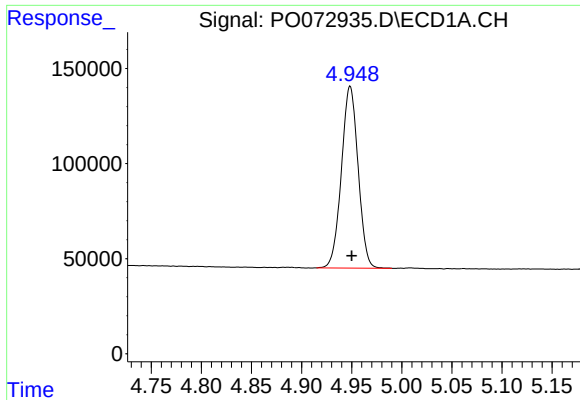

#1 Tetrachloro-m-xylene


R.T.: 4.948 min
Delta R.T.: -0.002 min
Response: 1107074
Conc: 24.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
2020-10-27-EB

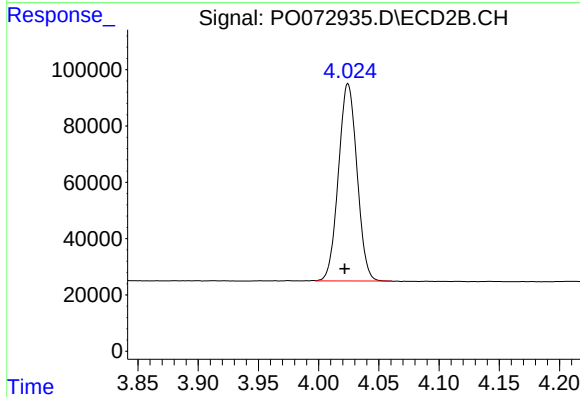


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.003 min
Response: 751553
Conc: 21.44 ng/ml

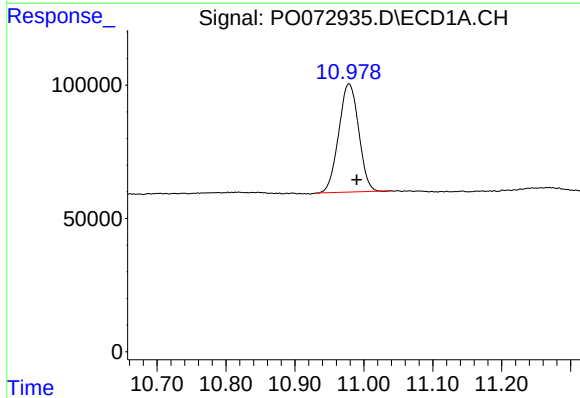

#2 Decachlorobiphenyl

R.T.: 10.979 min
Delta R.T.: -0.011 min
Response: 816936
Conc: 22.11 ng/ml

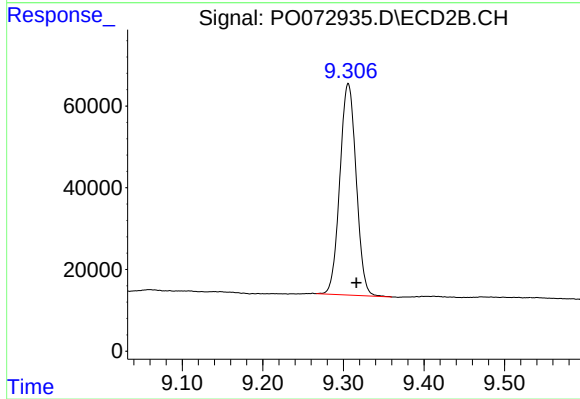

#2 Decachlorobiphenyl

R.T.: 9.306 min
Delta R.T.: -0.010 min
Response: 727934
Conc: 21.83 ng/ml