

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
Data File : PO072936.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2020 20:44
Operator : DD\AJ
Sample : L4557-31
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2020-10-28-EB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:33:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.948	4.025	946349	650079	20.525	18.549
2) SA Decachlor...	10.979	9.305	755724	676558	20.455	20.287

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
Data File : PO072936.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2020 20:44
Operator : DD\AJ
Sample : L4557-31
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2020-10-28-EB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:33:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

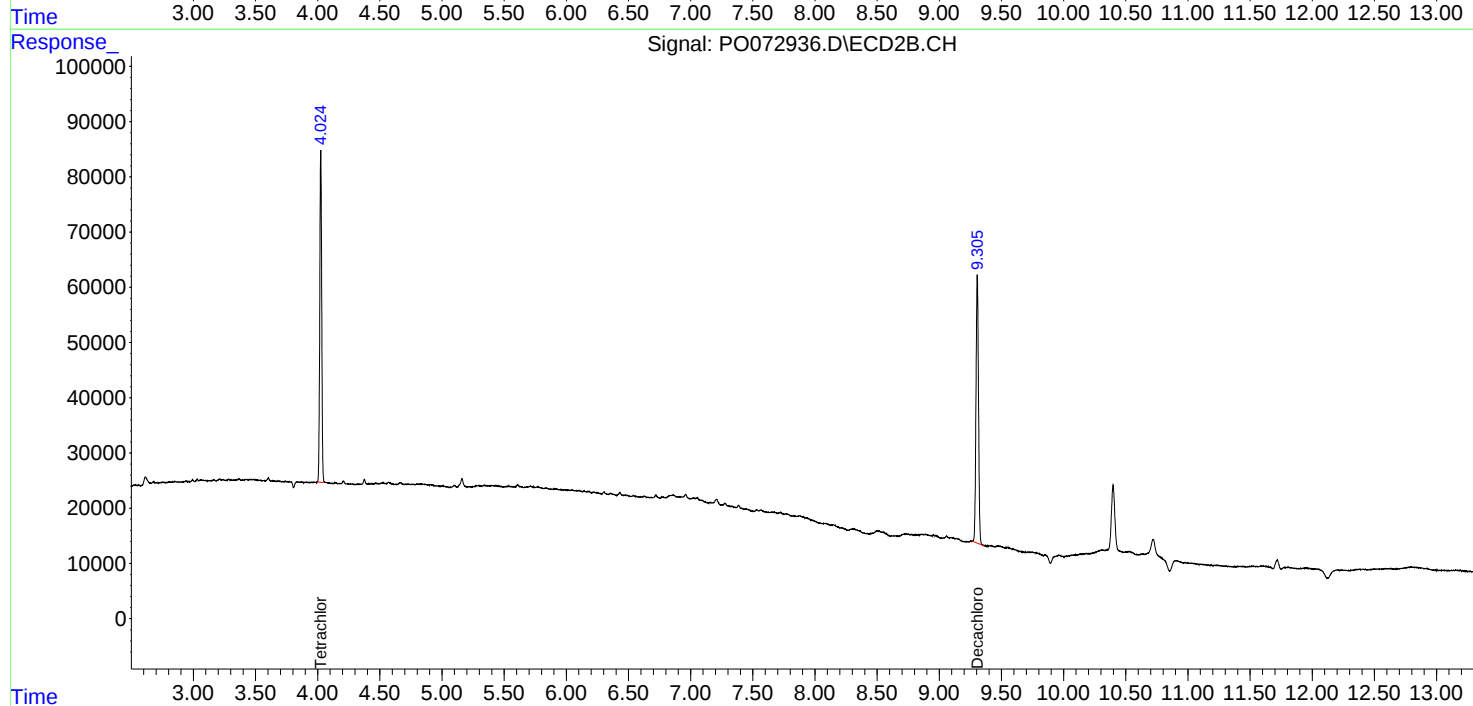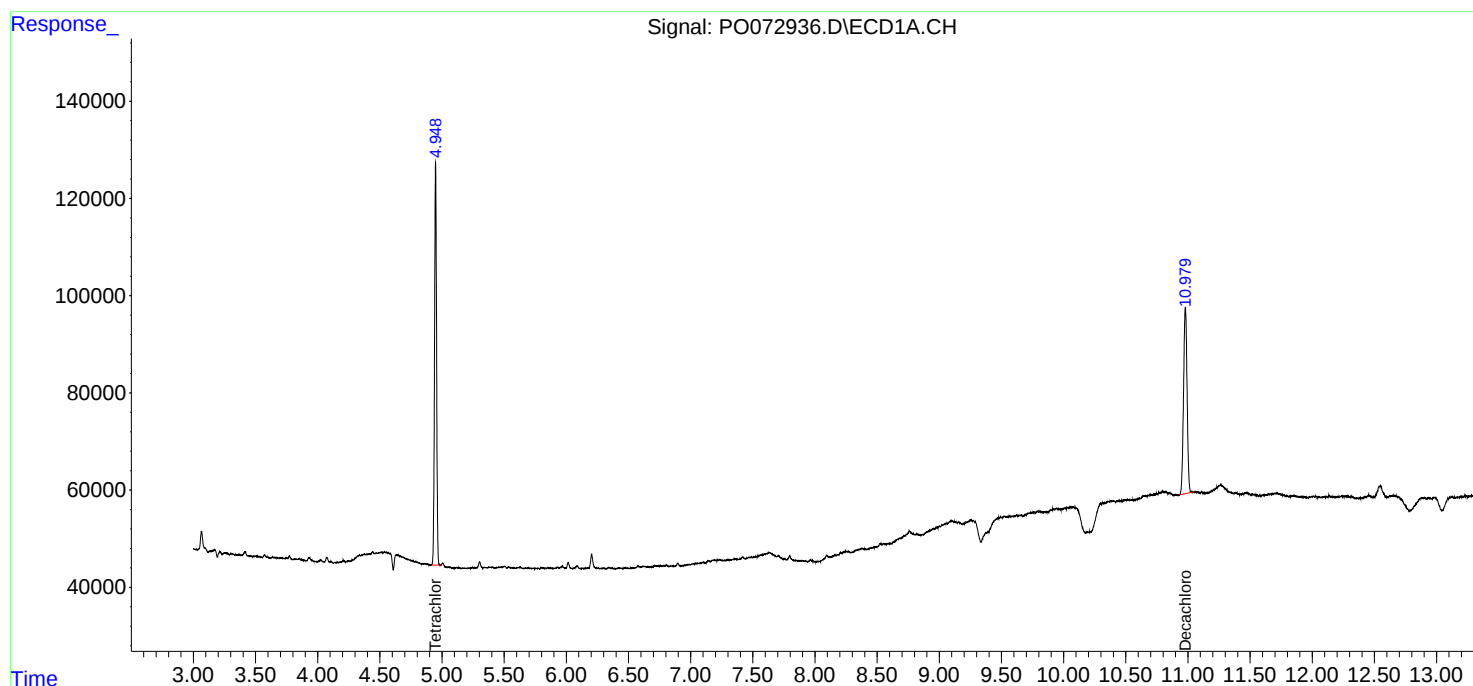


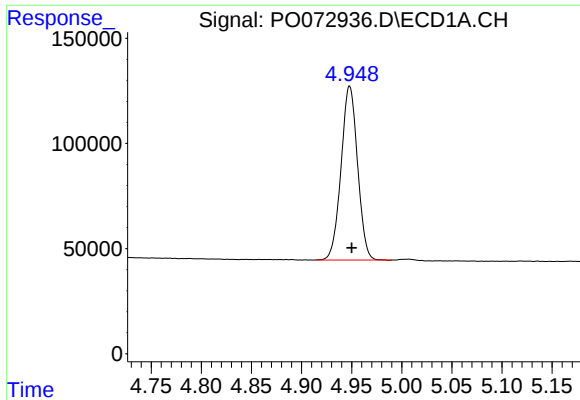

#1 Tetrachloro-m-xylene


R.T.: 4.948 min
Delta R.T.: -0.002 min
Response: 946349
Conc: 20.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
2020-10-28-EB

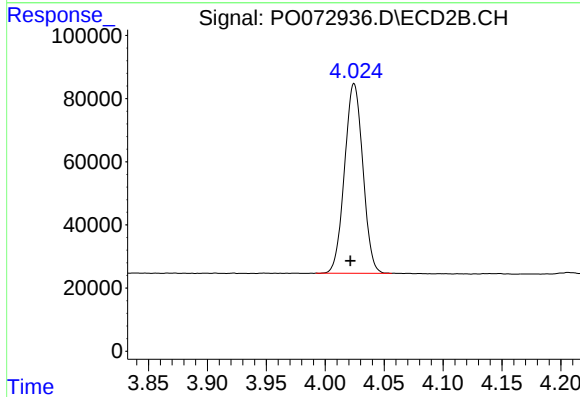


#1 Tetrachloro-m-xylene

R.T.: 4.025 min
Delta R.T.: 0.003 min
Response: 650079
Conc: 18.55 ng/ml

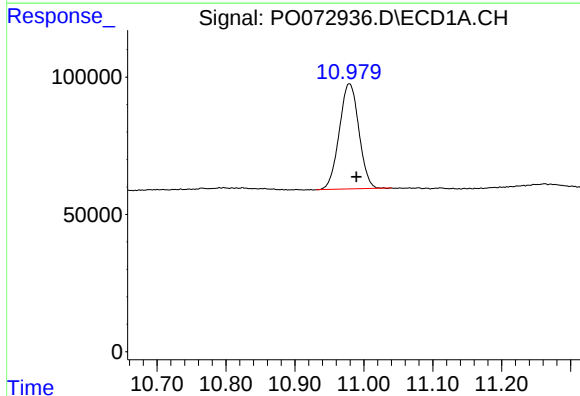

#2 Decachlorobiphenyl

R.T.: 10.979 min
Delta R.T.: -0.010 min
Response: 755724
Conc: 20.46 ng/ml

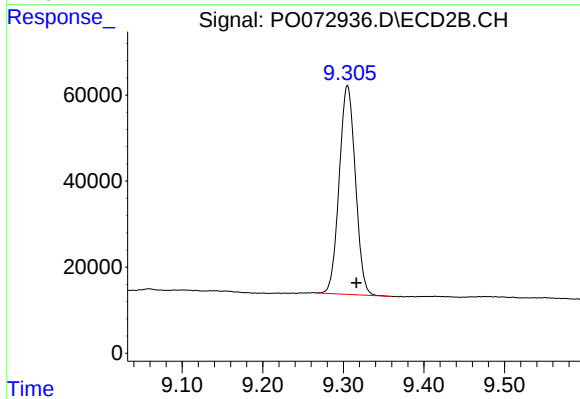

#2 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: -0.011 min
Response: 676558
Conc: 20.29 ng/ml