

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
 Data File : PO072958.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Oct 2020 3:00
 Operator : DD\AJ
 Sample : L4541-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2015

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 07:57:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.947	4.024	779799	531928	16.913	15.177
2) SA Decachlor...	10.974f	9.303	221058	185810	5.983	5.572

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
Data File : PO072958.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Oct 2020 3:00
Operator : DD\AJ
Sample : L4541-10
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2015

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:57:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

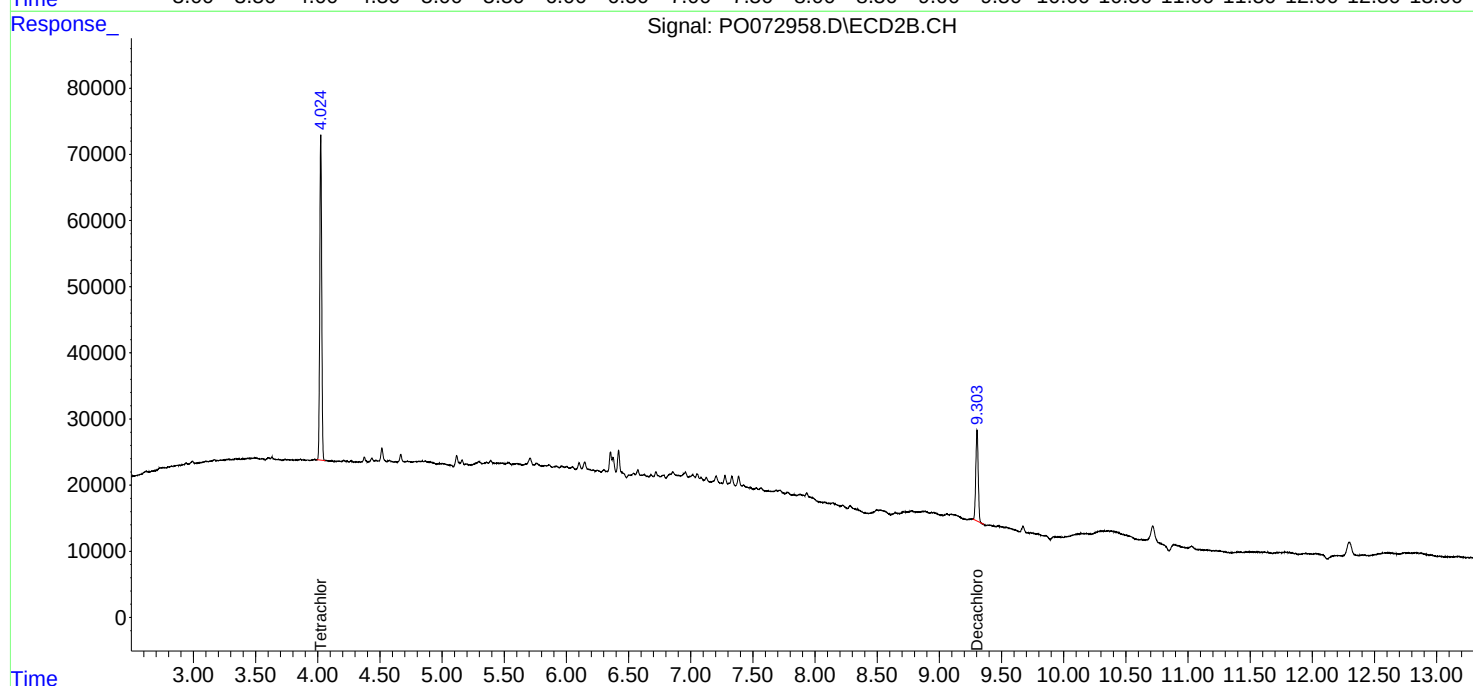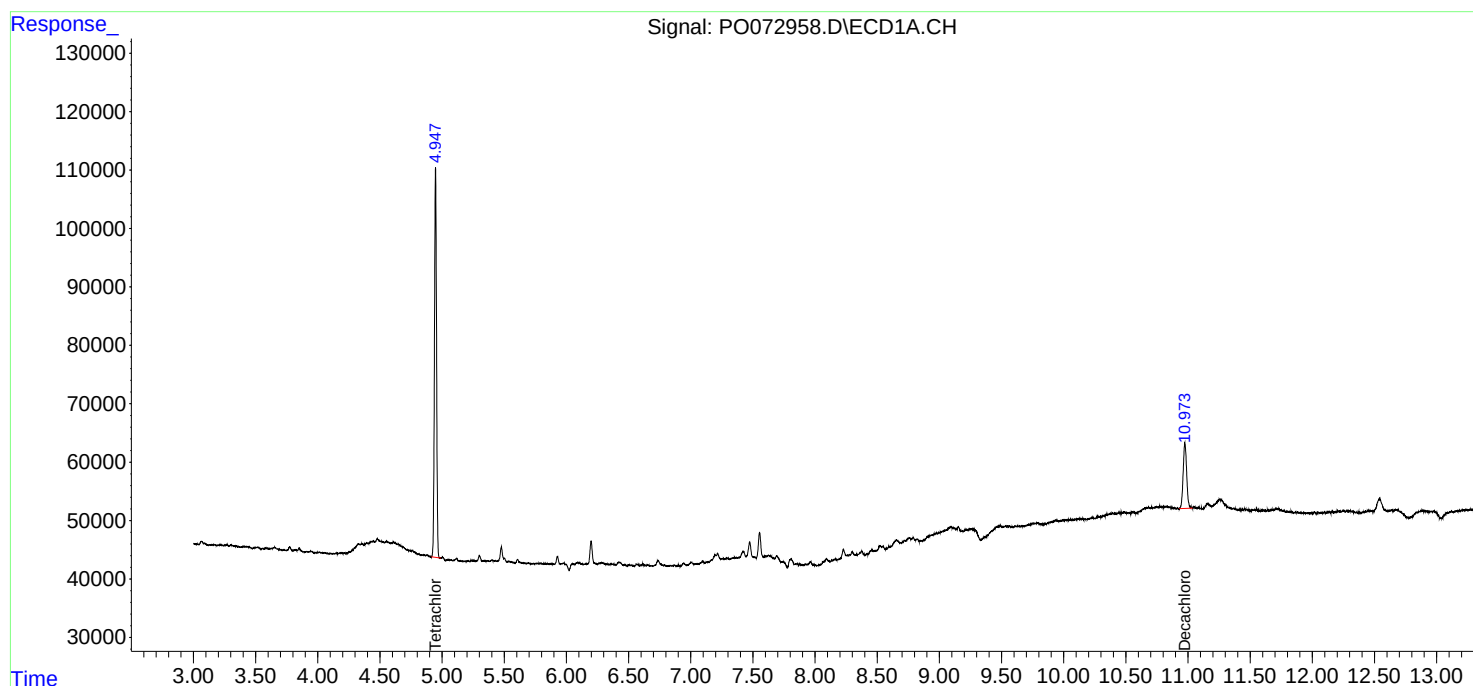


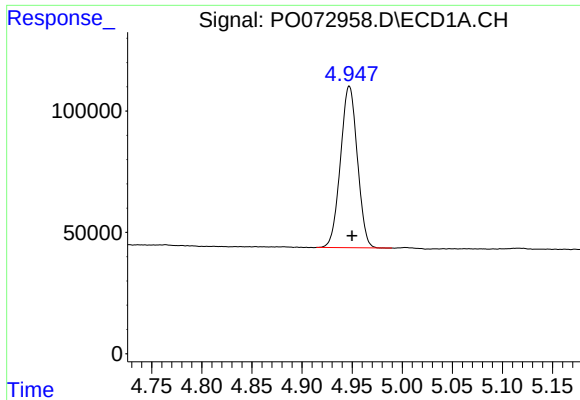

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: -0.003 min
Response: 779799
Conc: 16.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
2015

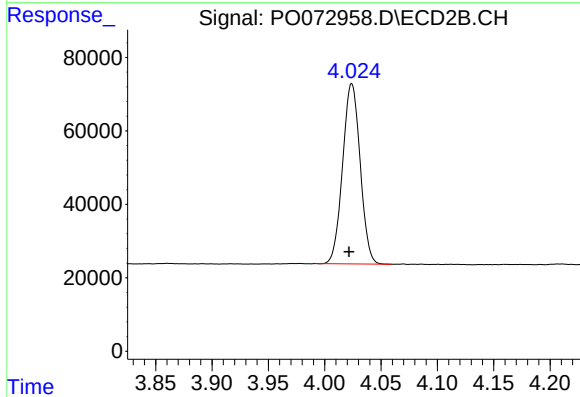


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.002 min
Response: 531928
Conc: 15.18 ng/ml

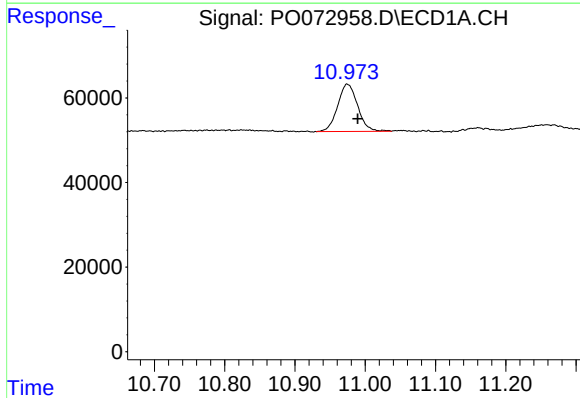

#2 Decachlorobiphenyl

R.T.: 10.974 min
Delta R.T.: -0.015 min
Response: 221058
Conc: 5.98 ng/ml

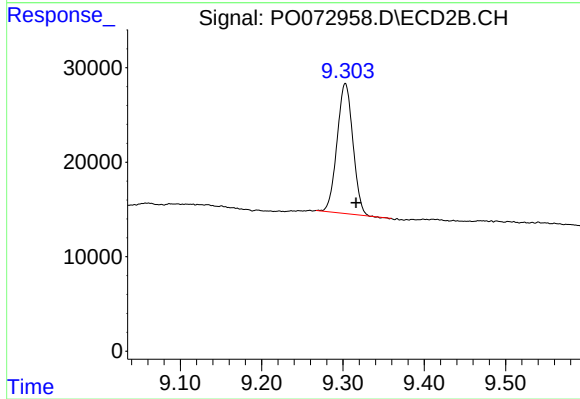

#2 Decachlorobiphenyl

R.T.: 9.303 min
Delta R.T.: -0.013 min
Response: 185810
Conc: 5.57 ng/ml