

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
 Data File : PO072959.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Oct 2020 3:17
 Operator : DD\AJ
 Sample : L4553-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 07:57:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 31 07:06:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.950	4.027	1286145	894722	27.895	25.529
2)	SA Decachlor...	10.984	9.311	888094	705595	24.038	21.158

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103120\
Data File : P0072959.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Oct 2020 3:17
Operator : DD\AJ
Sample : L4553-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 07:57:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102620.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 31 07:06:26 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

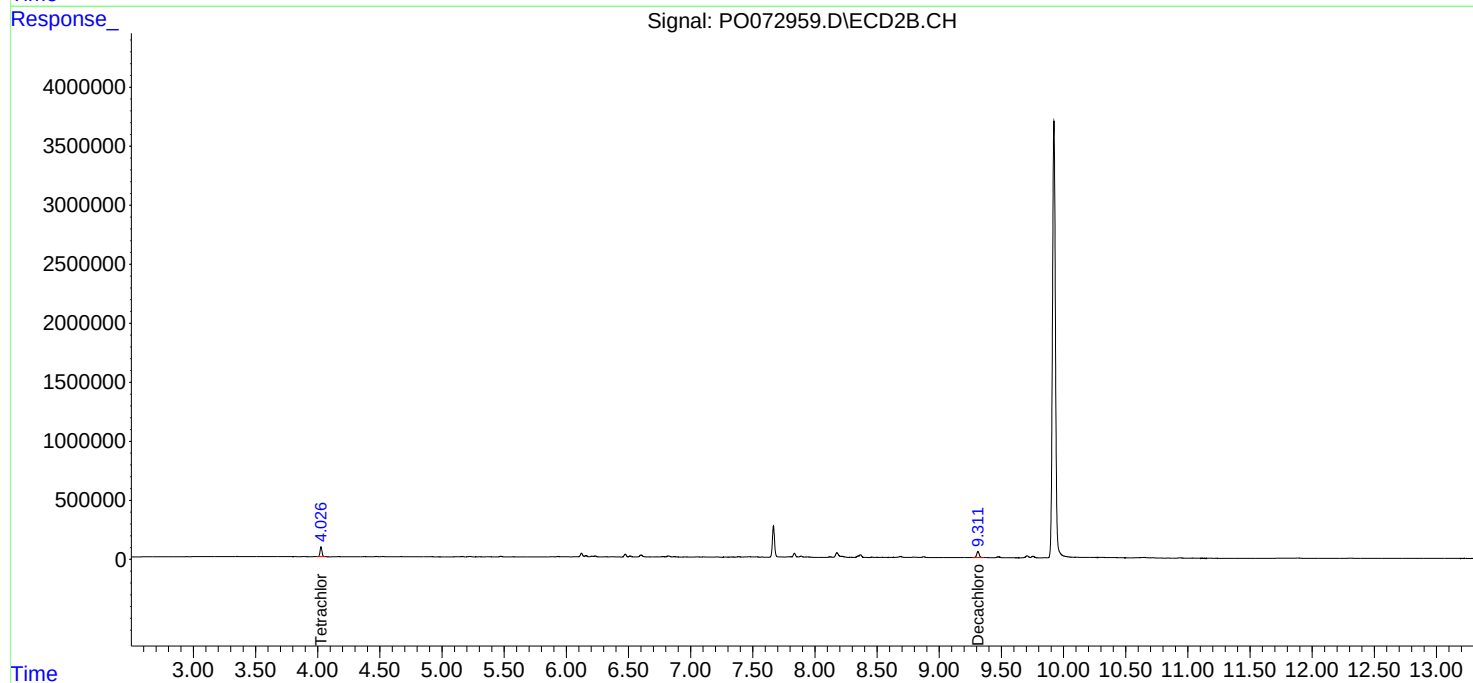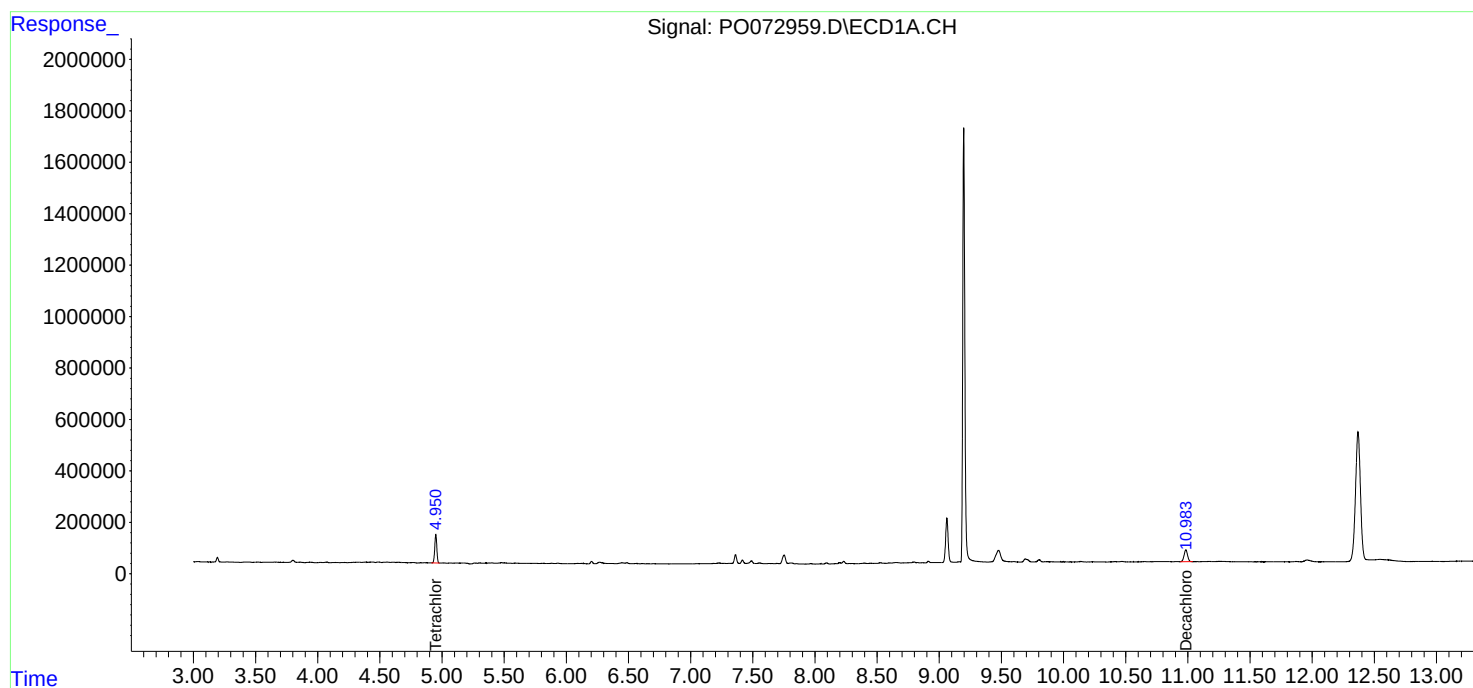


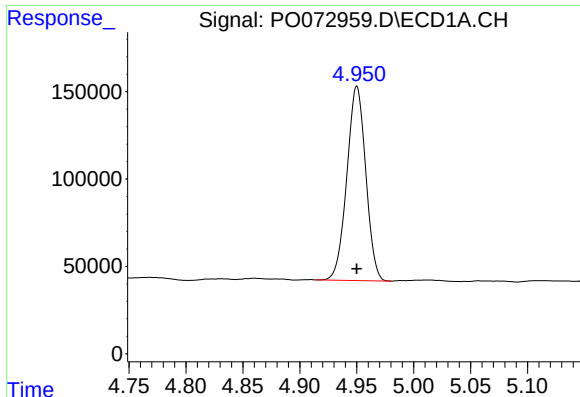

#1 Tetrachloro-m-xylene


R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 1286145
Conc: 27.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1

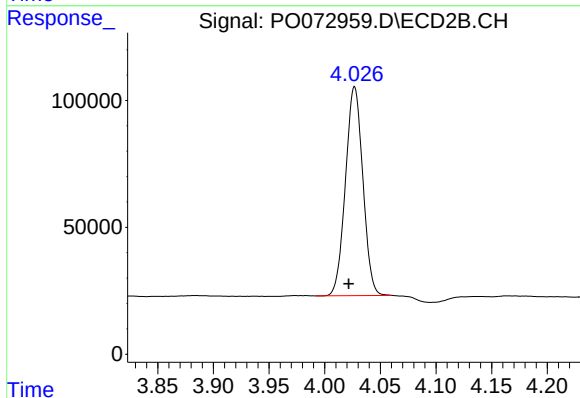


#1 Tetrachloro-m-xylene

R.T.: 4.027 min
Delta R.T.: 0.005 min
Response: 894722
Conc: 25.53 ng/ml

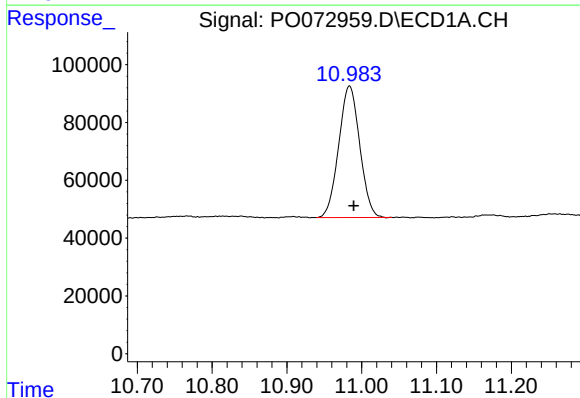

#2 Decachlorobiphenyl

R.T.: 10.984 min
Delta R.T.: -0.006 min
Response: 888094
Conc: 24.04 ng/ml

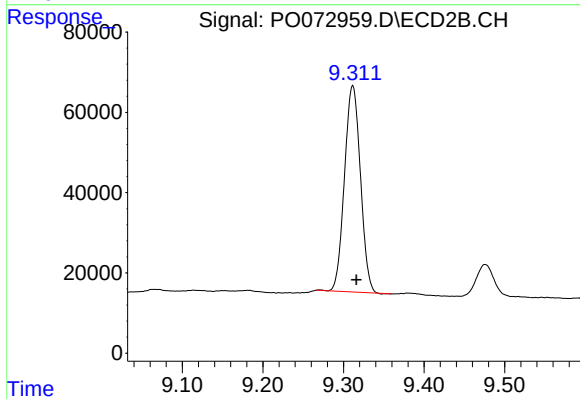

#2 Decachlorobiphenyl

R.T.: 9.311 min
Delta R.T.: -0.005 min
Response: 705595
Conc: 21.16 ng/ml