

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103123\
 Data File : P0099194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2023 13:13
 Operator : YP/AJ
 Sample : 05107-20RE
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1050RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/02/2023
 Supervised By :mohammad ahmed 11/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 11:03:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 25 06:04:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.469	3.626	29312803	4871933	14.835m	6.770 #
2) SA Decachlor...	10.268	8.622	5862699	2632485	5.175	4.906

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103123\
Data File : PO099194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2023 13:13
Operator : YP/AJ
Sample : 05107-20RE
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1050RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/02/2023
Supervised By :mohammad ahmed 11/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 11:03:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102523.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 25 06:04:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

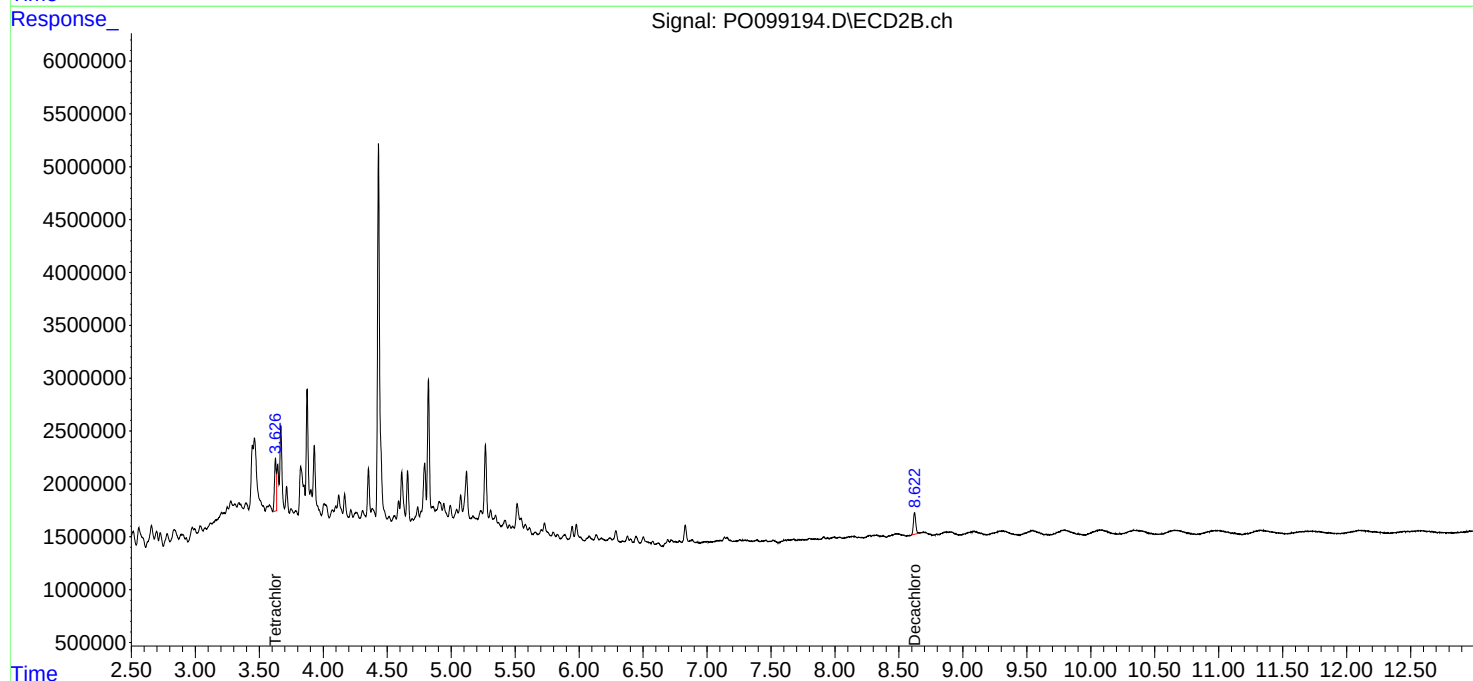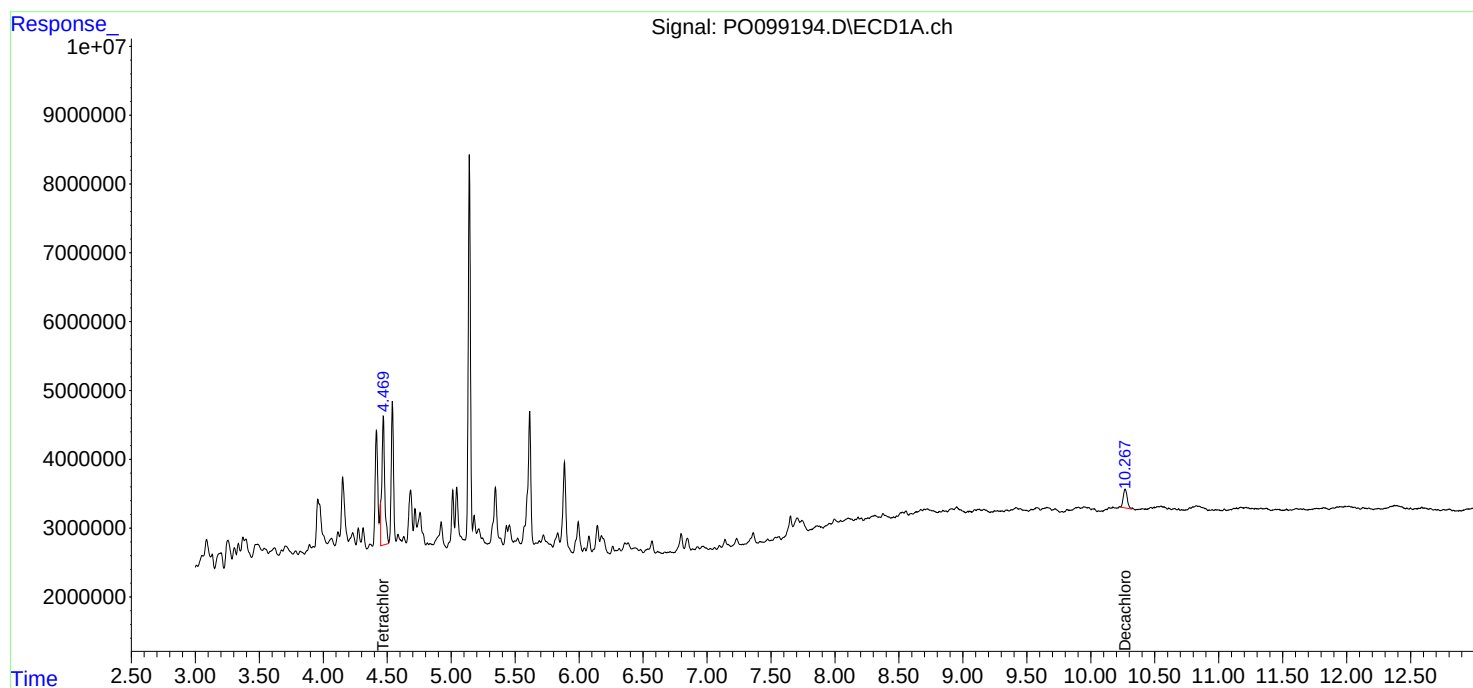

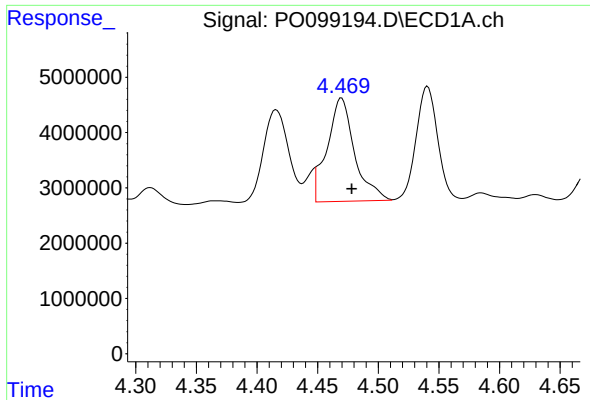


#1 Tetrachloro-m-xylene

R.T.: 4.469 min
Delta R.T.: -0.009 min
Response: 29312803
Conc: 14.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
1050RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/02/2023
Supervised By :mohammad ahmed 11/02/2023

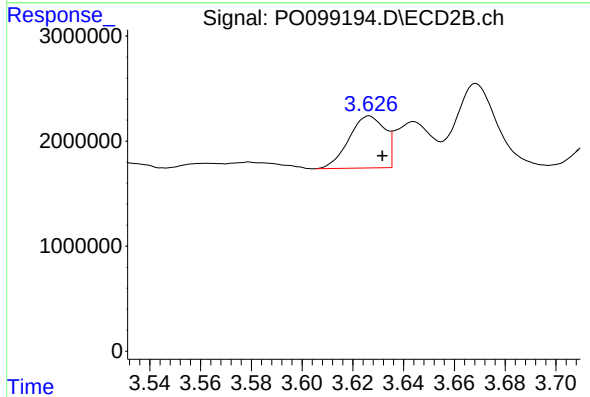


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: -0.005 min
Response: 4871933
Conc: 6.77 ng/ml

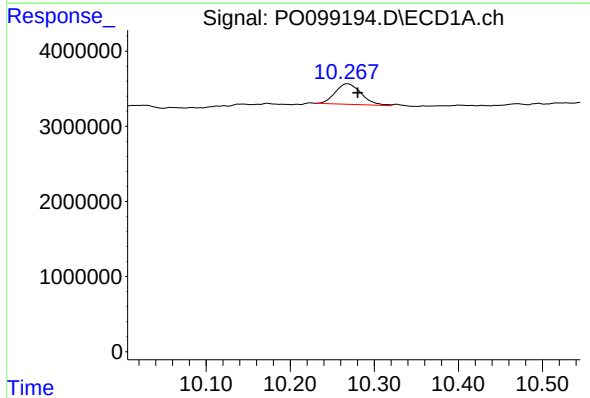

#2 Decachlorobiphenyl

R.T.: 10.268 min
Delta R.T.: -0.012 min
Response: 5862699
Conc: 5.18 ng/ml

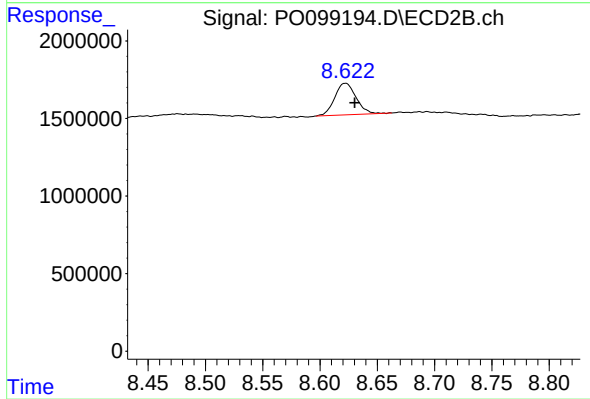

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: -0.008 min
Response: 2632485
Conc: 4.91 ng/ml