

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103125\
 Data File : P0114823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2025 18:57
 Operator : YP/AJ
 Sample : Q3505-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 10-10-25-WATER

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/03/2025
 Supervised By :Yogesh Patel 11/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 23:19:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0100925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 02:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.349	3.653	14344630	9661391	2.642m	2.414
2) SA Decachlor...	9.942	8.649	11308192	9176950	3.106	2.753

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103125\
Data File : PO114823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2025 18:57
Operator : YP/AJ
Sample : Q3505-04
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
10-10-25-WATER


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/03/2025
Supervised By :Yogesh Patel 11/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 23:19:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO100925.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 02:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

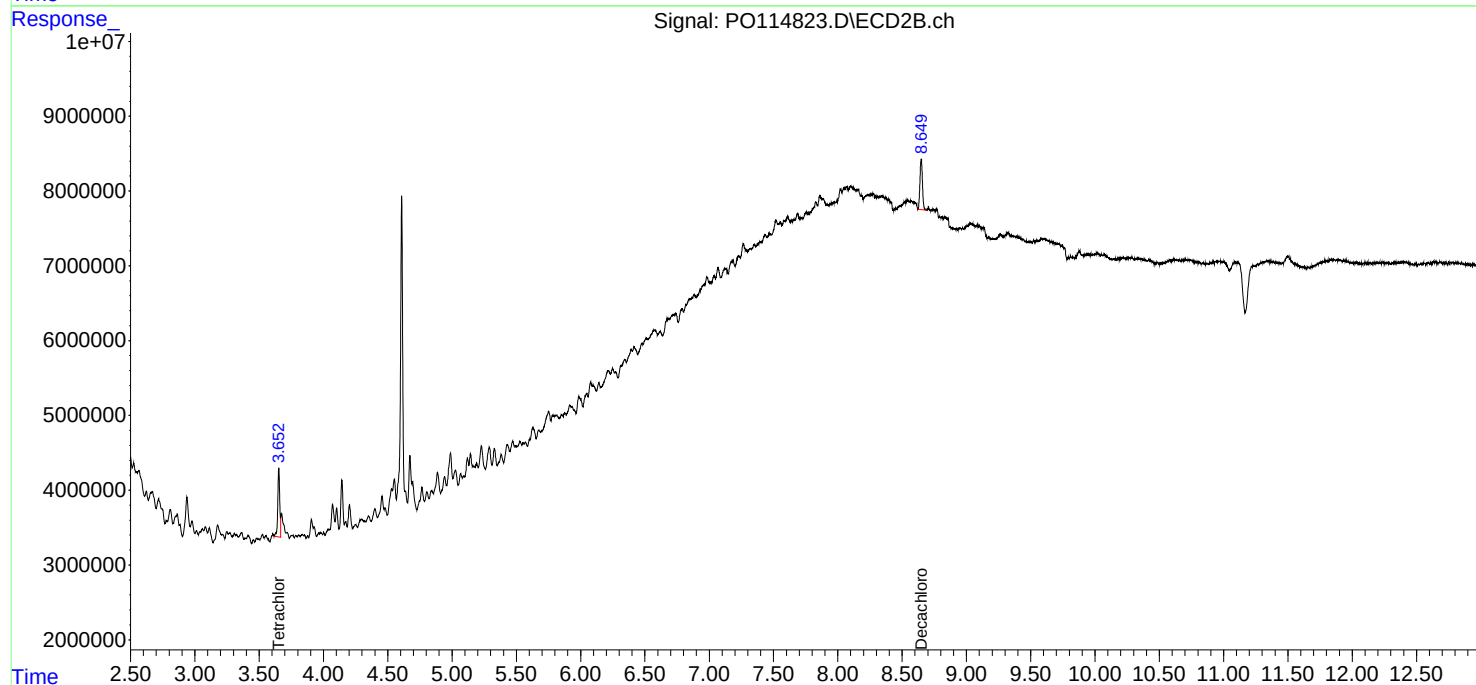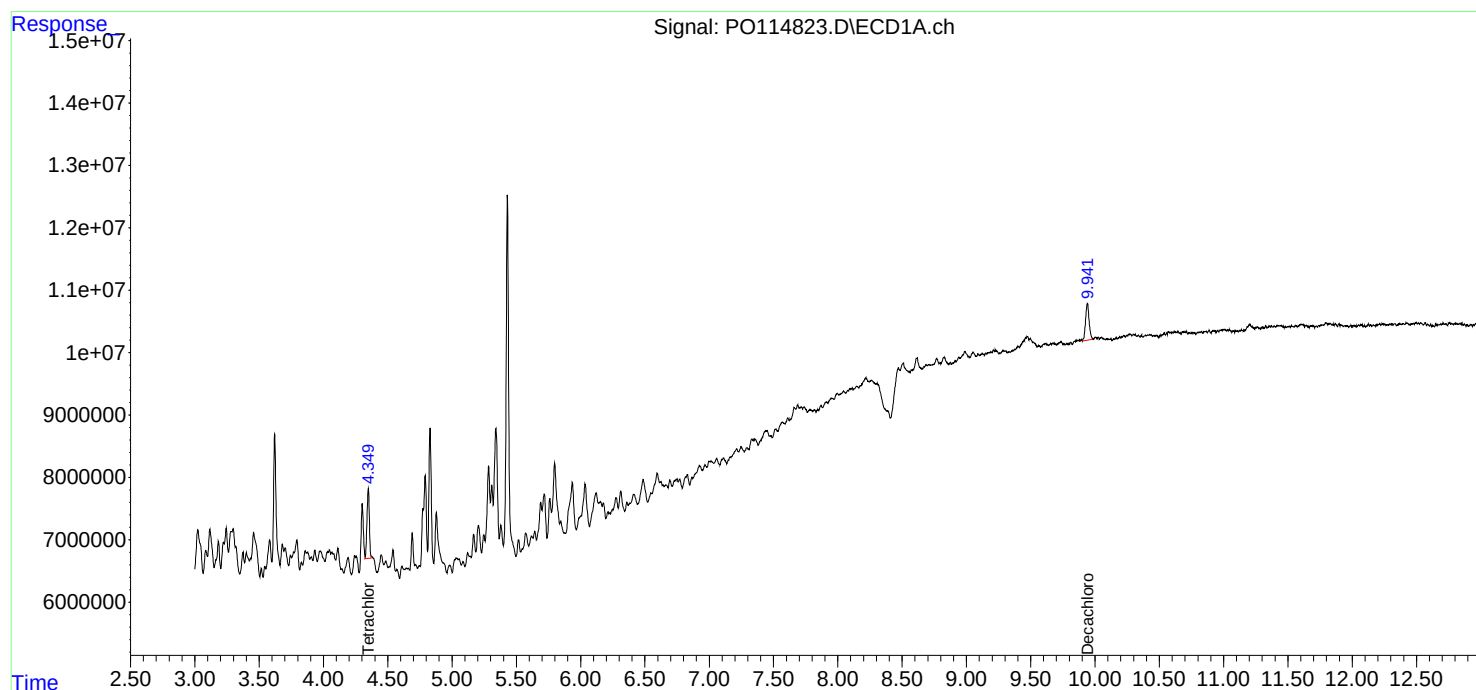

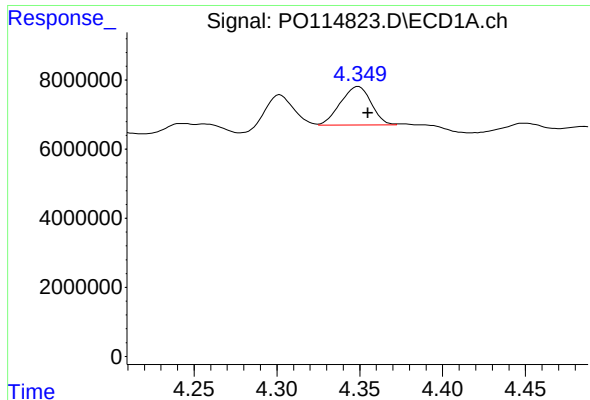


#1 Tetrachloro-m-xylene

R.T.: 4.349 min
Delta R.T.: -0.006 min
Response: 14344630
Conc: 2.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
10-10-25-WATER


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/03/2025
Supervised By :Yogesh Patel 11/03/2025

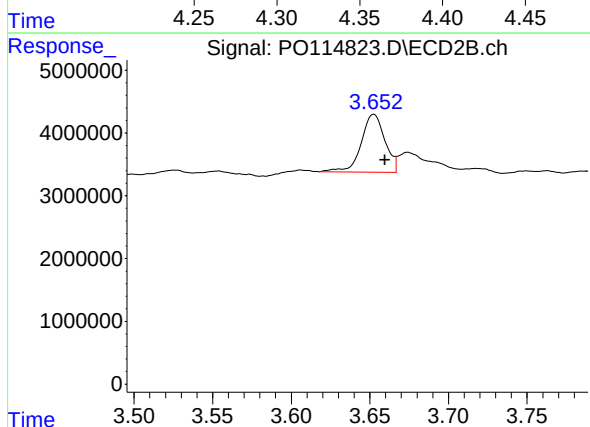


#1 Tetrachloro-m-xylene

R.T.: 3.653 min
Delta R.T.: -0.007 min
Response: 9661391
Conc: 2.41 ng/ml

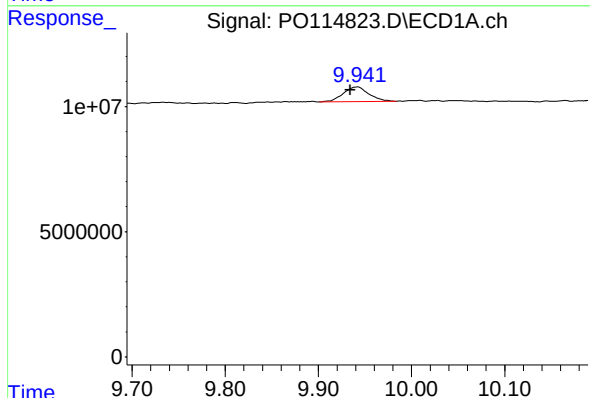

#2 Decachlorobiphenyl

R.T.: 9.942 min
Delta R.T.: 0.008 min
Response: 11308192
Conc: 3.11 ng/ml

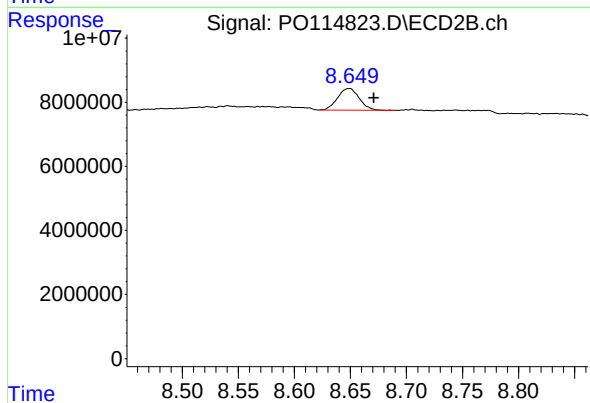

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.022 min
Response: 9176950
Conc: 2.75 ng/ml