

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
 Data File : PO050872.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 12:12
 Operator : SM/SJ
 Sample : J5741-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 14:27:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.357	3.348	13408257	5764612	26.824	26.522
2)	SA Decachlor...	10.015	8.094	5485929	4051877	17.650	15.841
Target Compounds							
9)	L2 AR-1221-2	0.000	3.628	0	74002	N.D.	58.148 #
14)	L3 AR-1232-4	0.000	4.683	0	74952	N.D.	33.622 #
19)	L4 AR-1242-4	0.000	4.683	0	74952	N.D.	15.690 #
23)	L5 AR-1248-3	0.000	4.683	0	74952	N.D.	10.722 #
30)	L6 AR-1254-5	0.000	6.267	0	23288	N.D.	0.871 #
36)	L8 AR-1262-1	0.000	6.267	0	23288	N.D.	0.828 #
38)	L8 AR-1262-3	0.000	7.004	0	53847	N.D.	2.999 #
41)	L9 AR-1268-1	0.000	7.004	0	53847	N.D.	0.978 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
Data File : PO050872.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 12:12
Operator : SM/SJ
Sample : J5741-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 14:27:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

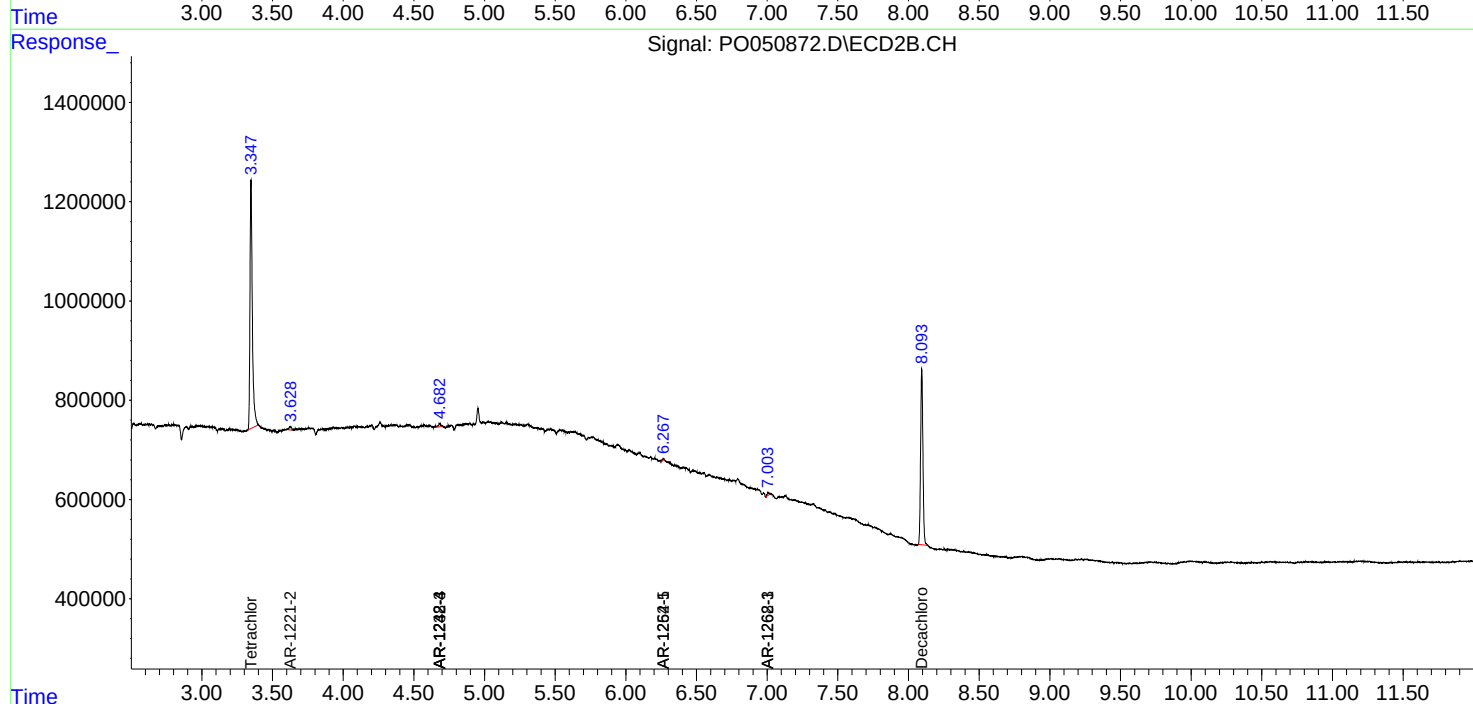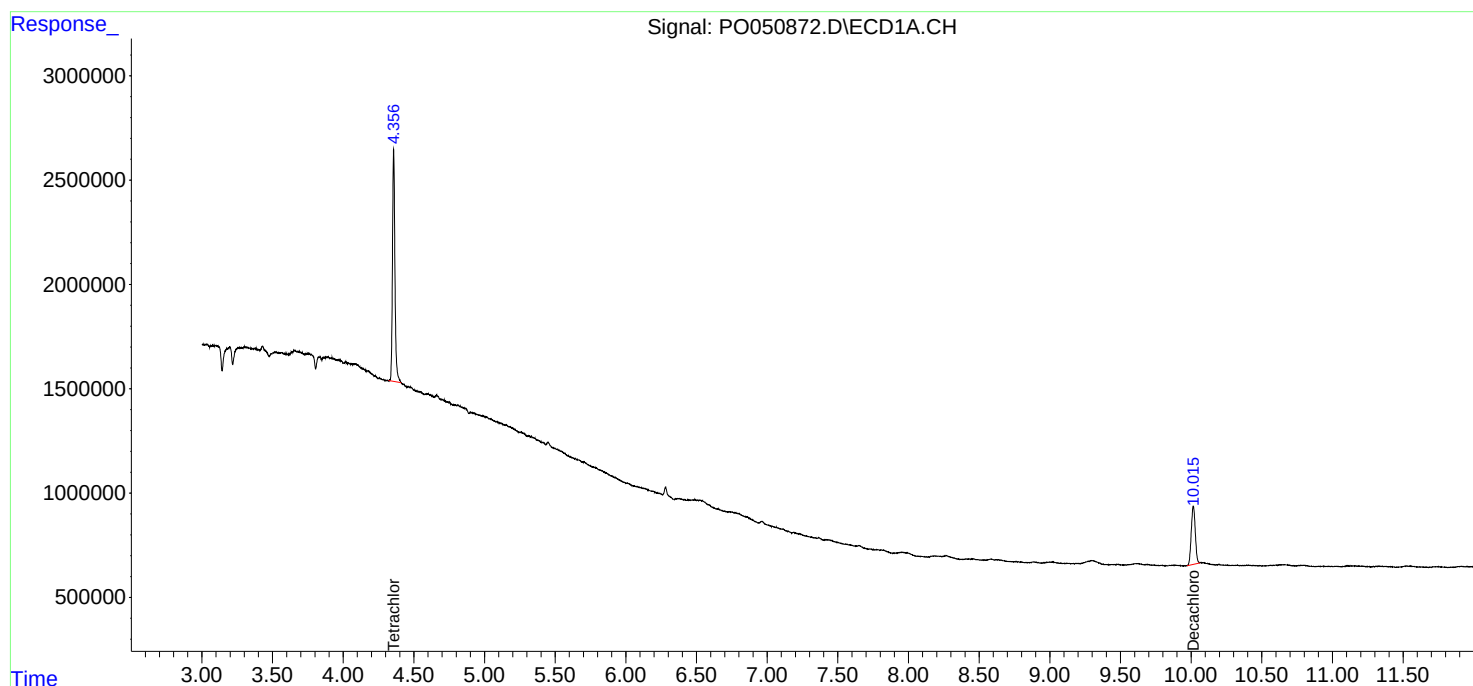


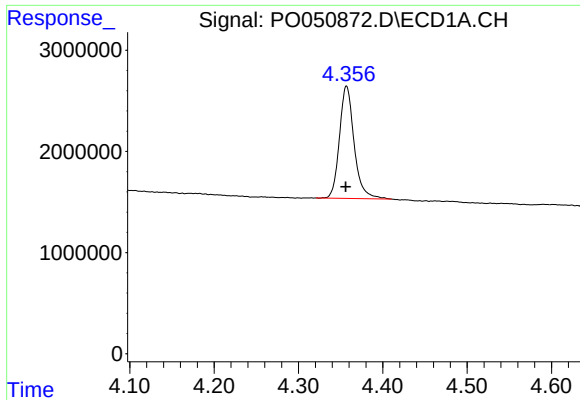

#1 Tetrachloro-m-xylene


R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 13408257
Conc: 26.82 ng/ml

Instrument :
ECD_O
ClientSampleId :

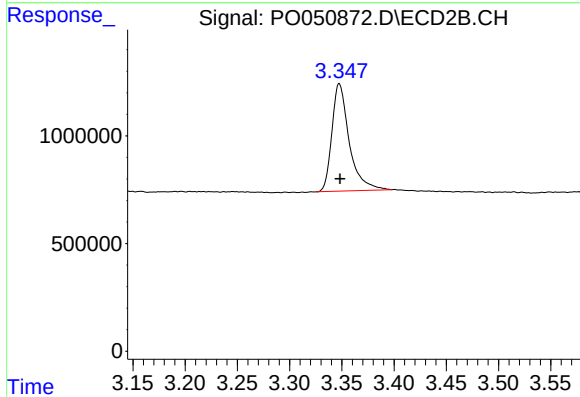


#1 Tetrachloro-m-xylene

R.T.: 3.348 min
Delta R.T.: 0.000 min
Response: 5764612
Conc: 26.52 ng/ml

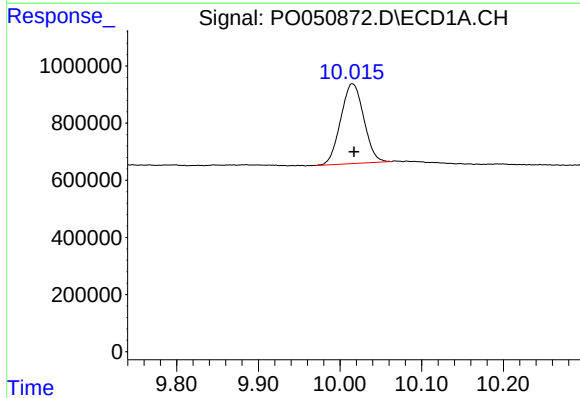


#2 Decachlorobiphenyl

R.T.: 10.015 min
Delta R.T.: -0.002 min
Response: 5485929
Conc: 17.65 ng/ml

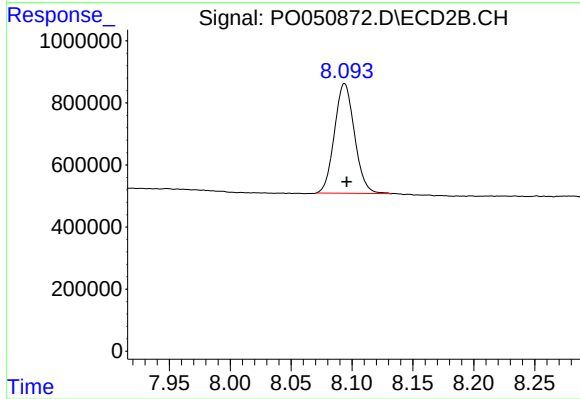

#2 Decachlorobiphenyl


R.T.: 8.094 min
Delta R.T.: -0.002 min
Response: 4051877
Conc: 15.84 ng/ml

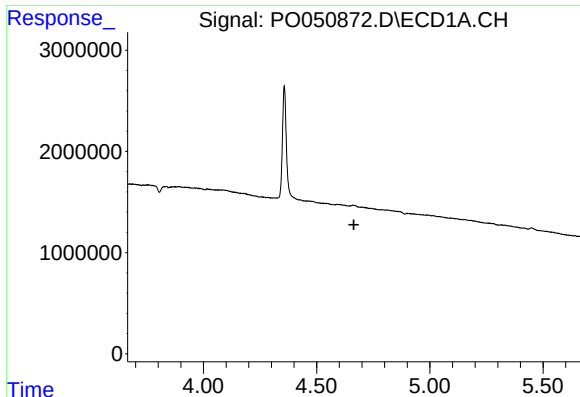

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.664 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

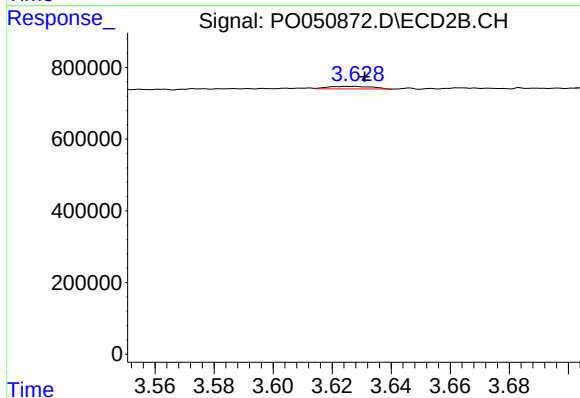


#9 AR-1221-2

R.T.: 3.628 min
Delta R.T.: -0.003 min
Response: 74002
Conc: 58.15 ng/ml

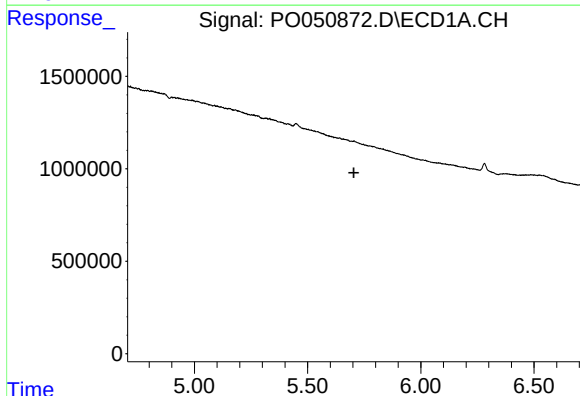


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.705 min
Response: 0
Conc: N.D.

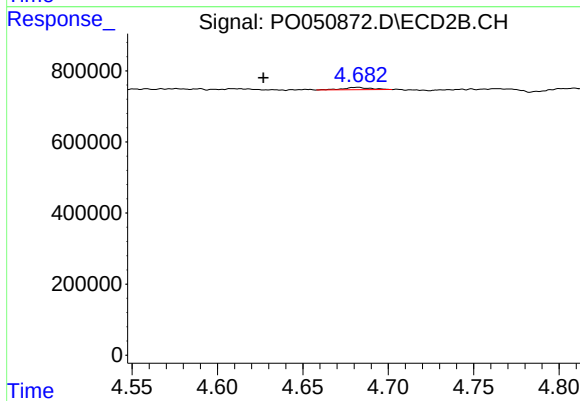

#14 AR-1232-4


R.T.: 4.683 min
Delta R.T.: 0.056 min
Response: 74952
Conc: 33.62 ng/ml

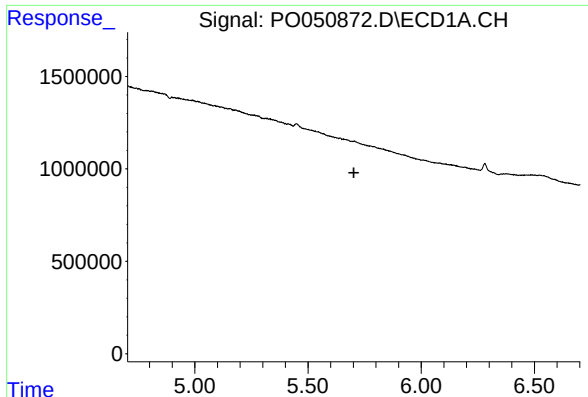

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T. : 5.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

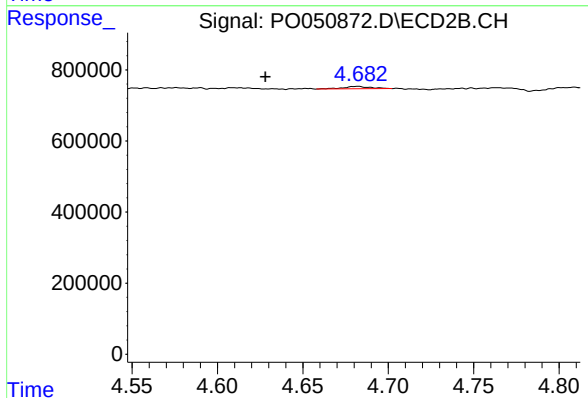


#19 AR-1242-4

R.T.: 4.683 min
Delta R.T.: 0.055 min
Response: 74952
Conc: 15.69 ng/ml

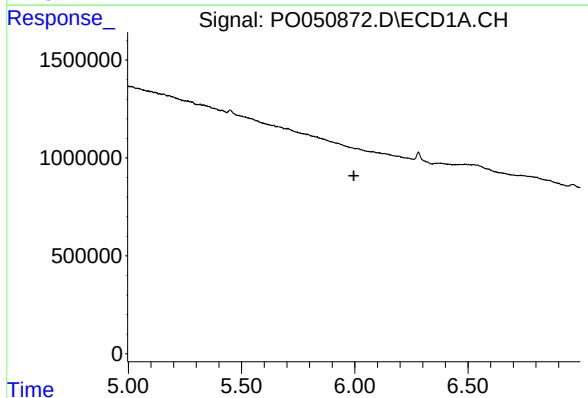


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

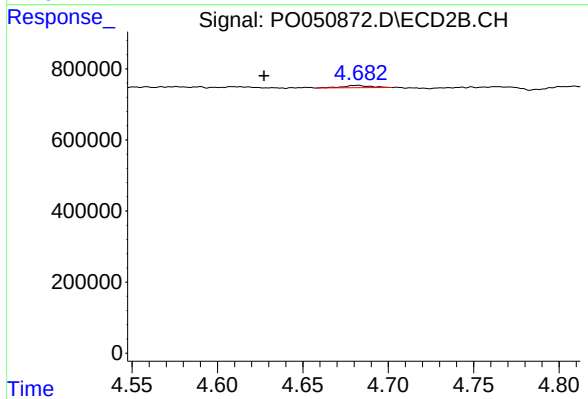

#23 AR-1248-3


R.T.: 4.683 min
Delta R.T.: 0.055 min
Response: 74952
Conc: 10.72 ng/ml

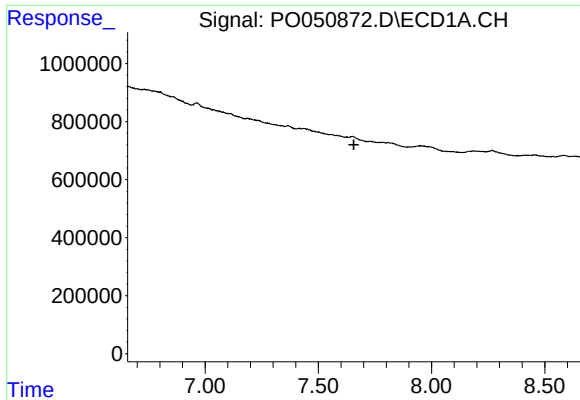

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.657 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

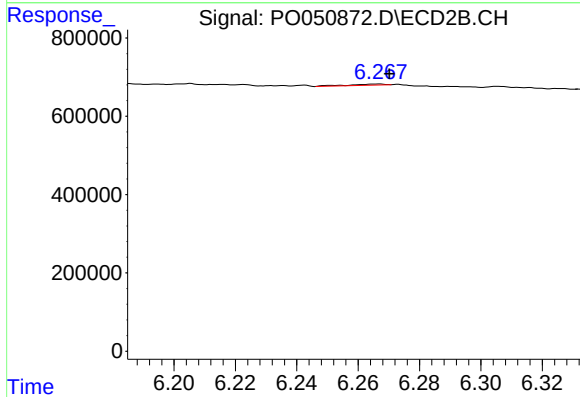


#30 AR-1254-5

R.T.: 6.267 min
Delta R.T.: -0.003 min
Response: 23288
Conc: 0.87 ng/ml

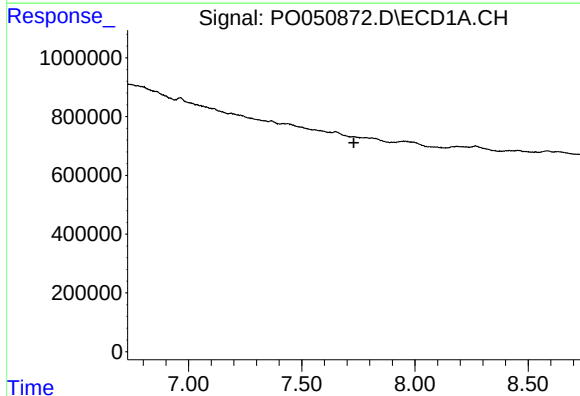


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 7.730 min
Response: 0
Conc: N.D.

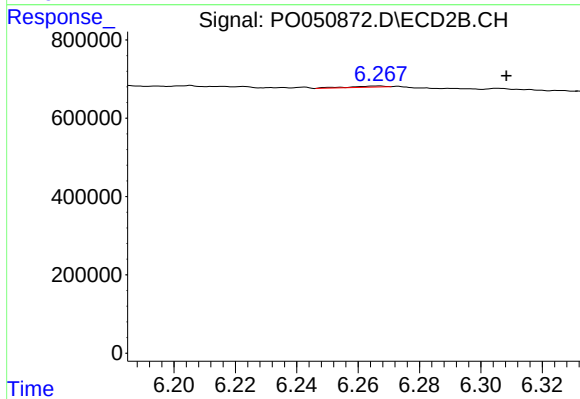

#36 AR-1262-1


R.T.: 6.267 min
Delta R.T.: -0.041 min
Response: 23288
Conc: 0.83 ng/ml

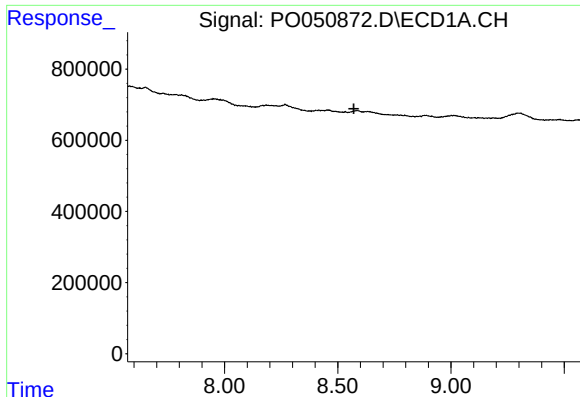

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

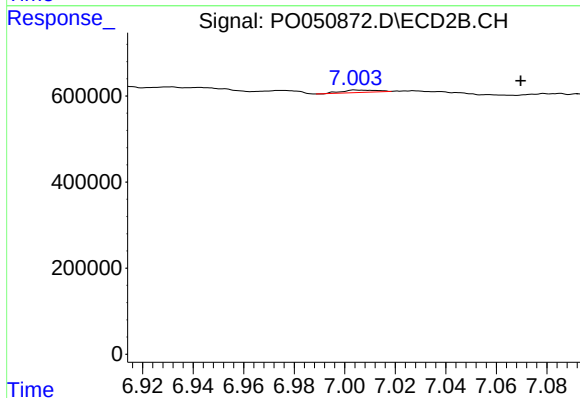


#38 AR-1262-3

R.T.: 7.004 min
Delta R.T.: -0.066 min
Response: 53847
Conc: 3.00 ng/ml

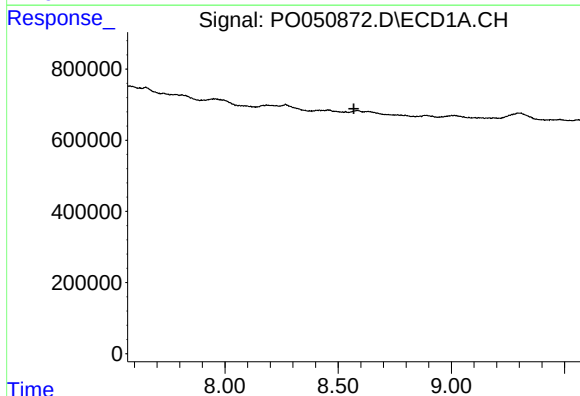

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.570 min
Response: 0
Conc: N.D.

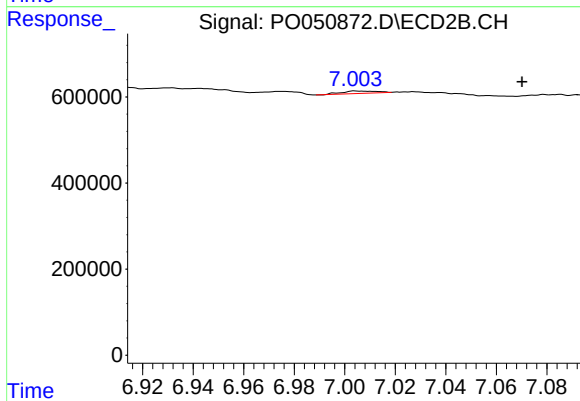

#41 AR-1268-1

R.T.: 7.004 min
Delta R.T.: -0.066 min
Response: 53847
Conc: 0.98 ng/ml