

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
 Data File : PO050903.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 22:47
 Operator : SM/SJ
 Sample : J5741-23
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:00:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.353	3.346	9015311	3916801	18.036	18.020
2)	SA Decachlor...	10.010	8.091	5192380	4356433	16.705	17.032
Target Compounds							
9)	L2 AR-1221-2	0.000	3.626	0	57160	N.D.	44.915 #
29)	L6 AR-1254-4	0.000	5.938	0	33132	N.D.	1.874 #
32)	L7 AR-1260-2	0.000	5.938	0	33132	N.D.	1.154 #
38)	L8 AR-1262-3	0.000	7.097	0	7179	N.D.	0.400 #
39)	L8 AR-1262-4	0.000	7.097	0	7179	N.D.	0.244 #
41)	L9 AR-1268-1	0.000	7.097	0	7179	N.D.	0.130 #
42)	L9 AR-1268-2	0.000	7.097	0	7179	N.D.	0.151 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
Data File : PO050903.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 22:47
Operator : SM/SJ
Sample : J5741-23
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:00:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

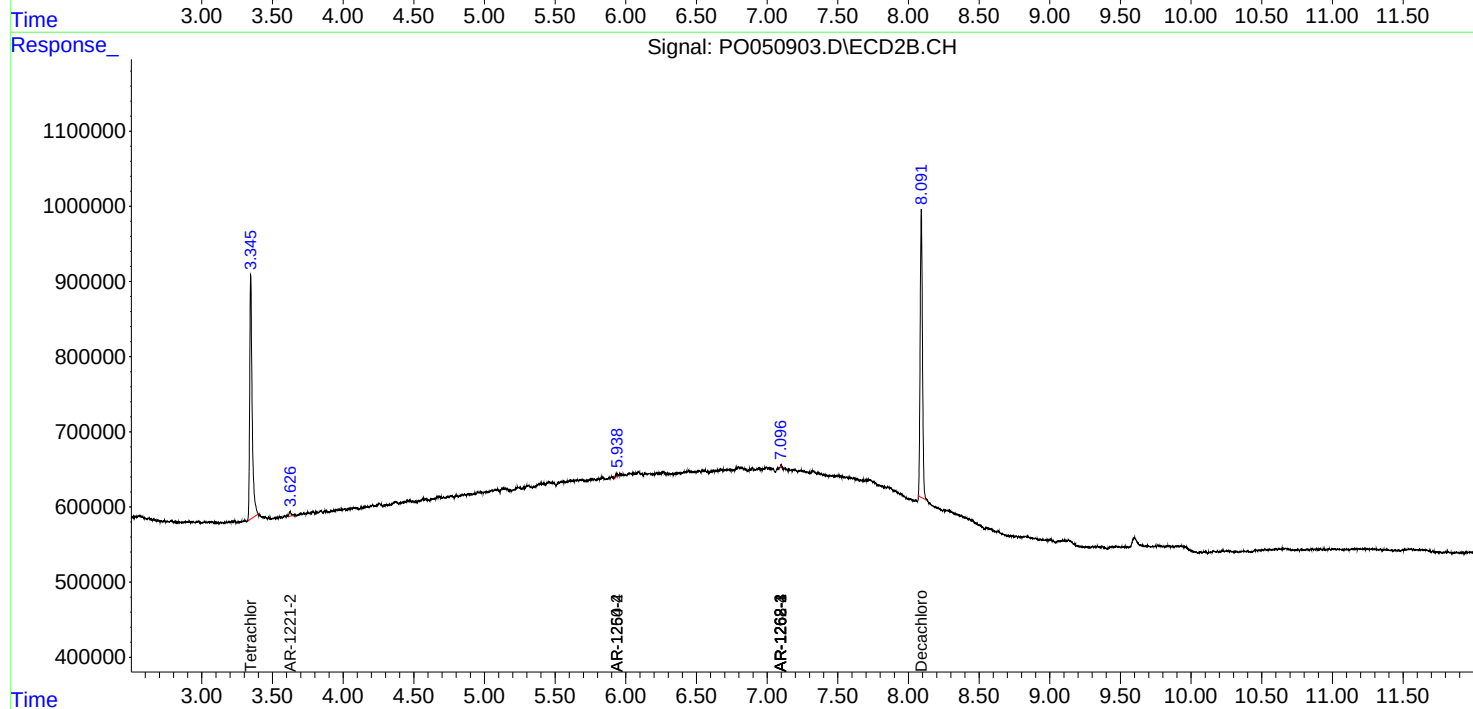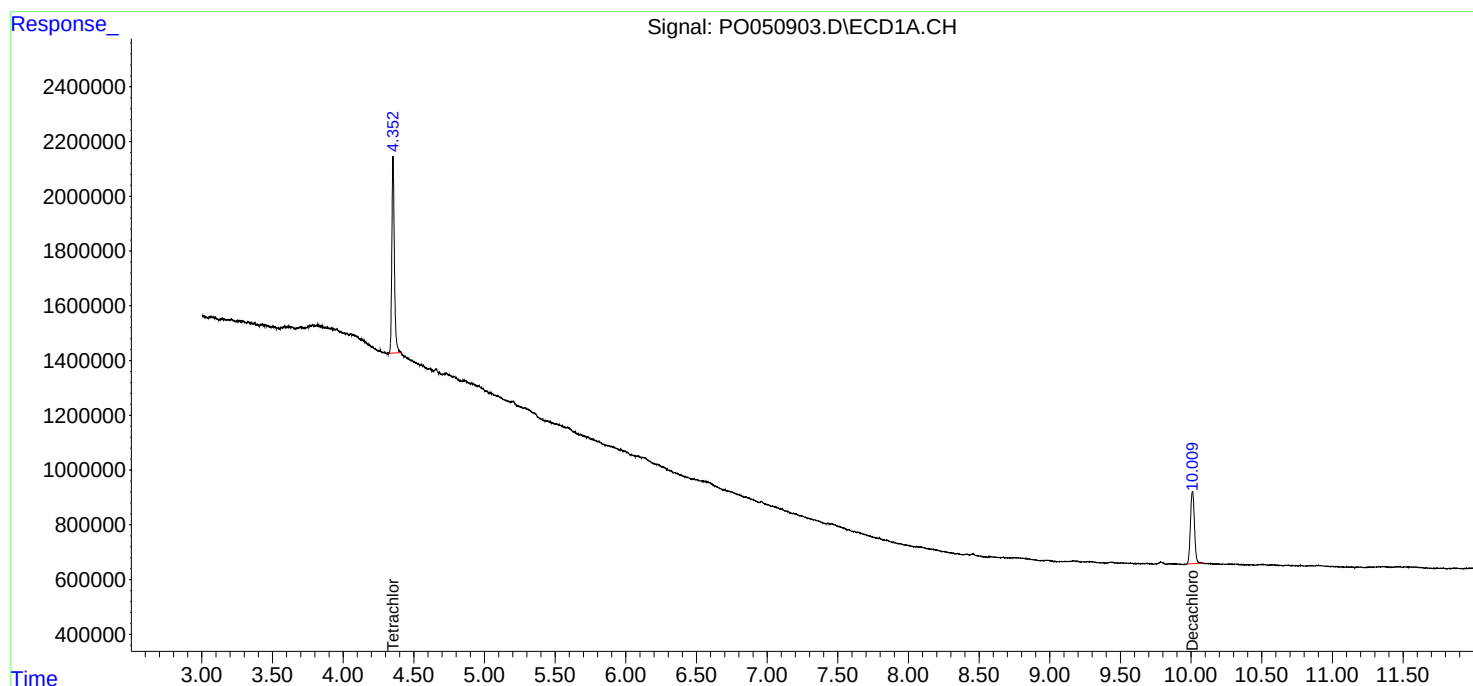


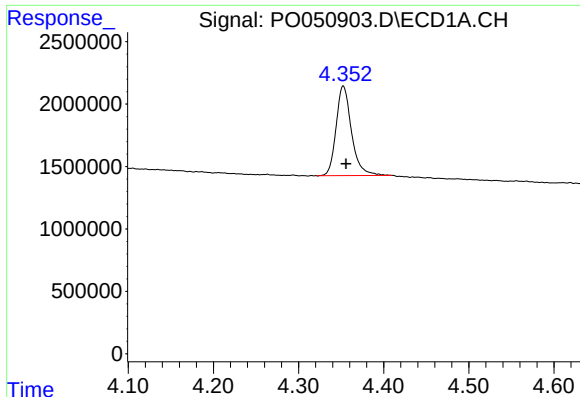

#1 Tetrachloro-m-xylene


R.T.: 4.353 min
Delta R.T.: -0.003 min
Response: 9015311
Conc: 18.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-6

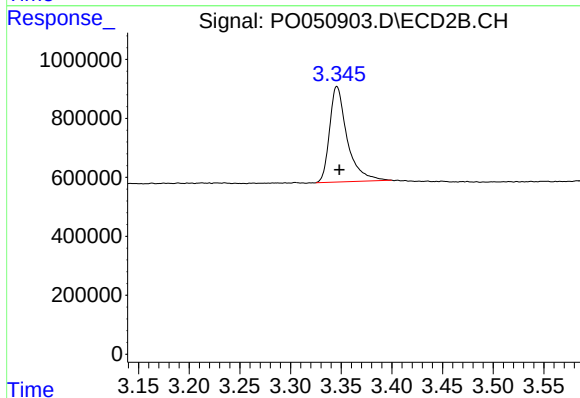


#1 Tetrachloro-m-xylene

R.T.: 3.346 min
Delta R.T.: -0.003 min
Response: 3916801
Conc: 18.02 ng/ml

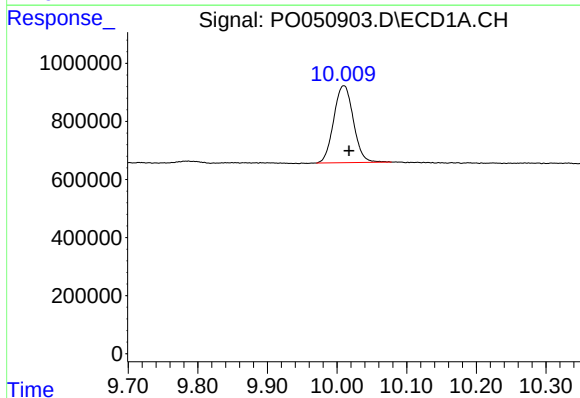


#2 Decachlorobiphenyl

R.T.: 10.010 min
Delta R.T.: -0.008 min
Response: 5192380
Conc: 16.71 ng/ml

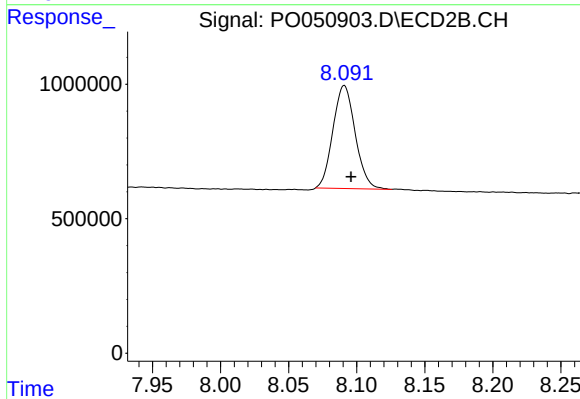

#2 Decachlorobiphenyl


R.T.: 8.091 min
Delta R.T.: -0.005 min
Response: 4356433
Conc: 17.03 ng/ml

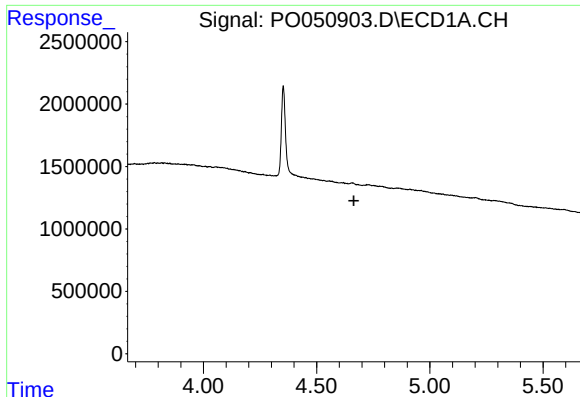

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.664 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-6

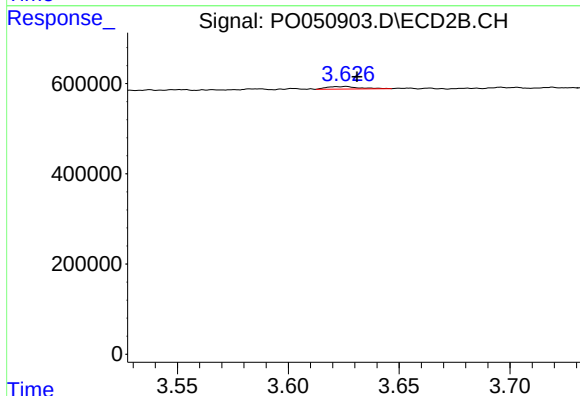


#9 AR-1221-2

R.T.: 3.626 min
Delta R.T.: -0.005 min
Response: 57160
Conc: 44.91 ng/ml

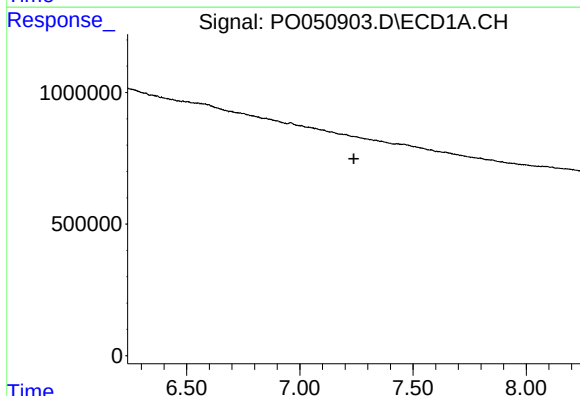


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T.: 7.239 min
Response: 0
Conc: N.D.

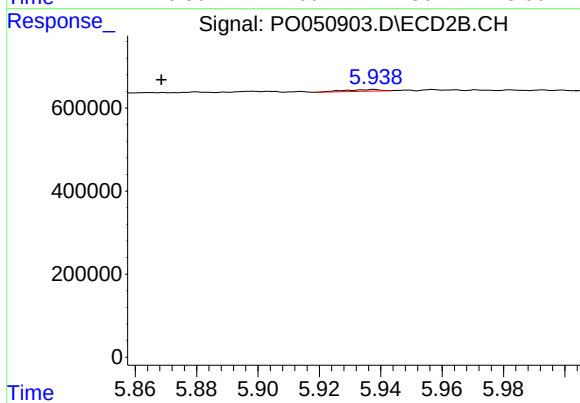

#29 AR-1254-4


R.T.: 5.938 min
Delta R.T.: 0.069 min
Response: 33132
Conc: 1.87 ng/ml

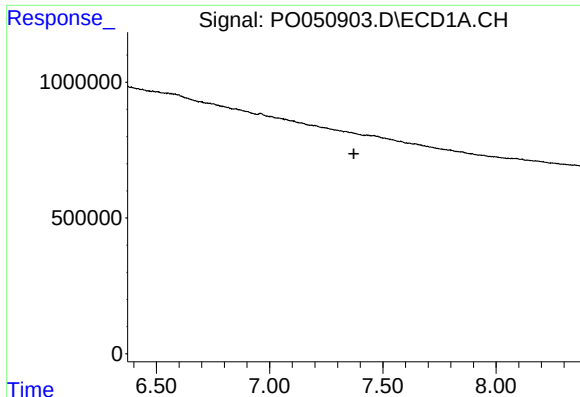

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-6

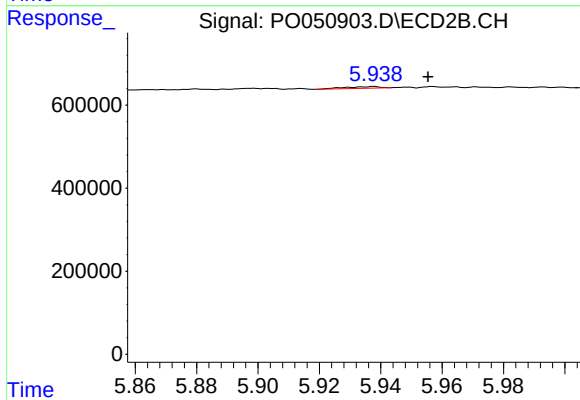


#32 AR-1260-2

R.T.: 5.938 min
Delta R.T.: -0.018 min
Response: 33132
Conc: 1.15 ng/ml

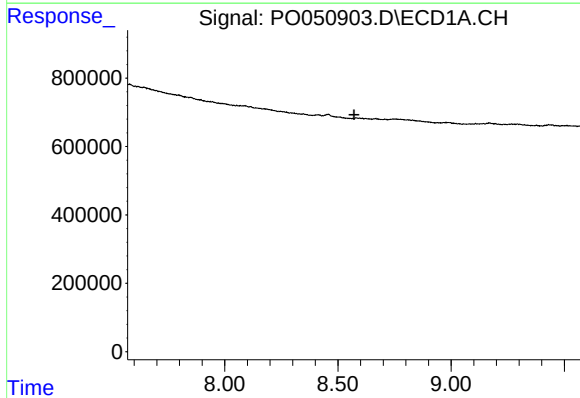


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.571 min
Response: 0
Conc: N.D.

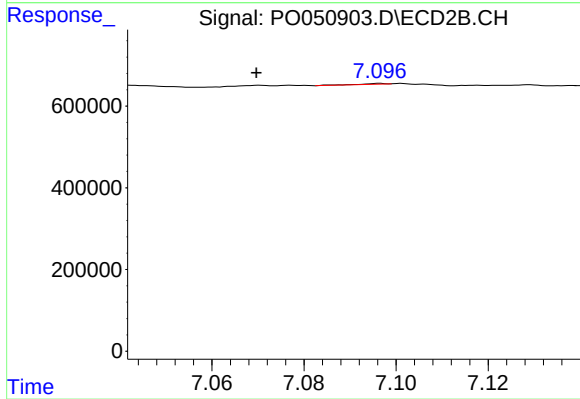

#38 AR-1262-3


R.T.: 7.097 min
Delta R.T.: 0.027 min
Response: 7179
Conc: 0.40 ng/ml

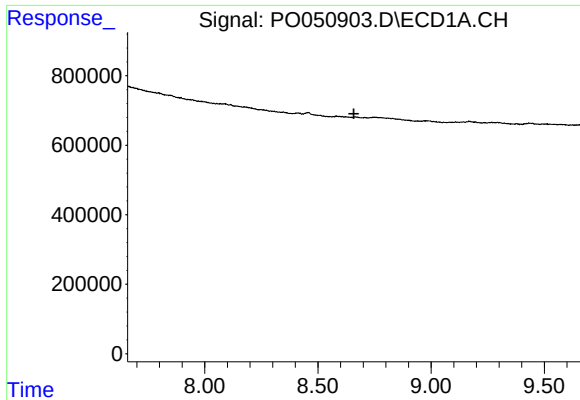

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.658 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-6

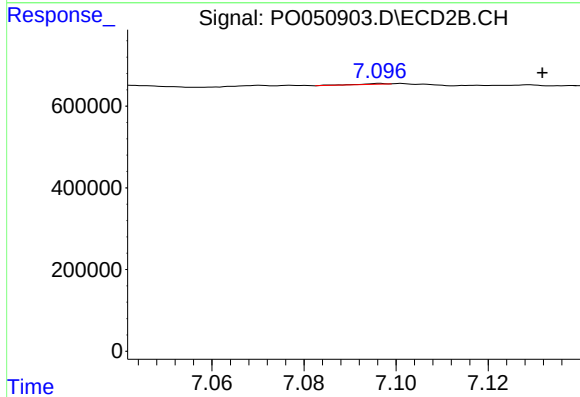


#39 AR-1262-4

R.T.: 7.097 min
Delta R.T.: -0.035 min
Response: 7179
Conc: 0.24 ng/ml

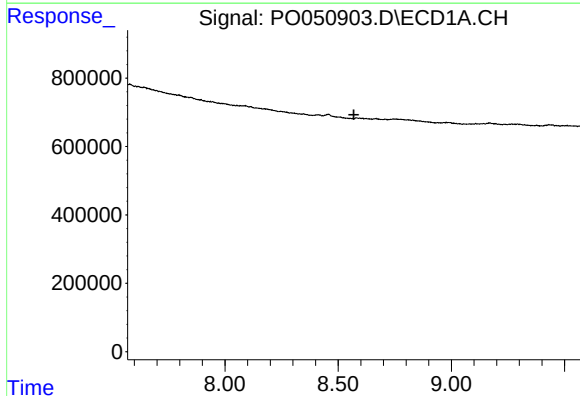


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.570 min
Response: 0
Conc: N.D.

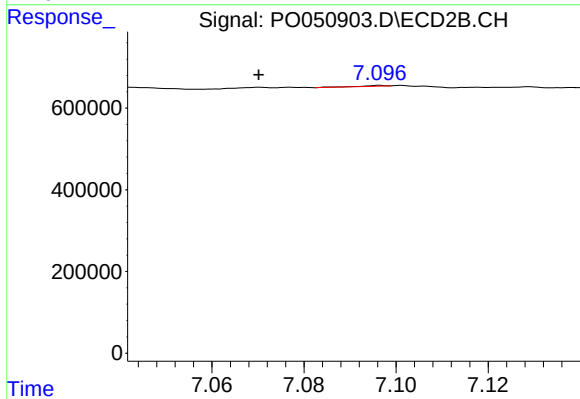

#41 AR-1268-1


R.T.: 7.097 min
Delta R.T.: 0.026 min
Response: 7179
Conc: 0.13 ng/ml

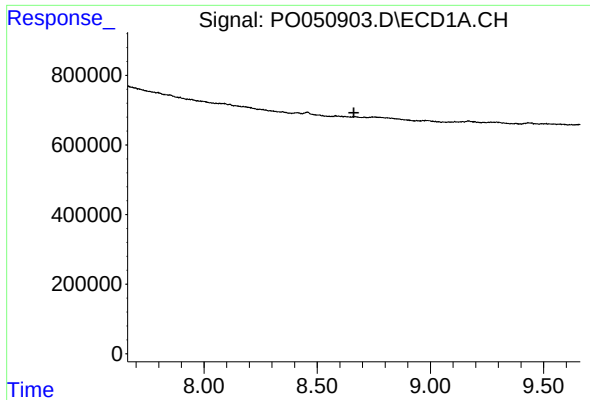

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.662 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-6

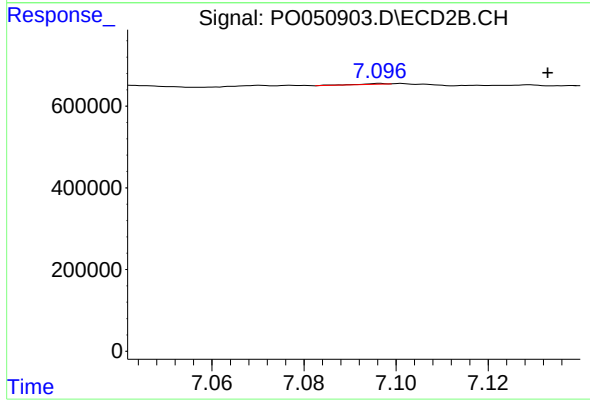

#42 AR-1268-2

R.T.: 7.097 min
Delta R.T.: -0.036 min
Response: 7179
Conc: 0.15 ng/ml