

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
 Data File : PO050907.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 23:55
 Operator : SM/SJ
 Sample : J5741-35
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:01:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.352	3.346	8675220	3677683	17.355	16.920
2)	SA Decachlor...	10.009	8.091	4890874	4040410	15.735	15.796
Target Compounds							
7)	L1 AR-1016-5	0.000	4.763	0	14703	N.D.	1.704 #
15)	L3 AR-1232-5	0.000	4.763	0	14703	N.D.	5.528 #
24)	L5 AR-1248-4	0.000	4.763	0	14703	N.D.	1.576 #
38)	L8 AR-1262-3	0.000	7.074	0	65017	N.D.	3.621 #
39)	L8 AR-1262-4	0.000	7.123	0	7584	N.D.	0.258 #
41)	L9 AR-1268-1	0.000	7.074	0	65017	N.D.	1.180 #
42)	L9 AR-1268-2	0.000	7.123	0	7584	N.D.	0.159 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
Data File : PO050907.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 23:55
Operator : SM/SJ
Sample : J5741-35
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:01:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

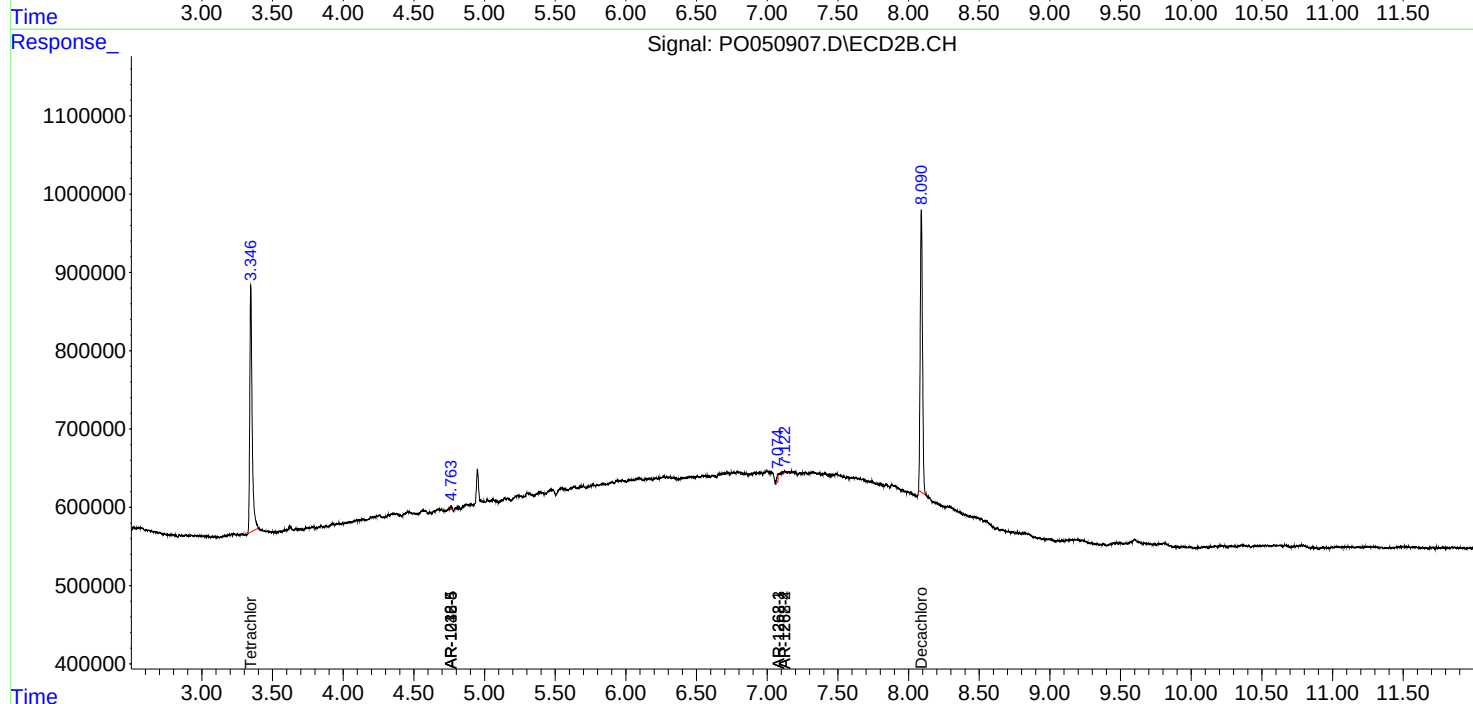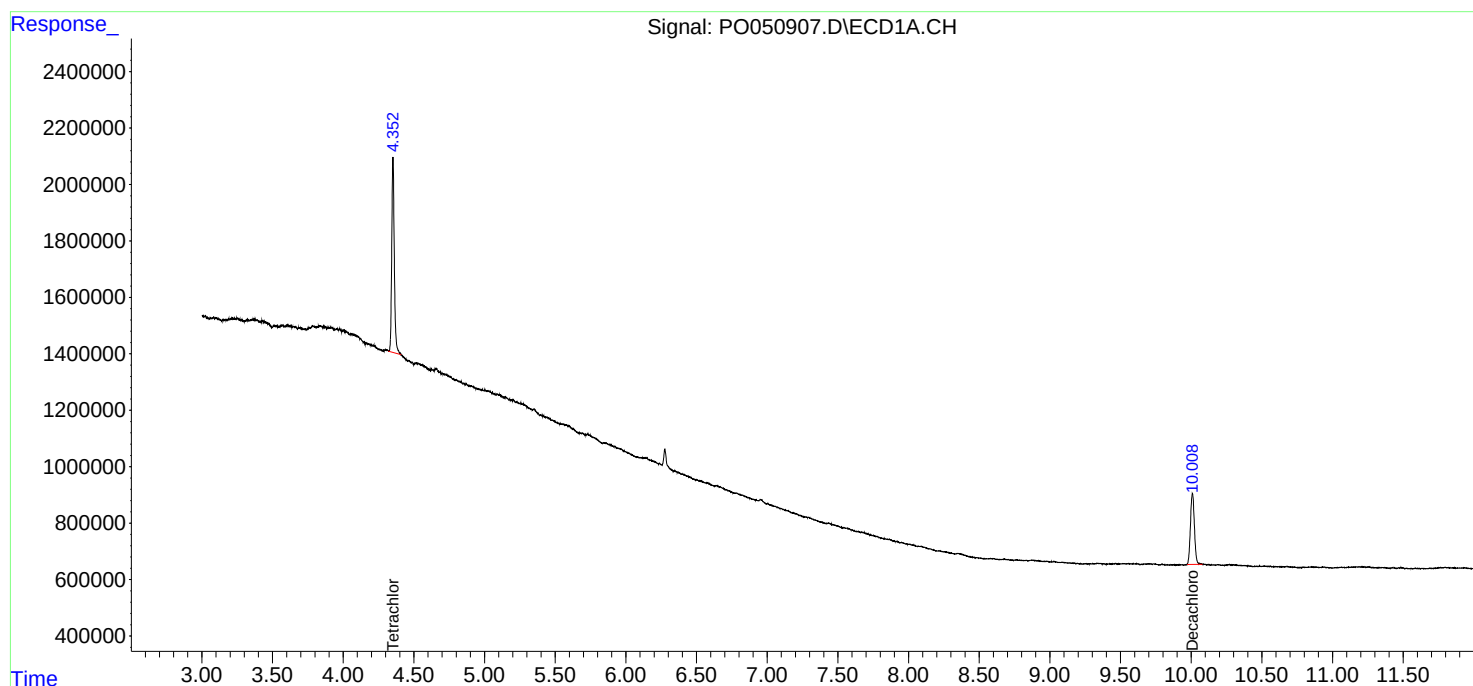


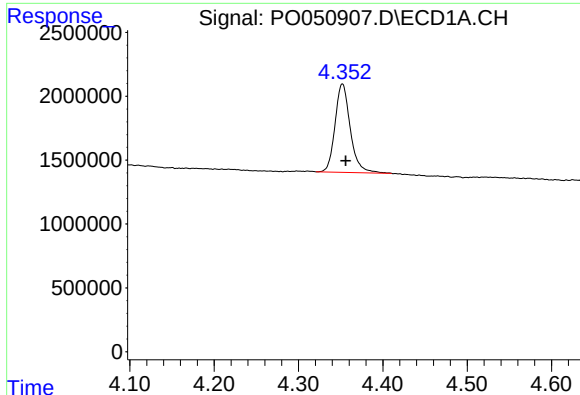

#1 Tetrachloro-m-xylene


R.T.: 4.352 min
Delta R.T.: -0.004 min
Response: 8675220
Conc: 17.36 ng/ml

Instrument :
ECD_O
ClientSampleId :

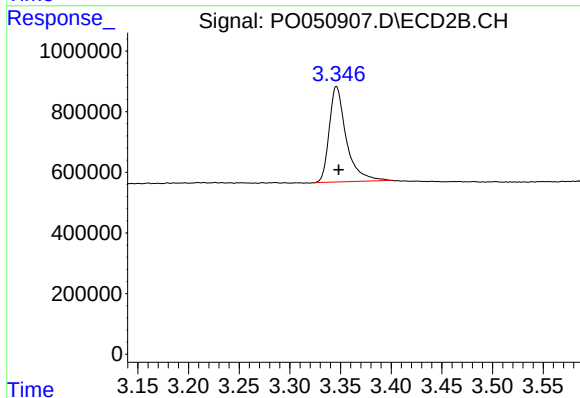


#1 Tetrachloro-m-xylene

R.T.: 3.346 min
Delta R.T.: -0.002 min
Response: 3677683
Conc: 16.92 ng/ml

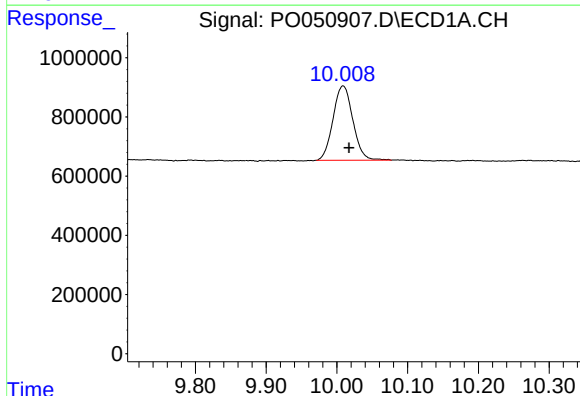


#2 Decachlorobiphenyl

R.T.: 10.009 min
Delta R.T.: -0.009 min
Response: 4890874
Conc: 15.74 ng/ml

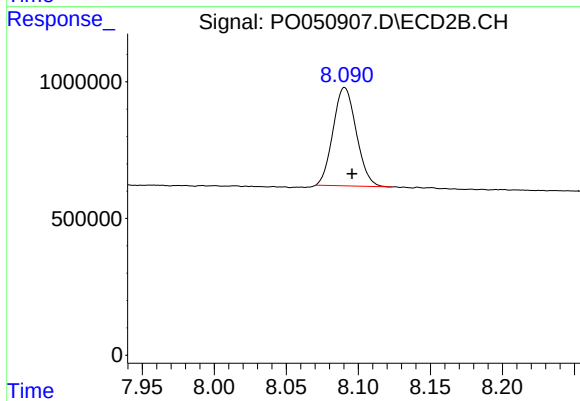

#2 Decachlorobiphenyl


R.T.: 8.091 min
Delta R.T.: -0.005 min
Response: 4040410
Conc: 15.80 ng/ml

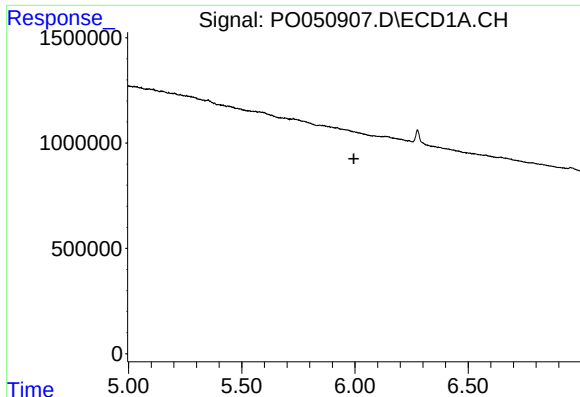

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.995 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

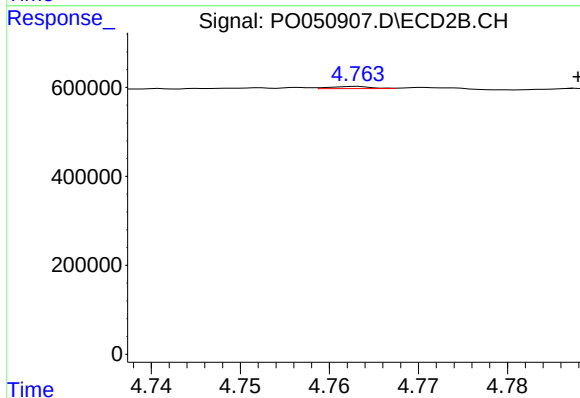


#7 AR-1016-5

R.T.: 4.763 min
Delta R.T.: -0.025 min
Response: 14703
Conc: 1.70 ng/ml

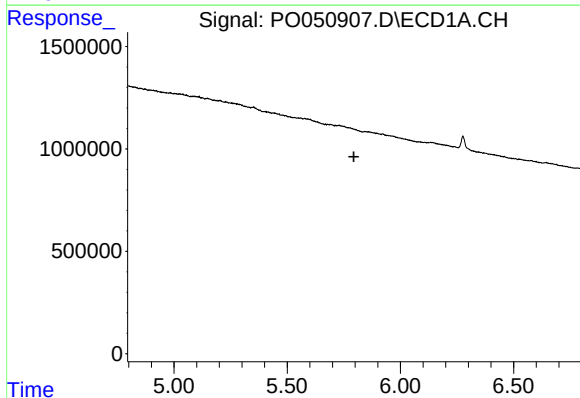


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.794 min
Response: 0
Conc: N.D.

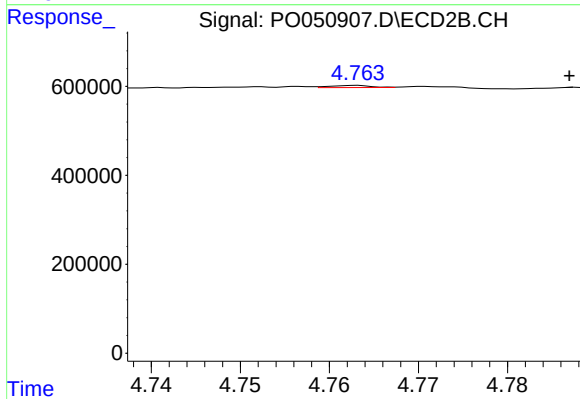

#15 AR-1232-5


R.T.: 4.763 min
Delta R.T.: -0.024 min
Response: 14703
Conc: 5.53 ng/ml

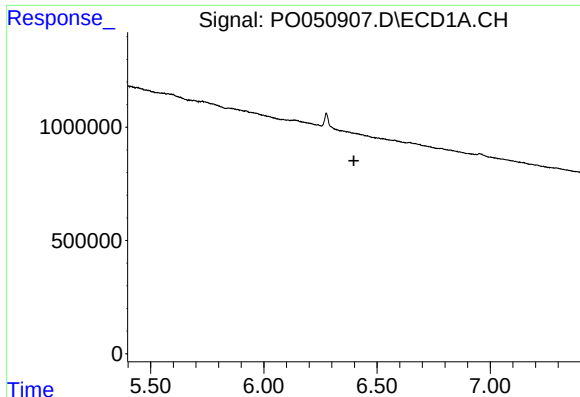

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

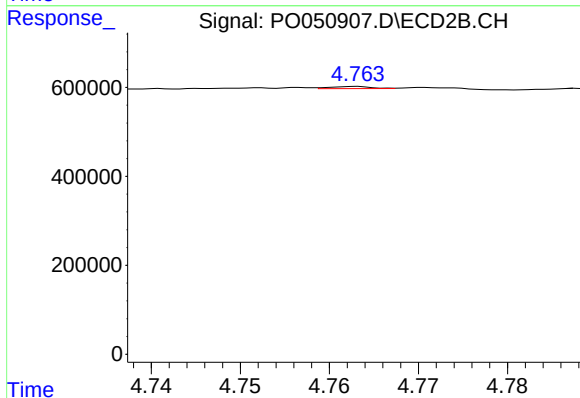


#24 AR-1248-4

R.T.: 4.763 min
Delta R.T.: -0.025 min
Response: 14703
Conc: 1.58 ng/ml

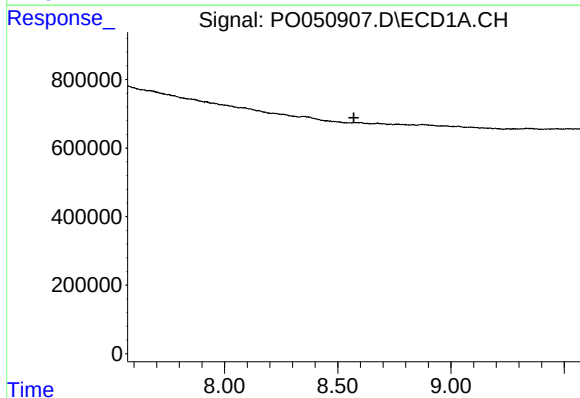


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.571 min
Response: 0
Conc: N.D.

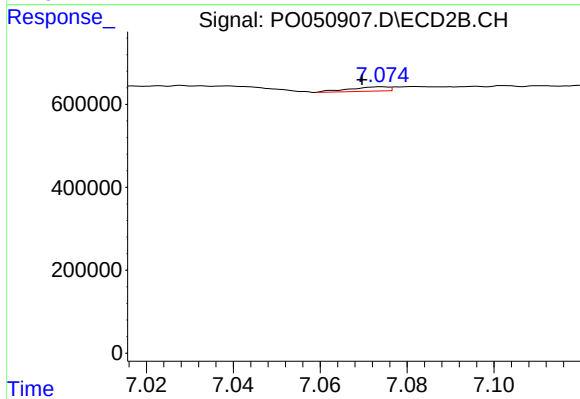

#38 AR-1262-3


R.T.: 7.074 min
Delta R.T.: 0.004 min
Response: 65017
Conc: 3.62 ng/ml

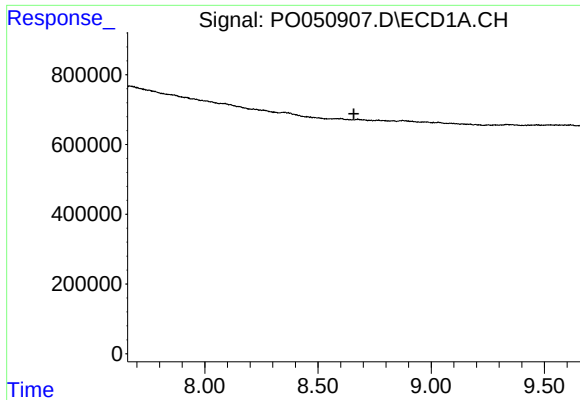

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.658 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

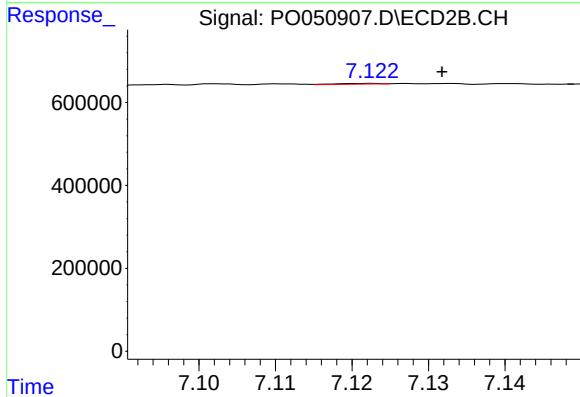


#39 AR-1262-4

R.T.: 7.123 min
Delta R.T.: -0.009 min
Response: 7584
Conc: 0.26 ng/ml

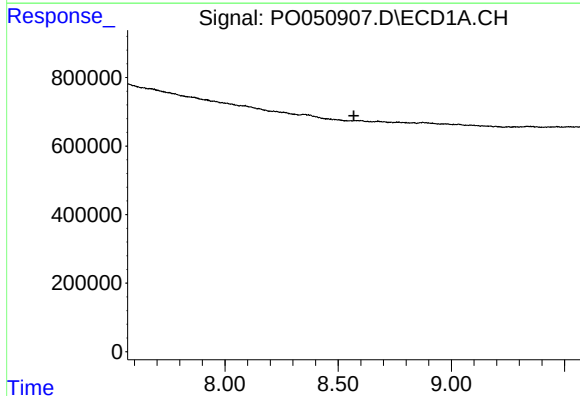


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.570 min
Response: 0
Conc: N.D.

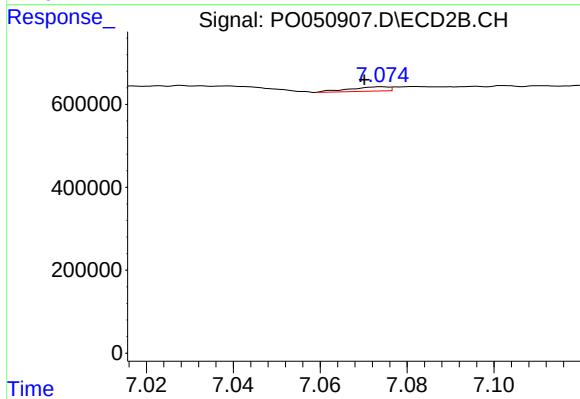

#41 AR-1268-1


R.T.: 7.074 min
Delta R.T.: 0.004 min
Response: 65017
Conc: 1.18 ng/ml

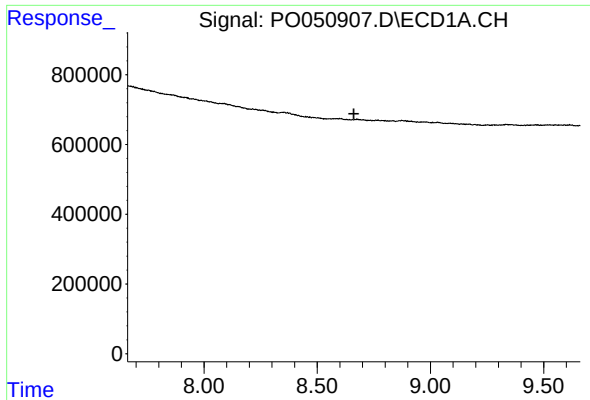

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.662 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

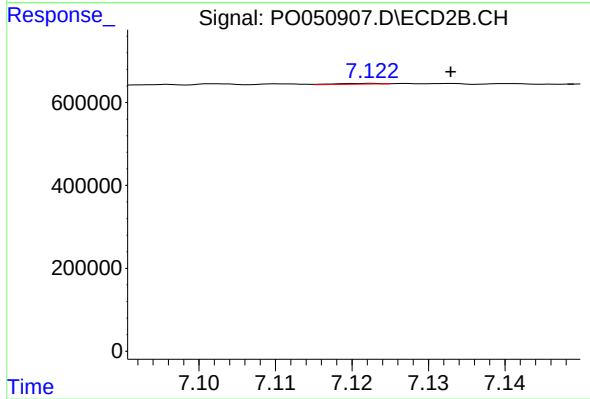

#42 AR-1268-2

R.T.: 7.123 min
Delta R.T.: -0.010 min
Response: 7584
Conc: 0.16 ng/ml