

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
 Data File : P0050889.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2018 18:17
 Operator : SM/SJ
 Sample : PB114245BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB114245BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 00:53:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.353	3.348	9702344	4022352	19.410	18.506
2) SA Decachlor...	10.011	8.091	5948657	4678705	19.138	18.291

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
Data File : PO050889.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 18:17
Operator : SM/SJ
Sample : PB114245BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB114245BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 00:53:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

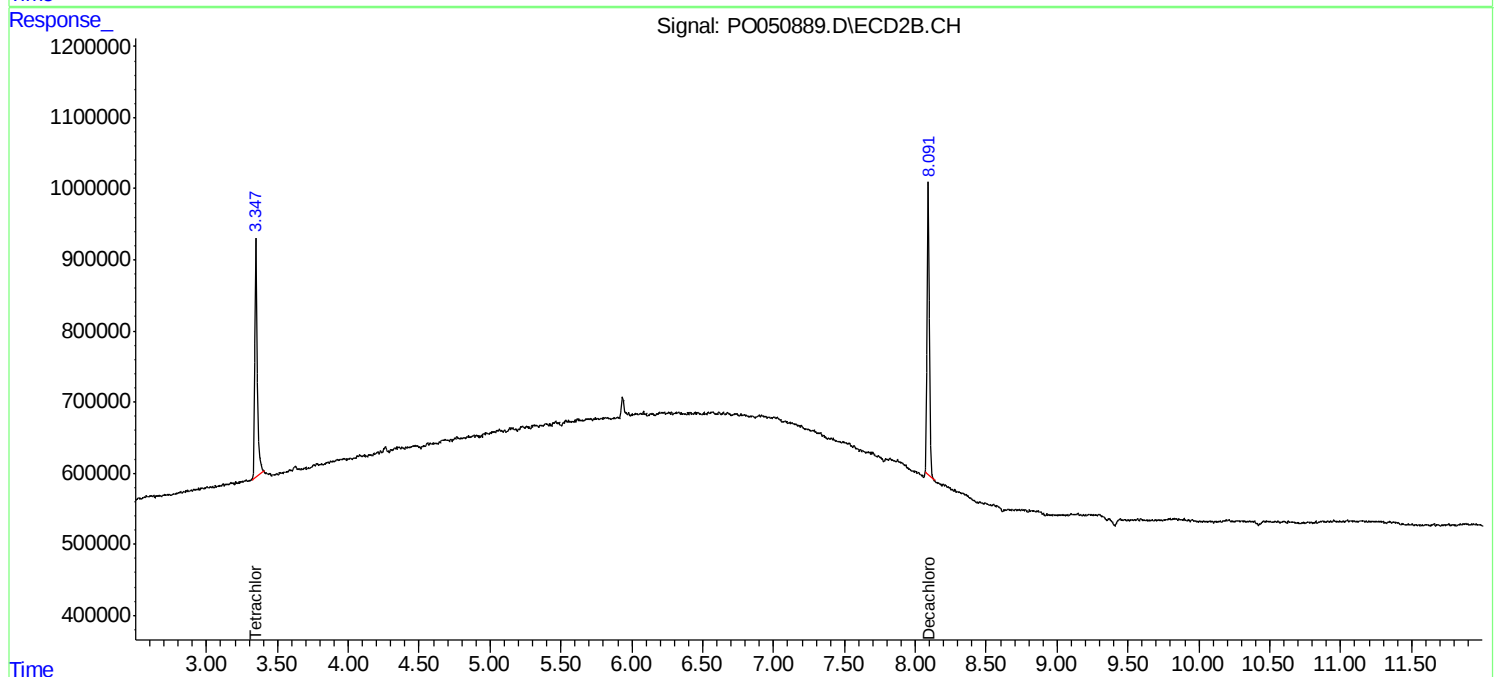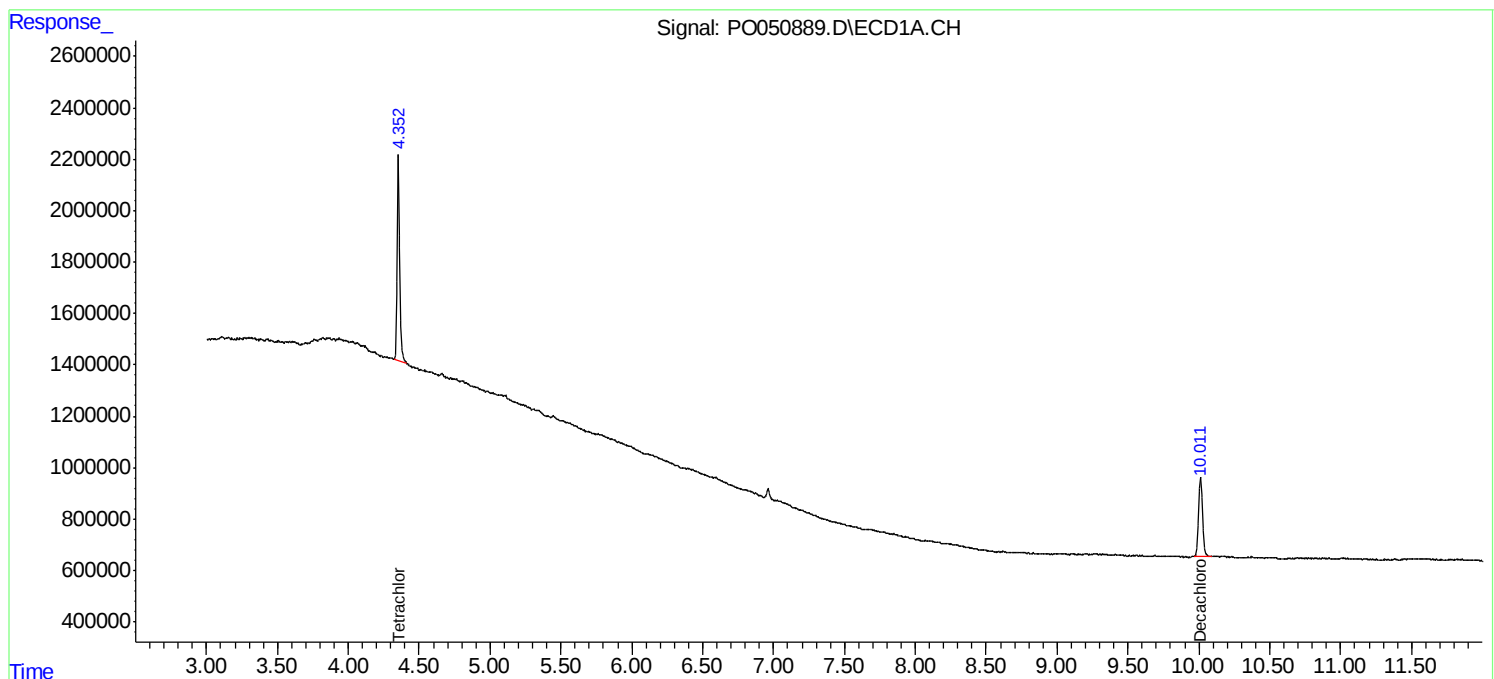


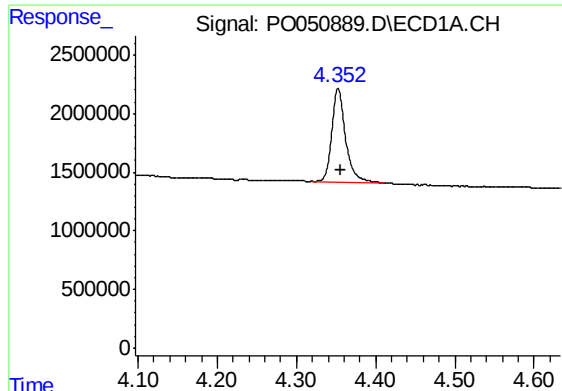

#1 Tetrachloro-m-xylene


R.T.: 4.353 min
Delta R.T.: -0.003 min
Response: 9702344
Conc: 19.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB114245BL

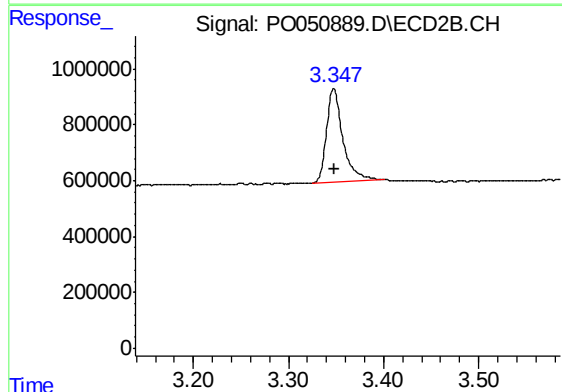


#1 Tetrachloro-m-xylene

R.T.: 3.348 min
Delta R.T.: 0.000 min
Response: 4022352
Conc: 18.51 ng/ml

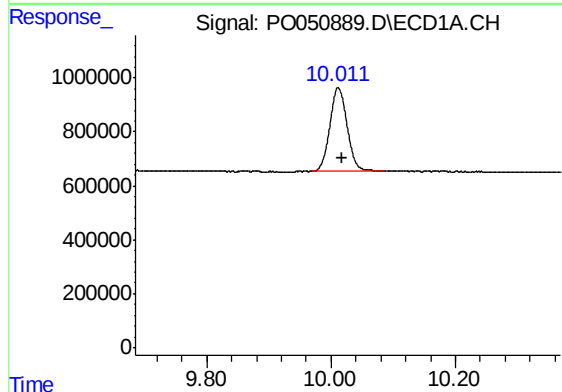

#2 Decachlorobiphenyl

R.T.: 10.011 min
Delta R.T.: -0.006 min
Response: 5948657
Conc: 19.14 ng/ml

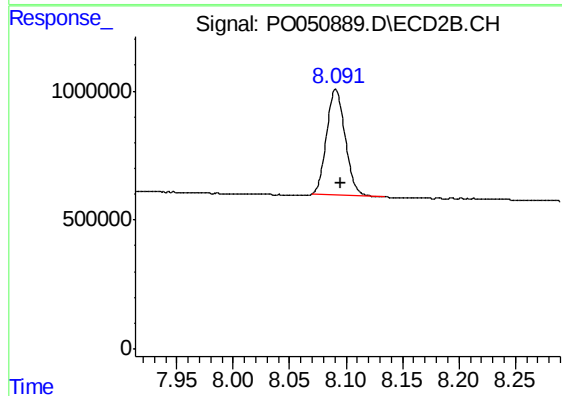

#2 Decachlorobiphenyl

R.T.: 8.091 min
Delta R.T.: -0.005 min
Response: 4678705
Conc: 18.29 ng/ml