

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
Data File : P0050903.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 22:47
Operator : SM/SJ
Sample : J5741-23
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:00:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.353	3.346	9015311	3916801	18.036	18.020
2)	SA Decachlor...	10.010	8.091	5192380	4486900	16.705	17.542m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
Data File : PO050903.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2018 22:47
Operator : SM/SJ
Sample : J5741-23
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:00:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

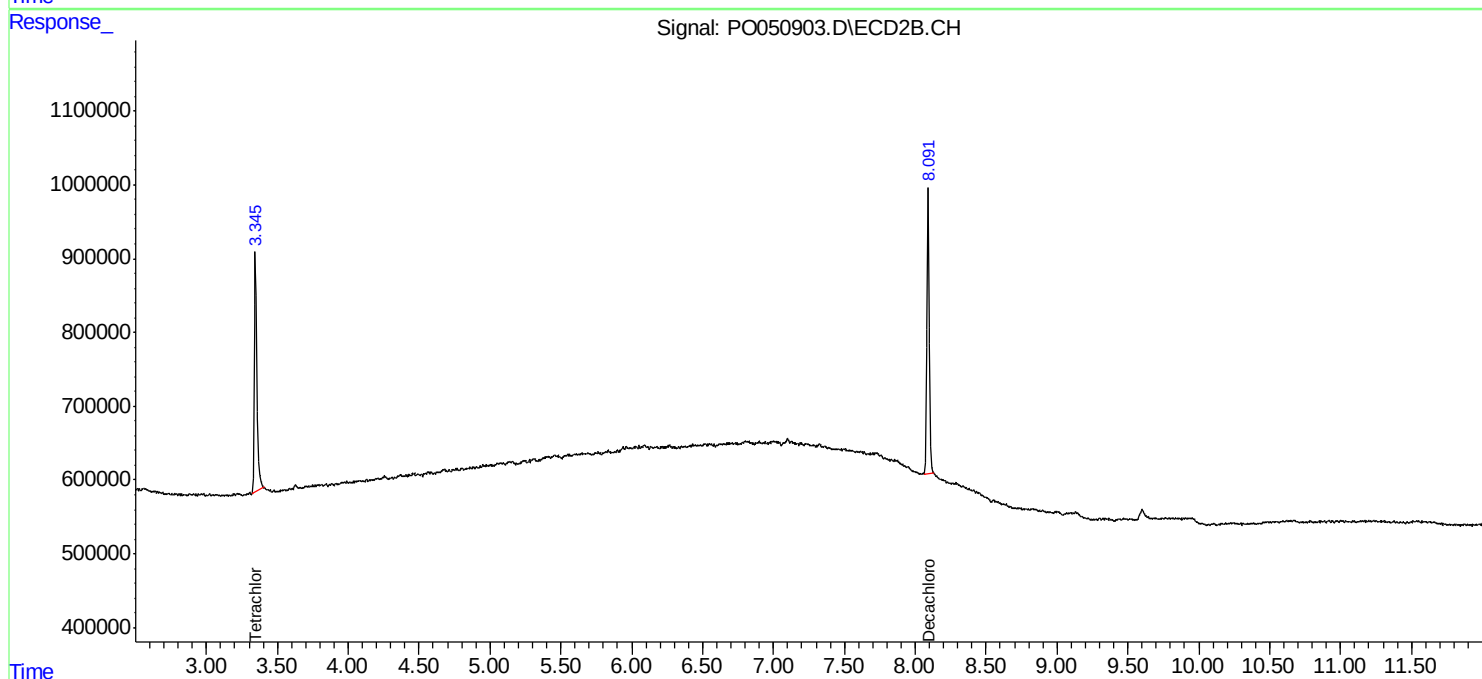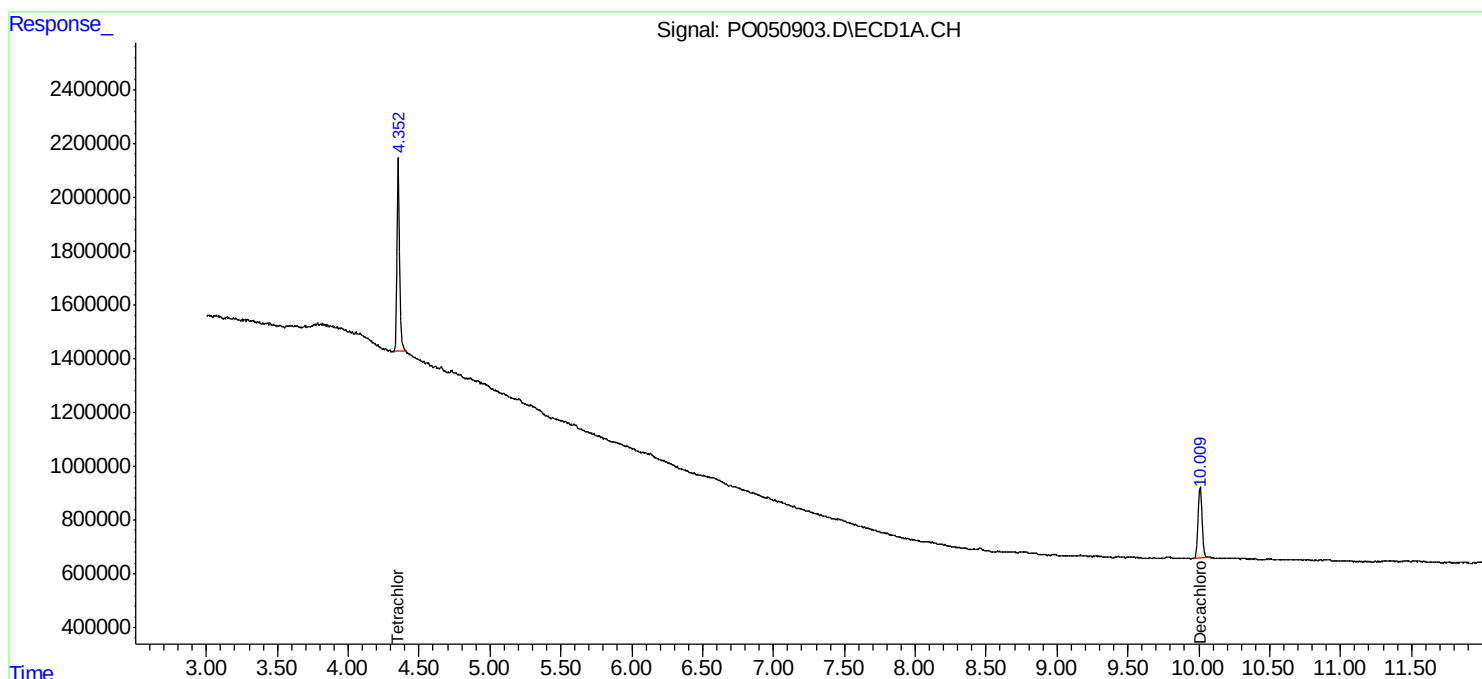


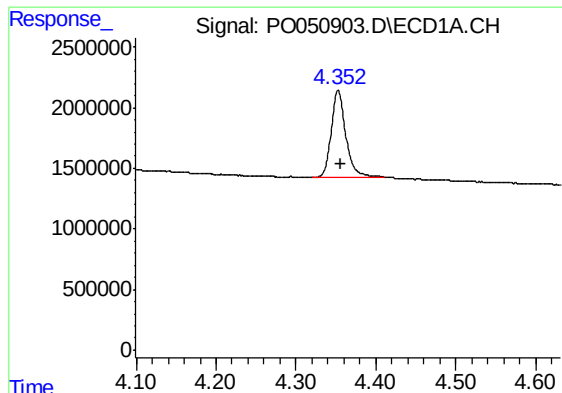

#1 Tetrachloro-m-xylene


R.T.: 4.353 min
Delta R.T.: -0.003 min
Response: 9015311
Conc: 18.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-6

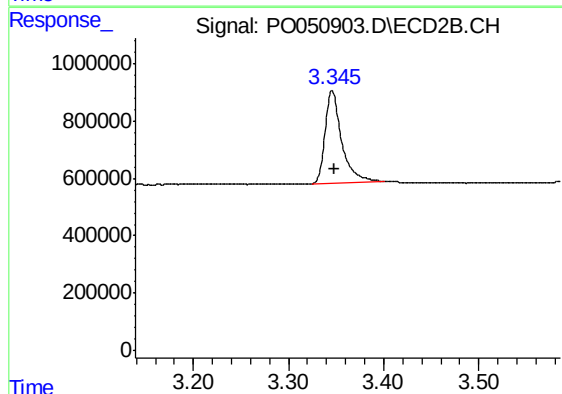


#1 Tetrachloro-m-xylene

R.T.: 3.346 min
Delta R.T.: -0.003 min
Response: 3916801
Conc: 18.02 ng/ml

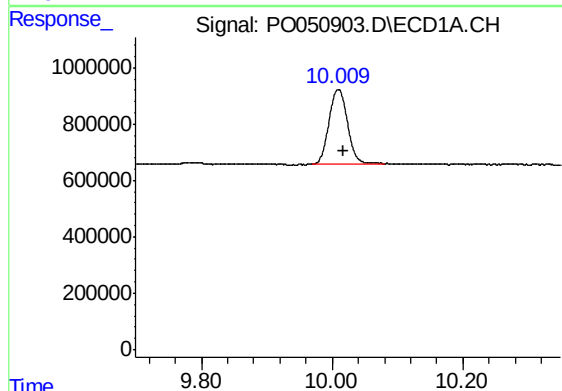

#2 Decachlorobiphenyl

R.T.: 10.010 min
Delta R.T.: -0.008 min
Response: 5192380
Conc: 16.71 ng/ml

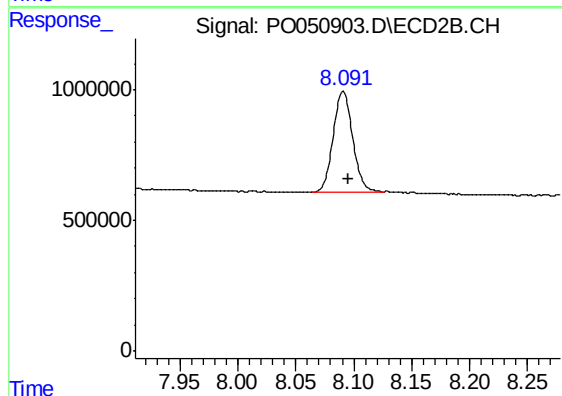

#2 Decachlorobiphenyl

R.T.: 8.091 min
Delta R.T.: -0.005 min
Response: 4486900
Conc: 17.54 ng/ml m