

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110118\
Data File : P0050916.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 2:26
Operator : SM/SJ
Sample : J5755-11
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2A-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 04:46:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.351	3.346	7345055	3072677	14.694	14.137
2)	SA Decachlor...	10.009	8.090	2988367	2677746	9.614	10.469m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110118\
Data File : P0050916.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 2:26
Operator : SM/SJ
Sample : J5755-11
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2A-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 04:46:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

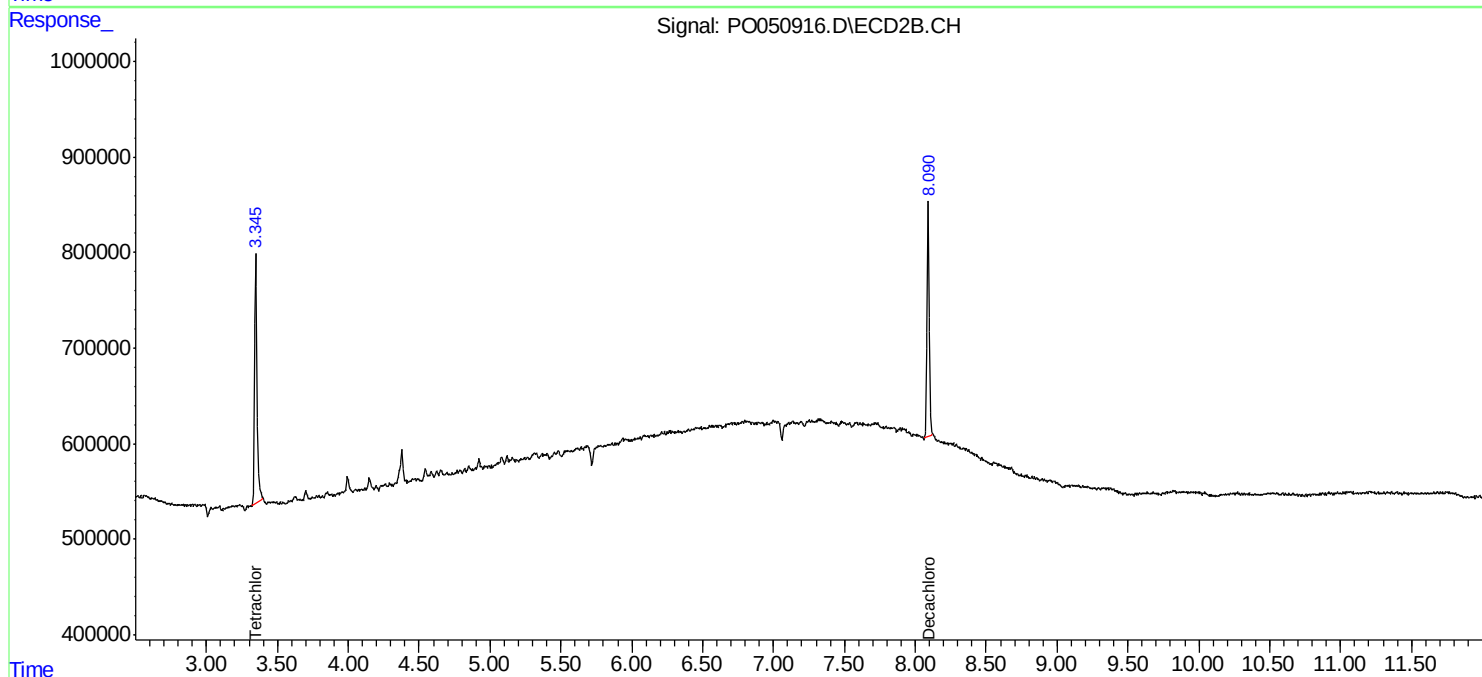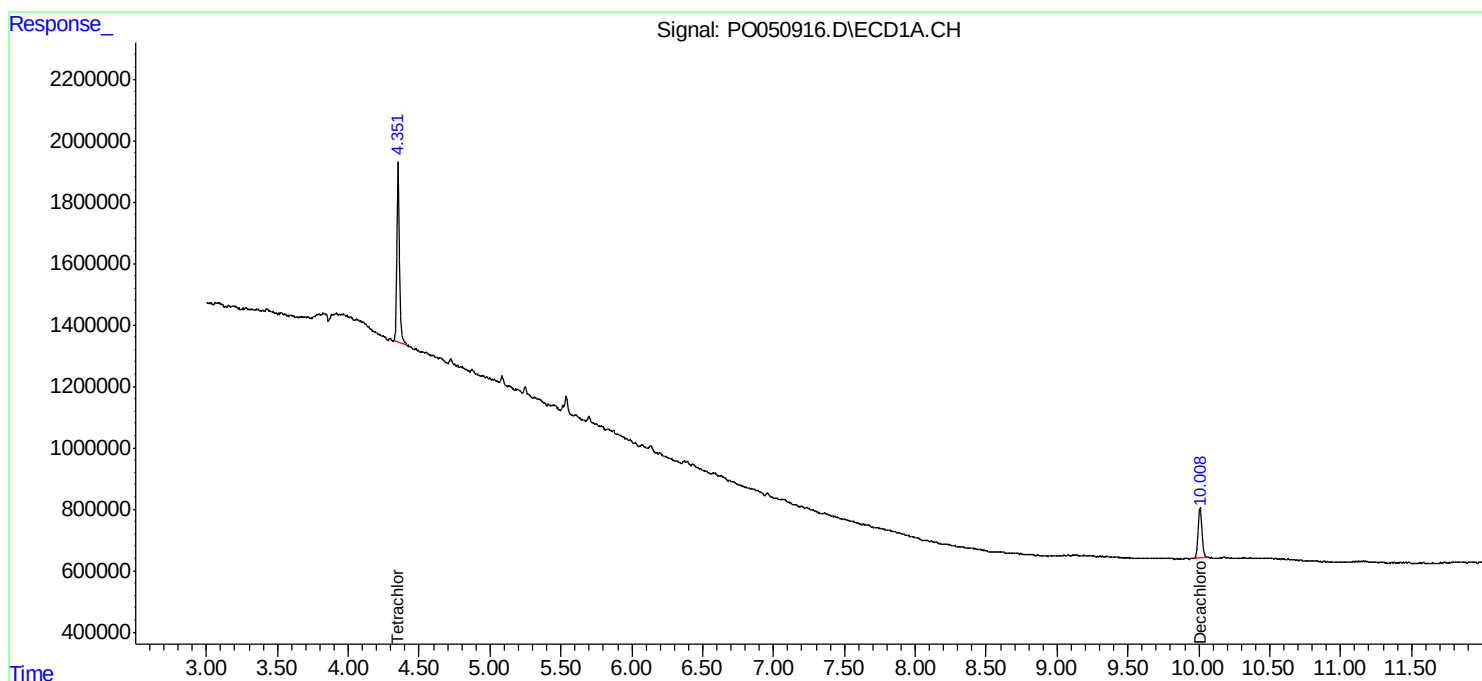


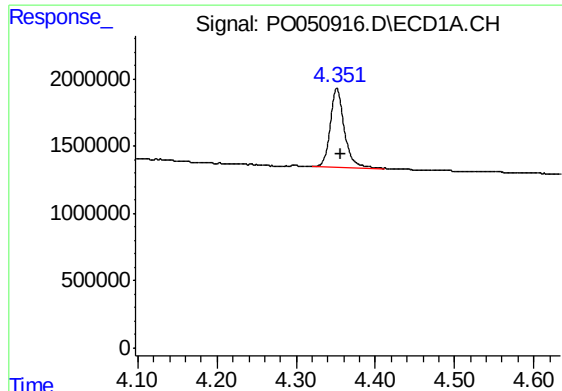

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.005 min
Response: 7345055
Conc: 14.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2A-D

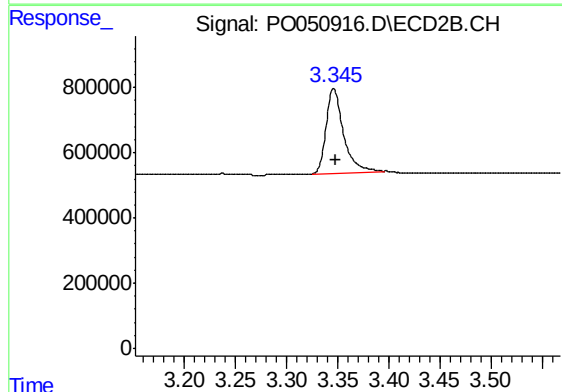


#1 Tetrachloro-m-xylene

R.T.: 3.346 min
Delta R.T.: -0.003 min
Response: 3072677
Conc: 14.14 ng/ml

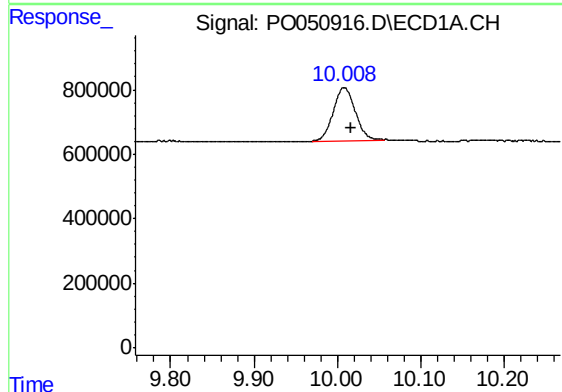

#2 Decachlorobiphenyl

R.T.: 10.009 min
Delta R.T.: -0.009 min
Response: 2988367
Conc: 9.61 ng/ml

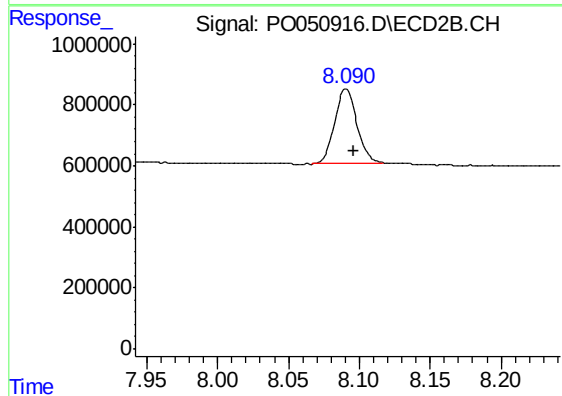

#2 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: -0.005 min
Response: 2677746
Conc: 10.47 ng/ml m