

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110121\
 Data File : PO082373.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2021 13:25
 Operator : AJ\MA
 Sample : M4404-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-2021-2A

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/02/2021
 Supervised By :mohammad ahmed 11/02/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 14:56:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 29 11:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.979	3.975	1045447	423401	12.938	14.350
2) SA Decachlor...	11.114	9.317	970197	389094	17.456	15.277m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110121\
Data File : PO082373.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2021 13:25
Operator : AJ\MA
Sample : M4404-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MOO-2021-2A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/02/2021
Supervised By :mohammad ahmed 11/02/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 14:56:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

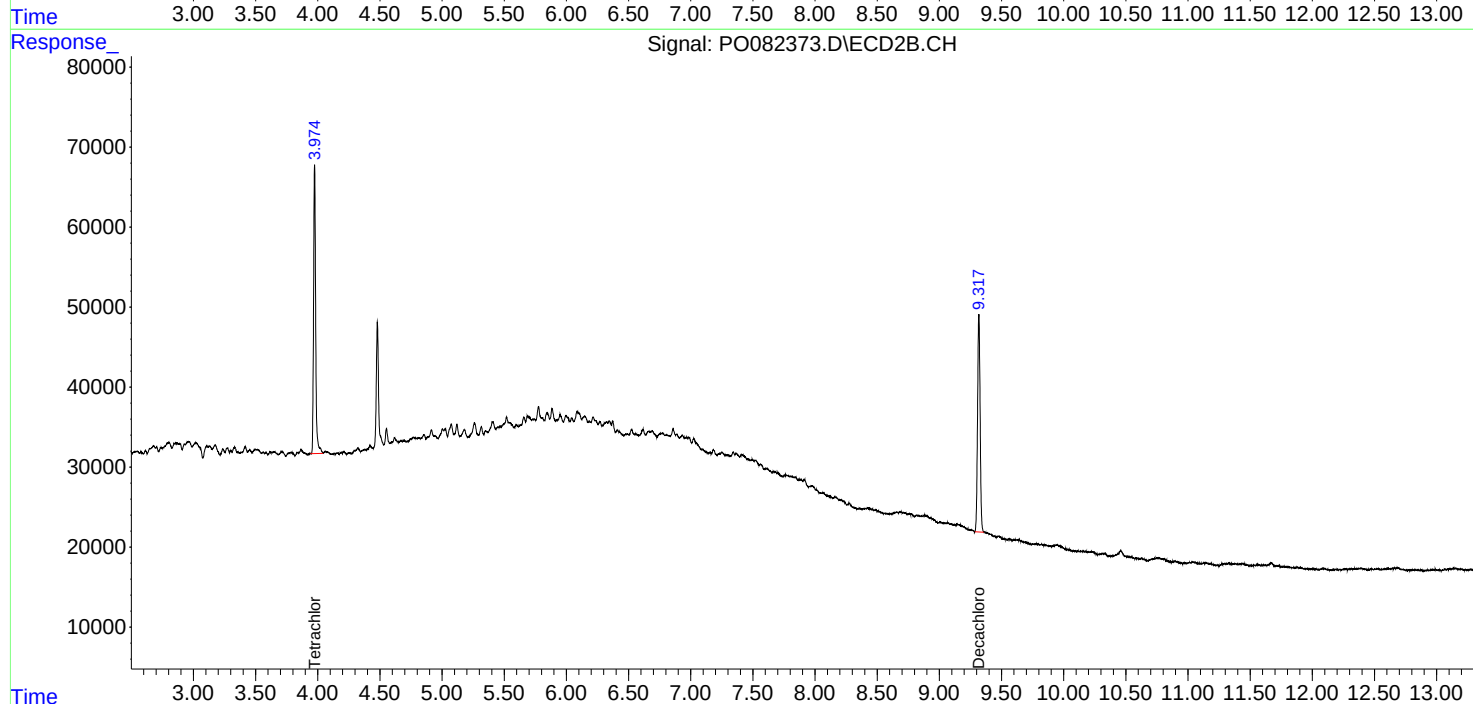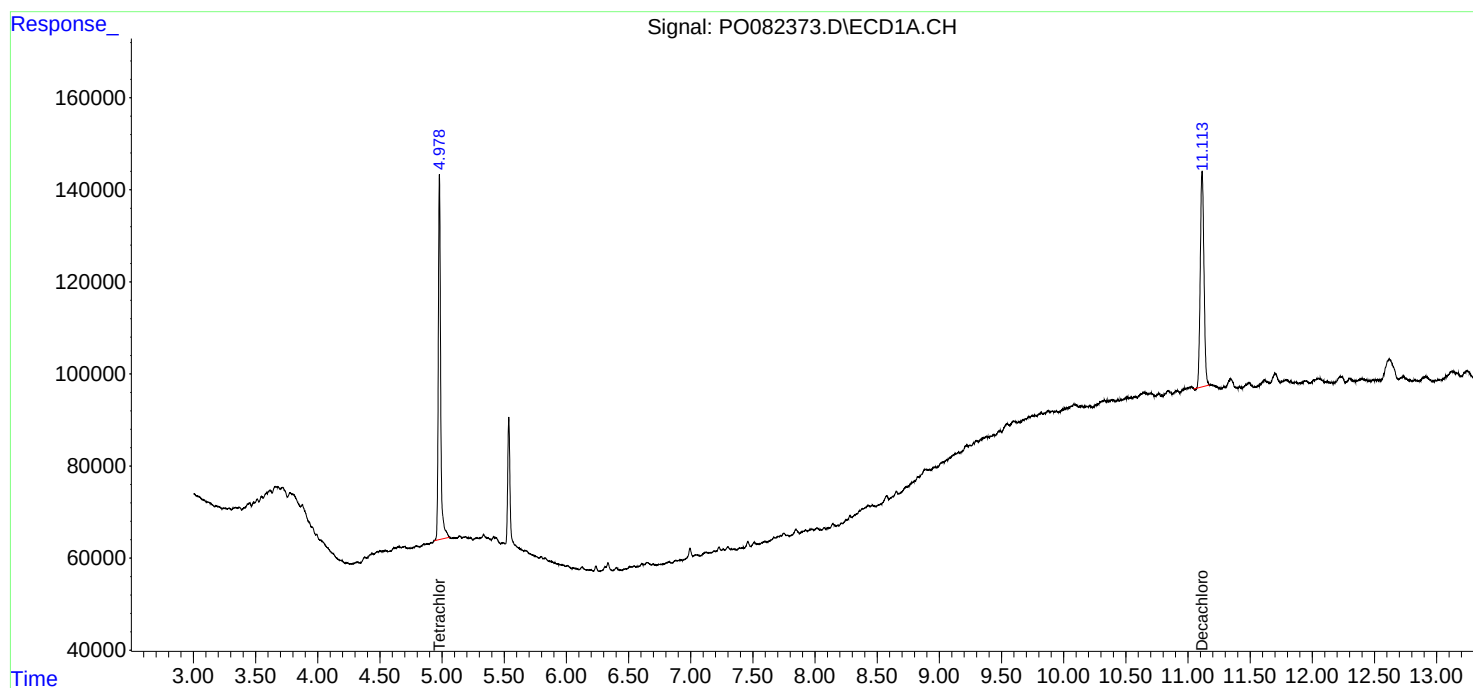

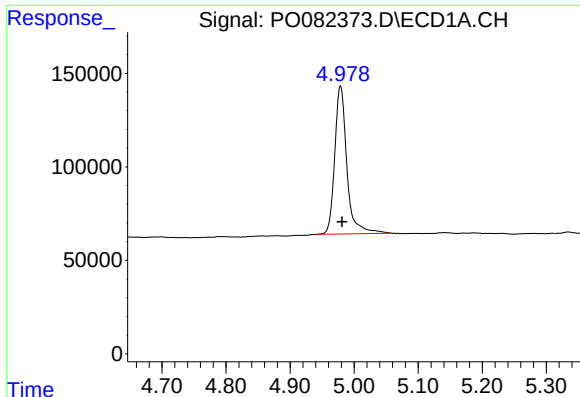


#1 Tetrachloro-m-xylene

R.T.: 4.979 min
Delta R.T.: -0.002 min
Response: 1045447
Conc: 12.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2021-2A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/02/2021
Supervised By :mohammad ahmed 11/02/2021

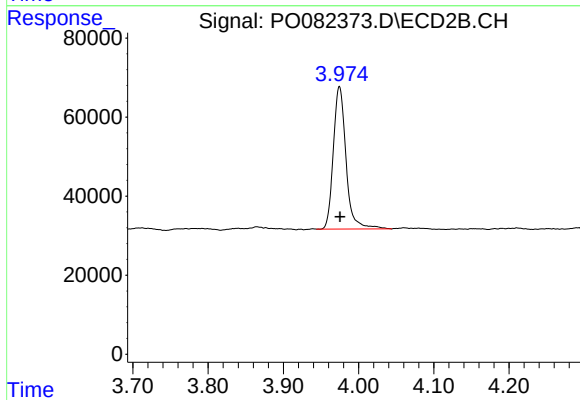


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: 0.000 min
Response: 423401
Conc: 14.35 ng/ml

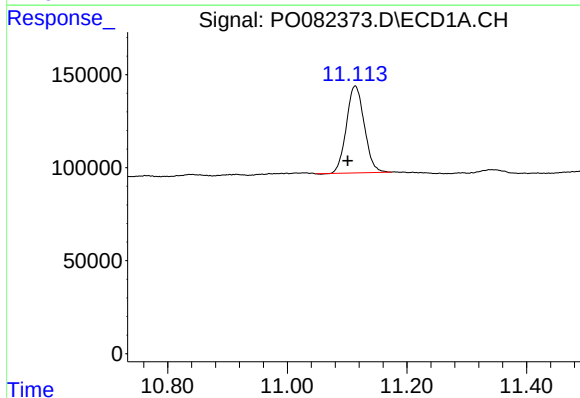

#2 Decachlorobiphenyl

R.T.: 11.114 min
Delta R.T.: 0.013 min
Response: 970197
Conc: 17.46 ng/ml

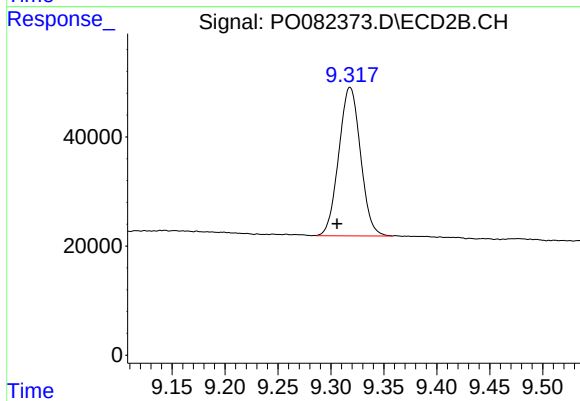

#2 Decachlorobiphenyl

R.T.: 9.317 min
Delta R.T.: 0.012 min
Response: 389094
Conc: 15.28 ng/ml m