

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110121\
 Data File : PO082375.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2021 13:59
 Operator : AJ\MA
 Sample : M4404-05 20X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-2021-3B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 14:56:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 29 11:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.976	3.971	39412	18702	0.488	0.634 #
2) SA Decachlor...	11.097	9.293	29067	13358	0.523	0.524

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110121\
Data File : PO082375.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2021 13:59
Operator : AJ\MA
Sample : M4404-05 20X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MOO-2021-3B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 14:56:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

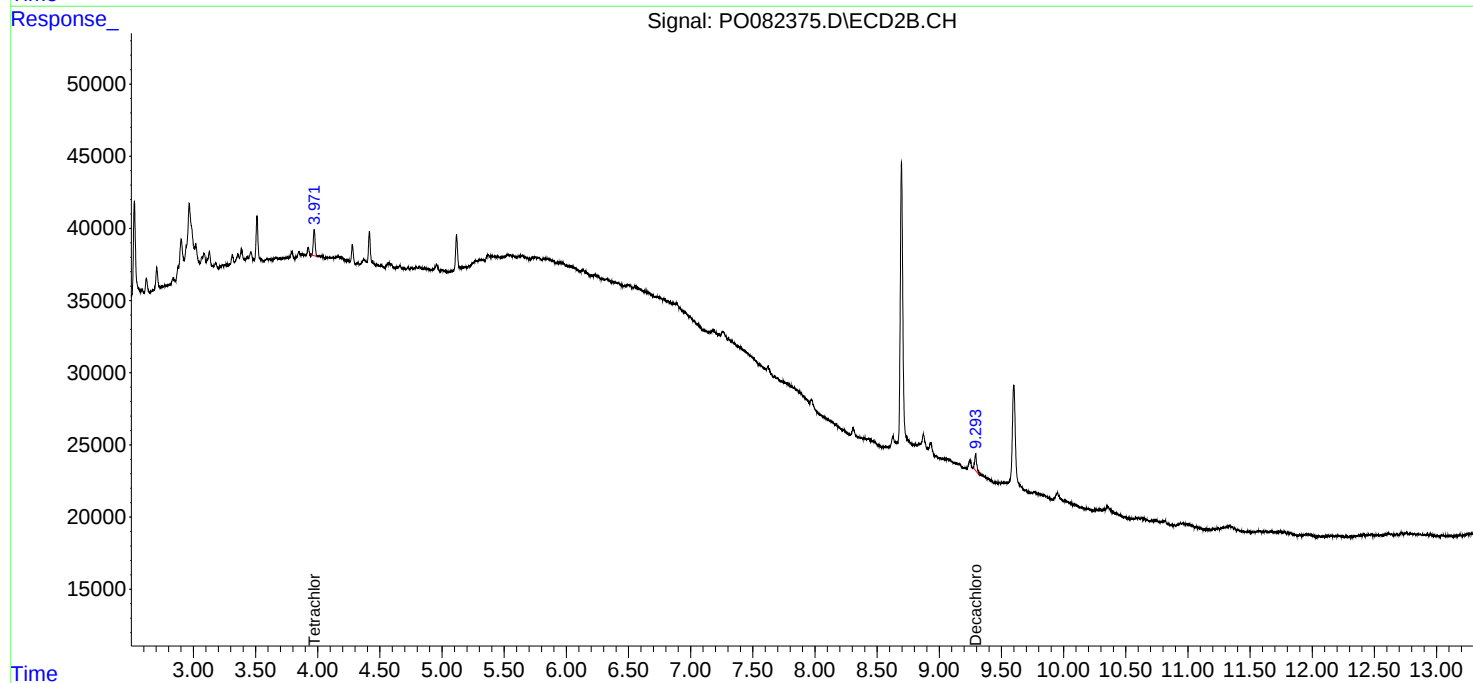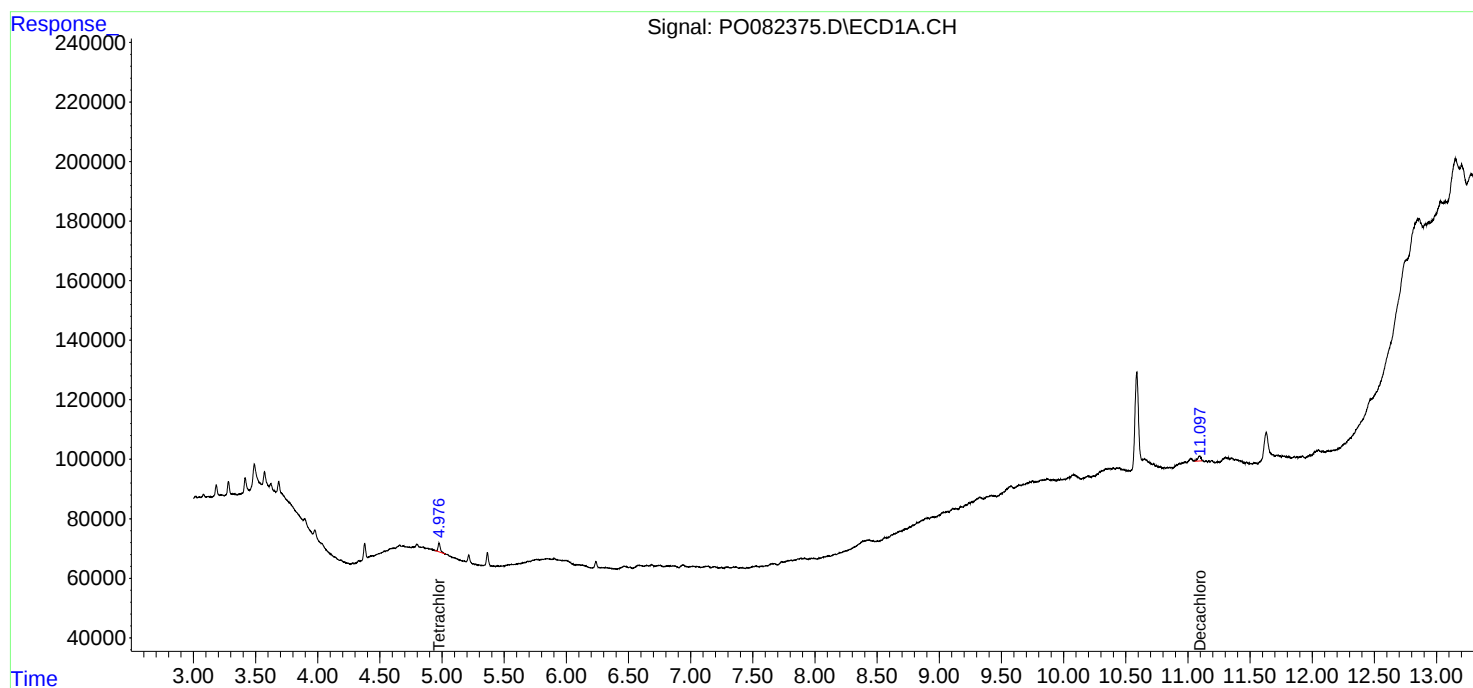


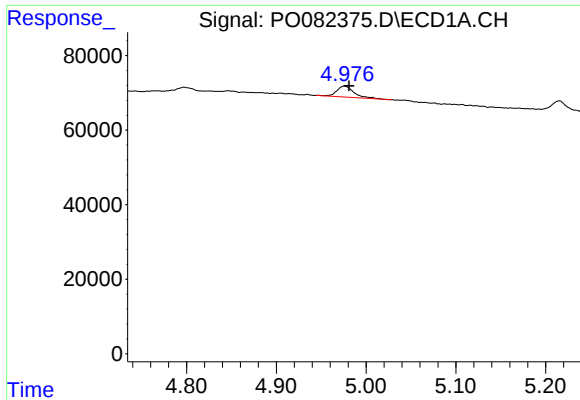

#1 Tetrachloro-m-xylene


R.T.: 4.976 min
Delta R.T.: -0.005 min
Response: 39412
Conc: 0.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2021-3B

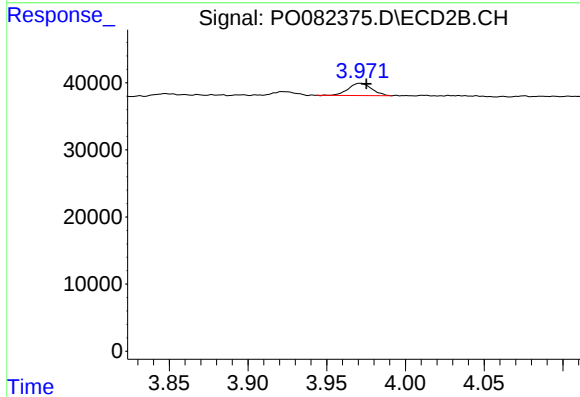


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: -0.004 min
Response: 18702
Conc: 0.63 ng/ml

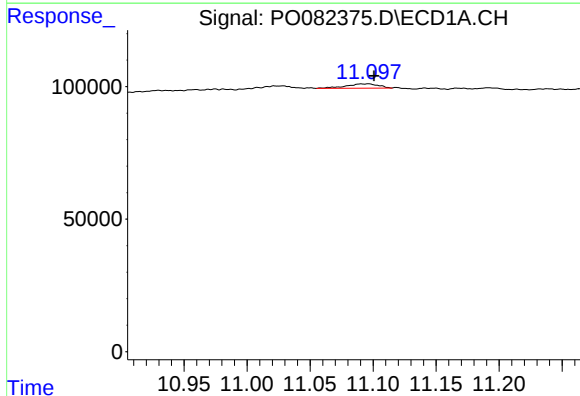

#2 Decachlorobiphenyl

R.T.: 11.097 min
Delta R.T.: -0.004 min
Response: 29067
Conc: 0.52 ng/ml

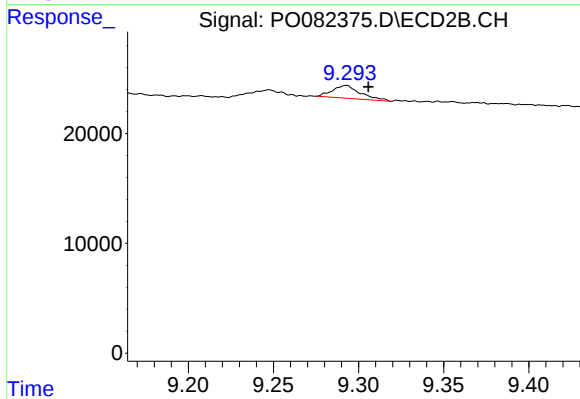

#2 Decachlorobiphenyl

R.T.: 9.293 min
Delta R.T.: -0.013 min
Response: 13358
Conc: 0.52 ng/ml