

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110121\
 Data File : PO082397.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2021 23:24
 Operator : AJ\MA
 Sample : M4427-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FDR-BH-4-20211029-7.5-8M

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 04:35:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 29 11:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.975	3.971	1420545	796256	17.580	26.988 #
2) SA Decachlor...	11.085	9.288	1372915	497316	24.702	19.526

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110121\
Data File : PO082397.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2021 23:24
Operator : AJ\MA
Sample : M4427-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FDR-BH-4-20211029-7.5-8M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 04:35:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 29 11:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

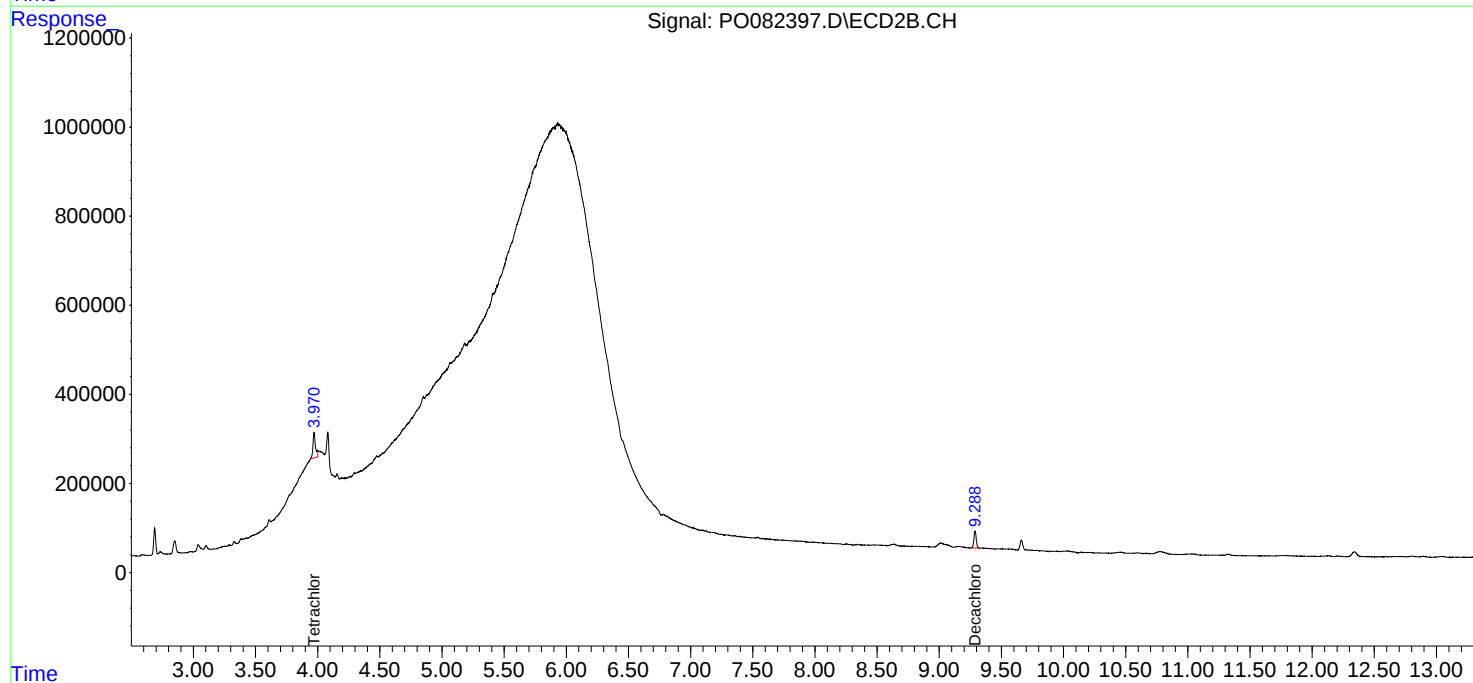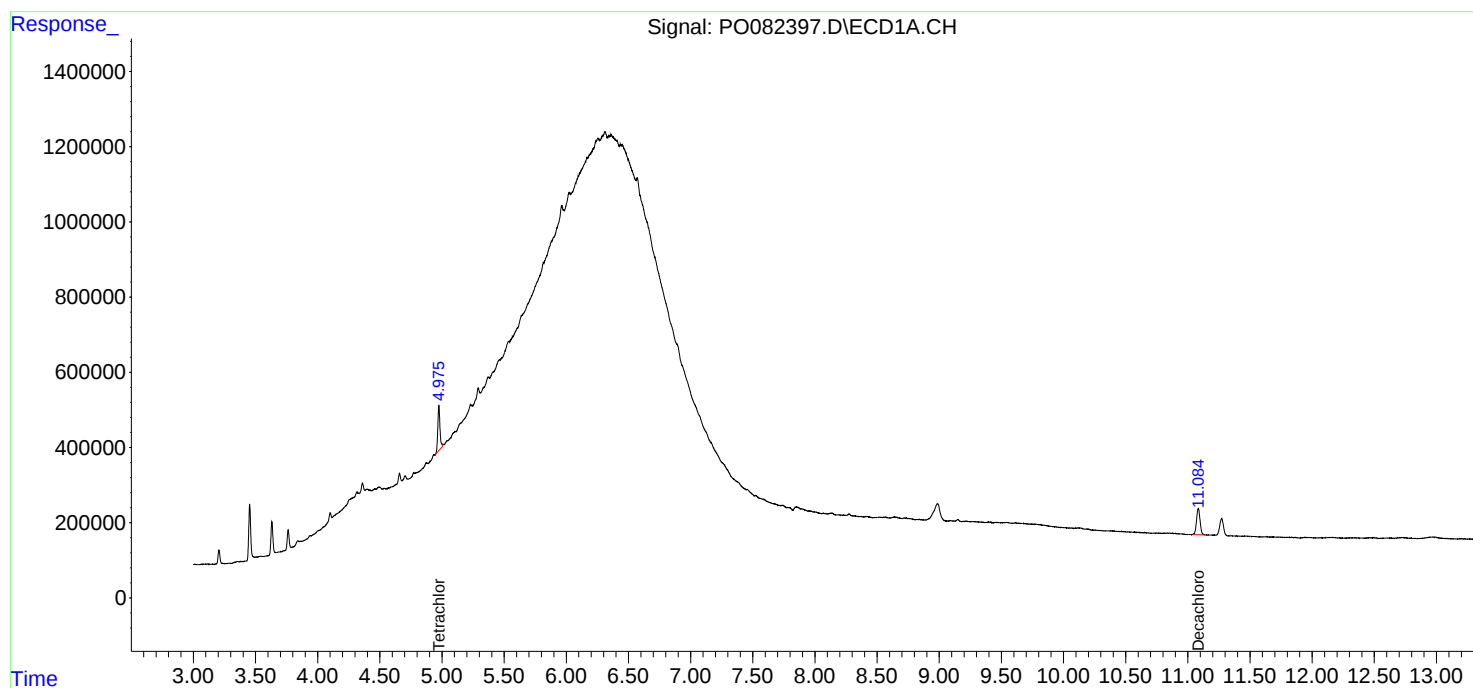


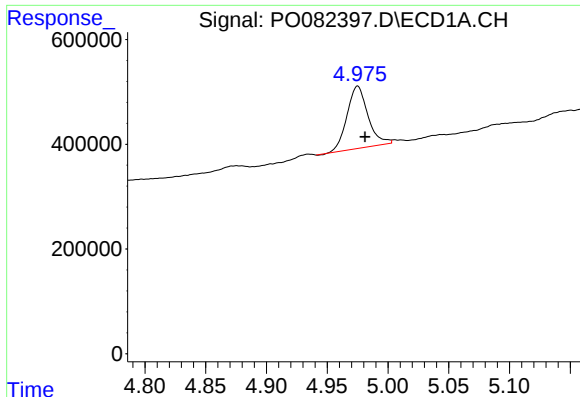

#1 Tetrachloro-m-xylene


R.T.: 4.975 min
Delta R.T.: -0.006 min
Response: 1420545
Conc: 17.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
FDR-BH-4-20211029-7.5-8M

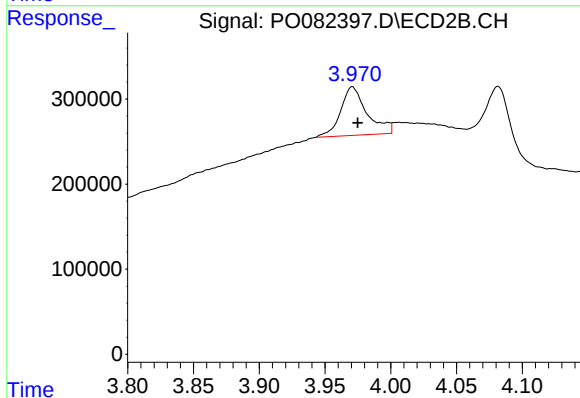


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: -0.004 min
Response: 796256
Conc: 26.99 ng/ml

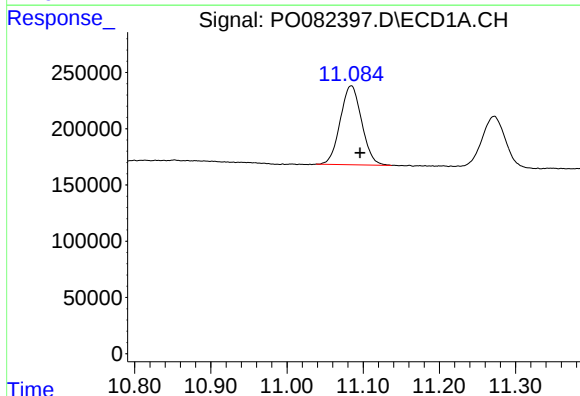

#2 Decachlorobiphenyl

R.T.: 11.085 min
Delta R.T.: -0.011 min
Response: 1372915
Conc: 24.70 ng/ml

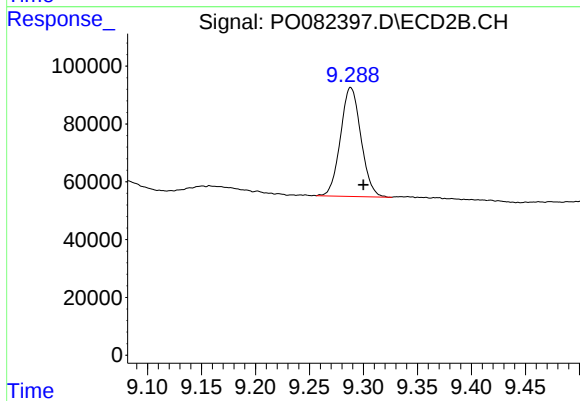

#2 Decachlorobiphenyl

R.T.: 9.288 min
Delta R.T.: -0.012 min
Response: 497316
Conc: 19.53 ng/ml