

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110122\
 Data File : P0090095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2022 21:35
 Operator : YP/AJ
 Sample : N5380-01MS
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-EMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 04:35:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.305	3.484	59557067	21168539	18.531	19.918
2)	SA Decachlor...	10.052	8.491	37890026	15891720	15.462	15.430
Target Compounds							
3)	L1 AR-1016-1	5.480	4.571	44899037	18111833	422.112	468.892
4)	L1 AR-1016-2	5.502	4.590	66566572	24991126	436.980	467.184
5)	L1 AR-1016-3	5.565	4.765	40827773	13136137	432.093	452.457
6)	L1 AR-1016-4	5.662	4.808	36159916	11197166	482.208	451.081
7)	L1 AR-1016-5	5.960	5.021	33945218	12871671	439.813	419.011
8)	L2 AR-1221-1	4.511	3.700	8551458	2467614	224.032	184.701
9)	L2 AR-1221-2	4.601	3.784	7070591	4292717	248.716	422.976 #
10)	L2 AR-1221-3	4.678	3.860	28247407	11743023	329.878	377.490
11)	L3 AR-1232-1	4.678	3.860	28247407	11743023	431.366	493.599
12)	L3 AR-1232-2	5.209	4.590	40386494	24991126	1050.586	1042.895
13)	L3 AR-1232-3	5.502	4.765	66566572	13136137	993.361	1034.435
14)	L3 AR-1232-4	5.662	4.851	36159916	13319864	1095.168	1092.463
15)	L3 AR-1232-5	5.756	5.021	29212360	12871671	1102.639	964.039
16)	L4 AR-1242-1	5.480	4.571	44899037	18111833	542.646	608.357
17)	L4 AR-1242-2	5.502	4.590	66566572	24991126	563.638	614.411
18)	L4 AR-1242-3	5.565	4.765	40827773	13136137	548.490	594.063
19)	L4 AR-1242-4	5.662	4.851	36159916	13319864	620.671	561.696
20)	L4 AR-1242-5	6.403	5.377	8056754	16875706	131.069	589.956 #
21)	L5 AR-1248-1	5.480	4.571	44899037	18111833	709.896	797.803
22)	L5 AR-1248-2	5.756	4.808	29212360	11197166	308.470	344.402
23)	L5 AR-1248-3	5.960	4.851	33945218	13319864	344.340	395.154
24)	L5 AR-1248-4	6.371	5.021	14504665	12871671	136.042	332.831 #
25)	L5 AR-1248-5	6.403	5.415	8056754	2655226	76.697	73.331
26)	L6 AR-1254-1	6.341	5.377	31405007	16875706	270.973	286.488
27)	L6 AR-1254-2	6.561	5.524	41710487	12381333	239.807	231.080
28)	L6 AR-1254-3	6.934	5.946	35177158	28641474	202.627	345.567 #
29)	L6 AR-1254-4	7.216	6.159	10408428	3214829	81.656	64.731
30)	L6 AR-1254-5	7.636	6.579	98435342	43675010	698.819	583.302
31)	L7 AR-1260-1	7.094	6.061	52777393	32343393	376.483	537.255 #
32)	L7 AR-1260-2	7.346	6.250	161.3E6	29621000	997.066	410.022 #
33)	L7 AR-1260-3	7.715	6.403	39283272	27798024	373.929	417.177
34)	L7 AR-1260-4	7.940	6.878	47865685	20184475	387.445	396.753
35)	L7 AR-1260-5	8.256	7.121	90503315	44538455	397.716	383.451
36)	L8 AR-1262-1	7.715	6.618	39283272	21710044	236.975	286.516
37)	L8 AR-1262-2	8.256	7.121	90503315	44538455	322.120	347.330
38)	L8 AR-1262-3	8.577	7.406	57694942	9262853	293.834	170.091 #
39)	L8 AR-1262-4	8.654	7.469	15486225	32469321	159.153	334.320 #
40)	L8 AR-1262-5	9.304	7.965	22715635	10362150	215.576	218.332
41)	L9 AR-1268-1	8.577	7.406	57694942	9262853	165.486	58.793 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110122\
 Data File : PO090095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2022 21:35
 Operator : YP/AJ
 Sample : N5380-01MS
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-EMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 04:35:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.654	7.469	15486225	32469321	49.641	231.416 #
43) L9	AR-1268-3	8.882	7.685	2024609	1278395	7.534	10.653 #
44) L9	AR-1268-4	9.304	7.965	22715635	10362150	194.950	190.797
45) L9	AR-1268-5	9.715	8.245	7539548	3502639	8.793	10.006



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110122\
Data File : PO090095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2022 21:35
Operator : YP/AJ
Sample : N5380-01MS
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-EMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 04:35:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

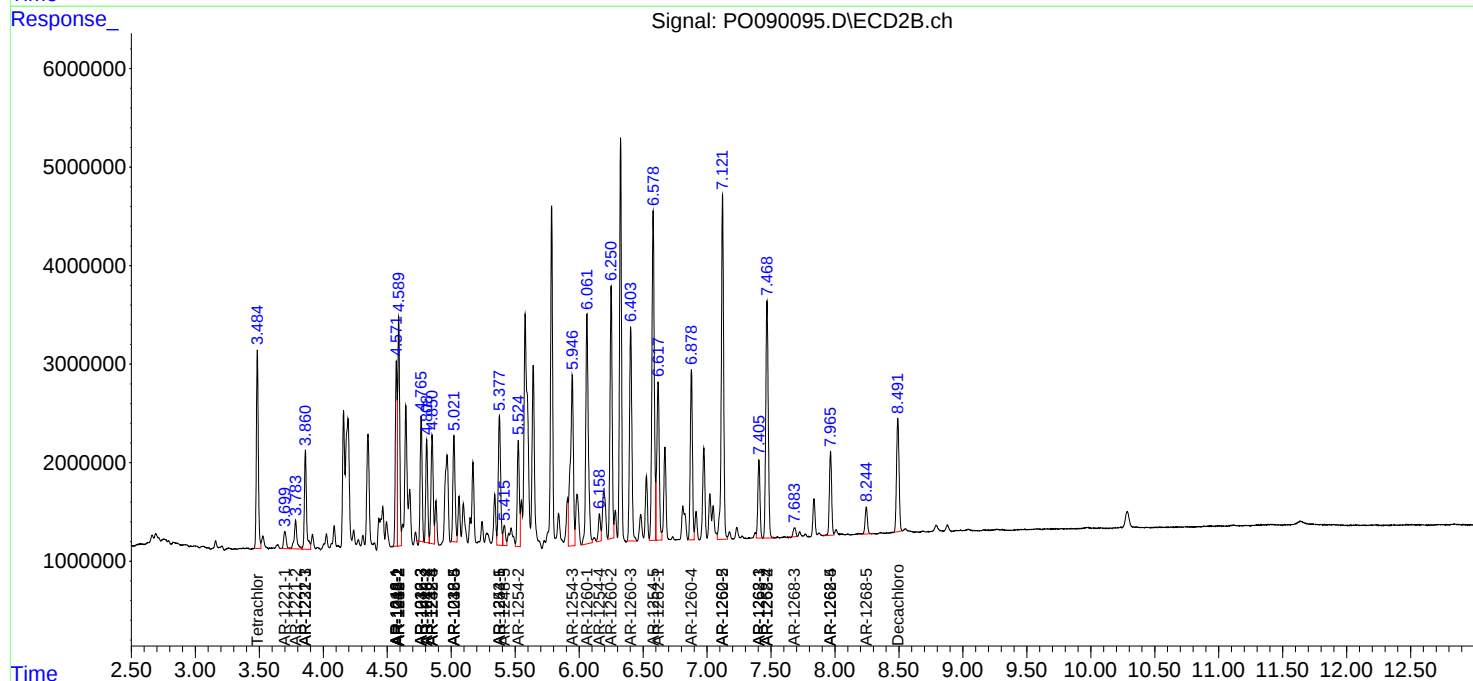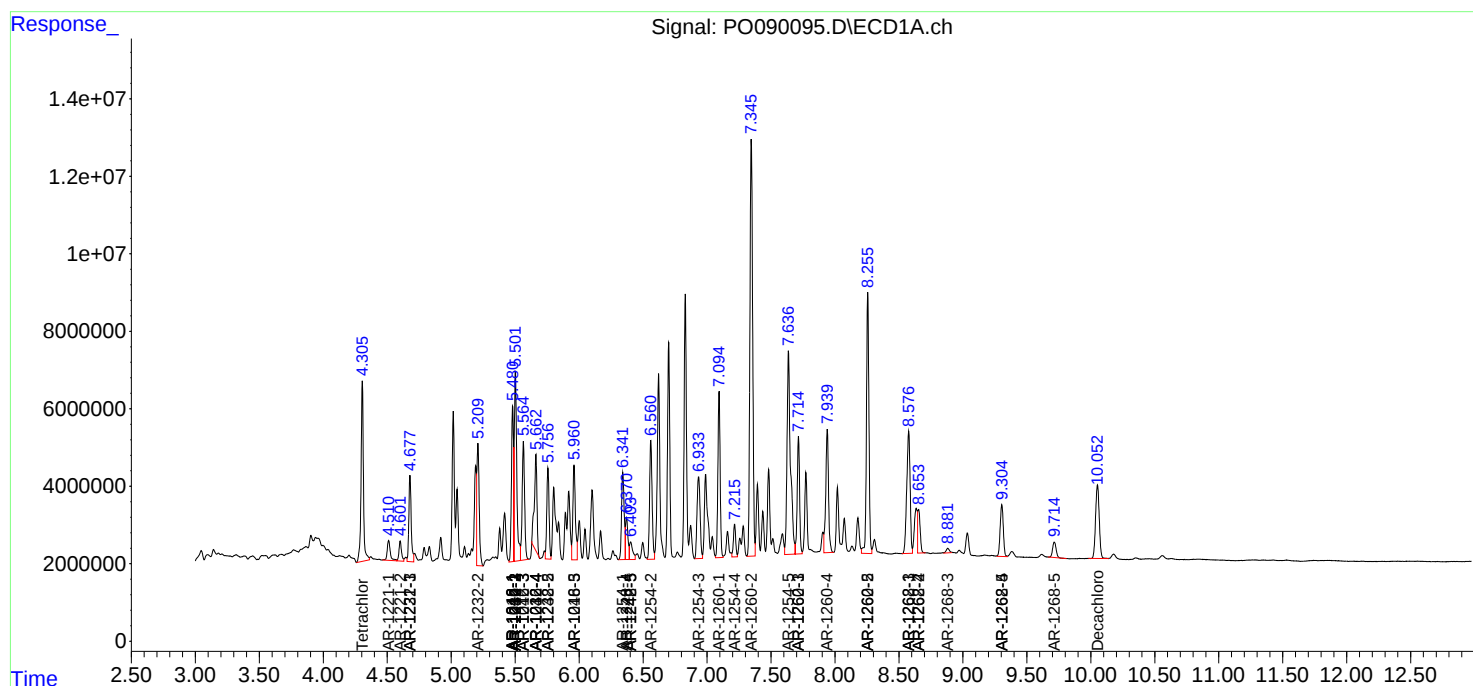


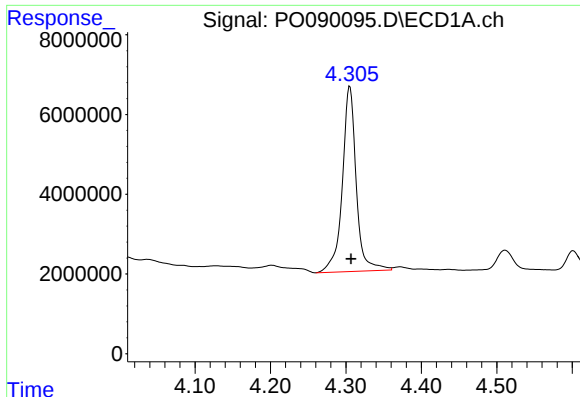

#1 Tetrachloro-m-xylene


R.T.: 4.305 min
Delta R.T.: -0.002 min
Response: 59557067
Conc: 18.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

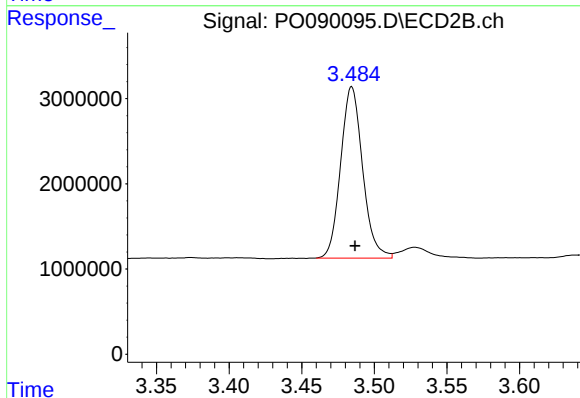


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 21168539
Conc: 19.92 ng/ml

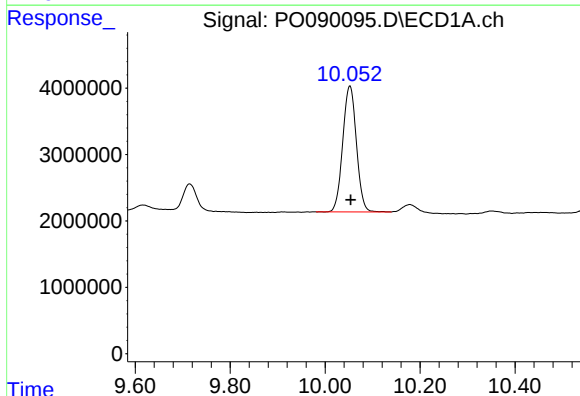


#2 Decachlorobiphenyl

R.T.: 10.052 min
Delta R.T.: -0.002 min
Response: 37890026
Conc: 15.46 ng/ml

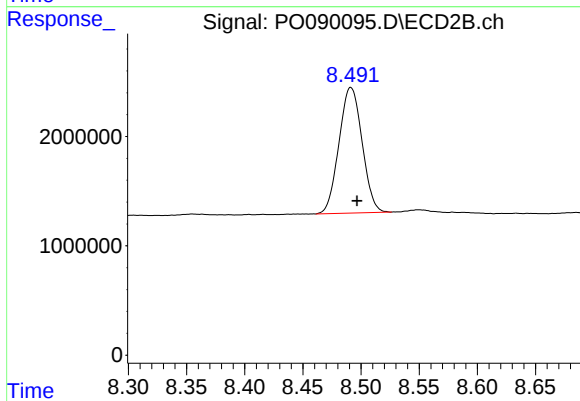

#2 Decachlorobiphenyl


R.T.: 8.491 min
Delta R.T.: -0.005 min
Response: 15891720
Conc: 15.43 ng/ml

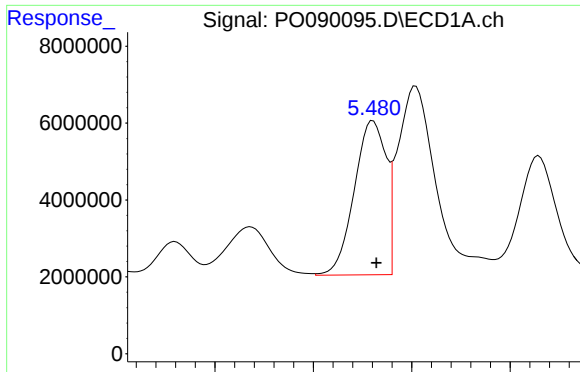

#3 AR-1016-1


R.T.: 5.480 min
Delta R.T.: -0.002 min
Response: 44899037
Conc: 422.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

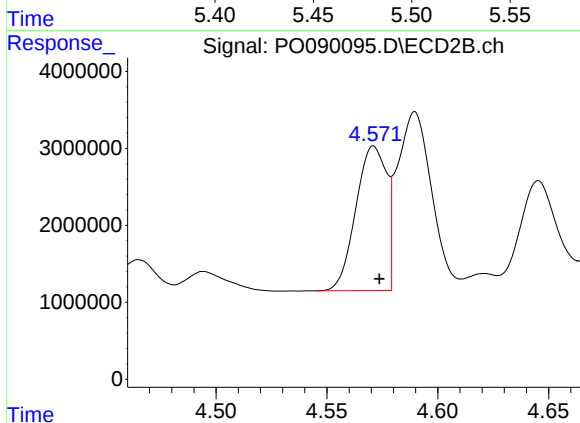


#3 AR-1016-1

R.T.: 4.571 min
Delta R.T.: -0.003 min
Response: 18111833
Conc: 468.89 ng/ml

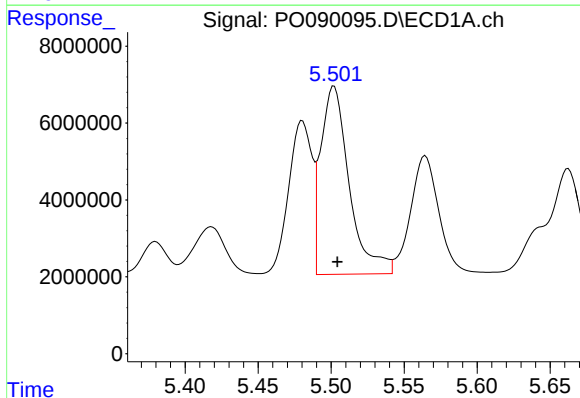


#4 AR-1016-2

R.T.: 5.502 min
Delta R.T.: -0.002 min
Response: 66566572
Conc: 436.98 ng/ml

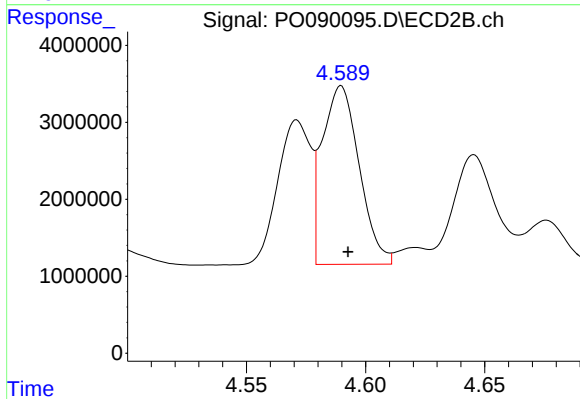

#4 AR-1016-2


R.T.: 4.590 min
Delta R.T.: -0.003 min
Response: 24991126
Conc: 467.18 ng/ml

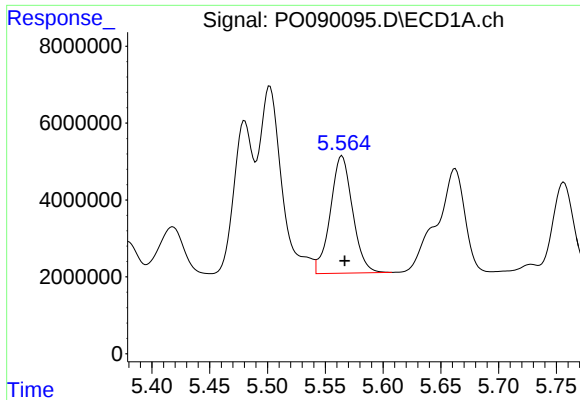

#5 AR-1016-3


R.T.: 5.565 min
Delta R.T.: -0.002 min
Response: 40827773
Conc: 432.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

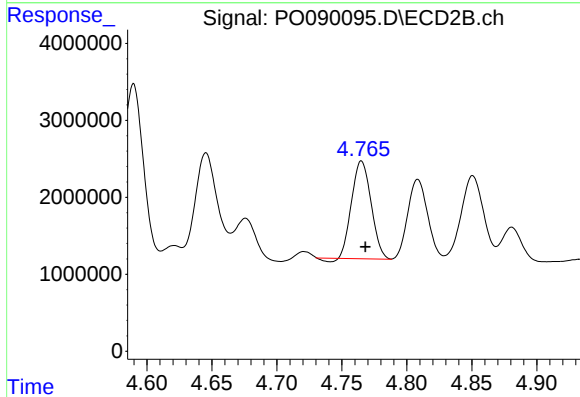


#5 AR-1016-3

R.T.: 4.765 min
Delta R.T.: -0.003 min
Response: 13136137
Conc: 452.46 ng/ml

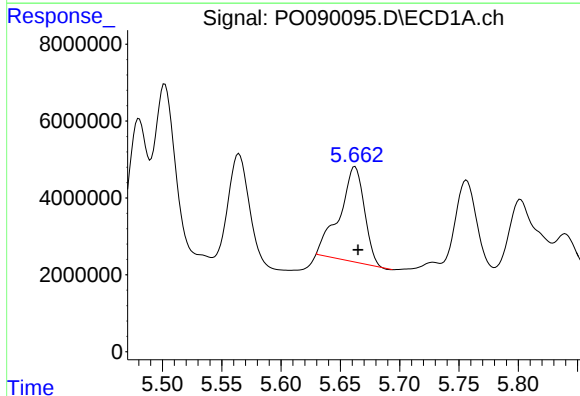


#6 AR-1016-4

R.T.: 5.662 min
Delta R.T.: -0.003 min
Response: 36159916
Conc: 482.21 ng/ml

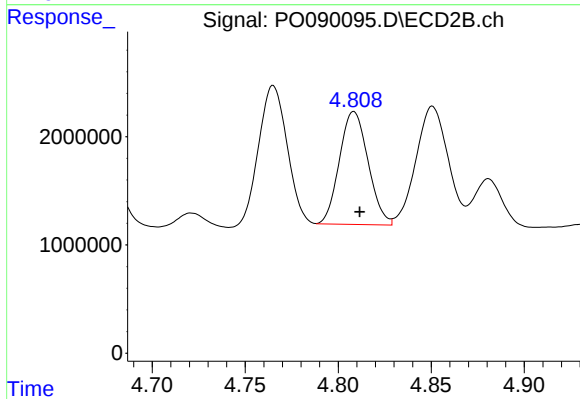

#6 AR-1016-4


R.T.: 4.808 min
Delta R.T.: -0.003 min
Response: 11197166
Conc: 451.08 ng/ml

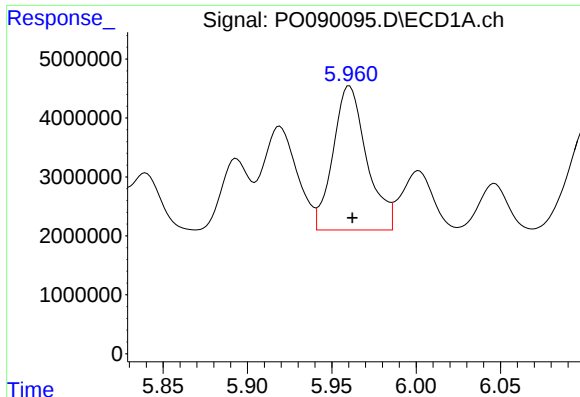

#7 AR-1016-5


R.T.: 5.960 min
Delta R.T.: -0.002 min
Response: 33945218
Conc: 439.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

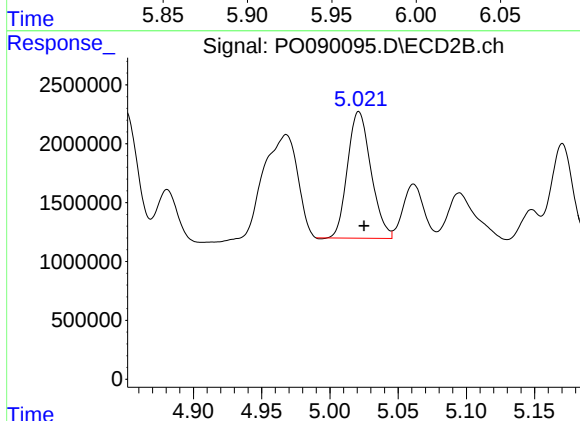


#7 AR-1016-5

R.T.: 5.021 min
Delta R.T.: -0.004 min
Response: 12871671
Conc: 419.01 ng/ml

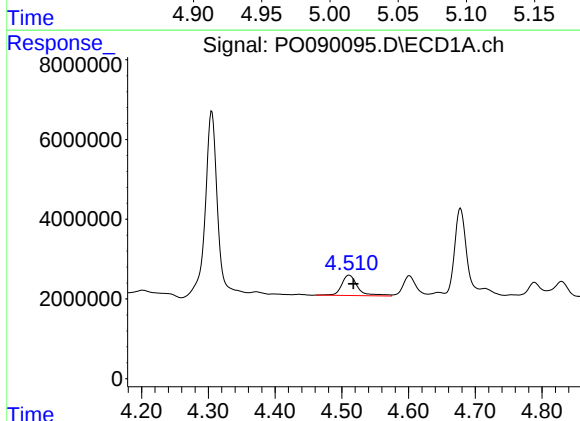


#8 AR-1221-1

R.T.: 4.511 min
Delta R.T.: -0.007 min
Response: 8551458
Conc: 224.03 ng/ml

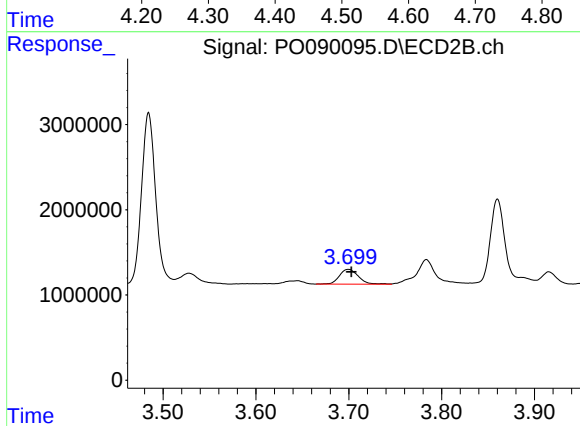

#8 AR-1221-1


R.T.: 3.700 min
Delta R.T.: -0.003 min
Response: 2467614
Conc: 184.70 ng/ml

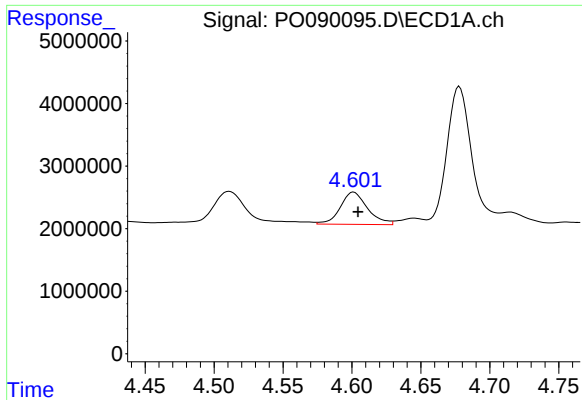

#9 AR-1221-2


R.T.: 4.601 min
Delta R.T.: -0.003 min
Response: 7070591
Conc: 248.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

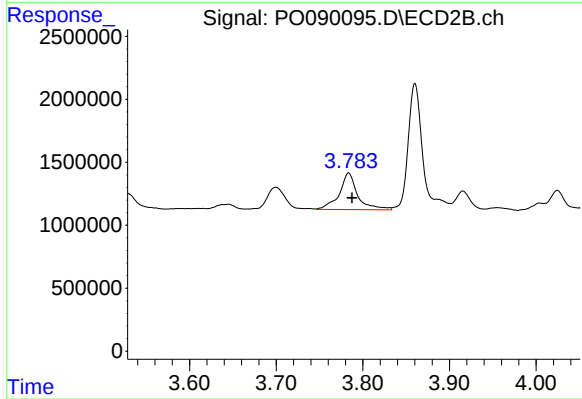


#9 AR-1221-2

R.T.: 3.784 min
Delta R.T.: -0.004 min
Response: 4292717
Conc: 422.98 ng/ml

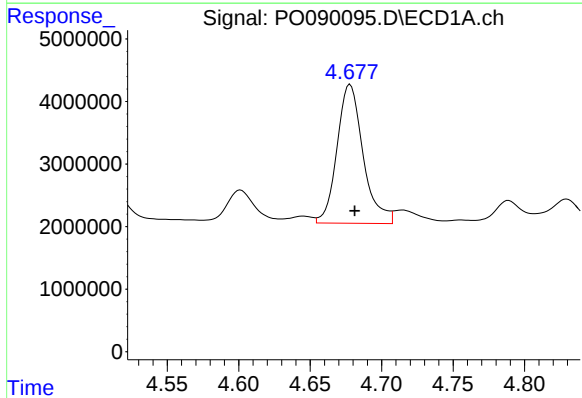


#10 AR-1221-3

R.T.: 4.678 min
Delta R.T.: -0.003 min
Response: 28247407
Conc: 329.88 ng/ml

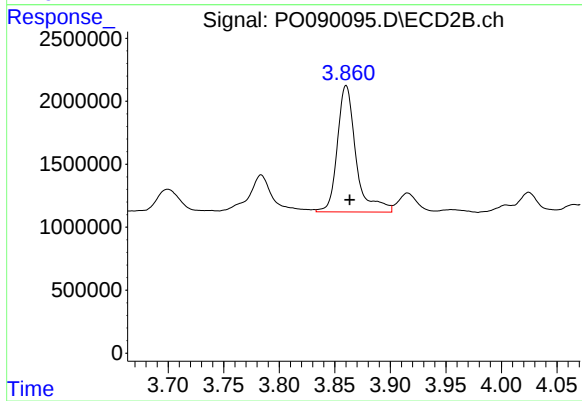

#10 AR-1221-3


R.T.: 3.860 min
Delta R.T.: -0.003 min
Response: 11743023
Conc: 377.49 ng/ml

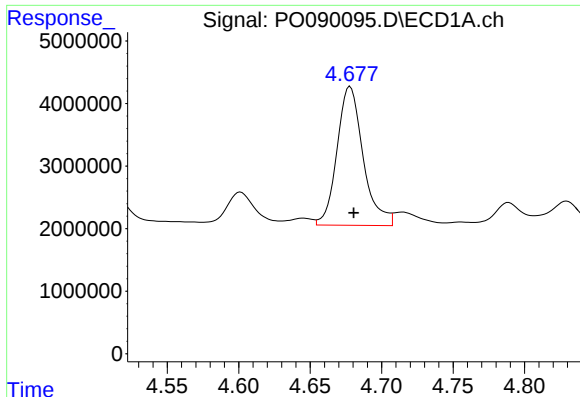

#11 AR-1232-1


R.T.: 4.678 min
Delta R.T.: -0.003 min
Response: 28247407
Conc: 431.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

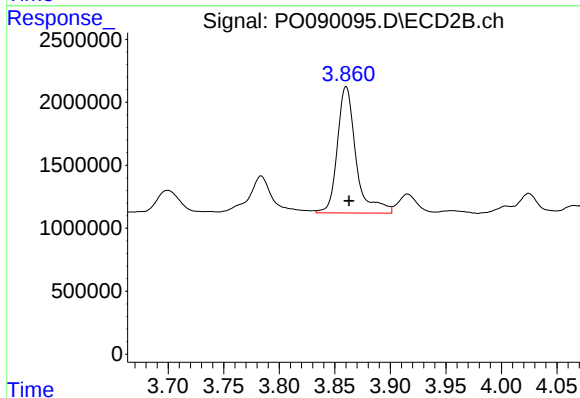


#11 AR-1232-1

R.T.: 3.860 min
Delta R.T.: -0.002 min
Response: 11743023
Conc: 493.60 ng/ml

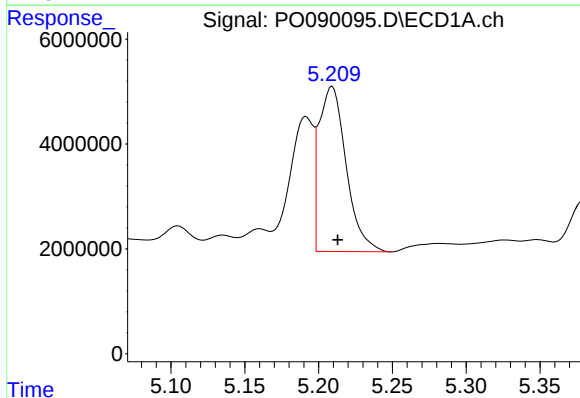


#12 AR-1232-2

R.T.: 5.209 min
Delta R.T.: -0.004 min
Response: 40386494
Conc: 1050.59 ng/ml

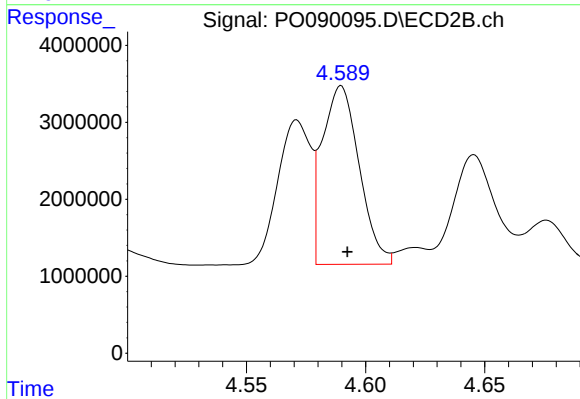

#12 AR-1232-2


R.T.: 4.590 min
Delta R.T.: -0.003 min
Response: 24991126
Conc: 1042.89 ng/ml

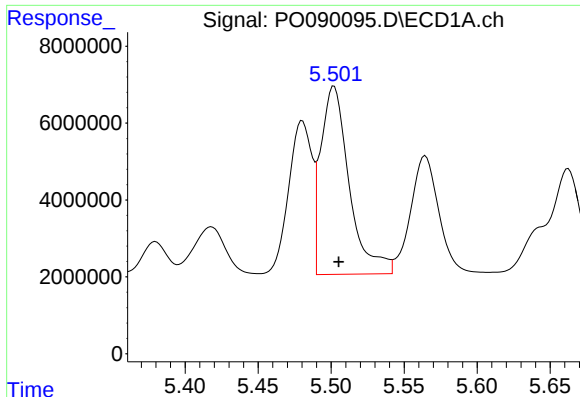

#13 AR-1232-3


R.T.: 5.502 min
Delta R.T.: -0.003 min
Response: 66566572
Conc: 993.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

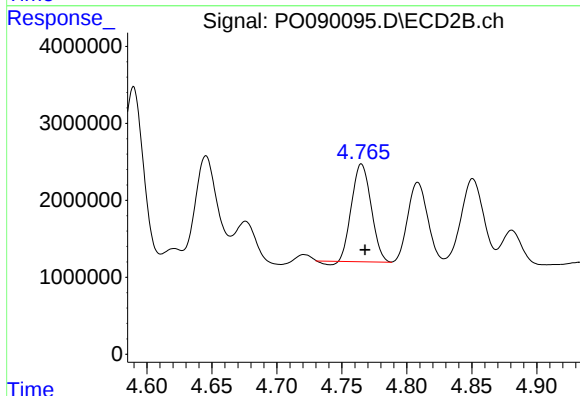


#13 AR-1232-3

R.T.: 4.765 min
Delta R.T.: -0.003 min
Response: 13136137
Conc: 1034.43 ng/ml

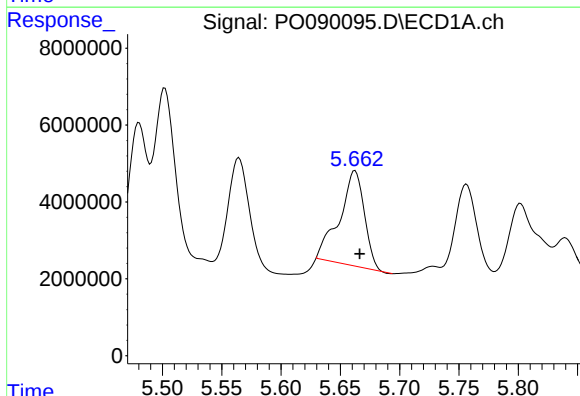


#14 AR-1232-4

R.T.: 5.662 min
Delta R.T.: -0.004 min
Response: 36159916
Conc: 1095.17 ng/ml

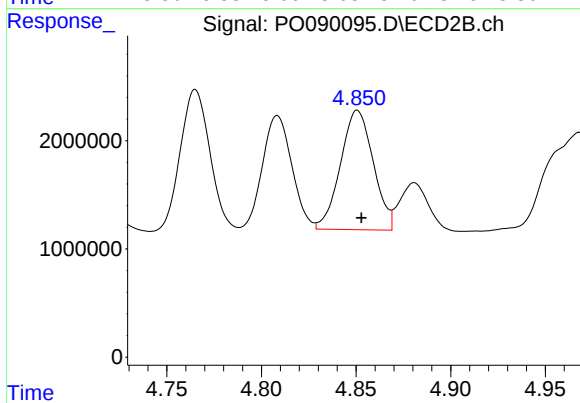

#14 AR-1232-4


R.T.: 4.851 min
Delta R.T.: -0.002 min
Response: 13319864
Conc: 1092.46 ng/ml

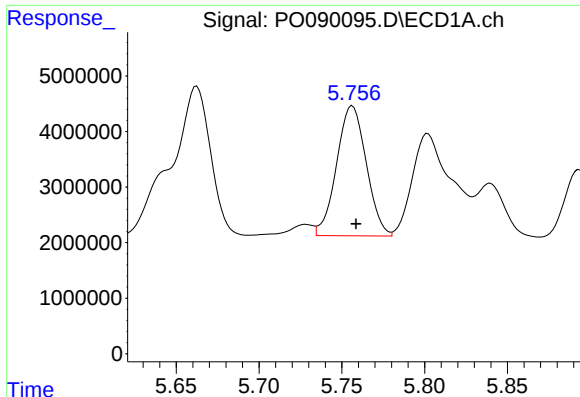

#15 AR-1232-5


R.T.: 5.756 min
Delta R.T.: -0.002 min
Response: 29212360
Conc: 1102.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

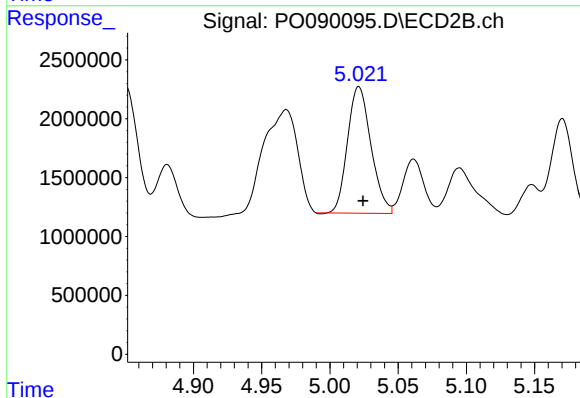


#15 AR-1232-5

R.T.: 5.021 min
Delta R.T.: -0.003 min
Response: 12871671
Conc: 964.04 ng/ml

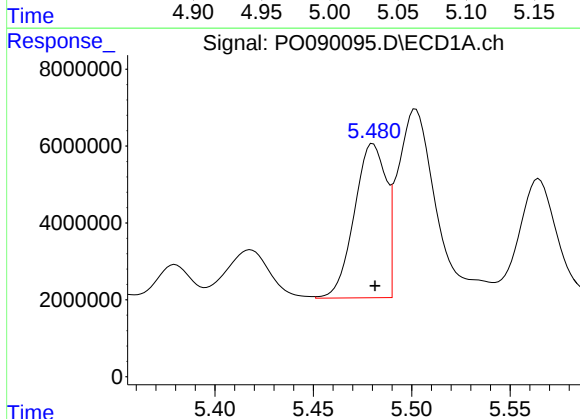


#16 AR-1242-1

R.T.: 5.480 min
Delta R.T.: -0.001 min
Response: 44899037
Conc: 542.65 ng/ml

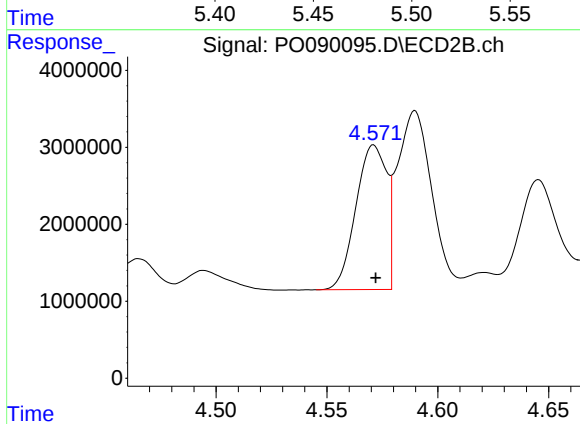

#16 AR-1242-1


R.T.: 4.571 min
Delta R.T.: 0.000 min
Response: 18111833
Conc: 608.36 ng/ml

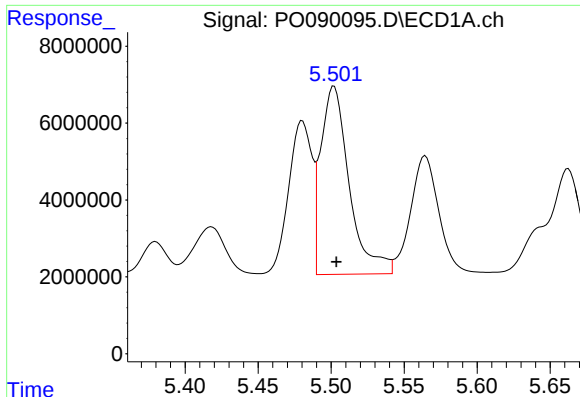

#17 AR-1242-2


R.T.: 5.502 min
Delta R.T.: -0.001 min
Response: 66566572
Conc: 563.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

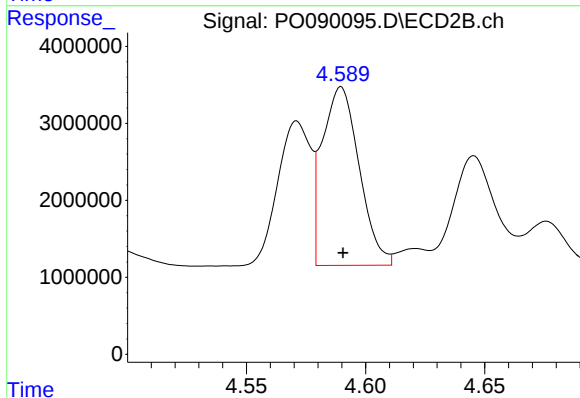


#17 AR-1242-2

R.T.: 4.590 min
Delta R.T.: 0.000 min
Response: 24991126
Conc: 614.41 ng/ml

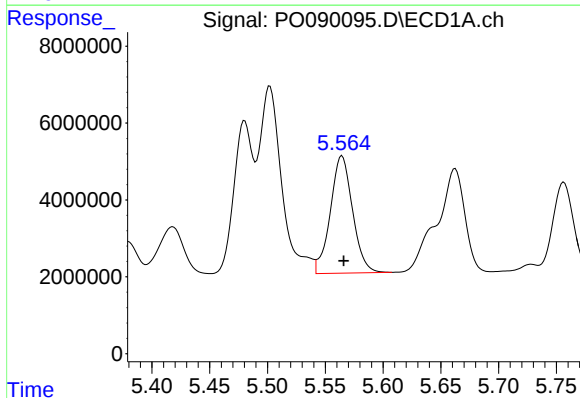


#18 AR-1242-3

R.T.: 5.565 min
Delta R.T.: -0.002 min
Response: 40827773
Conc: 548.49 ng/ml

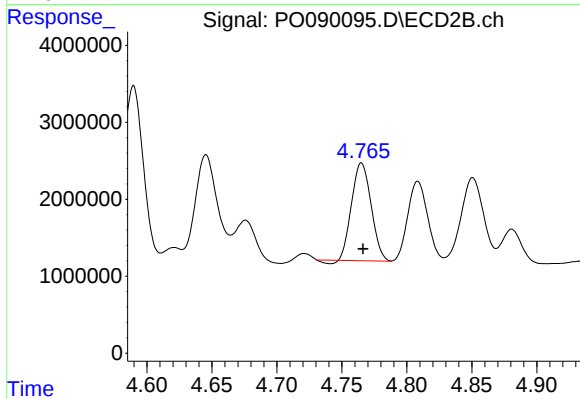

#18 AR-1242-3


R.T.: 4.765 min
Delta R.T.: -0.001 min
Response: 13136137
Conc: 594.06 ng/ml

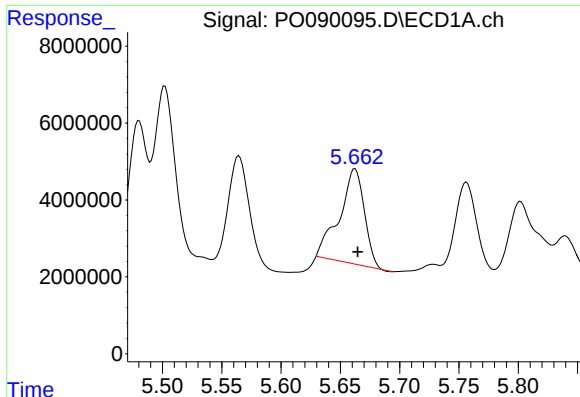

#19 AR-1242-4


R.T.: 5.662 min
Delta R.T.: -0.002 min
Response: 36159916
Conc: 620.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

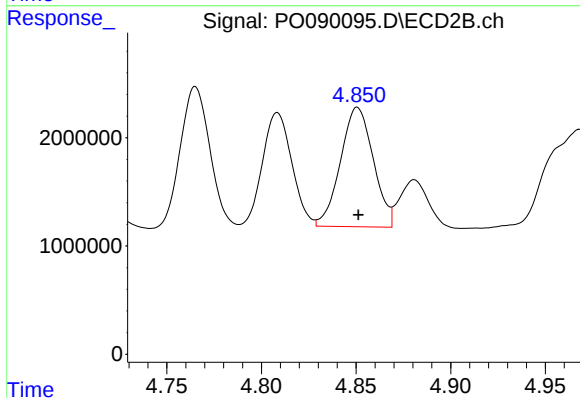


#19 AR-1242-4

R.T.: 4.851 min
Delta R.T.: 0.000 min
Response: 13319864
Conc: 561.70 ng/ml

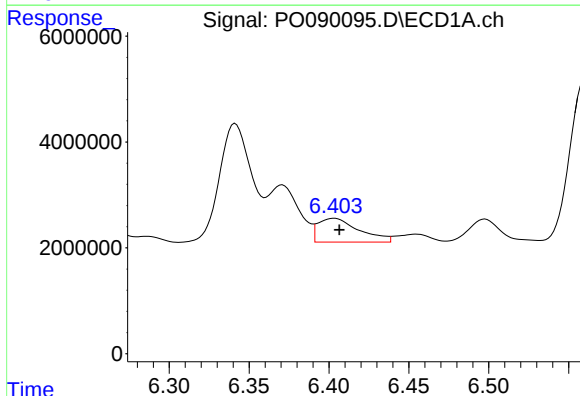


#20 AR-1242-5

R.T.: 6.403 min
Delta R.T.: -0.003 min
Response: 8056754
Conc: 131.07 ng/ml

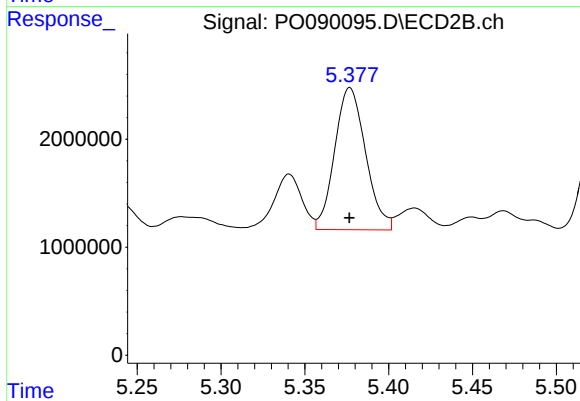

#20 AR-1242-5


R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 16875706
Conc: 589.96 ng/ml

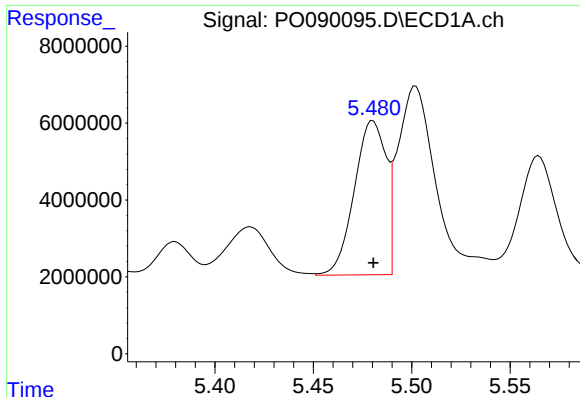

#21 AR-1248-1


R.T.: 5.480 min
Delta R.T.: 0.000 min
Response: 44899037
Conc: 709.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

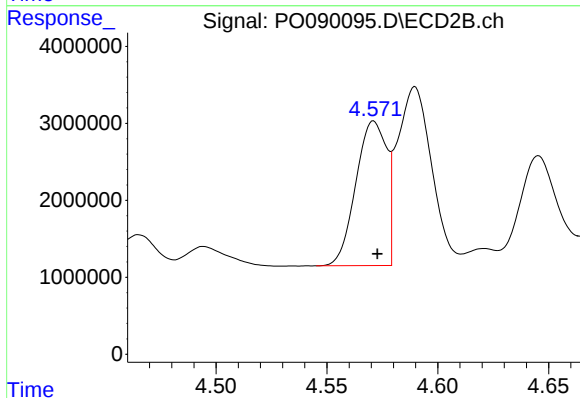


#21 AR-1248-1

R.T.: 4.571 min
Delta R.T.: -0.002 min
Response: 18111833
Conc: 797.80 ng/ml

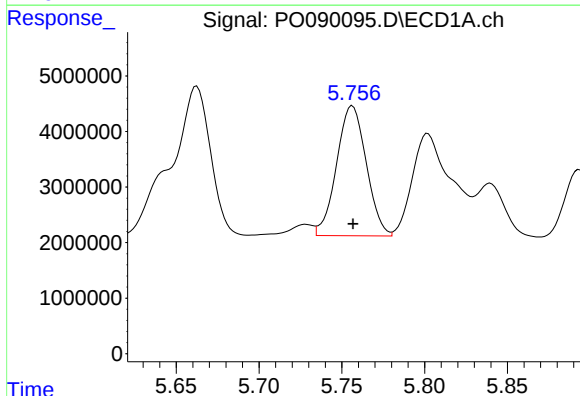


#22 AR-1248-2

R.T.: 5.756 min
Delta R.T.: 0.000 min
Response: 29212360
Conc: 308.47 ng/ml

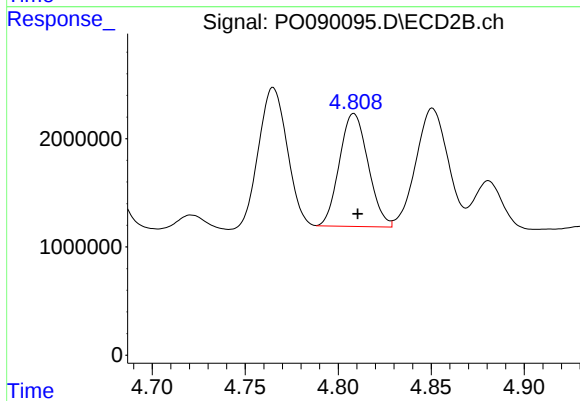

#22 AR-1248-2


R.T.: 4.808 min
Delta R.T.: -0.002 min
Response: 11197166
Conc: 344.40 ng/ml

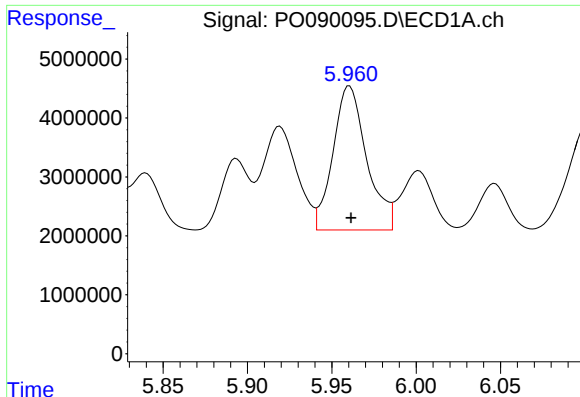

#23 AR-1248-3


R.T.: 5.960 min
Delta R.T.: 0.000 min
Response: 33945218
Conc: 344.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

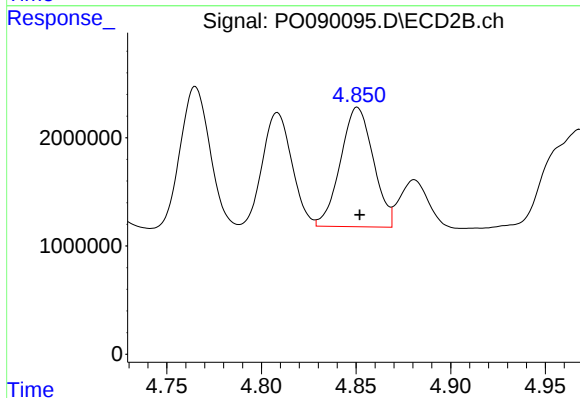


#23 AR-1248-3

R.T.: 4.851 min
Delta R.T.: -0.001 min
Response: 13319864
Conc: 395.15 ng/ml

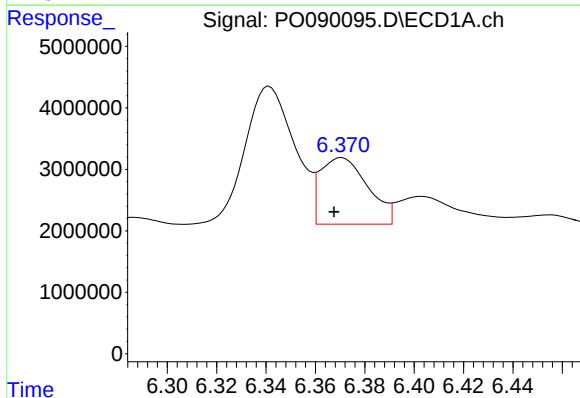


#24 AR-1248-4

R.T.: 6.371 min
Delta R.T.: 0.003 min
Response: 14504665
Conc: 136.04 ng/ml

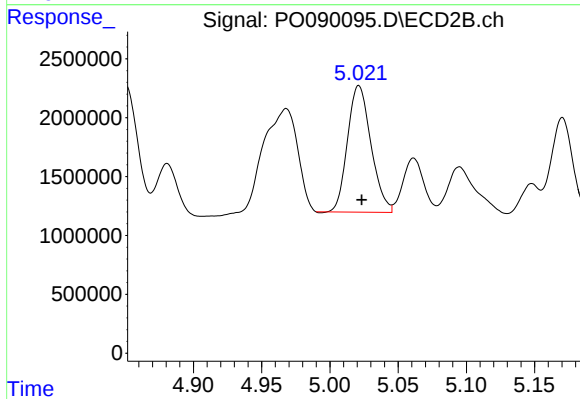

#24 AR-1248-4


R.T.: 5.021 min
Delta R.T.: -0.002 min
Response: 12871671
Conc: 332.83 ng/ml

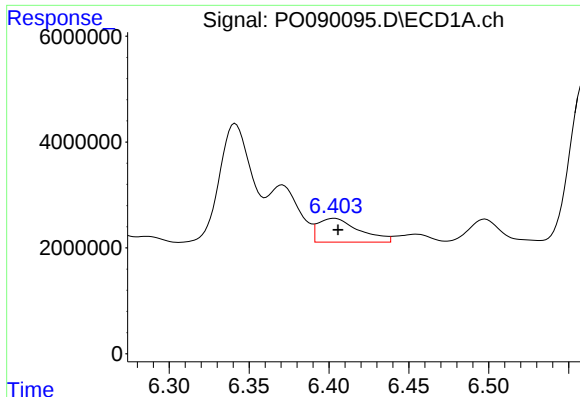

#25 AR-1248-5


R.T.: 6.403 min
Delta R.T.: -0.002 min
Response: 8056754
Conc: 76.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

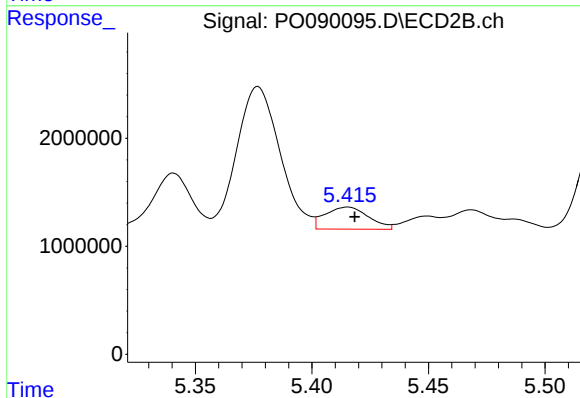


#25 AR-1248-5

R.T.: 5.415 min
Delta R.T.: -0.003 min
Response: 2655226
Conc: 73.33 ng/ml

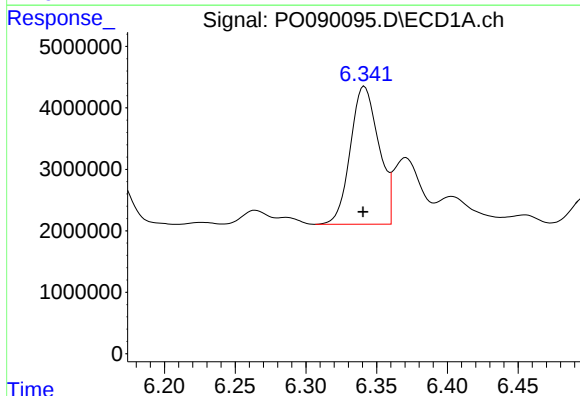


#26 AR-1254-1

R.T.: 6.341 min
Delta R.T.: 0.001 min
Response: 31405007
Conc: 270.97 ng/ml

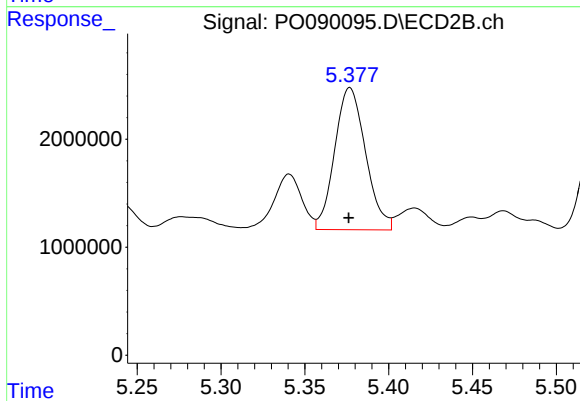

#26 AR-1254-1


R.T.: 5.377 min
Delta R.T.: 0.000 min
Response: 16875706
Conc: 286.49 ng/ml

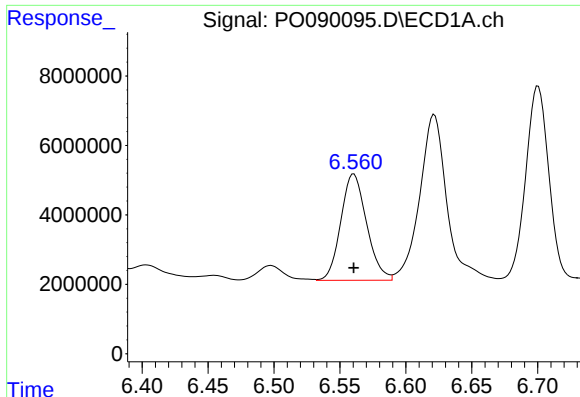

#27 AR-1254-2


R.T.: 6.561 min
Delta R.T.: 0.000 min
Response: 41710487
Conc: 239.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

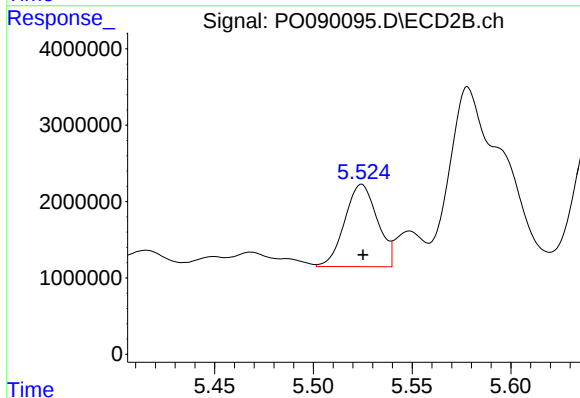


#27 AR-1254-2

R.T.: 5.524 min
Delta R.T.: 0.000 min
Response: 12381333
Conc: 231.08 ng/ml

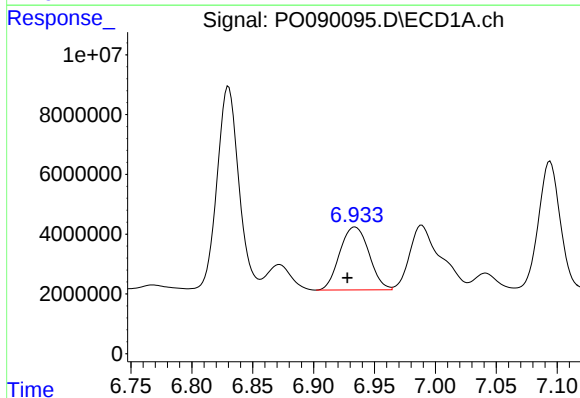


#28 AR-1254-3

R.T.: 6.934 min
Delta R.T.: 0.006 min
Response: 35177158
Conc: 202.63 ng/ml

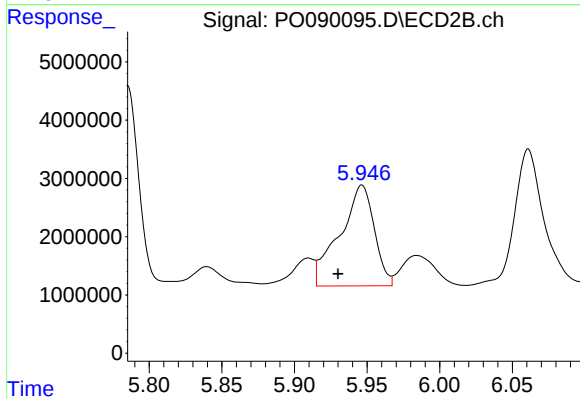

#28 AR-1254-3


R.T.: 5.946 min
Delta R.T.: 0.016 min
Response: 28641474
Conc: 345.57 ng/ml

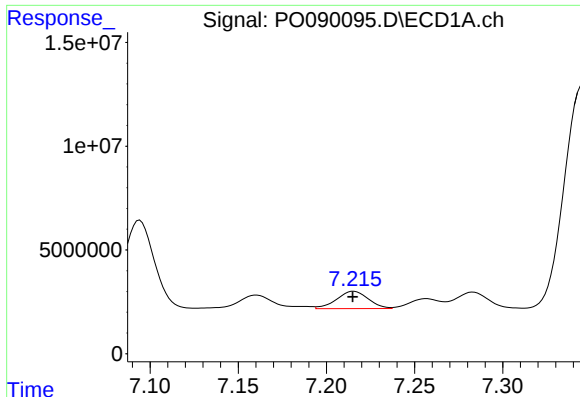

#29 AR-1254-4


R.T.: 7.216 min
Delta R.T.: 0.000 min
Response: 10408428
Conc: 81.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

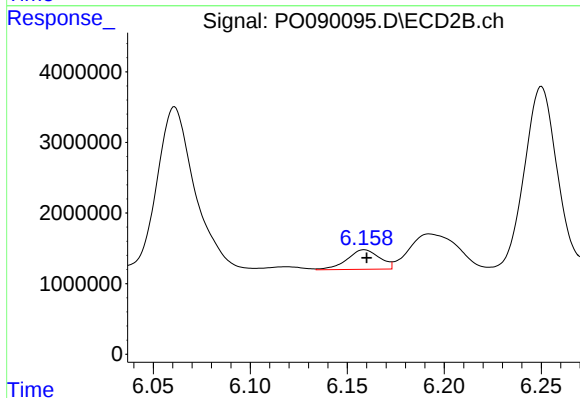


#29 AR-1254-4

R.T.: 6.159 min
Delta R.T.: -0.001 min
Response: 3214829
Conc: 64.73 ng/ml

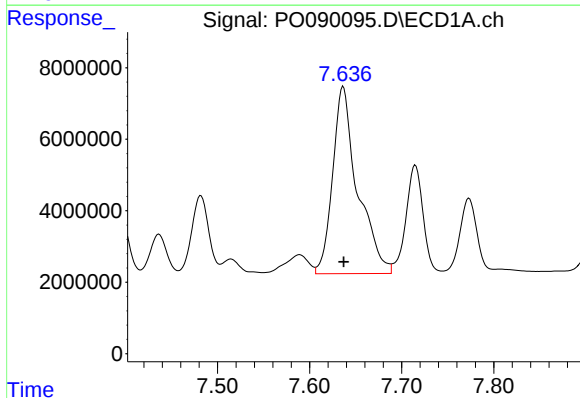


#30 AR-1254-5

R.T.: 7.636 min
Delta R.T.: 0.000 min
Response: 98435342
Conc: 698.82 ng/ml

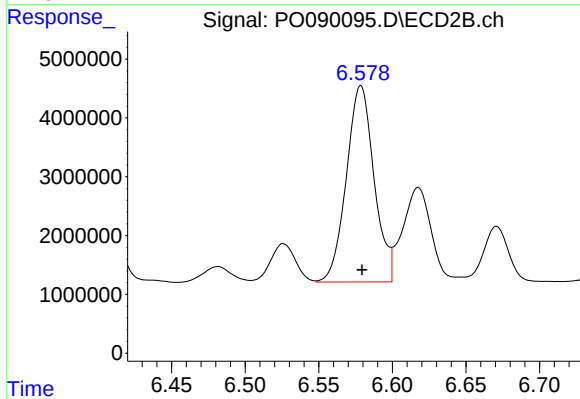

#30 AR-1254-5


R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 43675010
Conc: 583.30 ng/ml

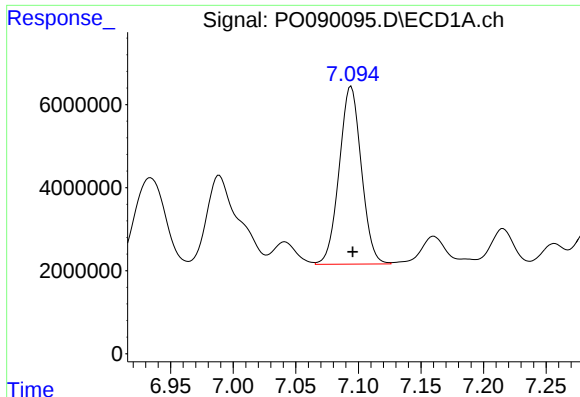

#31 AR-1260-1


R.T.: 7.094 min
Delta R.T.: -0.001 min
Response: 52777393
Conc: 376.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

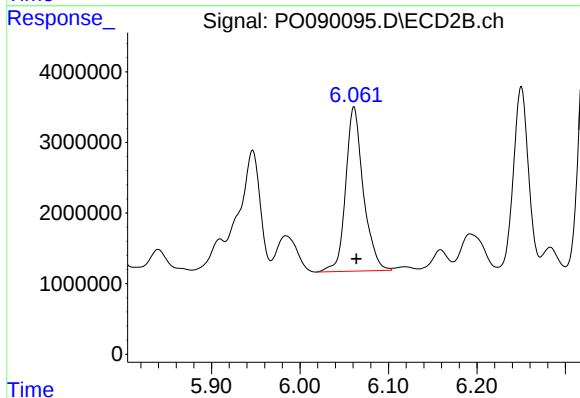


#31 AR-1260-1

R.T.: 6.061 min
Delta R.T.: -0.003 min
Response: 32343393
Conc: 537.25 ng/ml

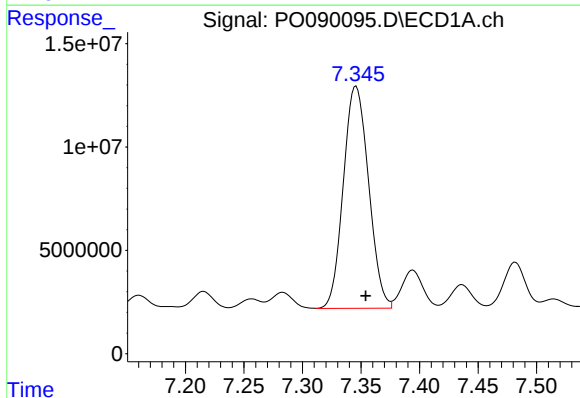


#32 AR-1260-2

R.T.: 7.346 min
Delta R.T.: -0.008 min
Response: 161305205
Conc: 997.07 ng/ml

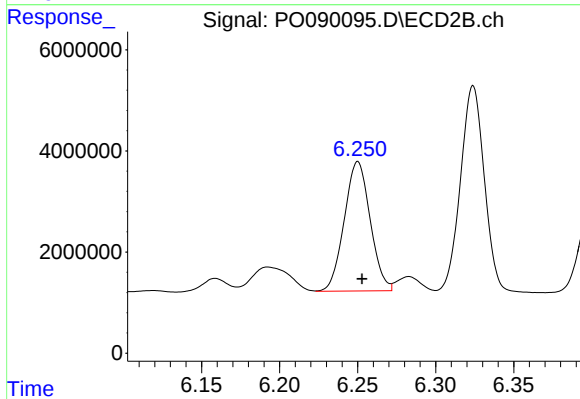

#32 AR-1260-2


R.T.: 6.250 min
Delta R.T.: -0.003 min
Response: 29621000
Conc: 410.02 ng/ml

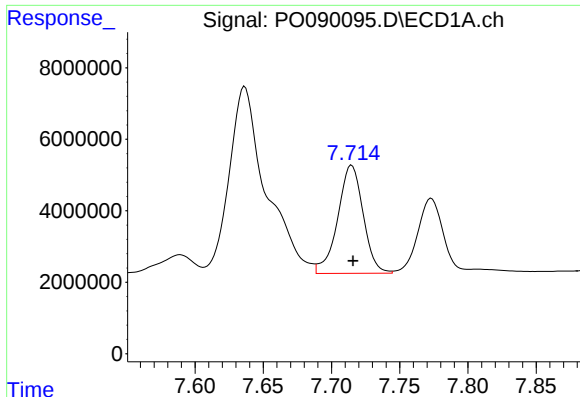

#33 AR-1260-3


R.T.: 7.715 min
Delta R.T.: -0.001 min
Response: 39283272
Conc: 373.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

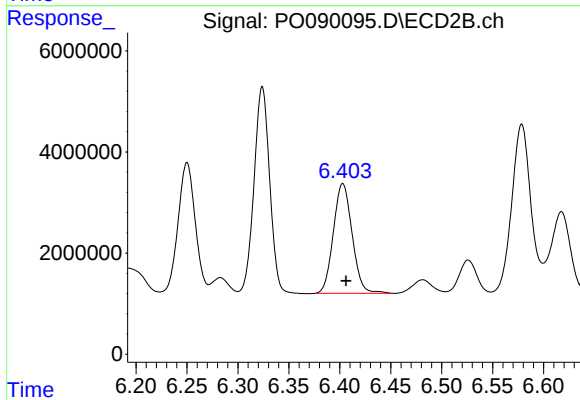


#33 AR-1260-3

R.T.: 6.403 min
Delta R.T.: -0.003 min
Response: 27798024
Conc: 417.18 ng/ml

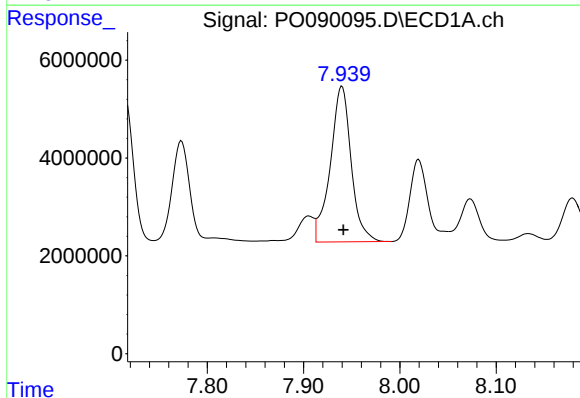


#34 AR-1260-4

R.T.: 7.940 min
Delta R.T.: -0.001 min
Response: 47865685
Conc: 387.45 ng/ml

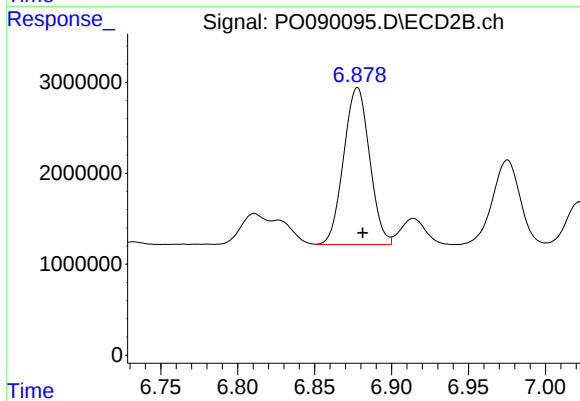

#34 AR-1260-4


R.T.: 6.878 min
Delta R.T.: -0.003 min
Response: 20184475
Conc: 396.75 ng/ml

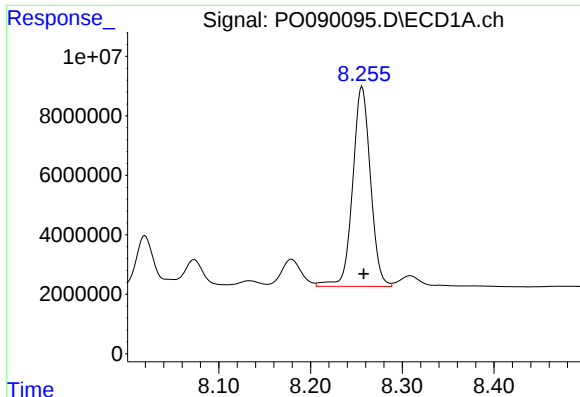

#35 AR-1260-5


R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 90503315
Conc: 397.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

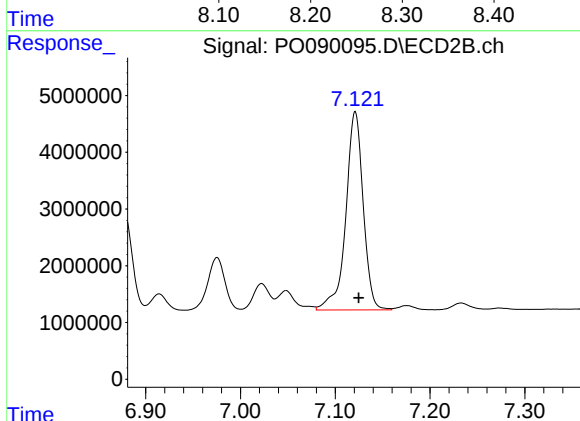


#35 AR-1260-5

R.T.: 7.121 min
Delta R.T.: -0.004 min
Response: 44538455
Conc: 383.45 ng/ml

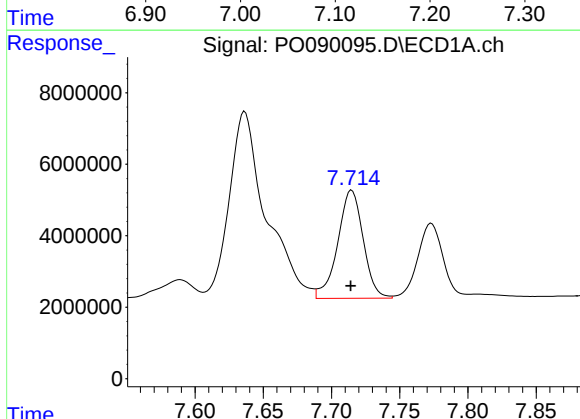


#36 AR-1262-1

R.T.: 7.715 min
Delta R.T.: 0.000 min
Response: 39283272
Conc: 236.98 ng/ml

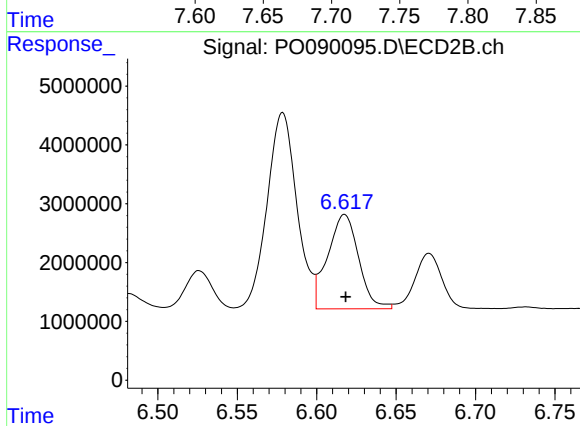

#36 AR-1262-1


R.T.: 6.618 min
Delta R.T.: 0.000 min
Response: 21710044
Conc: 286.52 ng/ml

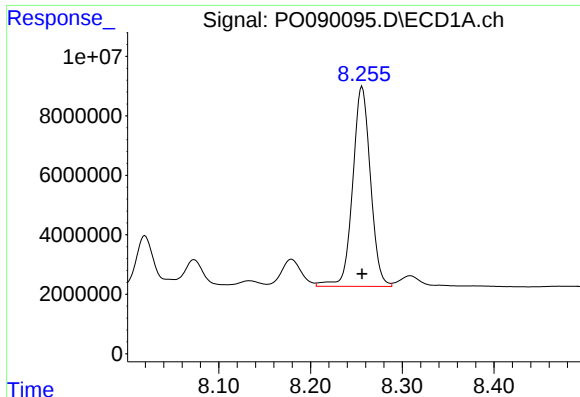

#37 AR-1262-2


R.T.: 8.256 min
Delta R.T.: 0.000 min
Response: 90503315
Conc: 322.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

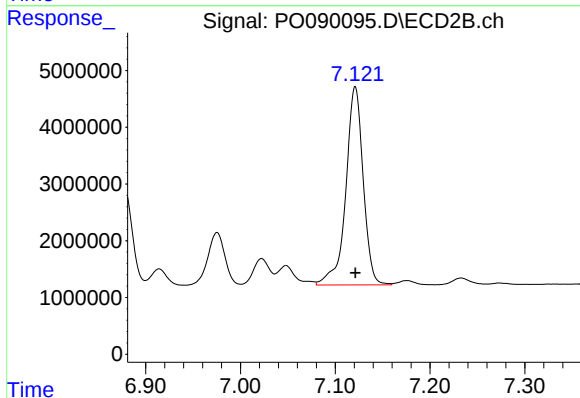


#37 AR-1262-2

R.T.: 7.121 min
Delta R.T.: 0.000 min
Response: 44538455
Conc: 347.33 ng/ml

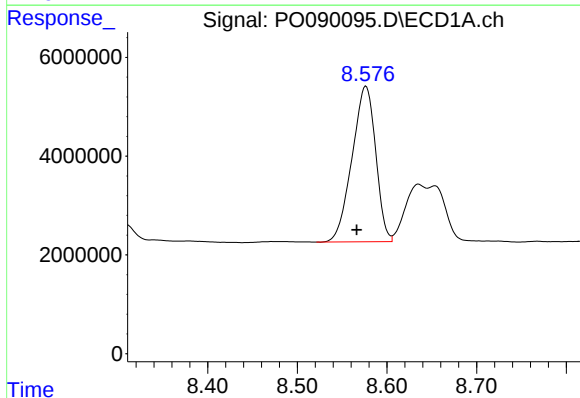


#38 AR-1262-3

R.T.: 8.577 min
Delta R.T.: 0.010 min
Response: 57694942
Conc: 293.83 ng/ml

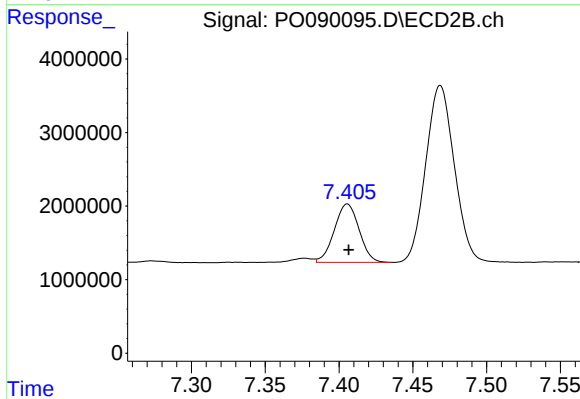

#38 AR-1262-3


R.T.: 7.406 min
Delta R.T.: 0.000 min
Response: 9262853
Conc: 170.09 ng/ml

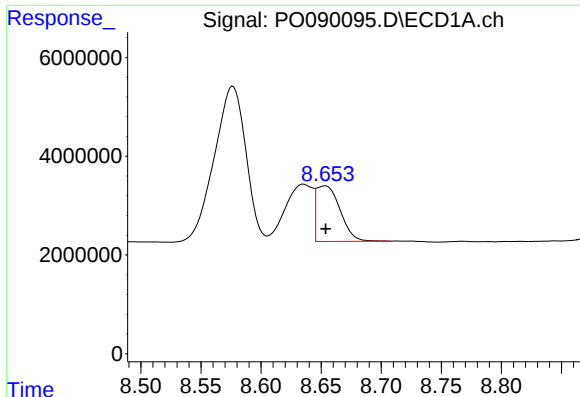

#39 AR-1262-4


R.T.: 8.654 min
Delta R.T.: 0.000 min
Response: 15486225
Conc: 159.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

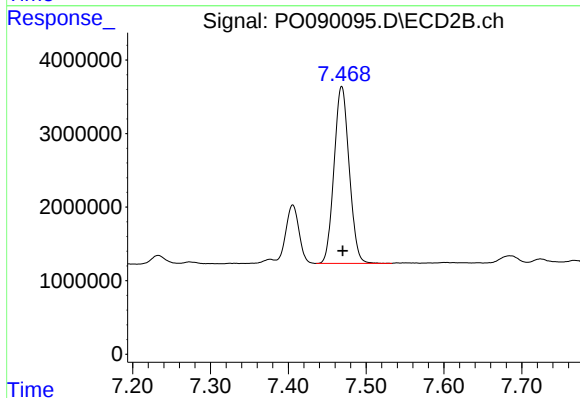


#39 AR-1262-4

R.T.: 7.469 min
Delta R.T.: -0.001 min
Response: 32469321
Conc: 334.32 ng/ml

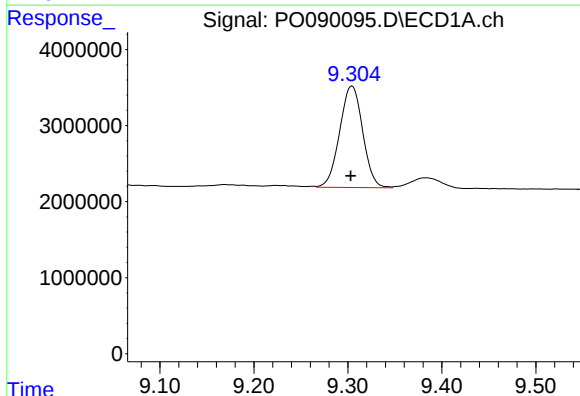


#40 AR-1262-5

R.T.: 9.304 min
Delta R.T.: 0.001 min
Response: 22715635
Conc: 215.58 ng/ml

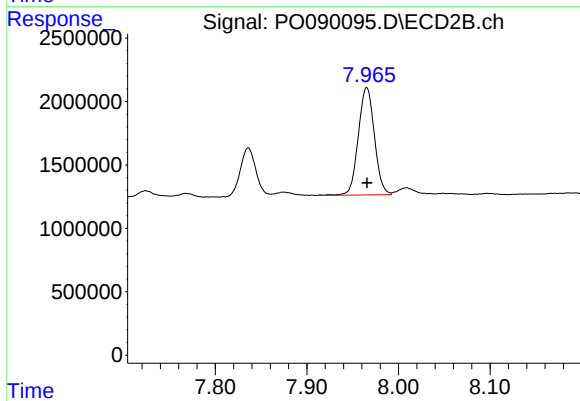

#40 AR-1262-5


R.T.: 7.965 min
Delta R.T.: 0.000 min
Response: 10362150
Conc: 218.33 ng/ml

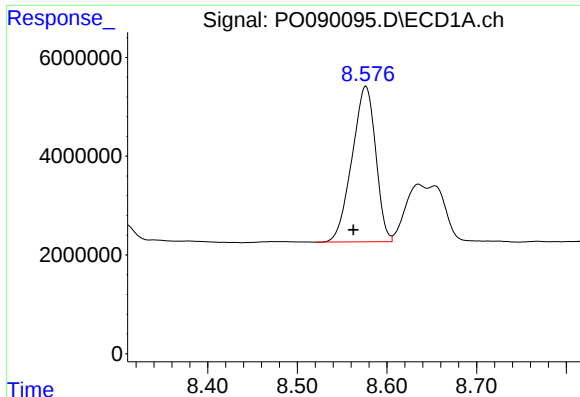

#41 AR-1268-1


R.T.: 8.577 min
Delta R.T.: 0.014 min
Response: 57694942
Conc: 165.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

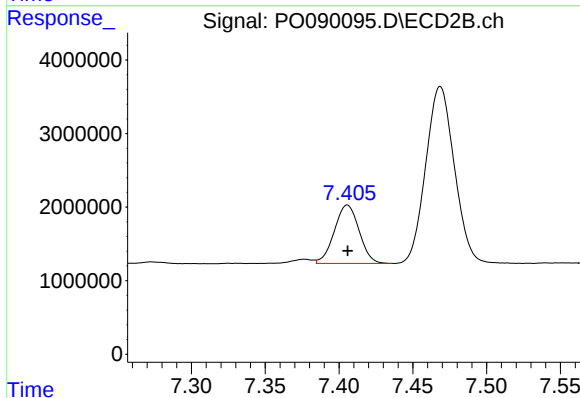


#41 AR-1268-1

R.T.: 7.406 min
Delta R.T.: 0.000 min
Response: 9262853
Conc: 58.79 ng/ml

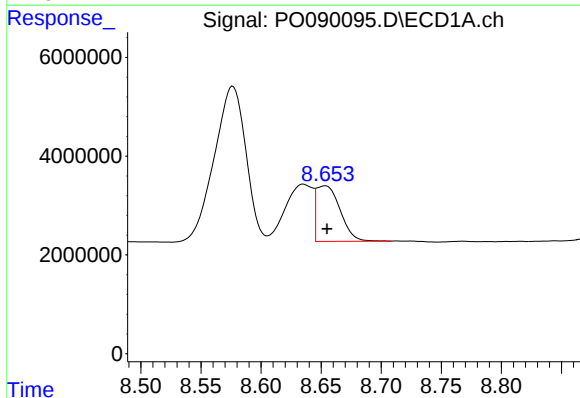


#42 AR-1268-2

R.T.: 8.654 min
Delta R.T.: -0.001 min
Response: 15486225
Conc: 49.64 ng/ml

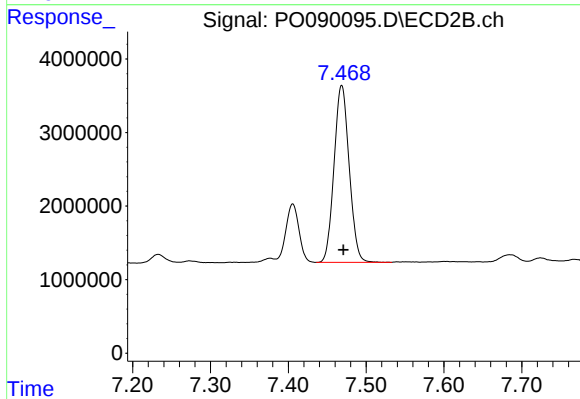

#42 AR-1268-2


R.T.: 7.469 min
Delta R.T.: -0.002 min
Response: 32469321
Conc: 231.42 ng/ml

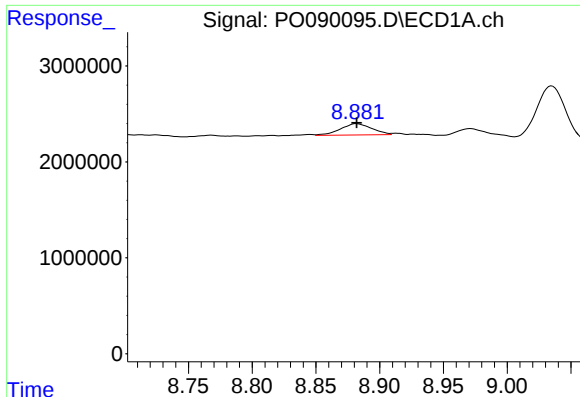

#43 AR-1268-3


R.T.: 8.882 min
Delta R.T.: 0.000 min
Response: 2024609
Conc: 7.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

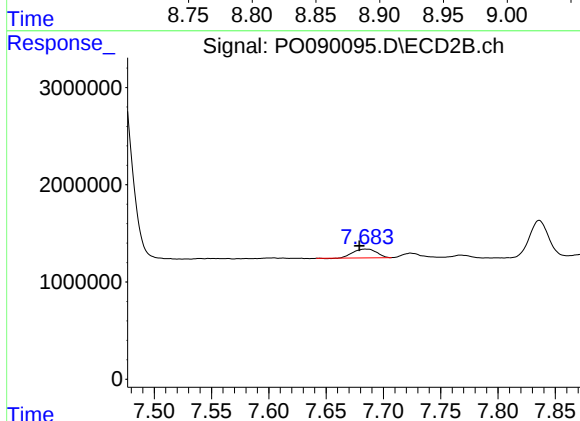


#43 AR-1268-3

R.T.: 7.685 min
Delta R.T.: 0.006 min
Response: 1278395
Conc: 10.65 ng/ml

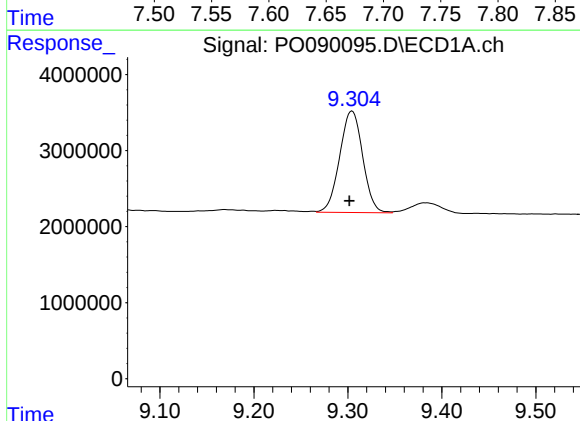


#44 AR-1268-4

R.T.: 9.304 min
Delta R.T.: 0.003 min
Response: 22715635
Conc: 194.95 ng/ml

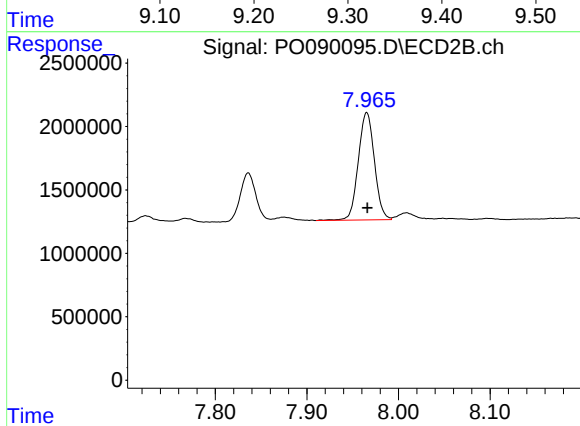

#44 AR-1268-4


R.T.: 7.965 min
Delta R.T.: 0.000 min
Response: 10362150
Conc: 190.80 ng/ml

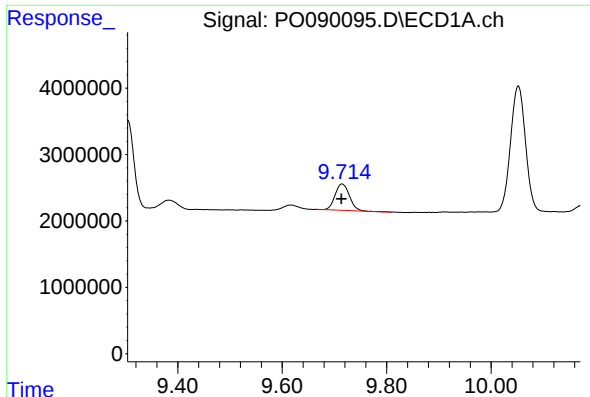

#45 AR-1268-5

R.T.: 9.715 min
Delta R.T.: 0.000 min
Response: 7539548
Conc: 8.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-EMS

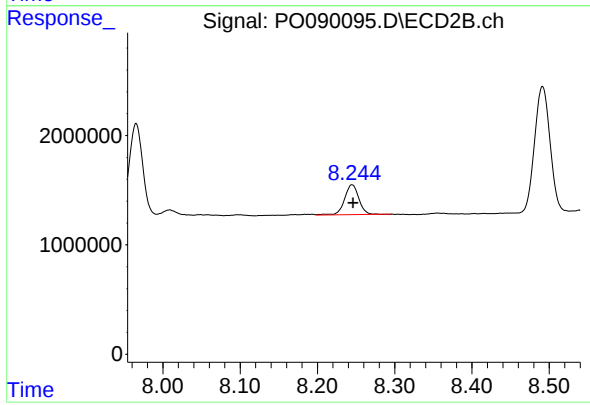

#45 AR-1268-5

R.T.: 8.245 min
Delta R.T.: -0.001 min
Response: 3502639
Conc: 10.01 ng/ml