

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110124\
 Data File : P0107599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 16:15
 Operator : YP/AJ
 Sample : P4662-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 102524-DRIP-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/04/2024
 Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 01:23:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.644	122.6E6	44093068	13.453m	13.700
2) SA Decachlor...	10.073	8.642	46495631	42548655	18.952	15.520
Target Compounds						
26) L6 AR-1254-1	6.378	5.527	7273937	3599122	27.066	21.841m
27) L6 AR-1254-2	6.597	5.674	12484252	3238148	33.079	22.338 #
28) L6 AR-1254-3	6.961	6.077	12474315	6945403	34.864	30.247
29) L6 AR-1254-4	7.246	6.305	10447904	4734618	45.542	36.582
30) L6 AR-1254-5	7.667	6.722	9321001	6230233	44.889m	32.610 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110124\
Data File : PO107599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 16:15
Operator : YP/AJ
Sample : P4662-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
102524-DRIP-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :Ankita Jodhani 11/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 01:23:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

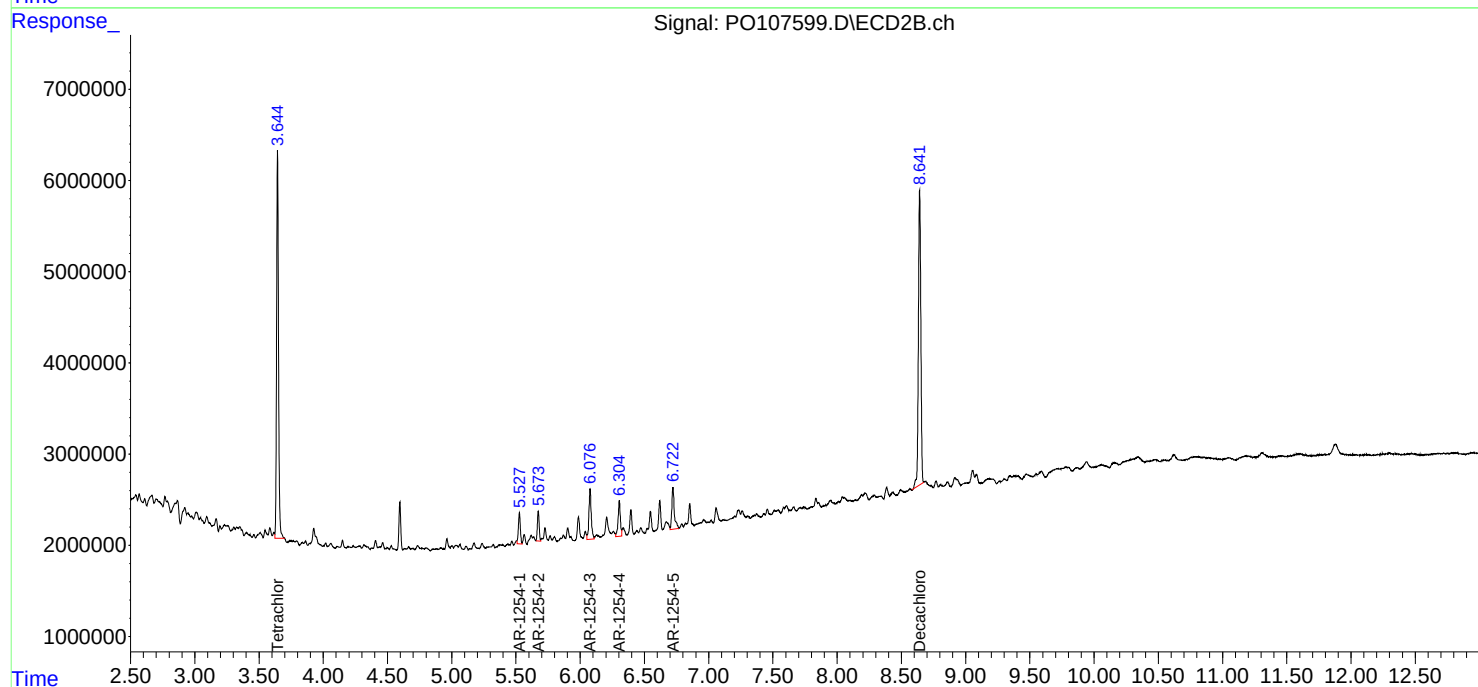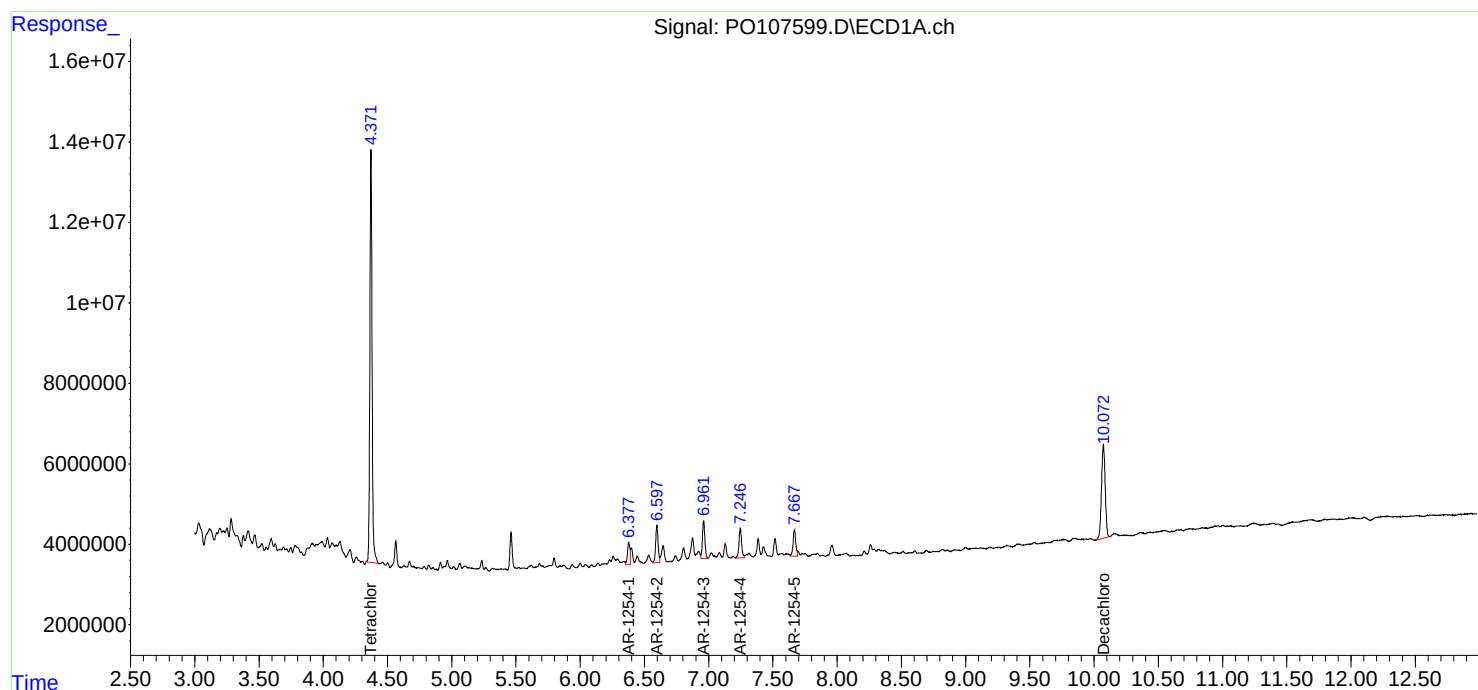

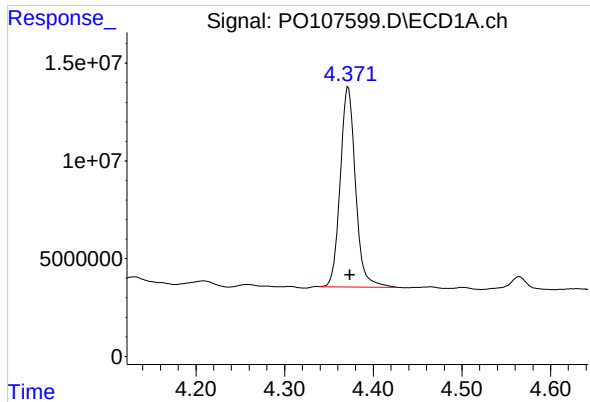


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 122607860
Conc: 13.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
102524-DRIP-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :Ankita Jodhani 11/04/2024

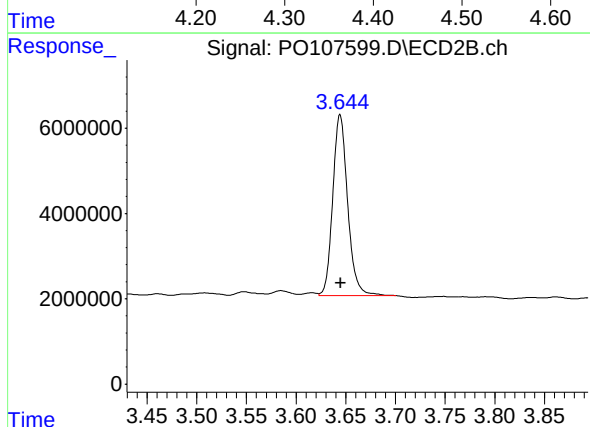


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.000 min
Response: 44093068
Conc: 13.70 ng/ml

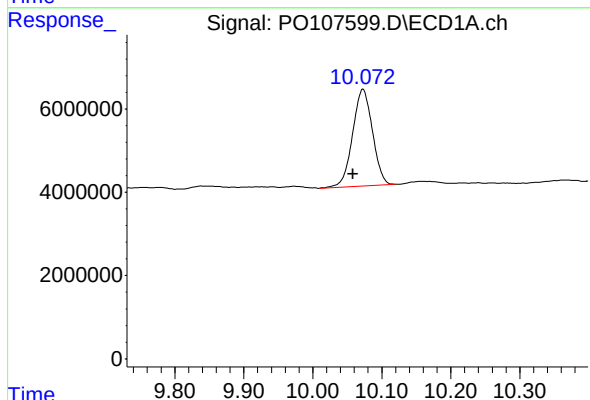


#2 Decachlorobiphenyl

R.T.: 10.073 min
Delta R.T.: 0.014 min
Response: 46495631
Conc: 18.95 ng/ml

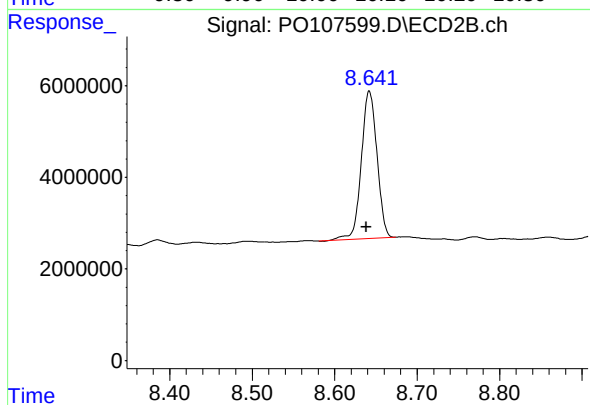

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: 0.003 min
Response: 42548655
Conc: 15.52 ng/ml

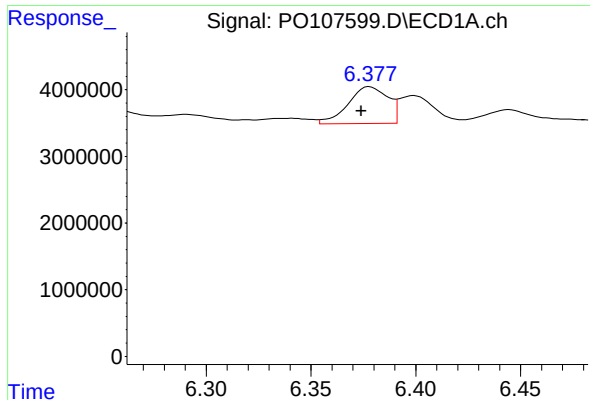


#26 AR-1254-1

R.T.: 6.378 min
Delta R.T.: 0.004 min
Response: 7273937
Conc: 27.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
102524-DRIP-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :Ankita Jodhani 11/04/2024

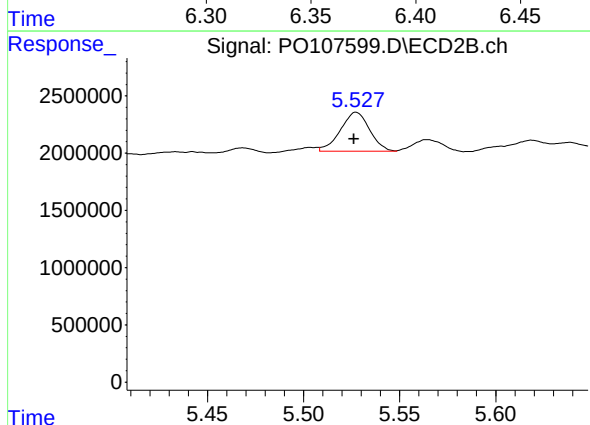


#26 AR-1254-1

R.T.: 5.527 min
Delta R.T.: 0.000 min
Response: 3599122
Conc: 21.84 ng/ml

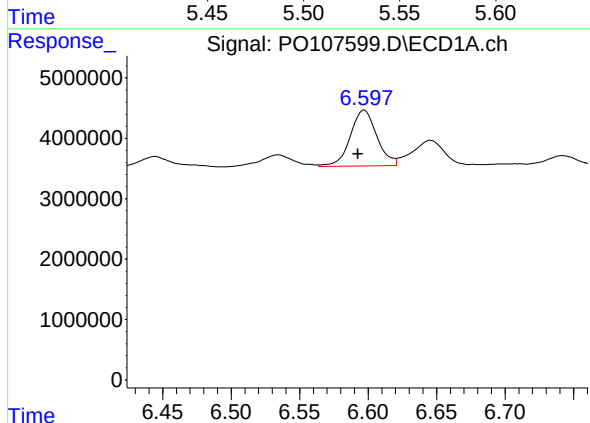


#27 AR-1254-2

R.T.: 6.597 min
Delta R.T.: 0.004 min
Response: 12484252
Conc: 33.08 ng/ml

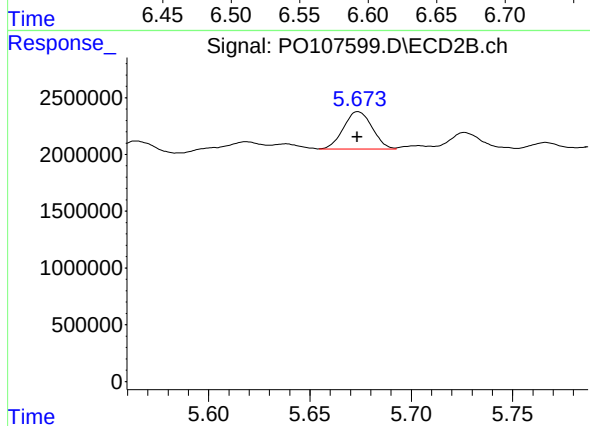

#27 AR-1254-2

R.T.: 5.674 min
Delta R.T.: 0.000 min
Response: 3238148
Conc: 22.34 ng/ml

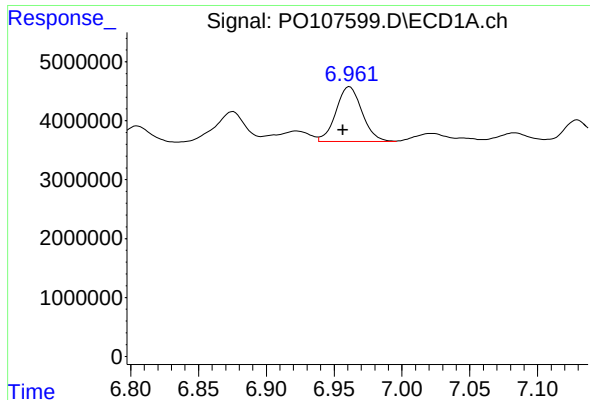


#28 AR-1254-3

R.T.: 6.961 min
Delta R.T.: 0.005 min
Response: 12474315
Conc: 34.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
102524-DRIP-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :Ankita Jodhani 11/04/2024

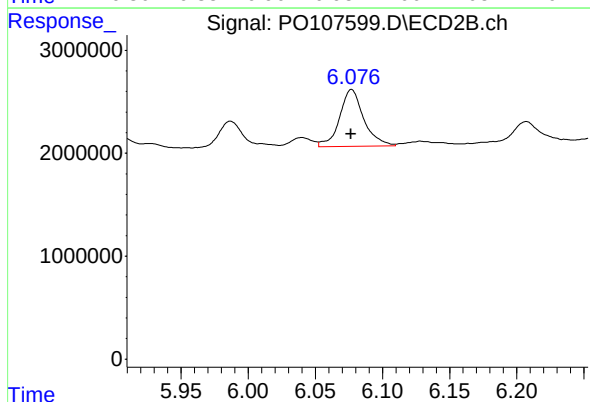


#28 AR-1254-3

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 6945403
Conc: 30.25 ng/ml

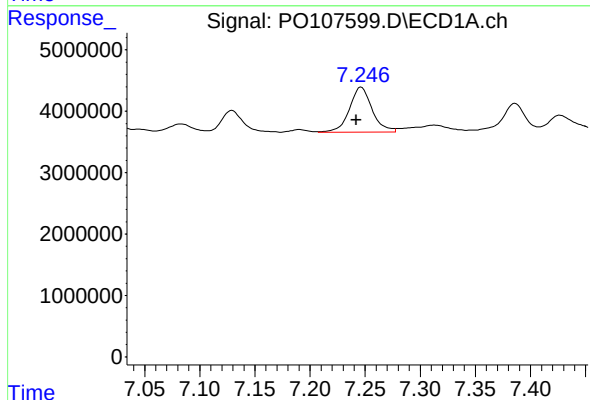


#29 AR-1254-4

R.T.: 7.246 min
Delta R.T.: 0.005 min
Response: 10447904
Conc: 45.54 ng/ml

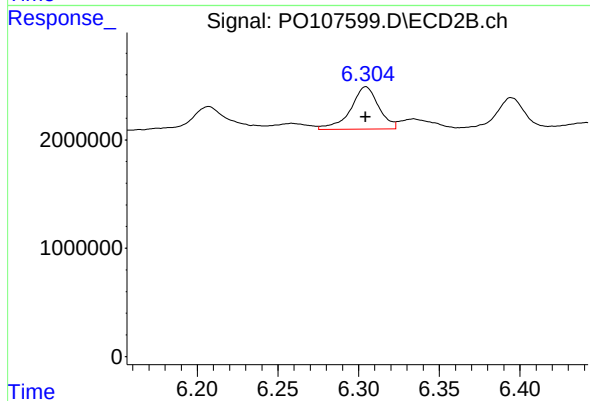

#29 AR-1254-4

R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 4734618
Conc: 36.58 ng/ml

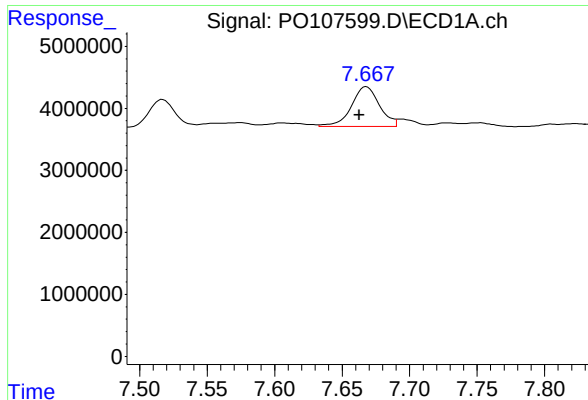


#30 AR-1254-5

R.T.: 7.667 min
Delta R.T.: 0.005 min
Response: 9321001
Conc: 44.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
102524-DRIP-A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/04/2024
Supervised By :Ankita Jodhani 11/04/2024

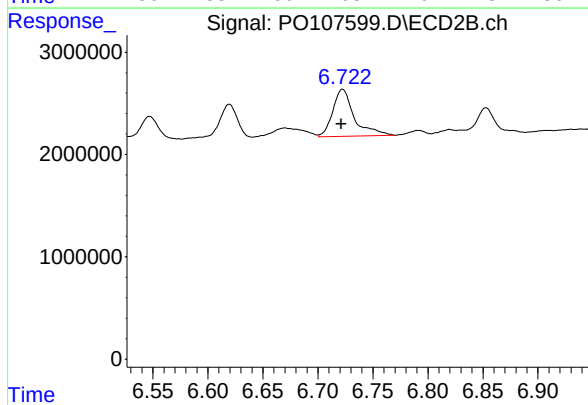

#30 AR-1254-5

R.T.: 6.722 min
Delta R.T.: 0.001 min
Response: 6230233
Conc: 32.61 ng/ml