

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110218\
 Data File : PO050946.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2018 12:03
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 23:00:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.354	3.346	12108441	4978328	24.224	22.904
2)	SA Decachlor...	10.012	8.091	6632058	5236575	21.337	20.472
Target Compounds							
7)	L1 AR-1016-5	0.000	4.810	0	690803	N.D.	80.051 #
15)	L3 AR-1232-5	0.000	4.810	0	690803	N.D.	259.728 #
20)	L4 AR-1242-5	0.000	5.062	0	59515	N.D.	9.238 #
24)	L5 AR-1248-4	0.000	4.810	0	690803	N.D.	74.032 #
26)	L6 AR-1254-1	0.000	5.062	0	59515	N.D.	3.104 #
28)	L6 AR-1254-3	0.000	5.602	0	10631	N.D.	0.376 #
29)	L6 AR-1254-4	0.000	5.929	0	23332	N.D.	1.320 #
32)	L7 AR-1260-2	0.000	5.937	0	28789	N.D.	1.003 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110218\
Data File : PO050946.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 12:03
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:00:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

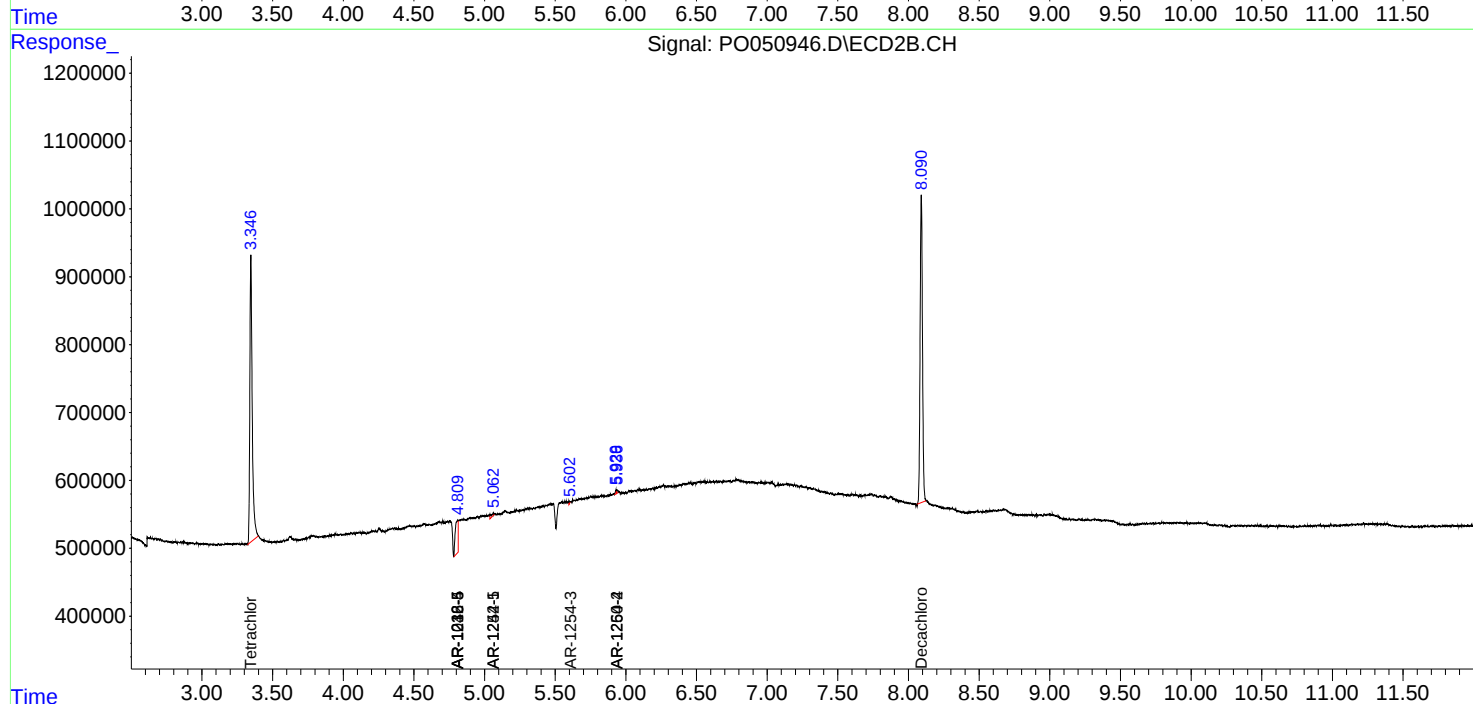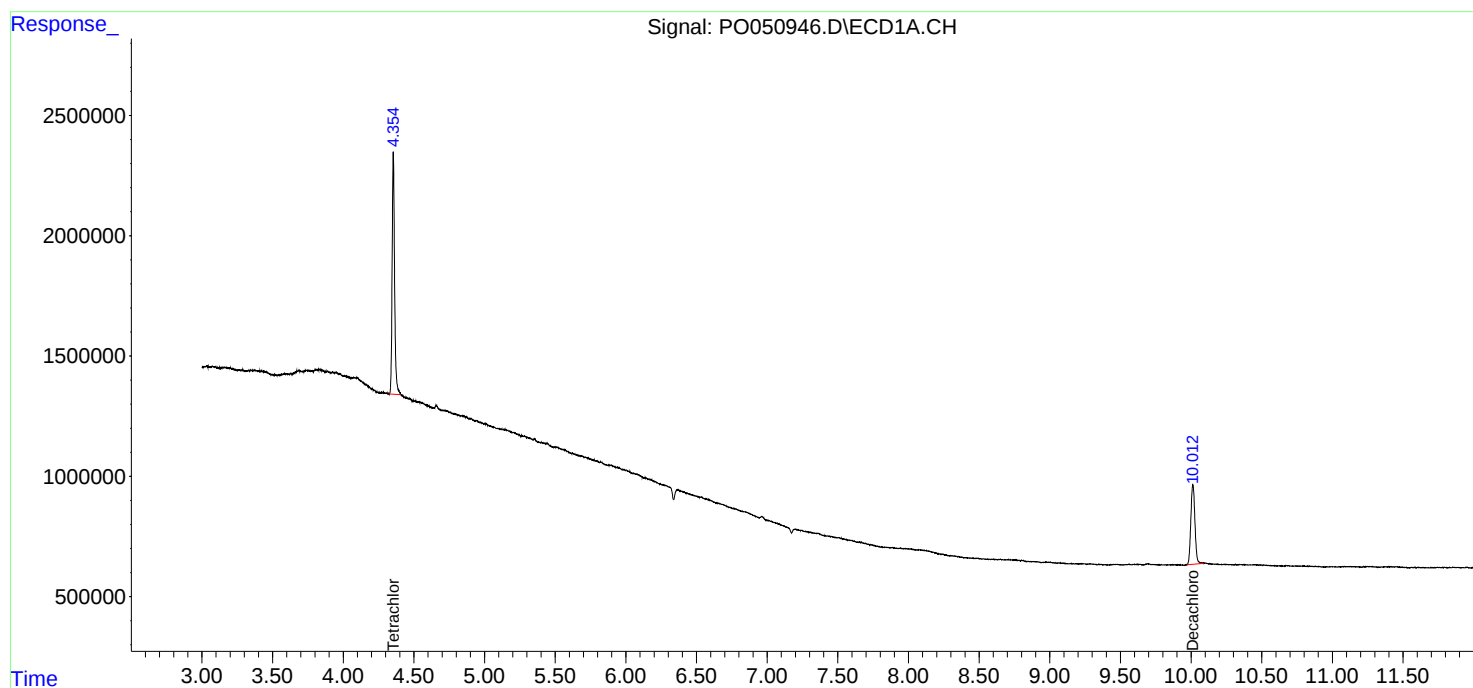


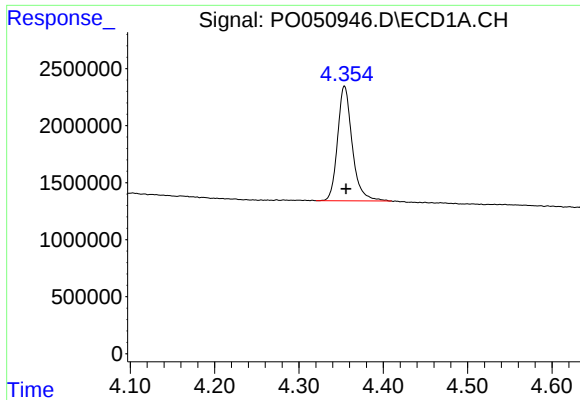

#1 Tetrachloro-m-xylene


R.T.: 4.354 min
Delta R.T.: -0.002 min
Response: 12108441
Conc: 24.22 ng/ml

Instrument :
ECD_O
ClientSampleId :

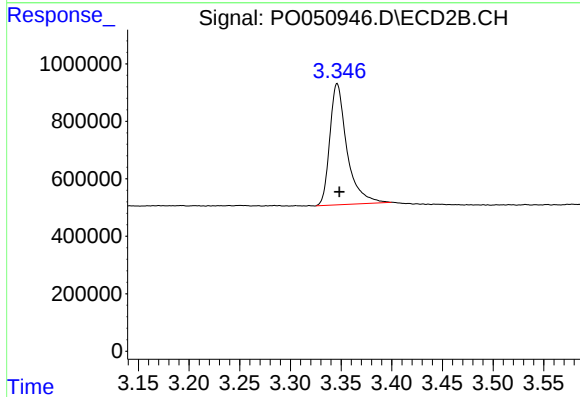


#1 Tetrachloro-m-xylene

R.T.: 3.346 min
Delta R.T.: -0.002 min
Response: 4978328
Conc: 22.90 ng/ml

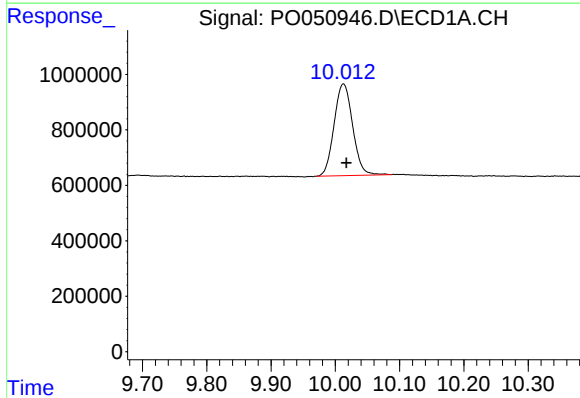


#2 Decachlorobiphenyl

R.T.: 10.012 min
Delta R.T.: -0.005 min
Response: 6632058
Conc: 21.34 ng/ml

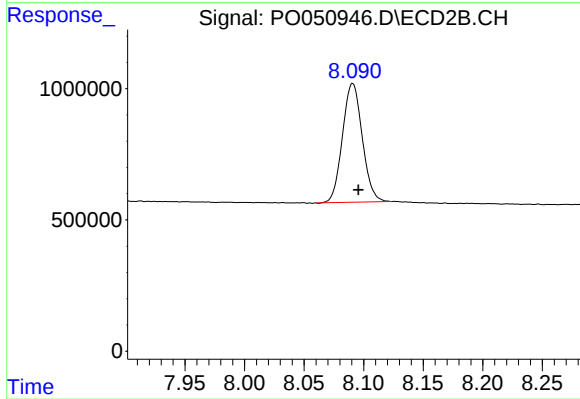

#2 Decachlorobiphenyl


R.T.: 8.091 min
Delta R.T.: -0.005 min
Response: 5236575
Conc: 20.47 ng/ml

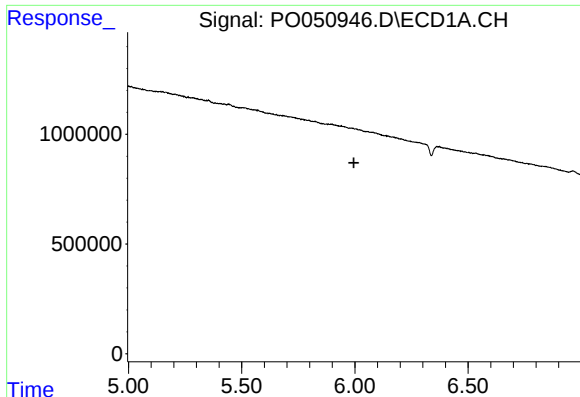

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.995 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

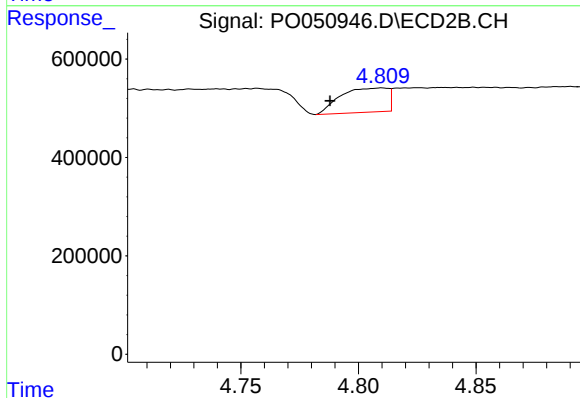


#7 AR-1016-5

R.T.: 4.810 min
Delta R.T.: 0.022 min
Response: 690803
Conc: 80.05 ng/ml

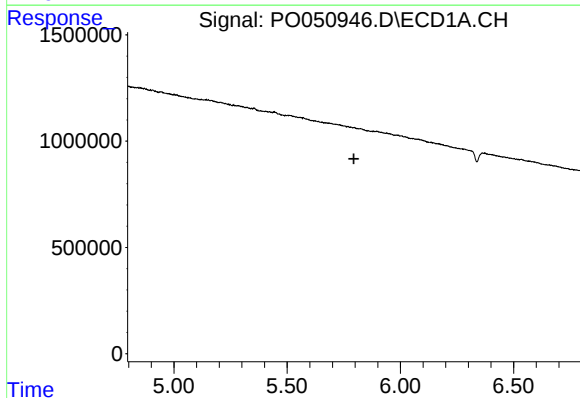


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.794 min
Response: 0
Conc: N.D.

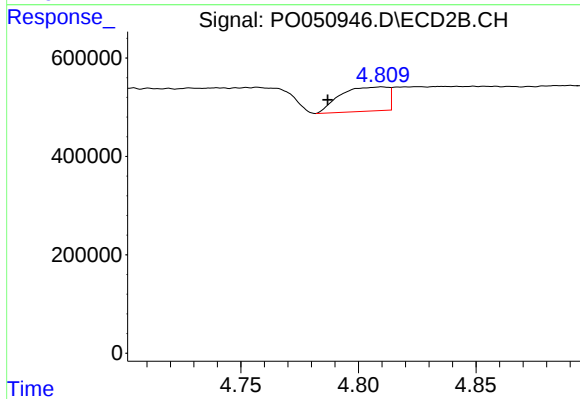

#15 AR-1232-5


R.T.: 4.810 min
Delta R.T.: 0.023 min
Response: 690803
Conc: 259.73 ng/ml

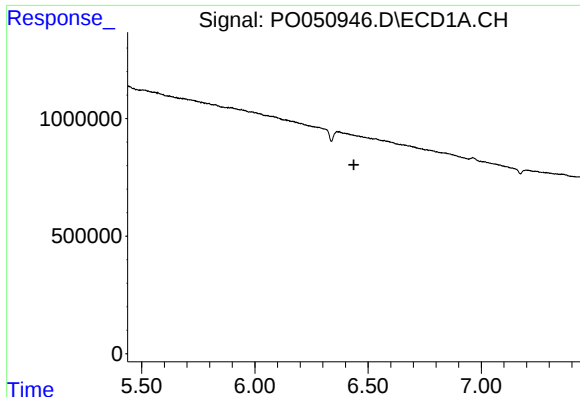

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

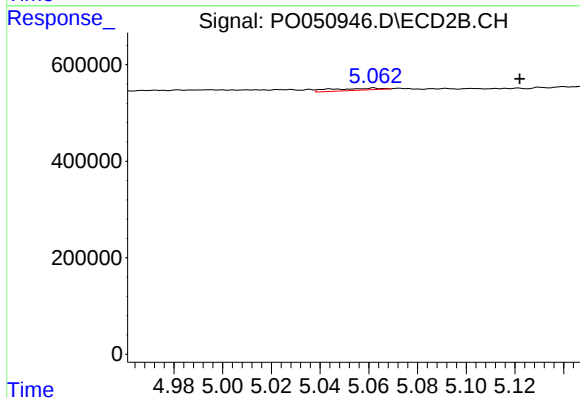


#20 AR-1242-5

R.T.: 5.062 min
Delta R.T.: -0.060 min
Response: 59515
Conc: 9.24 ng/ml

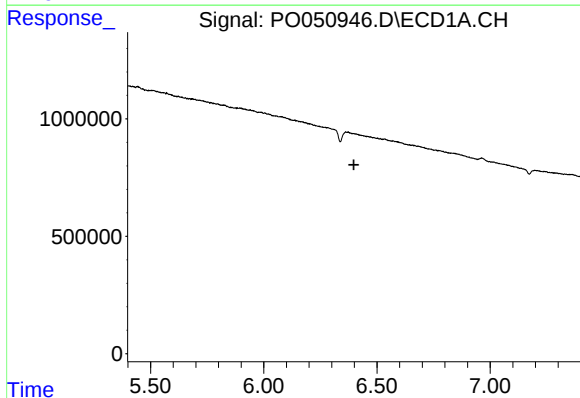


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

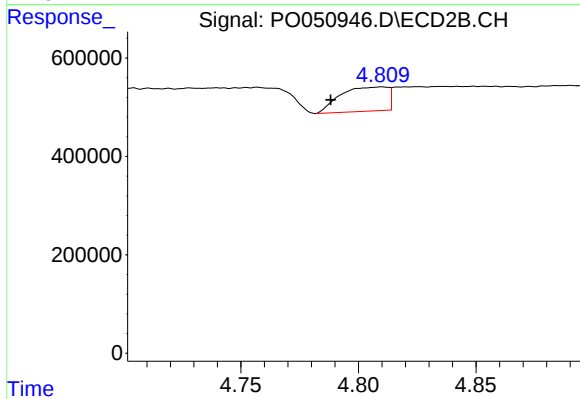

#24 AR-1248-4


R.T.: 4.810 min
Delta R.T.: 0.022 min
Response: 690803
Conc: 74.03 ng/ml

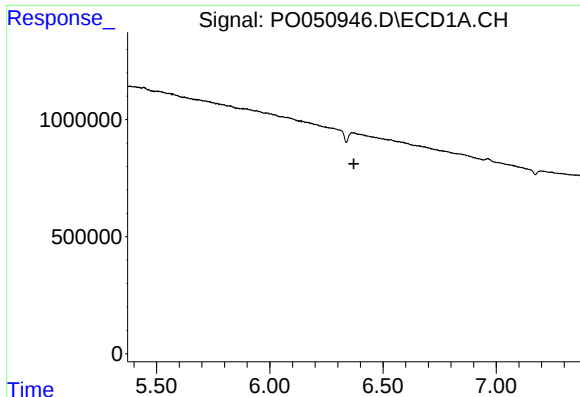

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

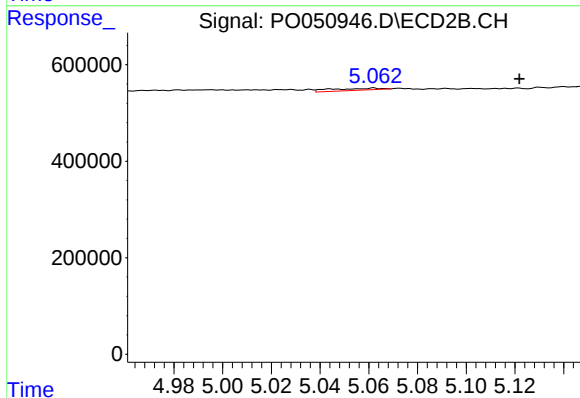


#26 AR-1254-1

R.T.: 5.062 min
Delta R.T.: -0.060 min
Response: 59515
Conc: 3.10 ng/ml

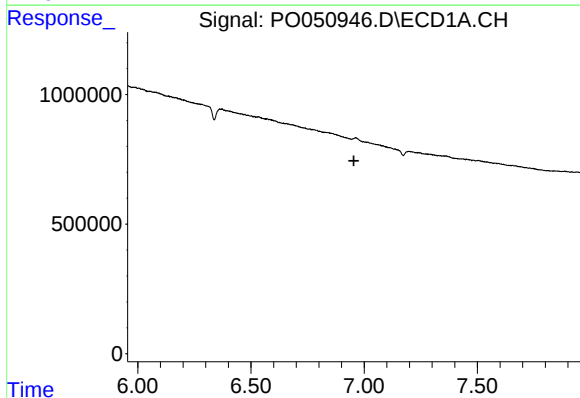


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.955 min
Response: 0
Conc: N.D.

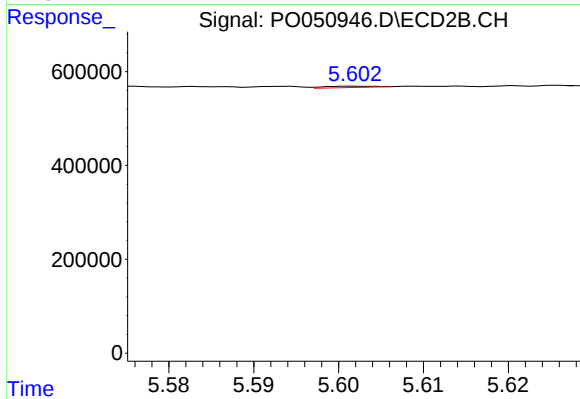

#28 AR-1254-3


R.T.: 5.602 min
Delta R.T.: -0.046 min
Response: 10631
Conc: 0.38 ng/ml

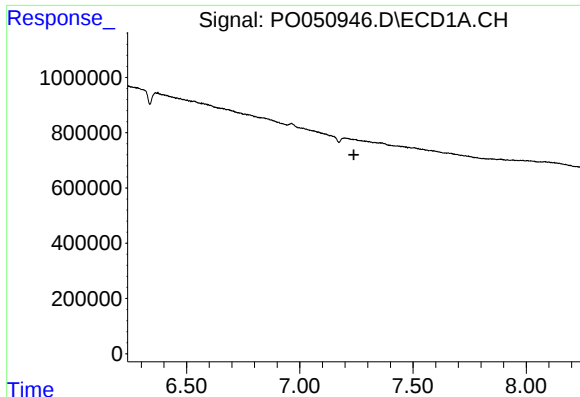

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

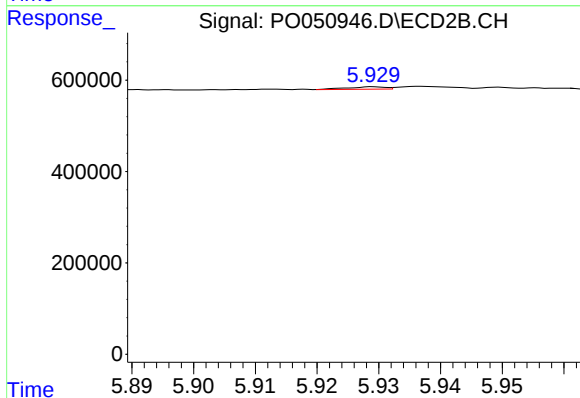


#29 AR-1254-4

R.T.: 5.929 min
Delta R.T.: 0.061 min
Response: 23332
Conc: 1.32 ng/ml

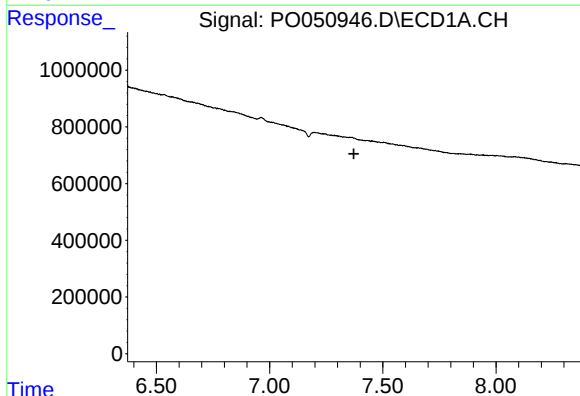

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

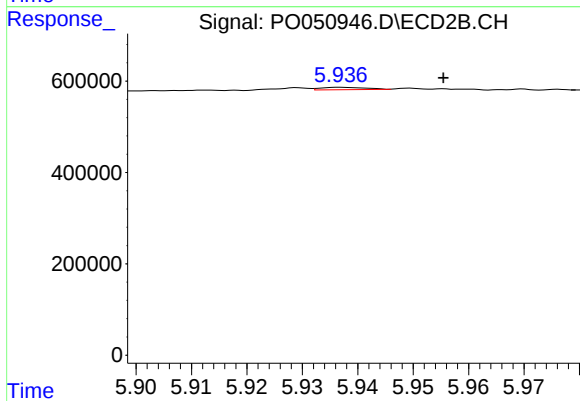

#32 AR-1260-2

R.T.: 5.937 min
Delta R.T.: -0.018 min
Response: 28789
Conc: 1.00 ng/ml