

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110218\
 Data File : P0050974.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2018 18:40
 Operator : SM/SJ
 Sample : J5789-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 103118-SIDI-E-D-M

Manual Integrations
 APPROVED

Sohil

11/6/2018 10:10:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 23:15:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.346	10772060	3990446	21.550	18.359m
2) SA Decachlor...	10.007	8.090	6371509	5753310	20.499	22.493

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110218\
Data File : PO050974.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2018 18:40
Operator : SM/SJ
Sample : J5789-05
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
103118-SIDI-E-D-M



Manual Integrations
APPROVED


Sohil

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:15:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

11/6/2018 10:10:11 AM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

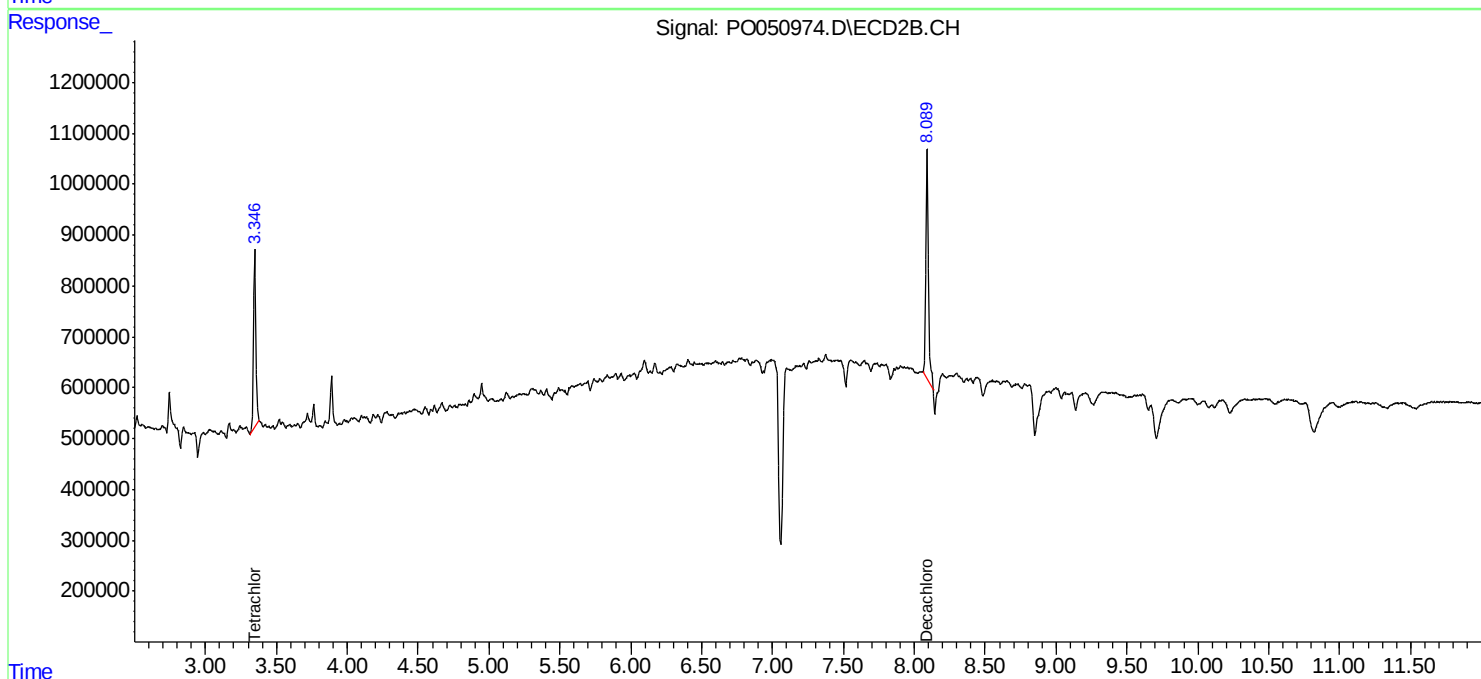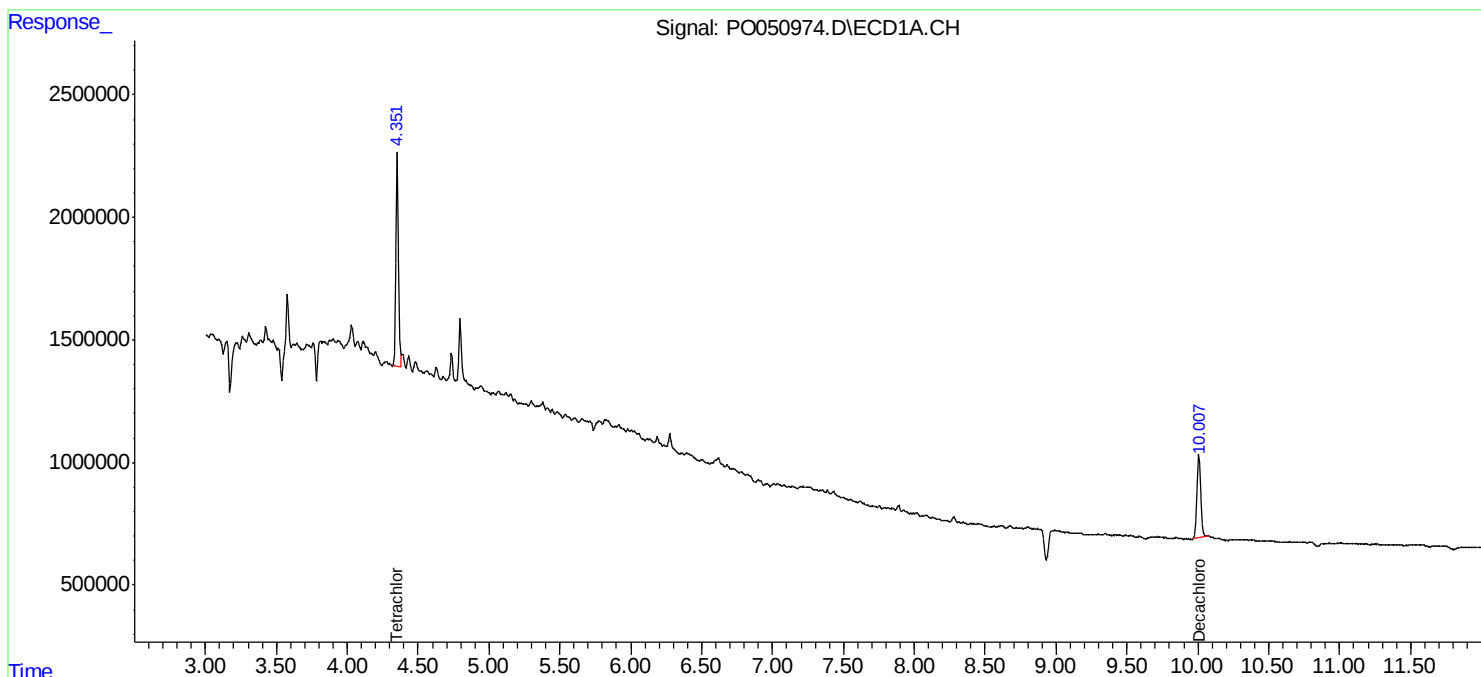

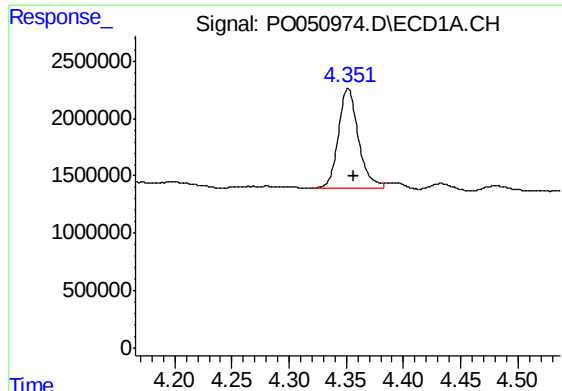

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.005 min
Response: 10772060
Conc: 21.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
103118-SIDI-E-D-M

Manual Integrations
APPROVED


Sohil

11/6/2018 10:10:11 AM

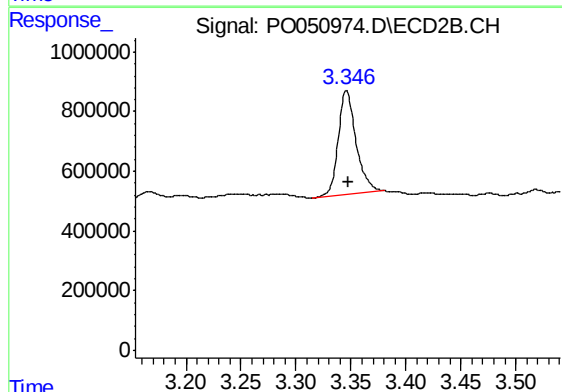


#1 Tetrachloro-m-xylene

R.T.: 3.346 min
Delta R.T.: -0.003 min
Response: 3990446
Conc: 18.36 ng/ml m

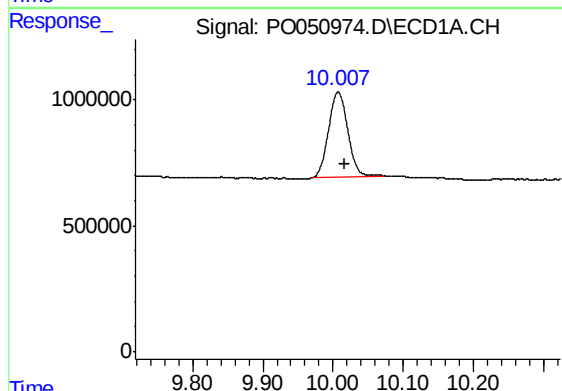

#2 Decachlorobiphenyl

R.T.: 10.007 min
Delta R.T.: -0.010 min
Response: 6371509
Conc: 20.50 ng/ml

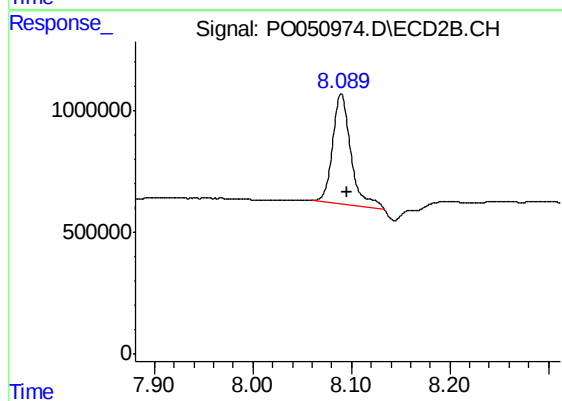

#2 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: -0.006 min
Response: 5753310
Conc: 22.49 ng/ml