

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110218\
 Data File : P0051002.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2018 2:33
 Operator : SM/SJ
 Sample : J5769-07
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LEFT-CORNER-BULDG-85

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 03:49:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.351	3.345	9227561	3803915	18.460	17.501
2)	SA Decachlor...	10.006	8.089	4410041	3734553	14.188	14.600

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110218\
Data File : PO051002.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2018 2:33
Operator : SM/SJ
Sample : J5769-07
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LEFT-CORNER-BULDG-85

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 03:49:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

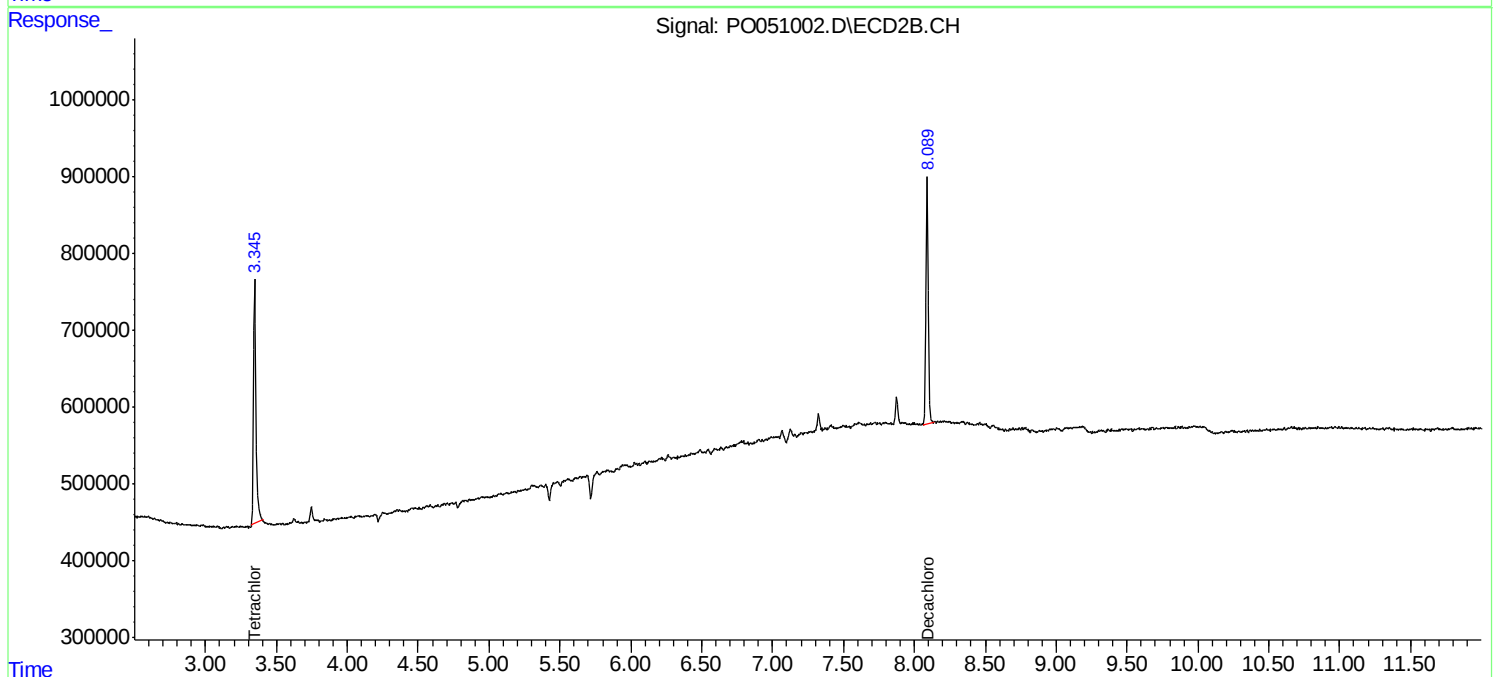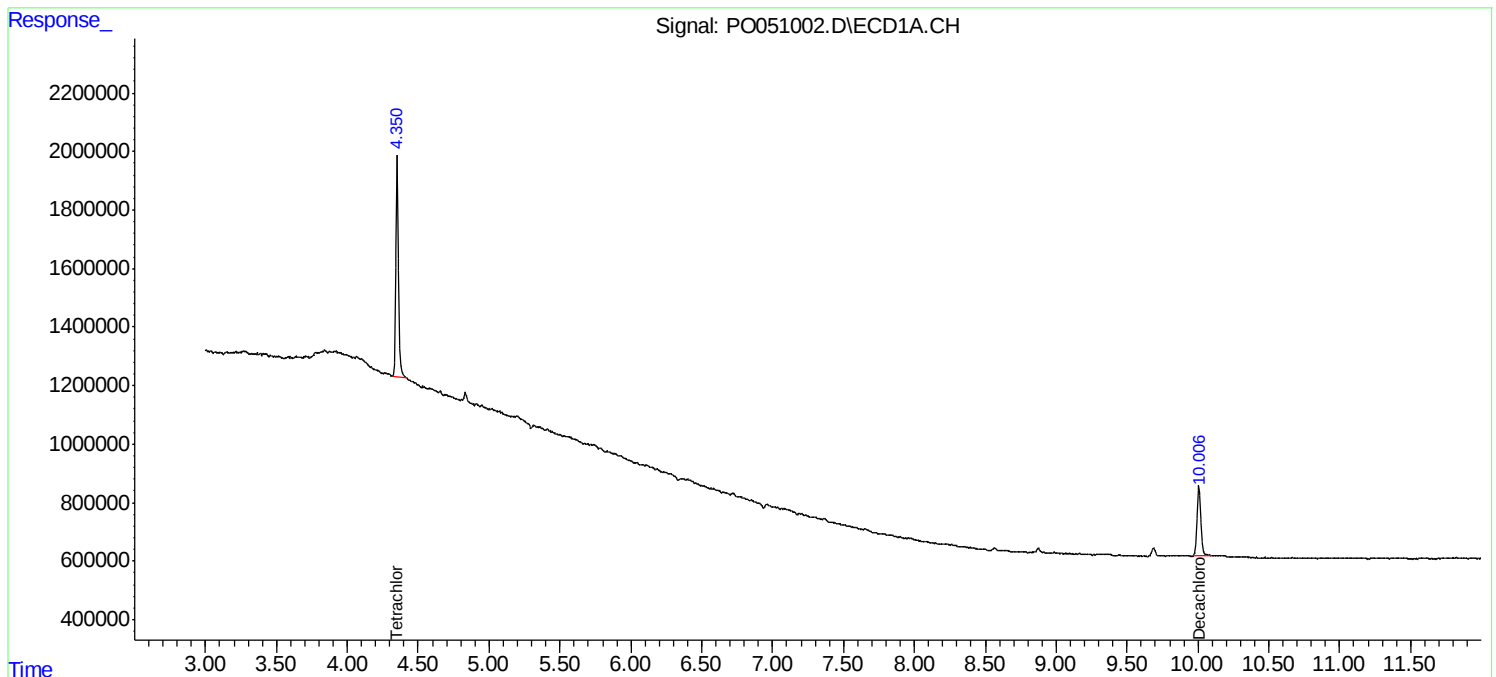


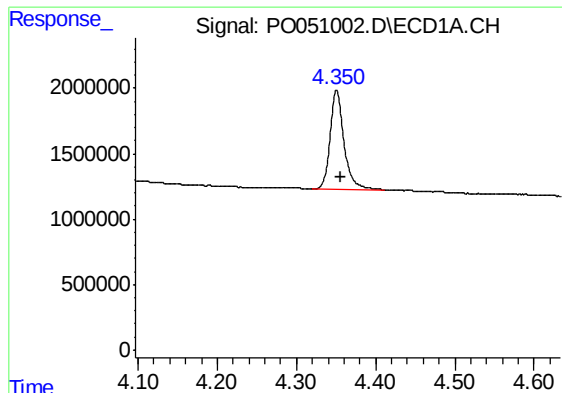

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.005 min
Response: 9227561
Conc: 18.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LEFT-CORNER-BULDG-85

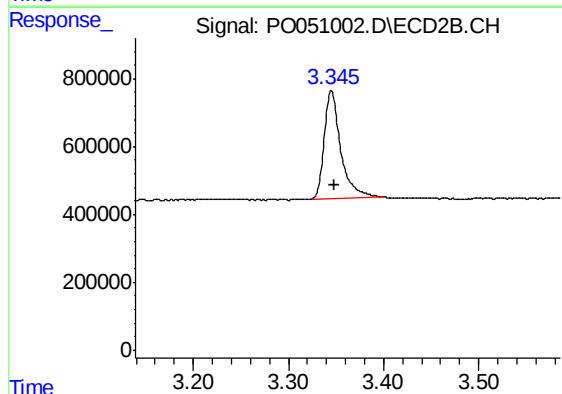


#1 Tetrachloro-m-xylene

R.T.: 3.345 min
Delta R.T.: -0.003 min
Response: 3803915
Conc: 17.50 ng/ml

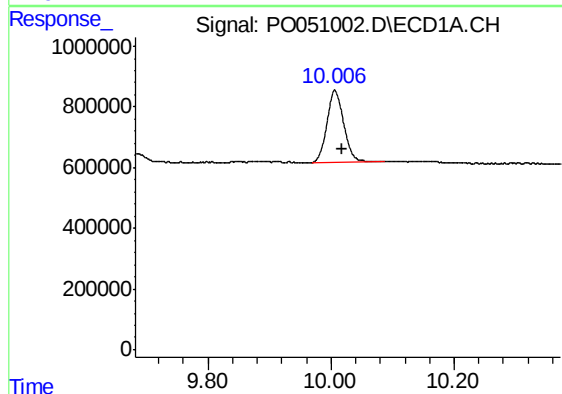

#2 Decachlorobiphenyl

R.T.: 10.006 min
Delta R.T.: -0.011 min
Response: 4410041
Conc: 14.19 ng/ml

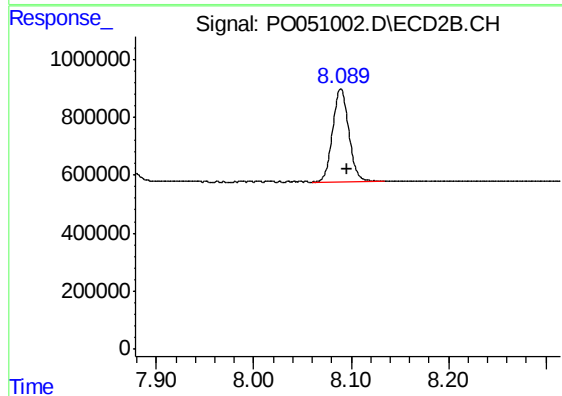

#2 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: -0.006 min
Response: 3734553
Conc: 14.60 ng/ml