

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110218\
Data File : P0051026.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2018 9:52
Operator : SM/SJ
Sample : J5794-11
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-10B-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 03:08:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.351	3.346	12631710	5196552	25.271	23.908
2)	SA Decachlor...	10.006	8.089	5290518	3471610	17.021	13.572

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110218\
Data File : P0051026.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2018 9:52
Operator : SM/SJ
Sample : J5794-11
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-10B-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 03:08:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

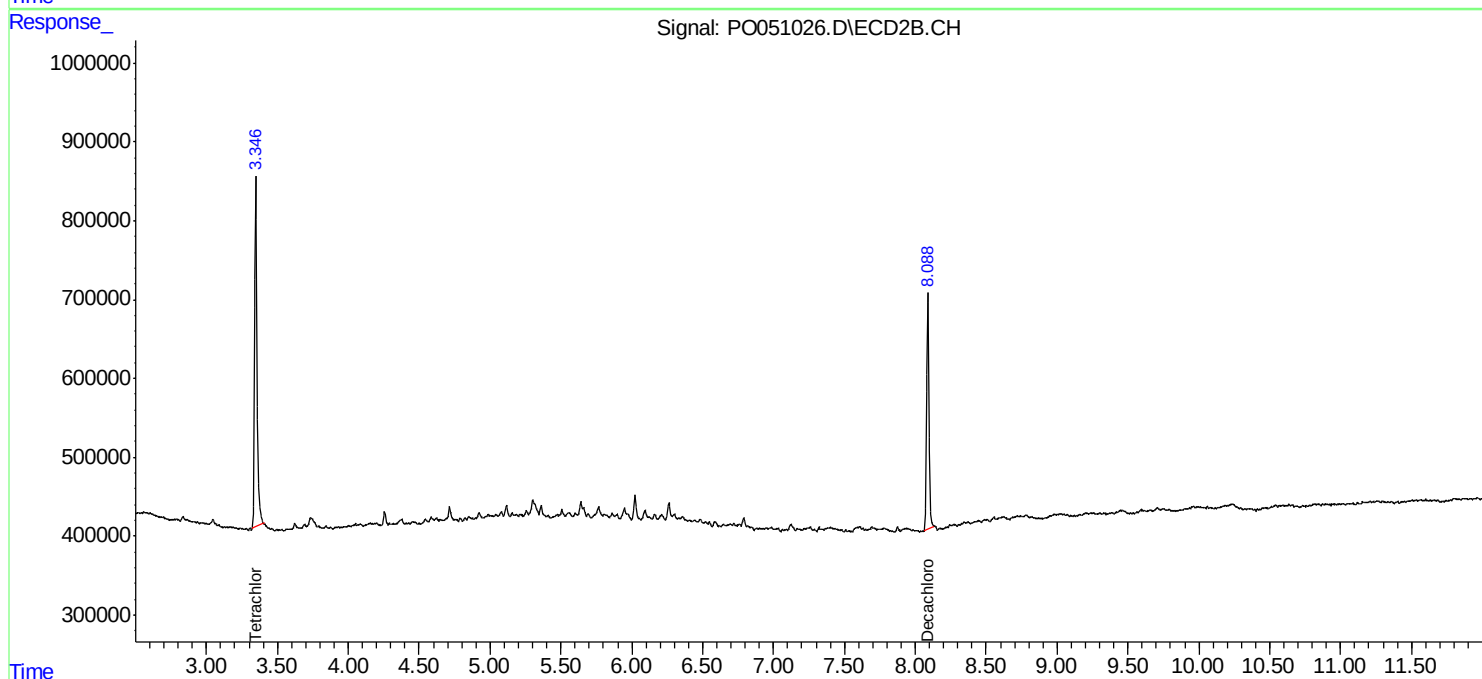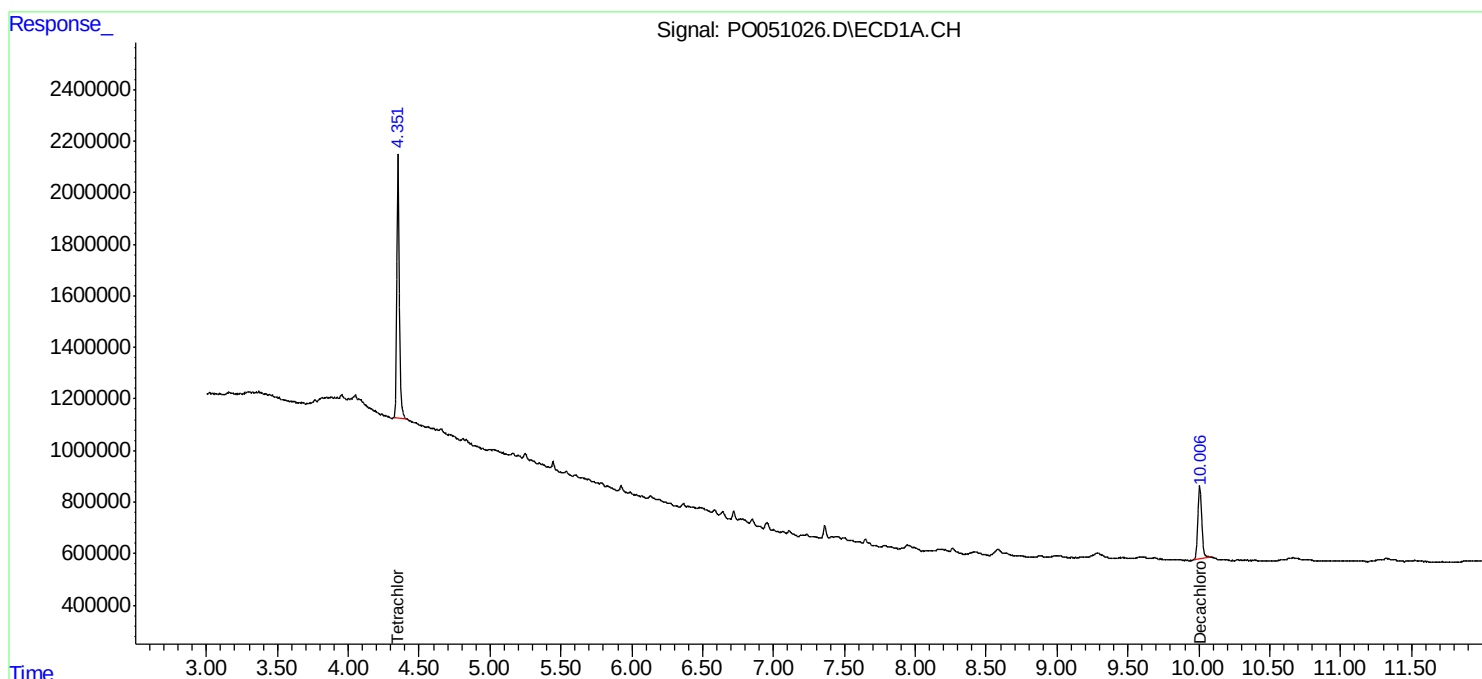


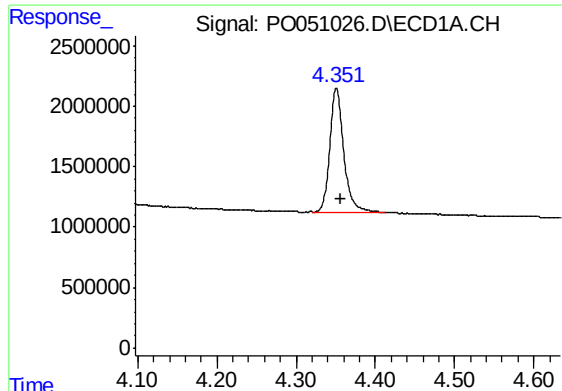

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.005 min
Response: 12631710
Conc: 25.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-10B-S

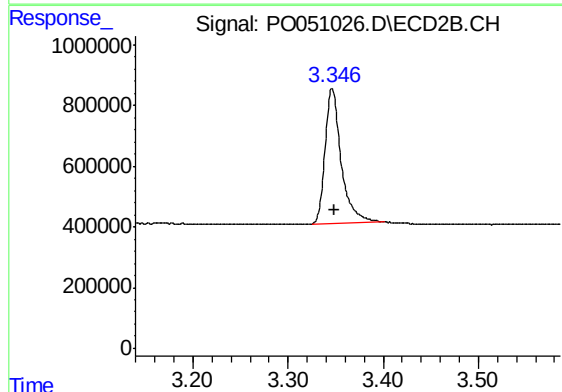


#1 Tetrachloro-m-xylene

R.T.: 3.346 min
Delta R.T.: -0.002 min
Response: 5196552
Conc: 23.91 ng/ml

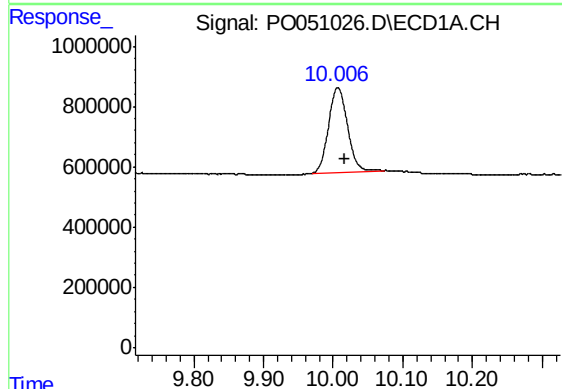

#2 Decachlorobiphenyl

R.T.: 10.006 min
Delta R.T.: -0.011 min
Response: 5290518
Conc: 17.02 ng/ml

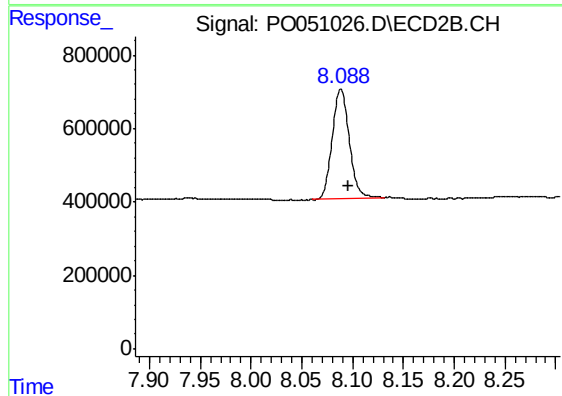

#2 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: -0.007 min
Response: 3471610
Conc: 13.57 ng/ml